
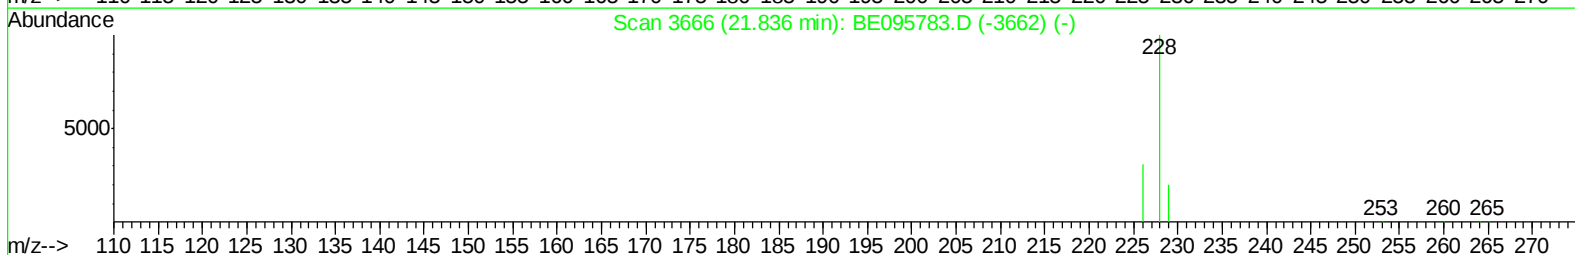
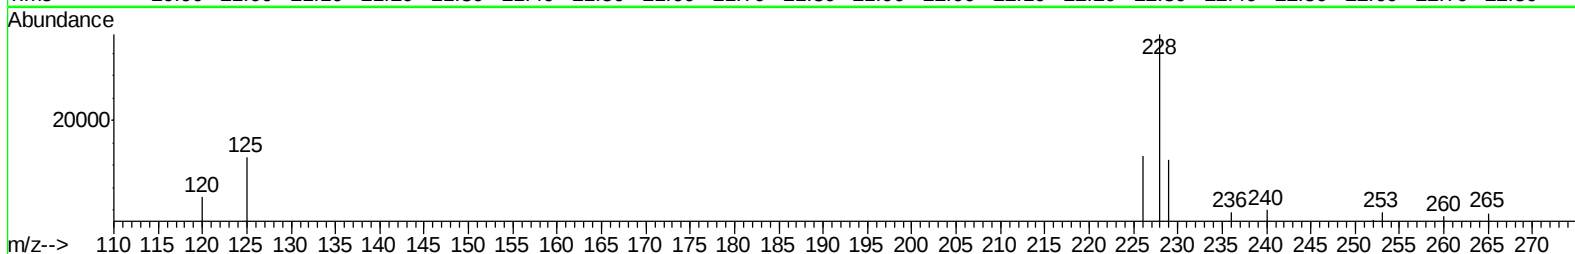


Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\  
Data File : BE095788.D  
Acq On : 15 Mar 2018 5:32  
Operator : SJ/JU  
Sample : J1835-15  
Misc :  
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Mar 15 08:48:52 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 15 05:35:28 2018  
Response via : Initial Calibration

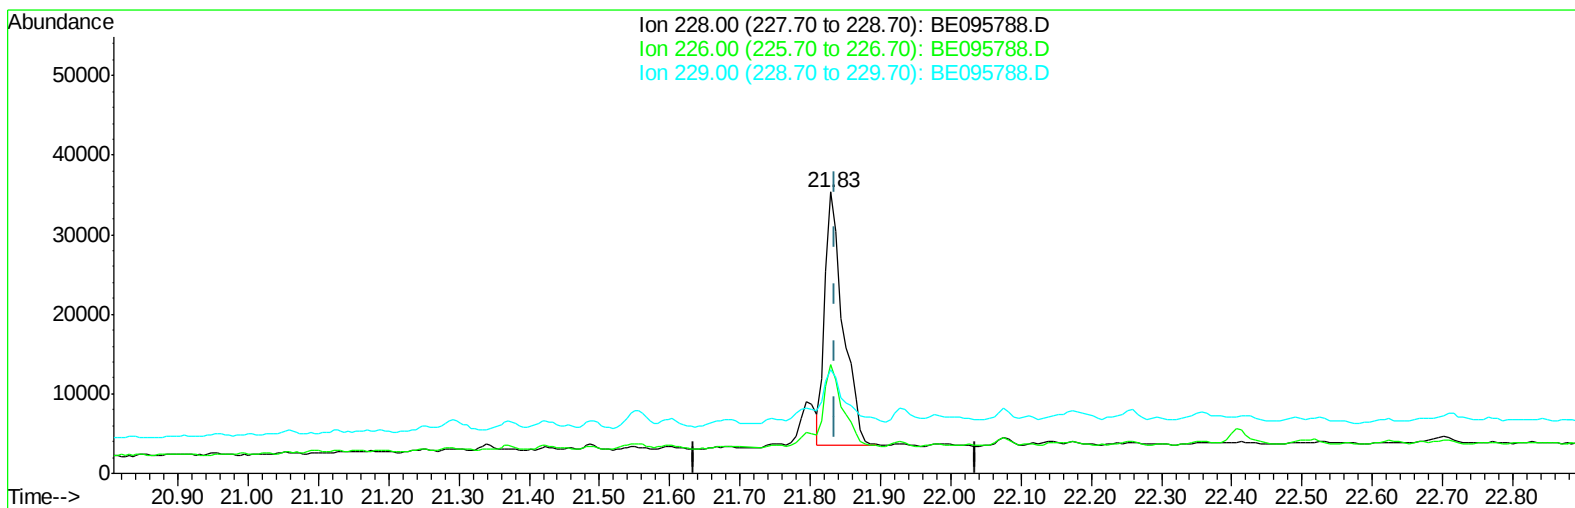

TIC: BE095788.D

(19) Chrysene

21.829min (-0.006) 1.97ng/ul m

response 57078

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 228.00 | 100   | 100    |
| 226.00 | 29.20 | 38.50# |
| 229.00 | 22.10 | 36.91# |
| 0.00   | 0.00  | 0.00   |