
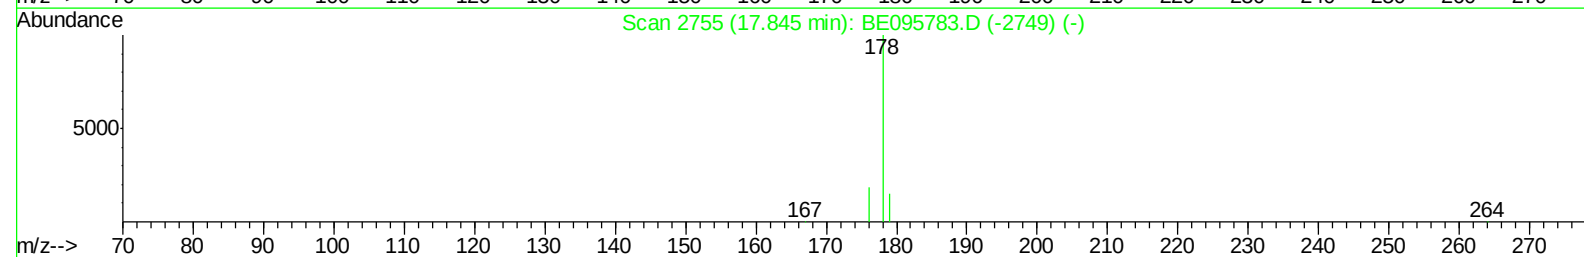
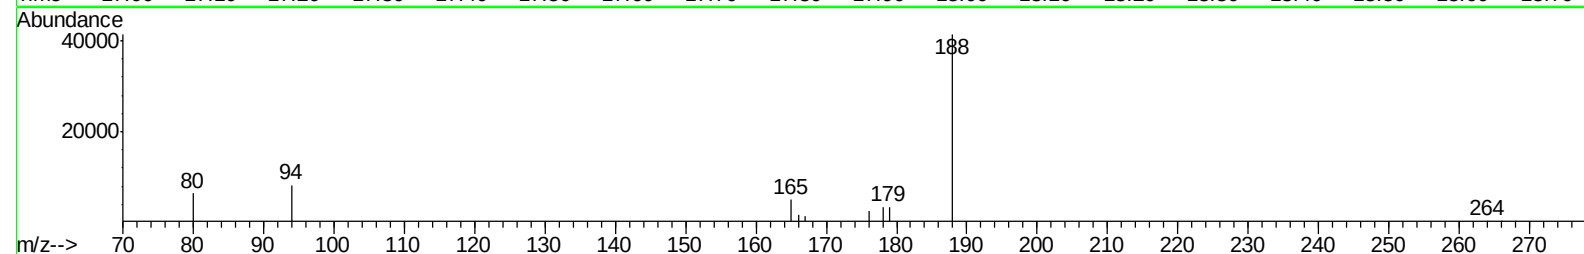


Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
Data File : BE095789.D
Acq On : 15 Mar 2018 6:08
Operator : SJ/JU
Sample : J1835-17
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Mar 15 08:55:22 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 15 05:35:28 2018
Response via : Initial Calibration

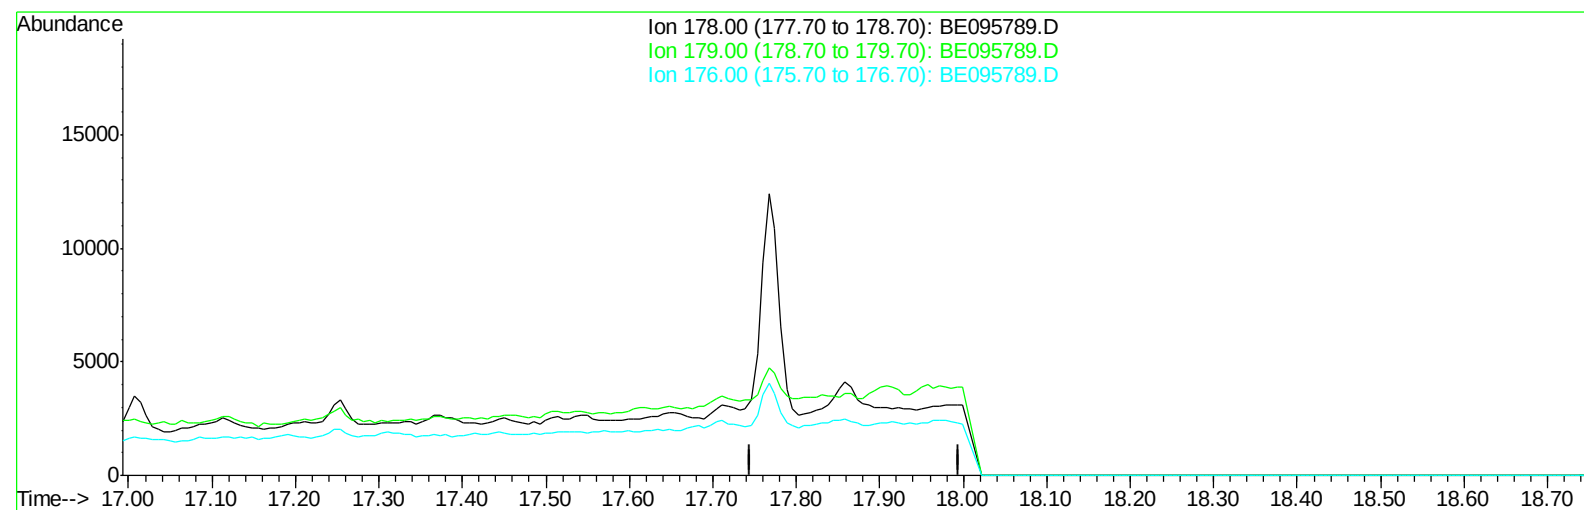

TIC: BE095789.D

(13) Anthracene

17.845min (-17.845) 0.00ng/ul

response 0

Ion	Exp%	Act%
178.00	100	0.00
179.00	22.60	0.00#
176.00	18.40	0.00#
0.00	0.00	0.00