
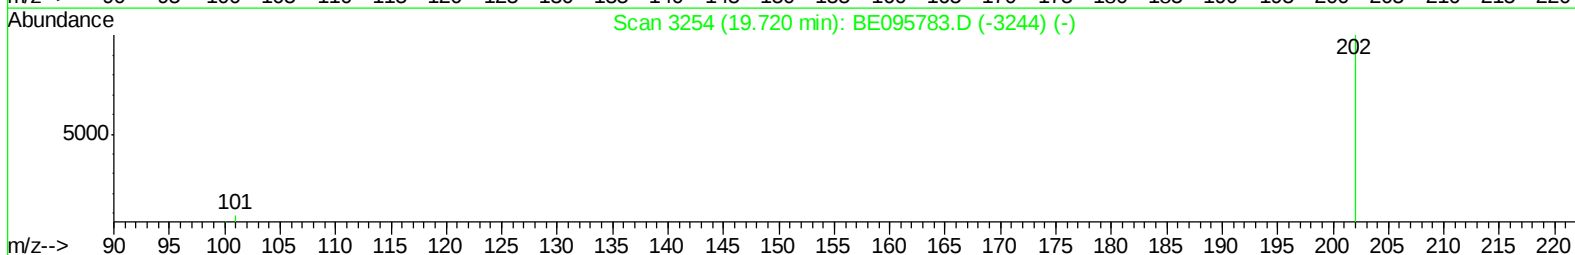
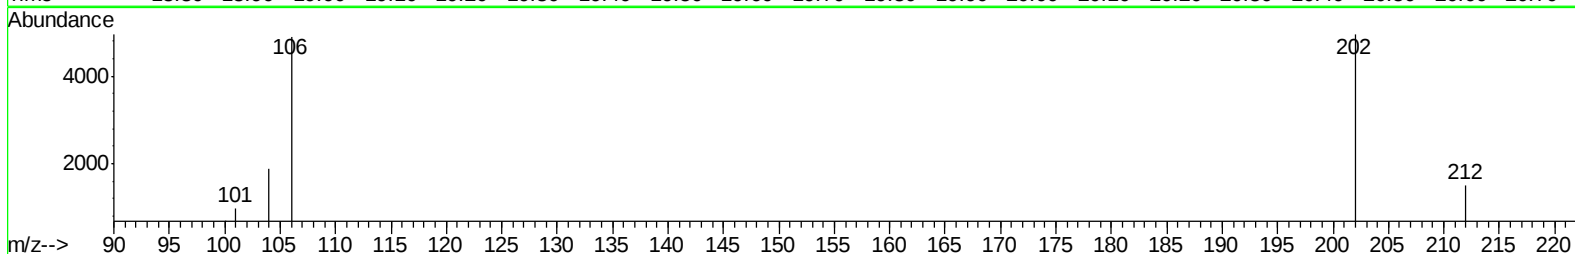


Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
Data File : BE095789.D
Acq On : 15 Mar 2018 6:08
Operator : SJ/JU
Sample : J1835-17
Misc :
ALS Vial : 33 Sample Multiplier: 1

Quant Time: Mar 15 08:55:22 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 15 05:35:28 2018
Response via : Initial Calibration

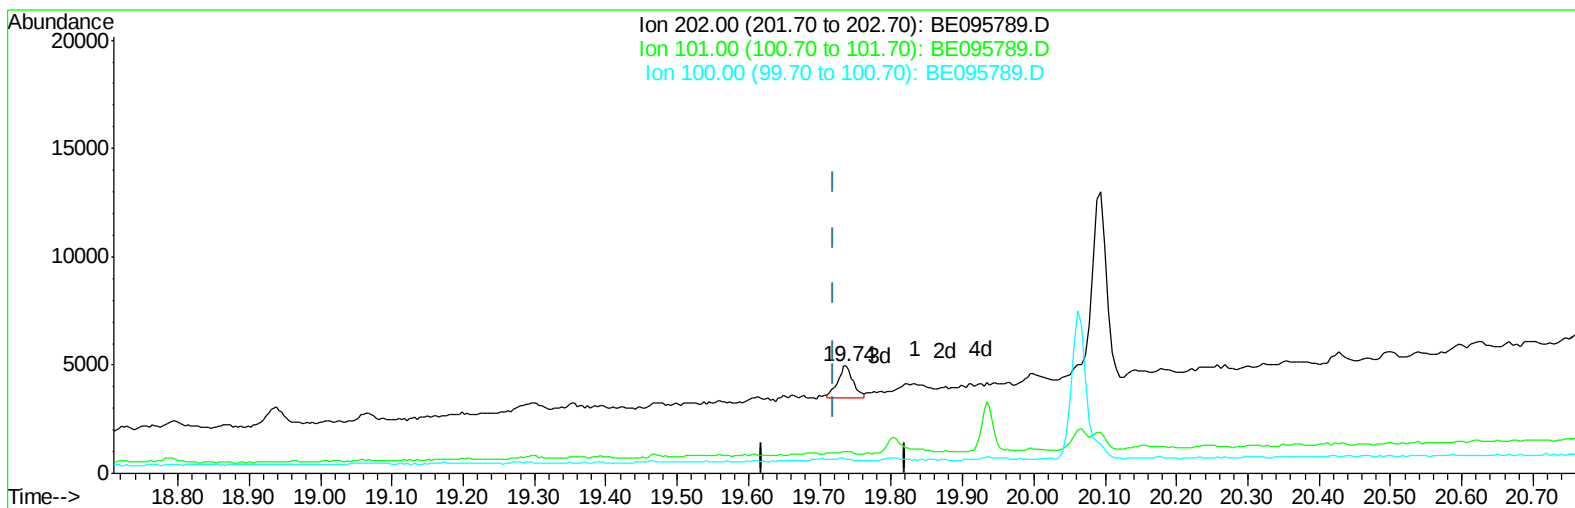

TIC: BE095789.D

(15) Fluoranthene (C)

19.737min (+0.018) 0.07ng/ul m

response 2281

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	19.78
100.00	19.50	13.68
0.00	0.00	0.00