
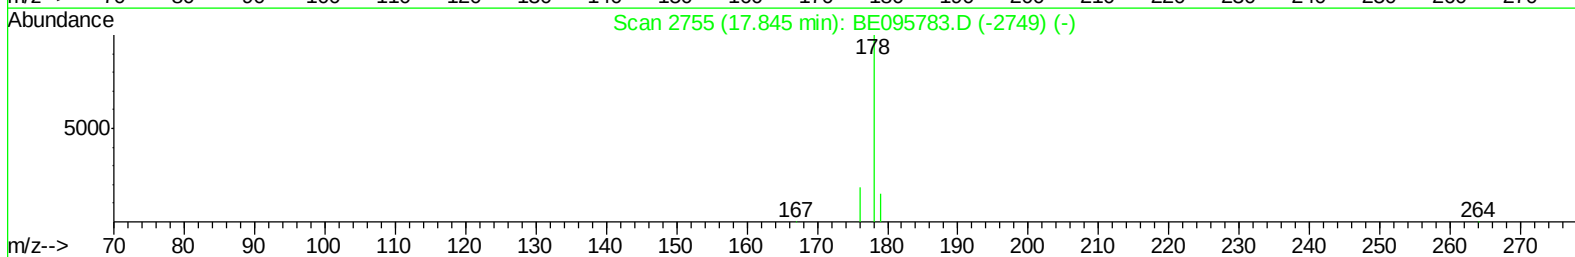
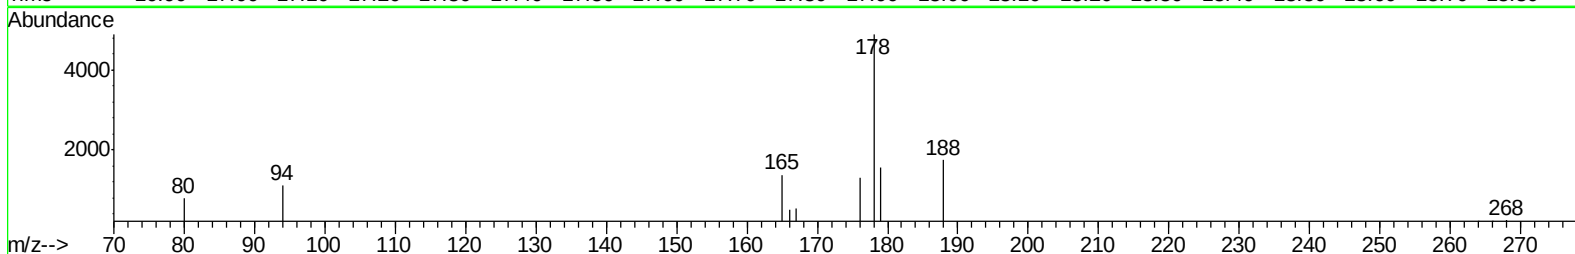


Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
Data File : BE095790.D
Acq On : 15 Mar 2018 6:43
Operator : SJ/JU
Sample : J1835-12
Misc :
ALS Vial : 34 Sample Multiplier: 1

Quant Time: Mar 15 08:59:29 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 15 05:35:28 2018
Response via : Initial Calibration

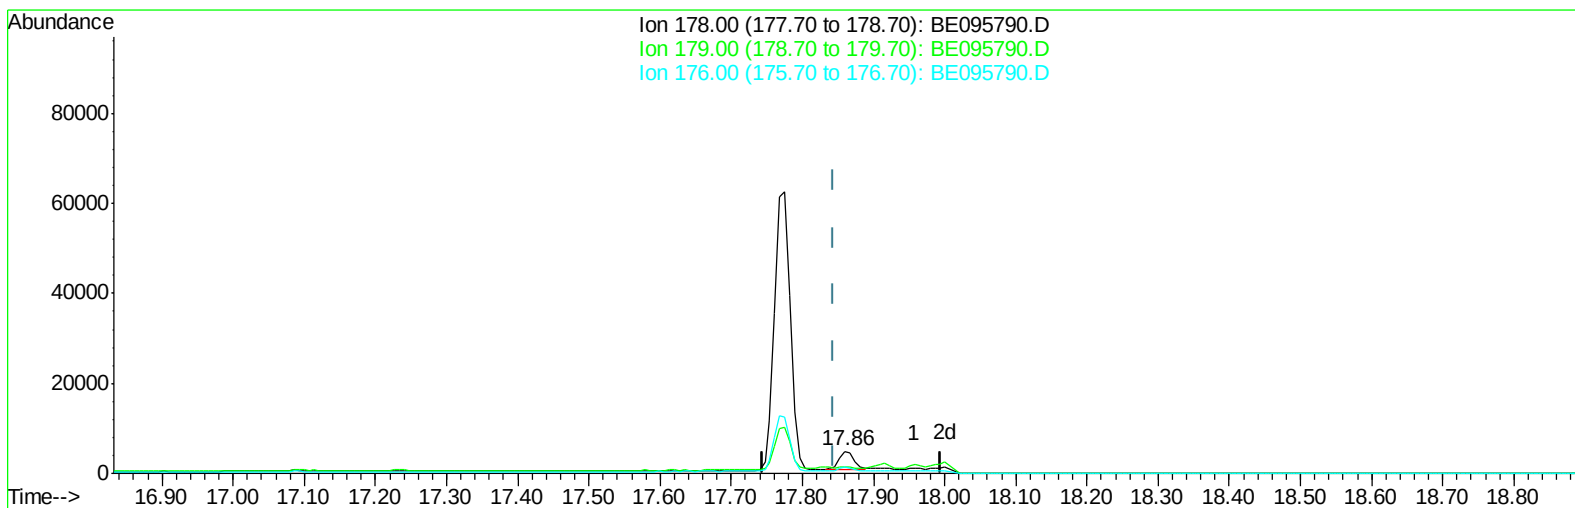

TIC: BE095790.D

(13) Anthracene

17.860min (+0.015) 0.26ng/ul m

response 5926

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	31.50#
176.00	18.40	26.73#
0.00	0.00	0.00