
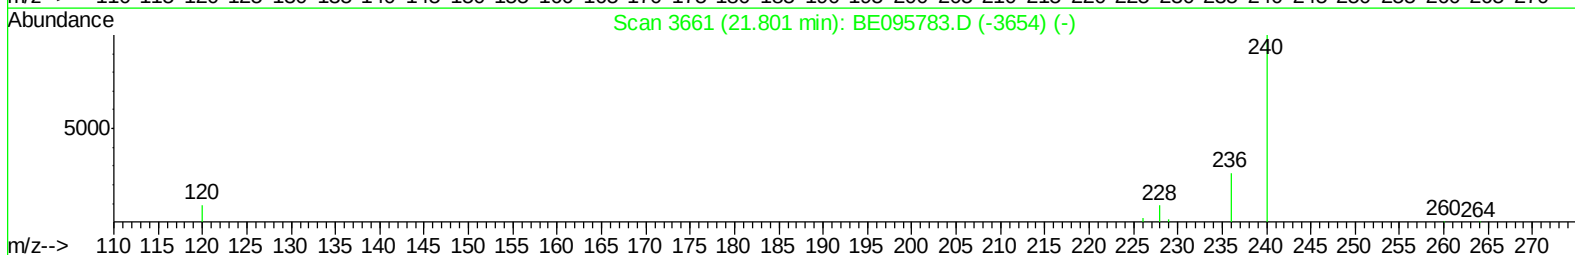
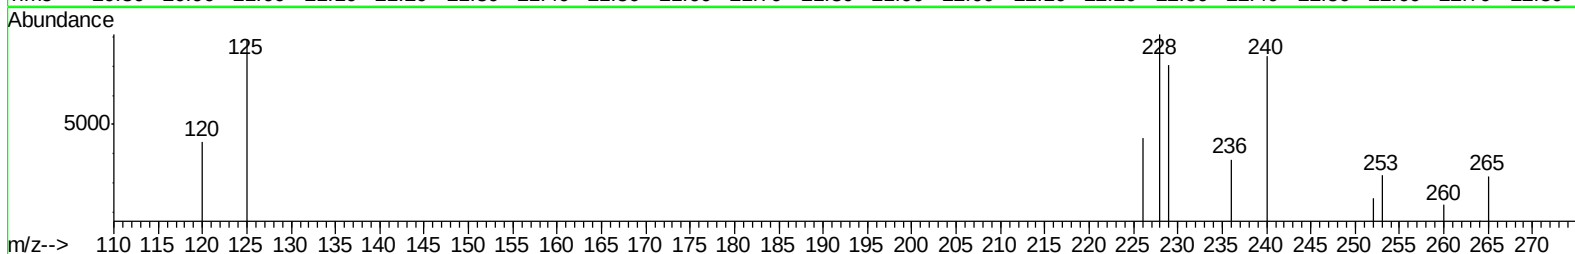


Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
Data File : BE095790.D
Acq On : 15 Mar 2018 6:43
Operator : SJ/JU
Sample : J1835-12
Misc :
ALS Vial : 34 Sample Multiplier: 1

Quant Time: Mar 15 08:59:29 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 15 05:35:28 2018
Response via : Initial Calibration

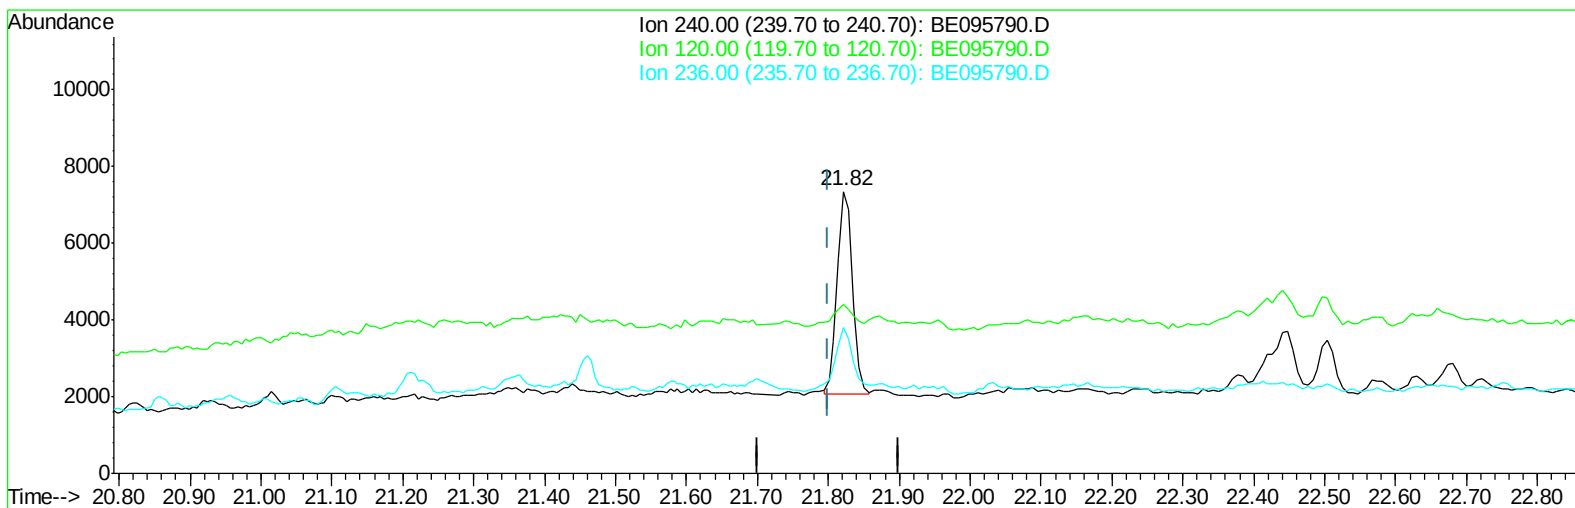

TIC: BE095790.D

(16) Chrysene-d12 (I)

21.822min (+0.021) 0.40ng/ul m

response 7856

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	60.06#
236.00	34.90	51.88#
0.00	0.00	0.00