
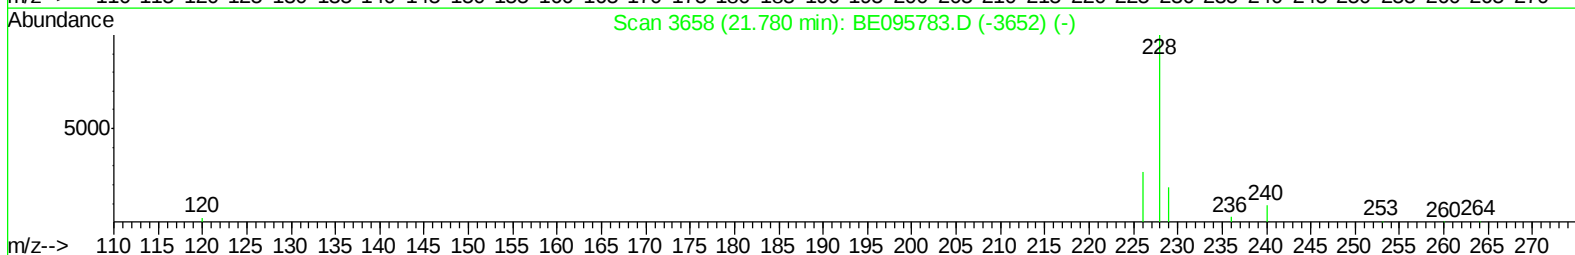
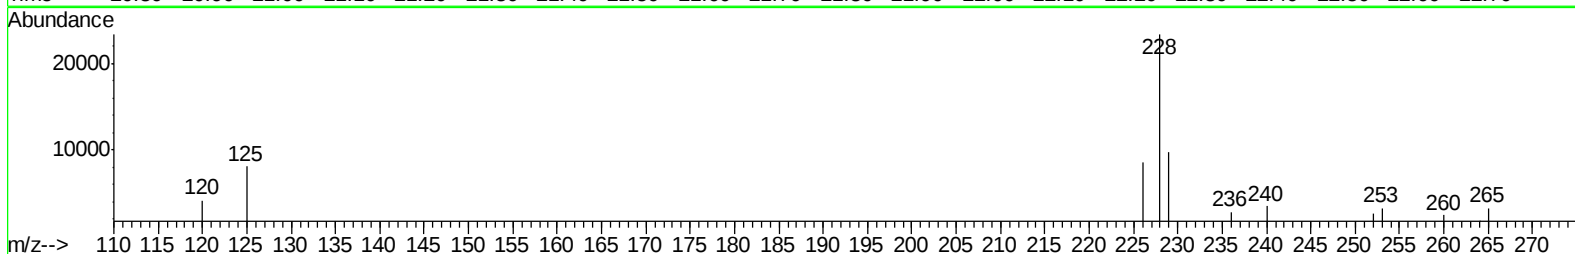


Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
Data File : BE095790.D
Acq On : 15 Mar 2018 6:43
Operator : SJ/JU
Sample : J1835-12
Misc :
ALS Vial : 34 Sample Multiplier: 1

Quant Time: Mar 15 09:01:05 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 15 05:35:28 2018
Response via : Initial Calibration

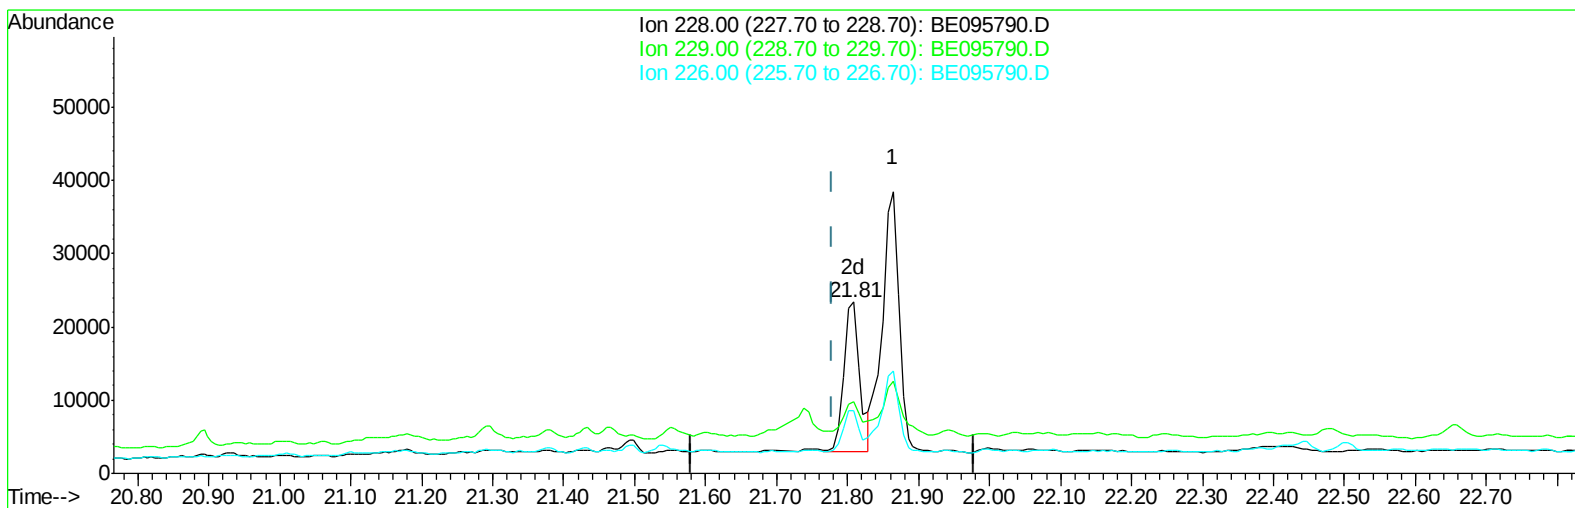

TIC: BE095790.D

(18) Benzo(a)anthracene

21.808min (+0.028) 1.25ng/ul m

response 31784

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	41.88#
226.00	21.30	36.67#
0.00	0.00	0.00