
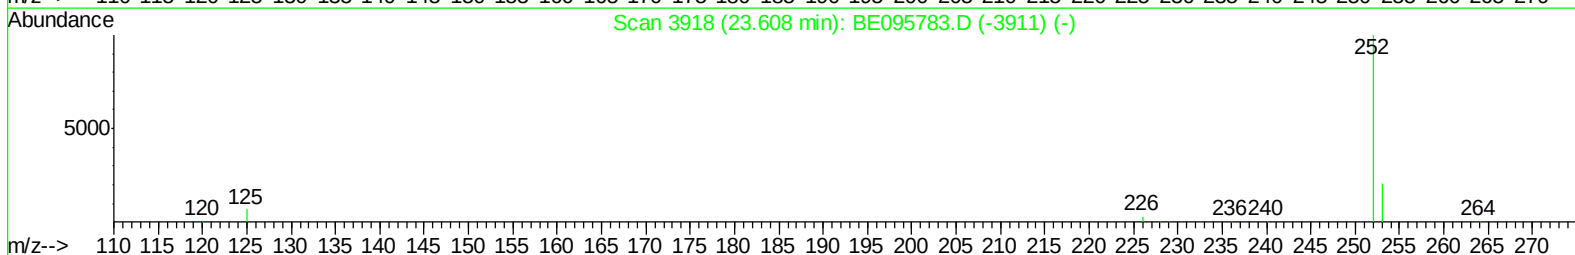
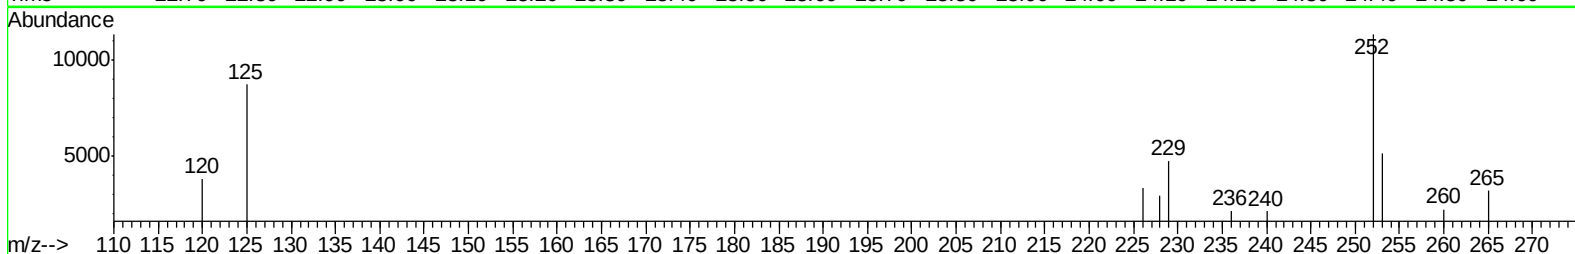


Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\  
Data File : BE095790.D  
Acq On : 15 Mar 2018 6:43  
Operator : SJ/JU  
Sample : J1835-12  
Misc :  
ALS Vial : 34 Sample Multiplier: 1

Quant Time: Mar 15 09:02:03 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 15 05:35:28 2018  
Response via : Initial Calibration

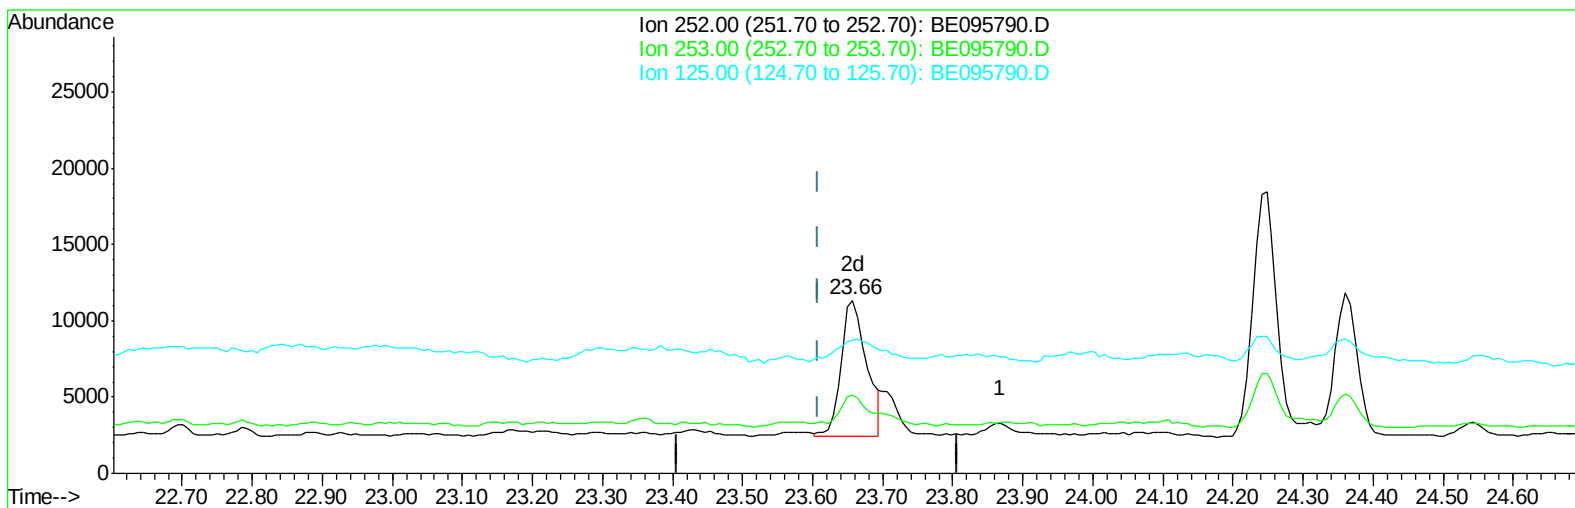

TIC: BE095790.D

(21) Benzo(b)fluoranthene

23.657min (+0.049) 0.86ng/ul m

response 22404

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 32.10 | 45.21  |
| 125.00 | 17.50 | 76.95# |
| 0.00   | 0.00  | 0.00   |