
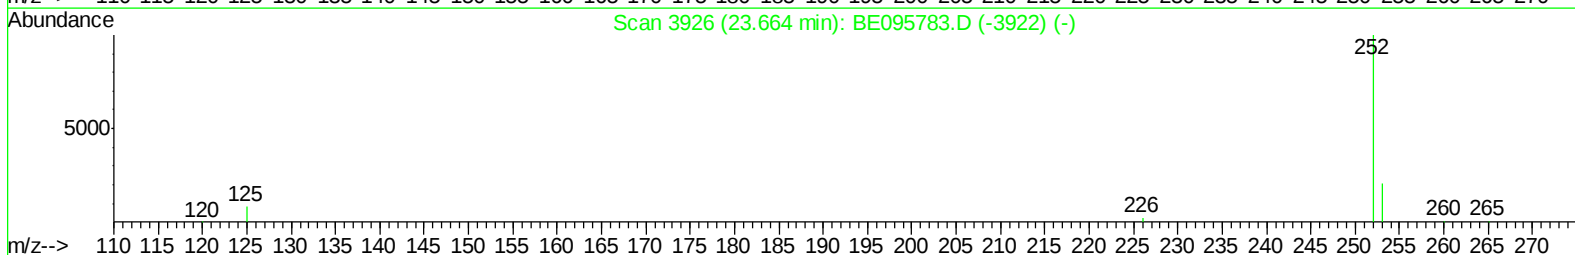
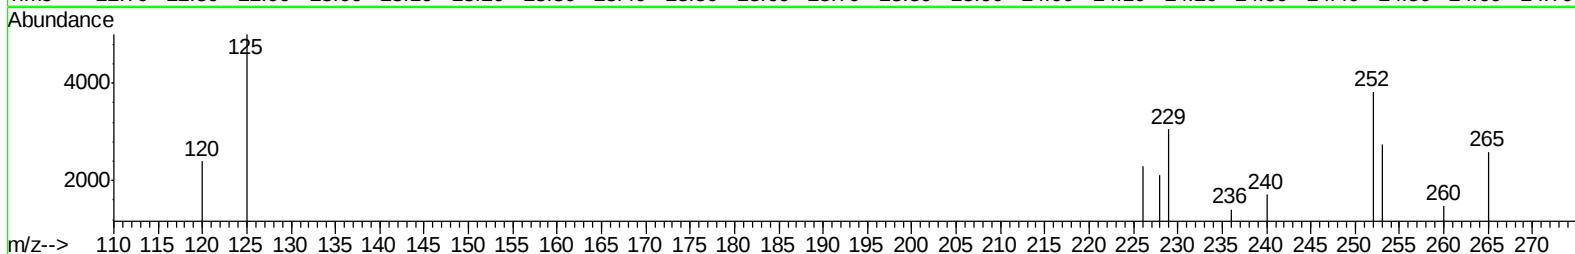


Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\  
Data File : BE095791.D  
Acq On : 15 Mar 2018 7:22  
Operator : SJ/JU  
Sample : J1835-13  
Misc :  
ALS Vial : 35 Sample Multiplier: 1

Quant Time: Mar 15 09:07:08 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 15 05:35:28 2018  
Response via : Initial Calibration

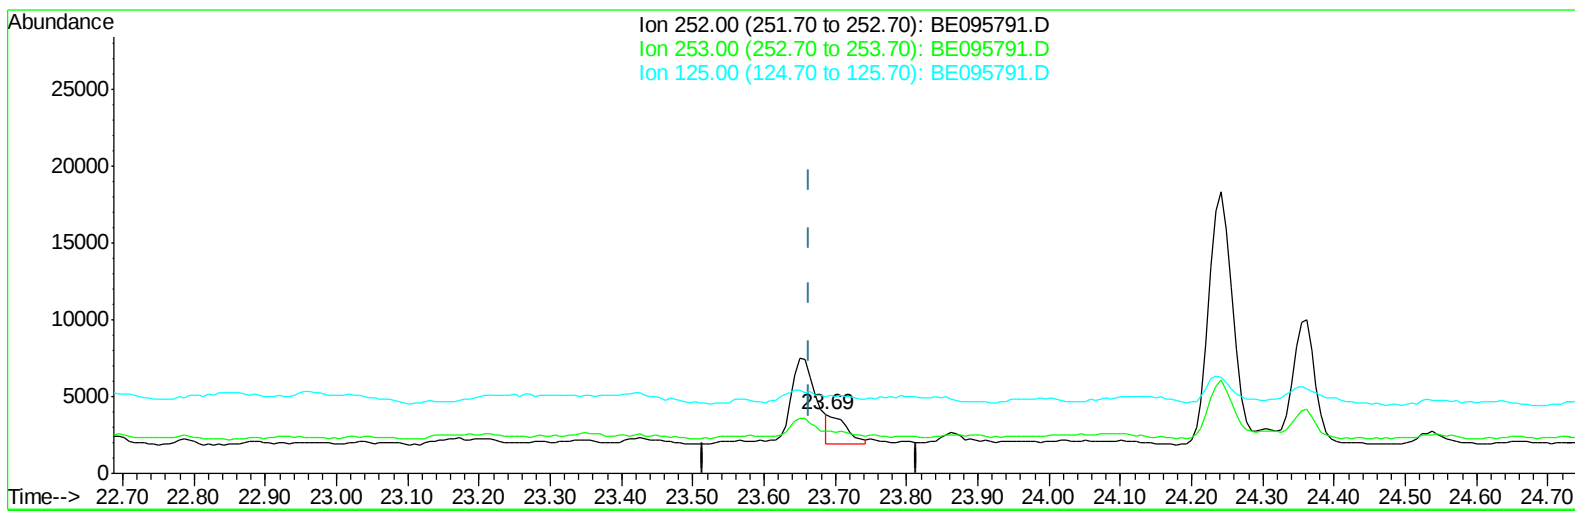

TIC: BE095791.D

(22) Benzo(k)fluoranthene

23.686min (+0.022) 0.12ng/ul m

response 3380

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 252.00 | 100   | 100     |
| 253.00 | 30.60 | 71.63#  |
| 125.00 | 17.10 | 130.99# |
| 0.00   | 0.00  | 0.00    |