
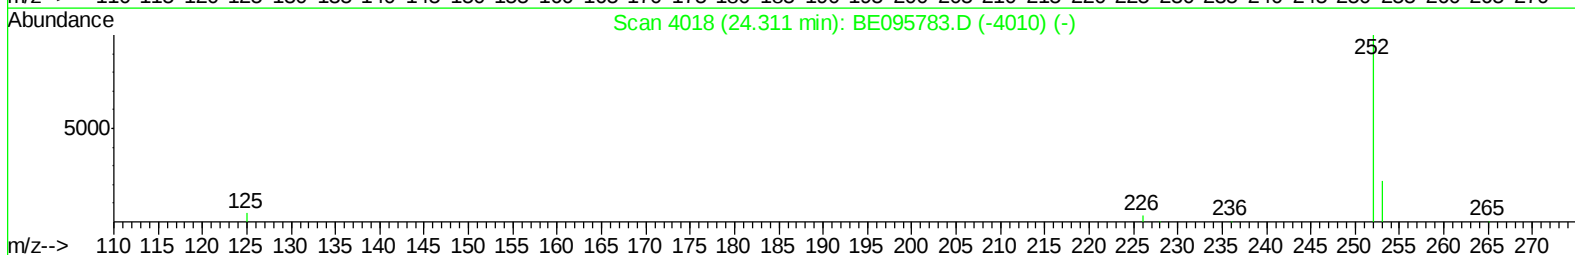
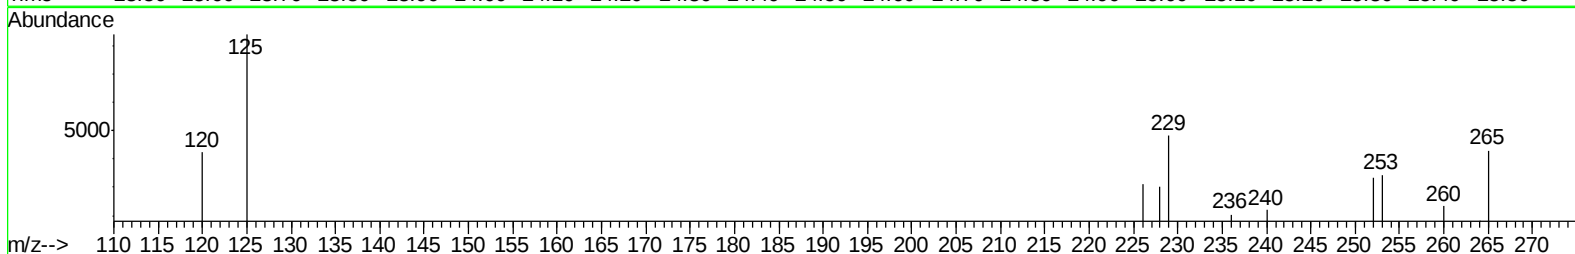


Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
Data File : BE095792.D
Acq On : 15 Mar 2018 7:58
Operator : SJ/JU
Sample : J1835-14
Misc :
ALS Vial : 36 Sample Multiplier: 1

Quant Time: Mar 15 09:14:34 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 15 05:35:28 2018
Response via : Initial Calibration

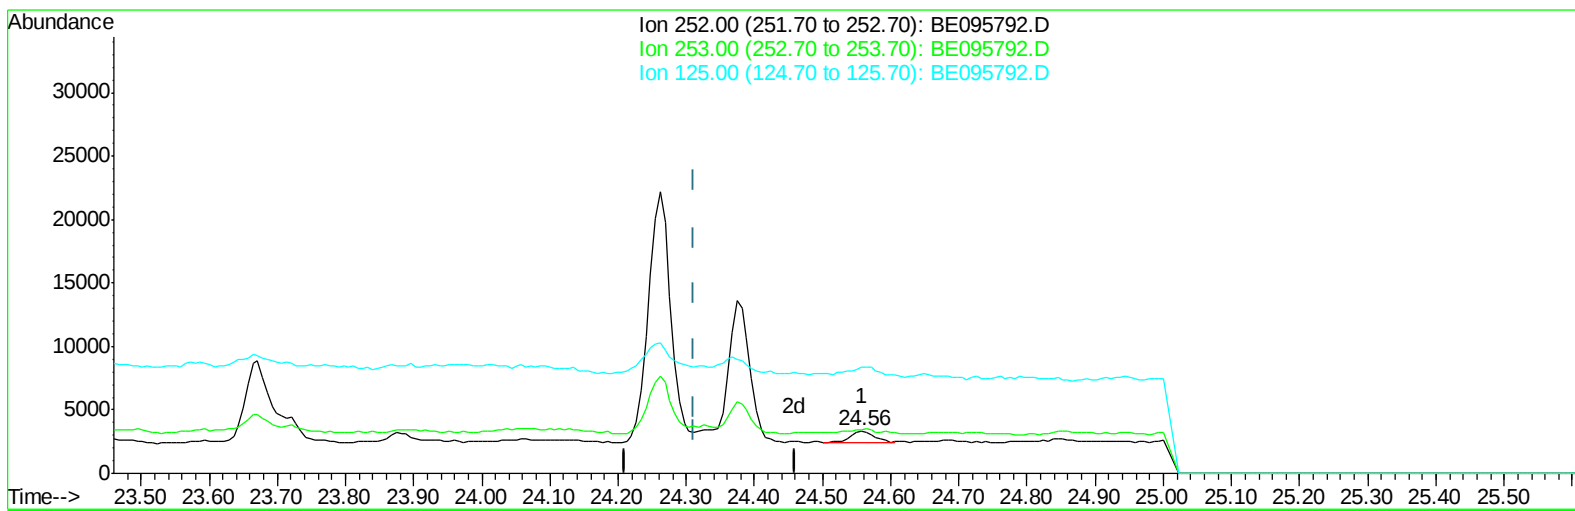

TIC: BE095792.D

(23) Benzo(a)pyrene (C)

24.557min (+0.246) 0.08ng/ul

response 2283

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	102.69#
125.00	22.60	251.30#
0.00	0.00	0.00