

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095772.D
 Acq On : 14 Mar 2018 19:59
 Operator : SJ/JU
 Sample : J1813-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Mar 15 03:10:35 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 15 03:09:28 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1799	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	5347	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3511	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.81	188	524963	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.79
20) Perylene-d12	24.26	264	475895	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.80	152	3155	0.35	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.98	166	922	0.064	ng/ul#	Ovalue 23


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
Data File : BE095772.D
Acq On : 14 Mar 2018 19:59
Operator : SJ/JU
Sample : J1813-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Mar 15 03:10:35 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 15 03:09:28 2018
Response via : Initial Calibration

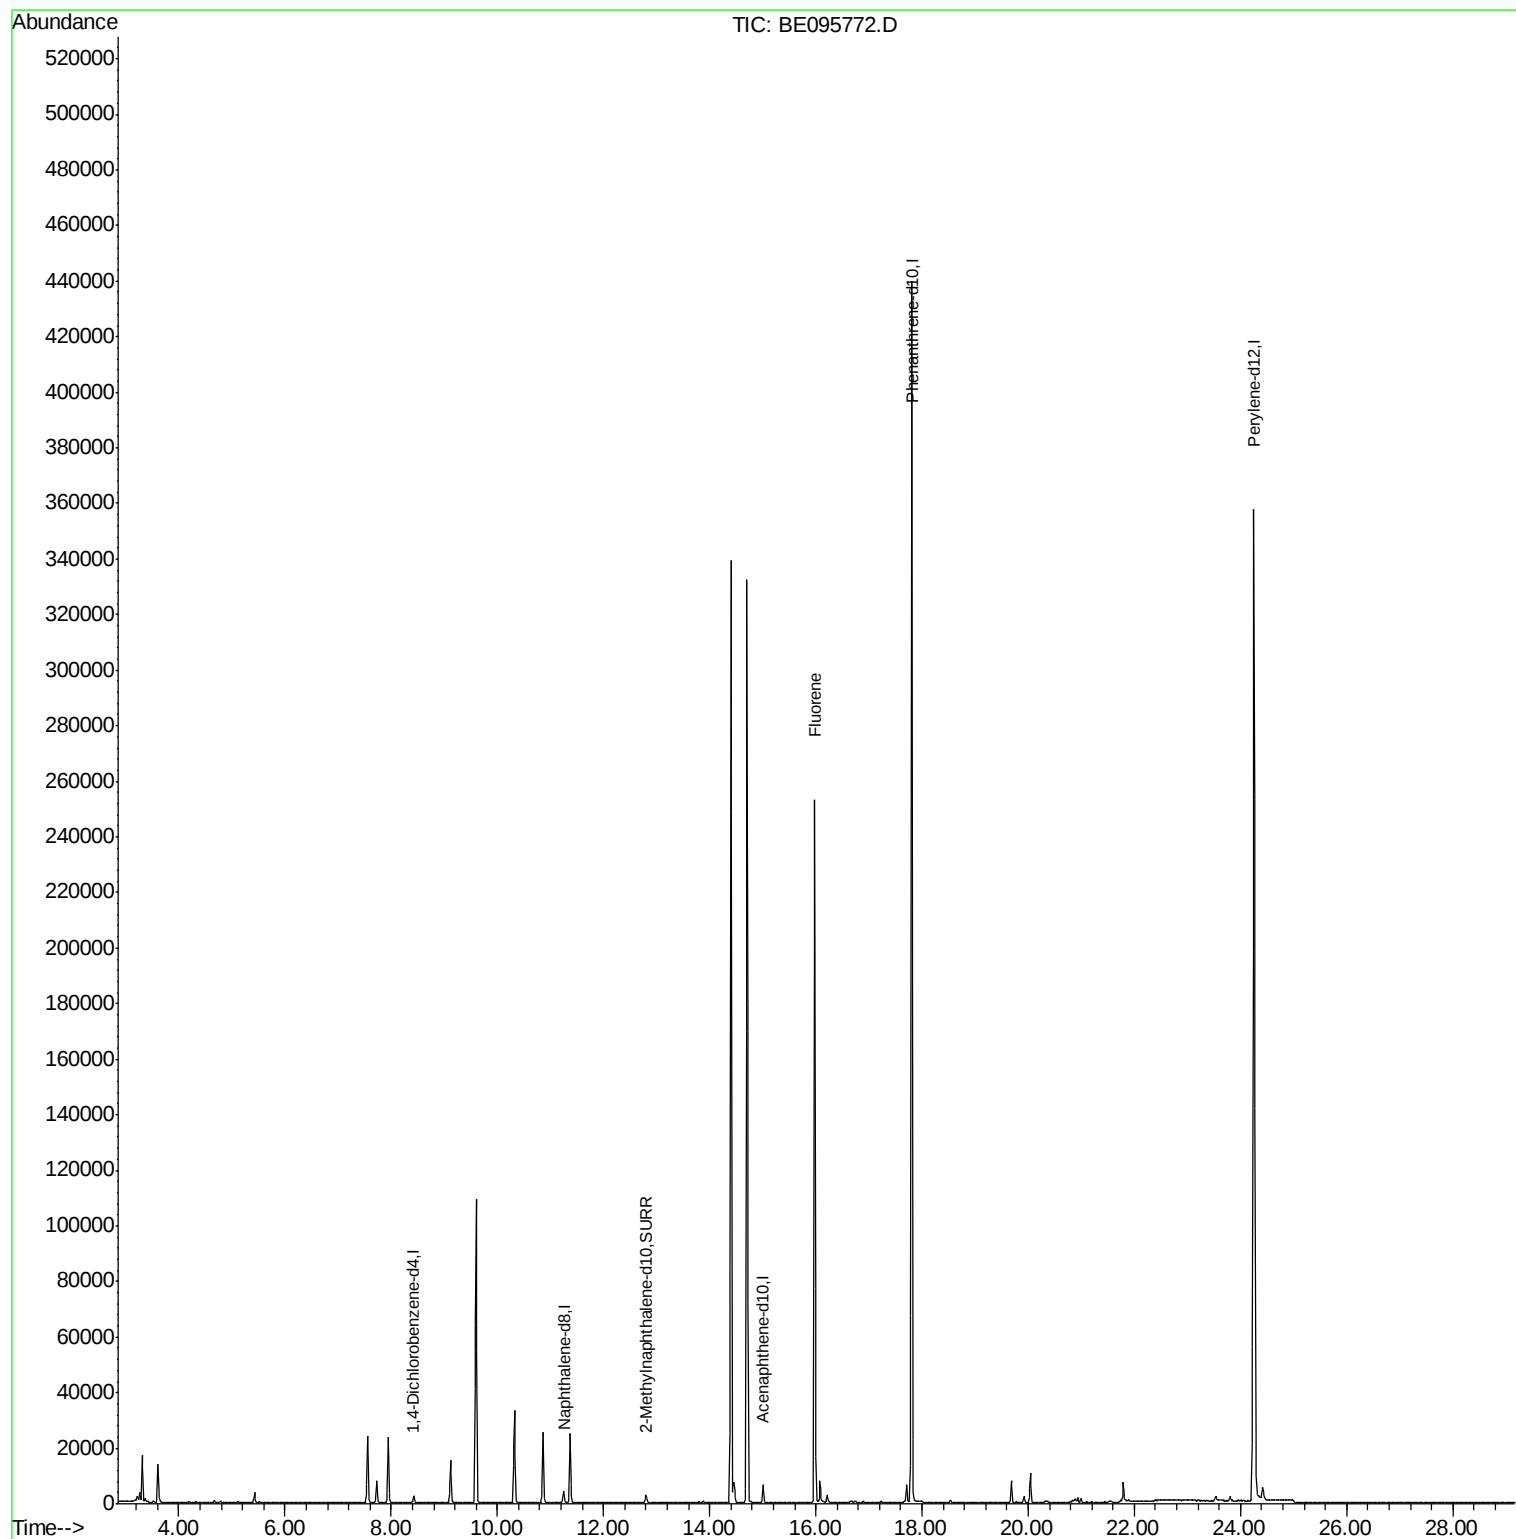

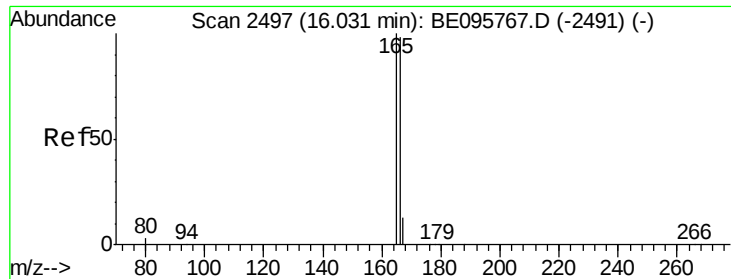

#9

Fluorene

Concen: 0.064 ng/ul

RT: 15.98 min Scan# 2490

Delta R.T. -0.05 min

Lab File: BE095772.D

Acq: 14 Mar 2018 19:59

Instrument :

BNA_E

ClientSampleId :


Tot Ion:166 Resp: 922

Ion Ratio Lower Upper

166 100

165 12.4 73.4 110.2#

167 39.0 14.6 22.0#

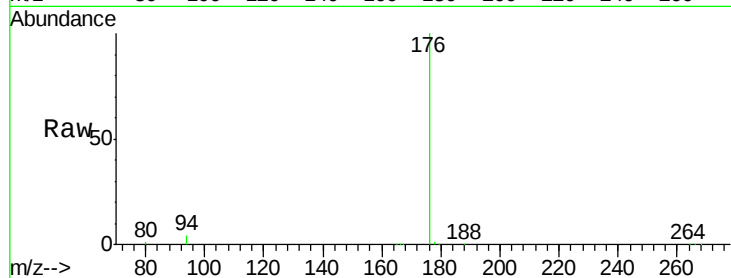

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

