

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095782.D
 Acq On : 15 Mar 2018 1:57
 Operator : SJ/JU
 Sample : J1835-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Mar 15 03:44:03 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 15 03:09:28 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	2079	0.40	ng/ul	0.00
2) Naphthalene-d8	11.25	136	6325	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3894	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.81	188	320151	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.79
20) Perylene-d12	24.26	264	301788	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.80	152	2090	0.20	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	11.30	128	931	0.053	ng/ul#	78
5) 2-Methylnaphthalene	12.87	142	1743	0.142	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
Data File : BE095782.D
Acq On : 15 Mar 2018 1:57
Operator : SJ/JU
Sample : J1835-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Mar 15 03:44:03 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 15 03:09:28 2018
Response via : Initial Calibration

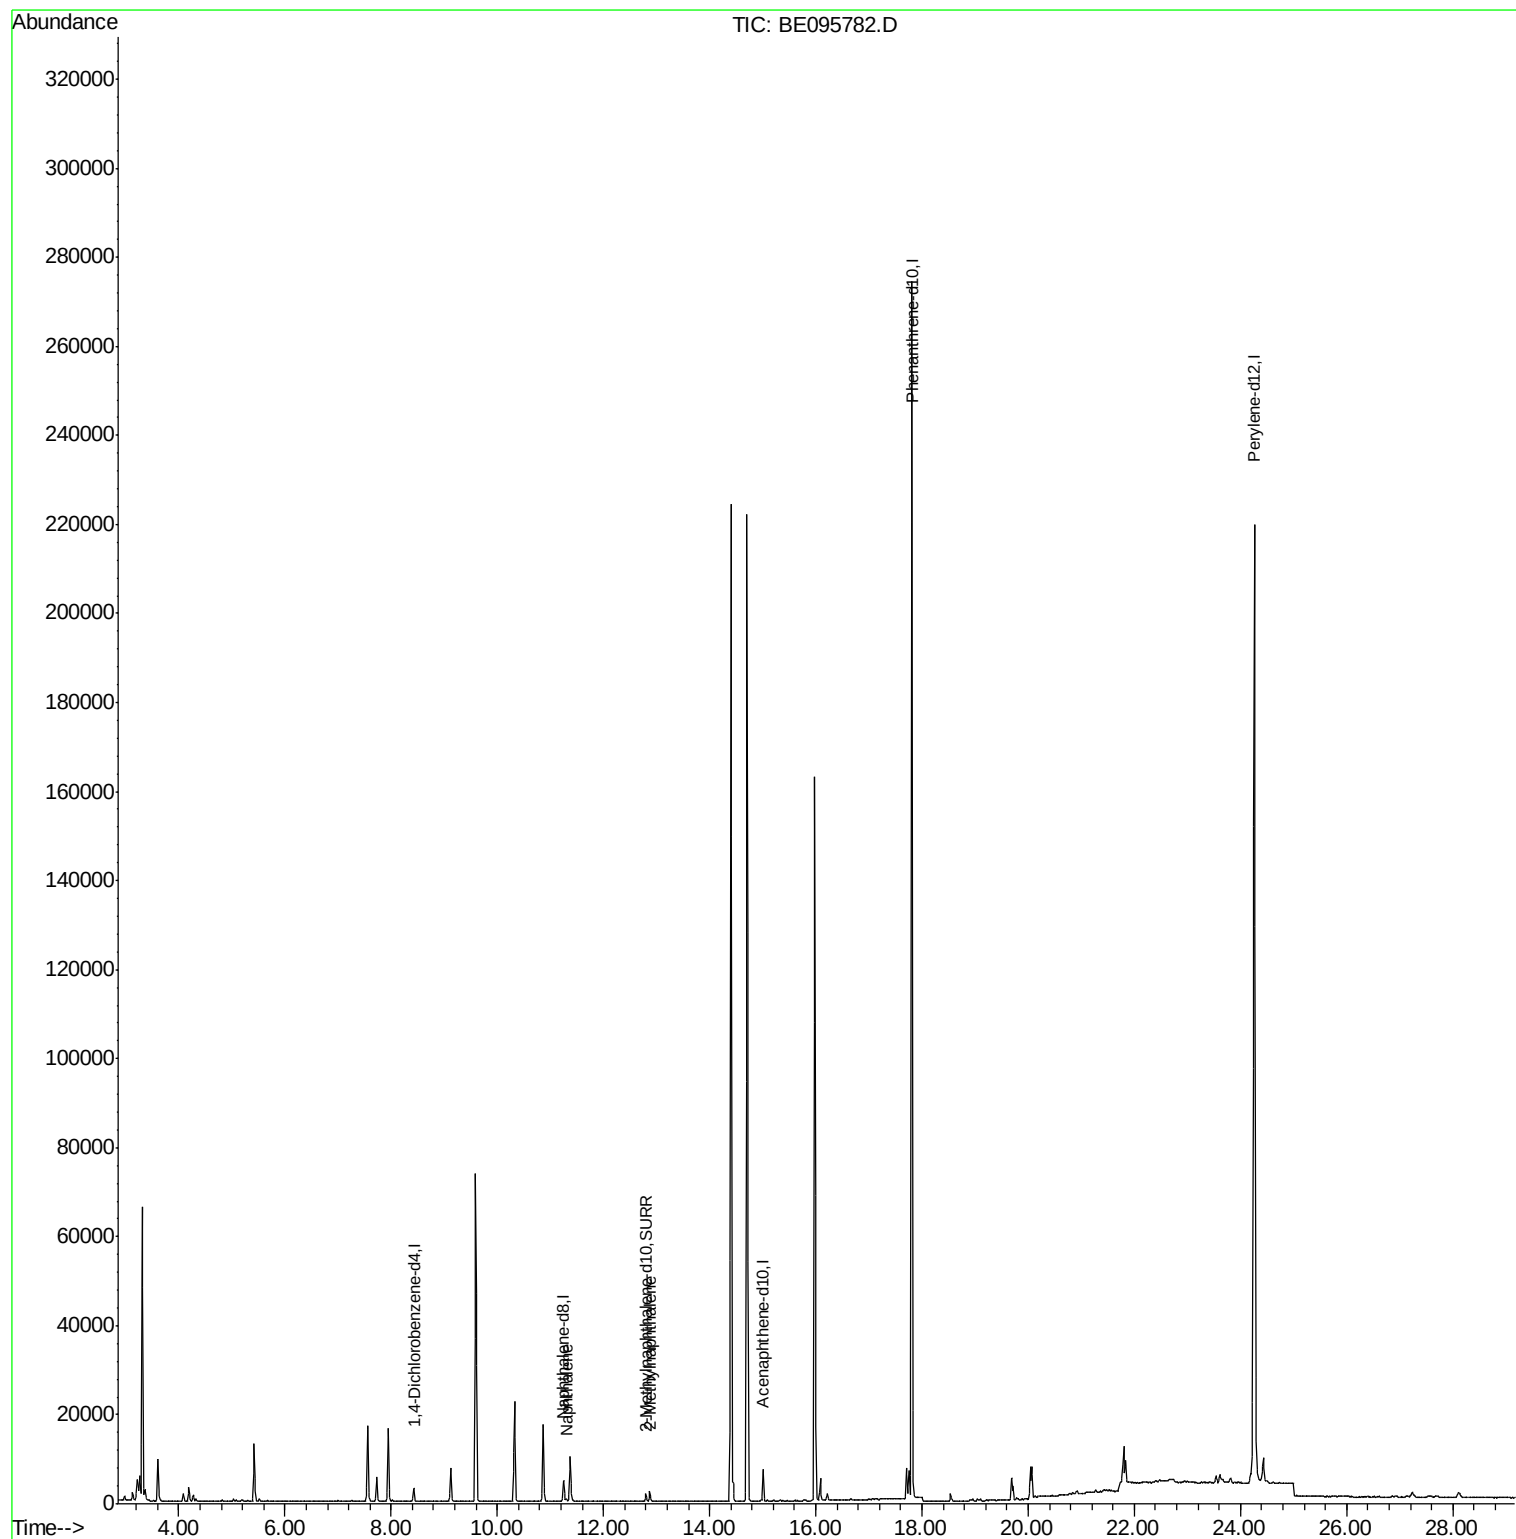

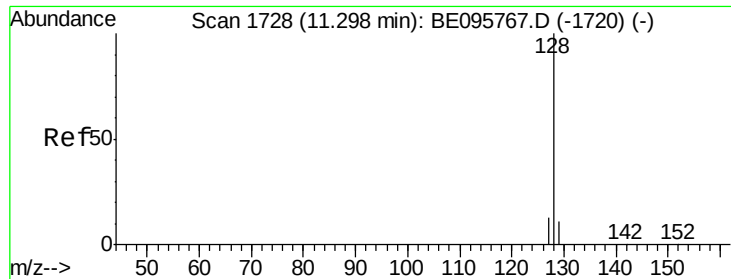

#3

Naphthalene

Concen: 0.053 ng/ul

RT: 11.30 min Scan# 1728

Delta R.T. 0.00 min

Lab File: BE095782.D

Acq: 15 Mar 2018 1:57

Instrument :

BNA_E

ClientSampleId :


Tot Ion:128 Resp: 931

Ion Ratio Lower Upper

128 100

129 18.9 11.3 16.9#




127 21.5 4.0 6.0#

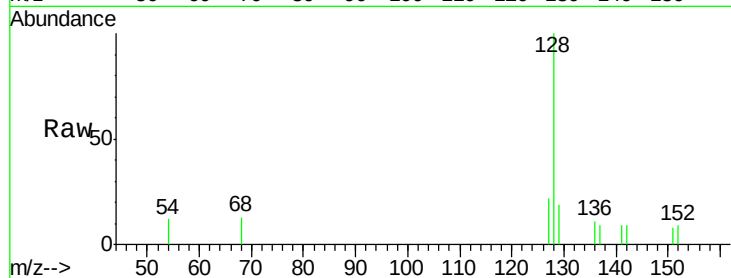

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

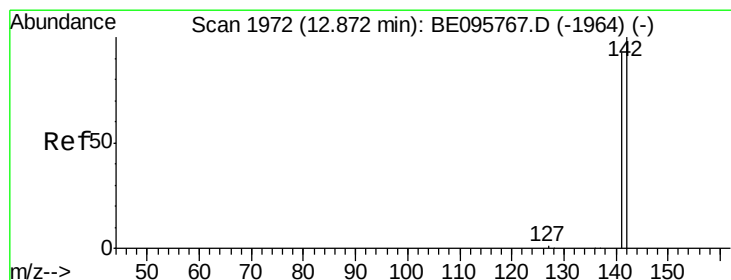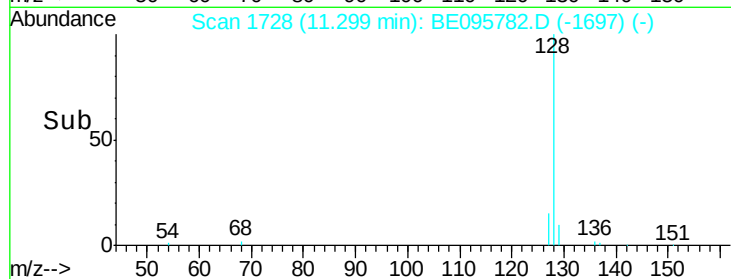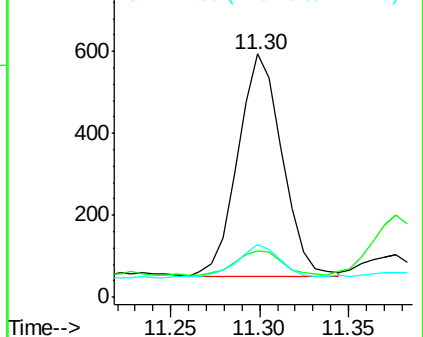

#5

2-Methylnaphthalene

Concen: 0.142 ng/ul

RT: 12.87 min Scan# 1972

Delta R.T. 0.00 min

Lab File: BE095782.D


Acq: 15 Mar 2018 1:57

Tgt Ion:142 Resp: 1743

Ion Ratio Lower Upper

142 100

141 93.6 72.6 108.8

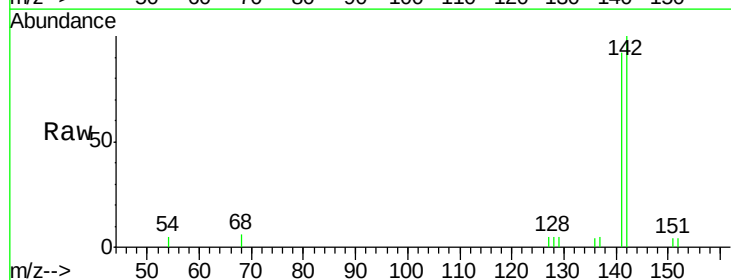

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

