


Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095793.D
 Acq On : 15 Mar 2018 8:34
 Operator : SJ/JU
 Sample : J1813-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1




Quant Time: Mar 15 11:10:44 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Qlast Update : Thu Mar 15 05:35:28 2018
 Response via : Initial Calibration

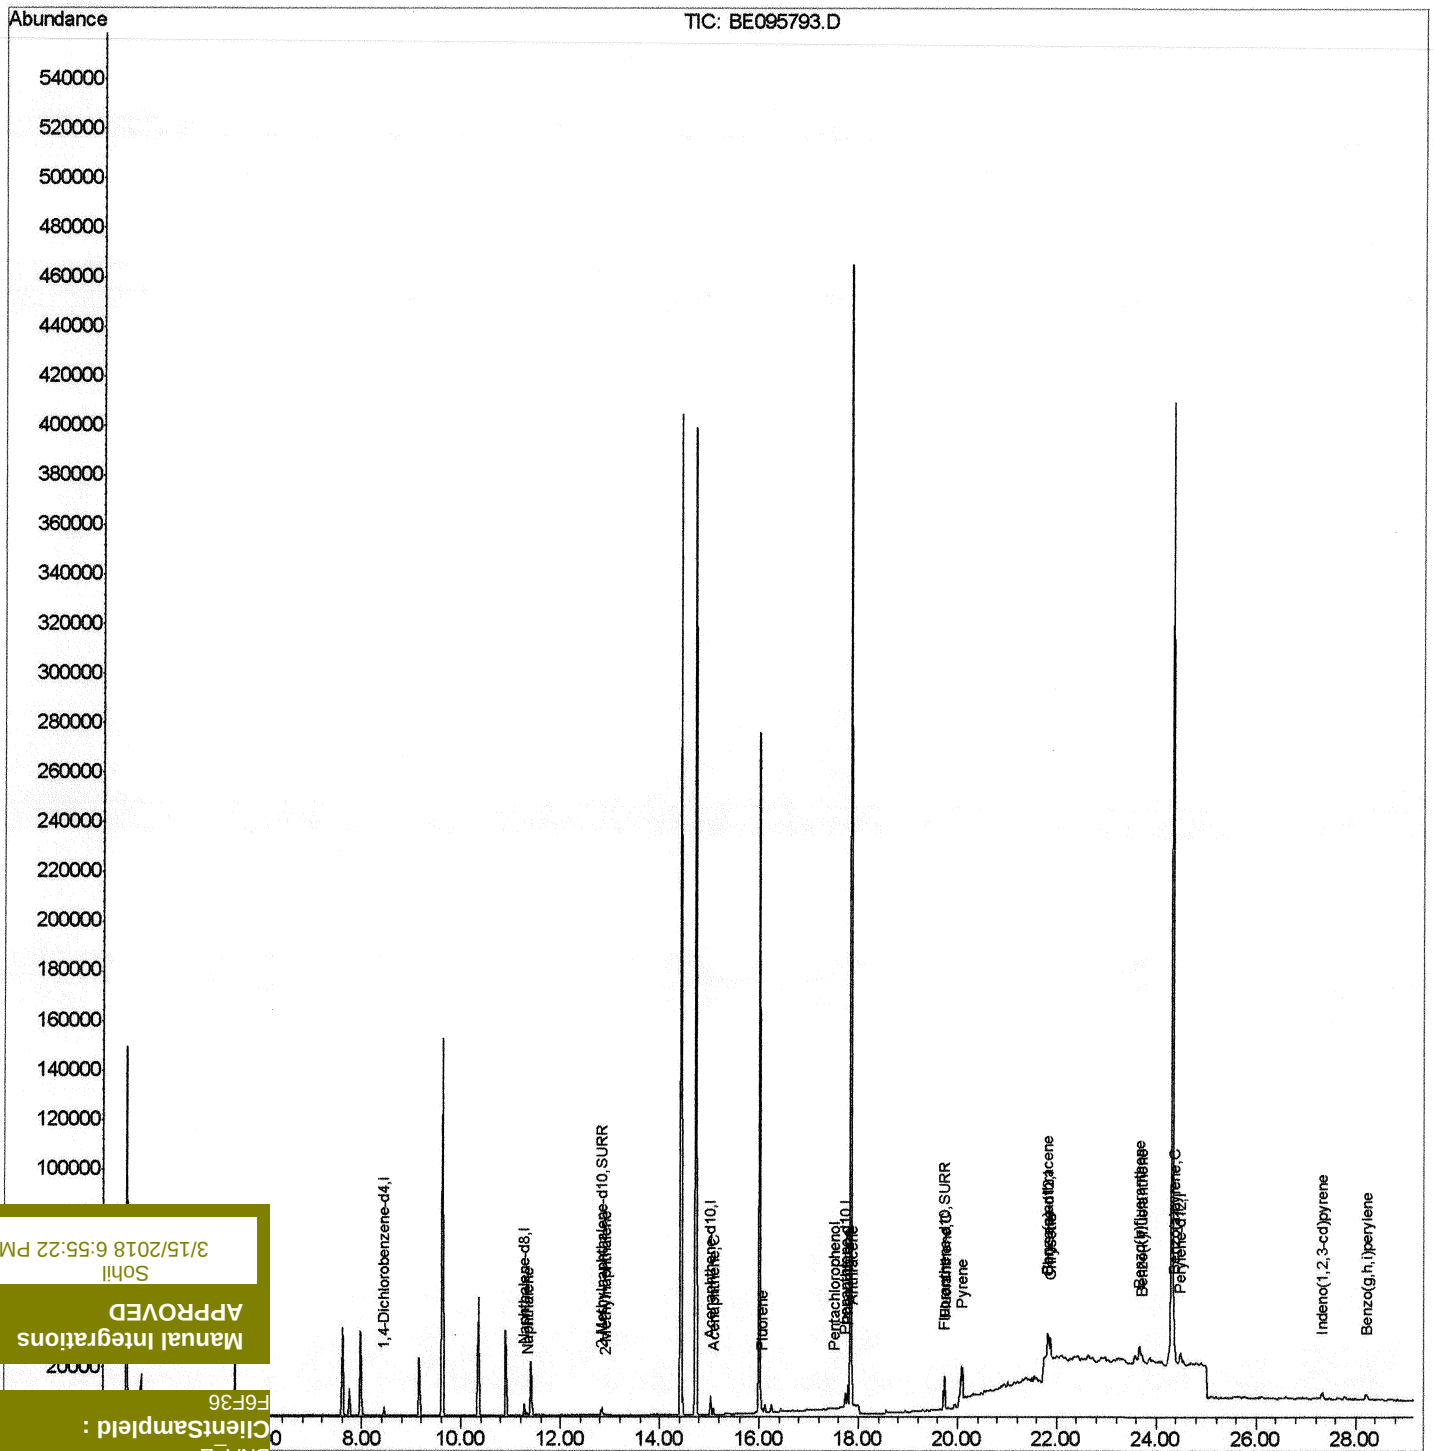

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095793.D
 Acq On : 15 Mar 2018 8:34
 Operator : SJ/JU
 Sample : J1813-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Mar 15 10:59:30 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Qlast Update : Thu Mar 15 05:35:28 2018
 Response via : Initial Calibration

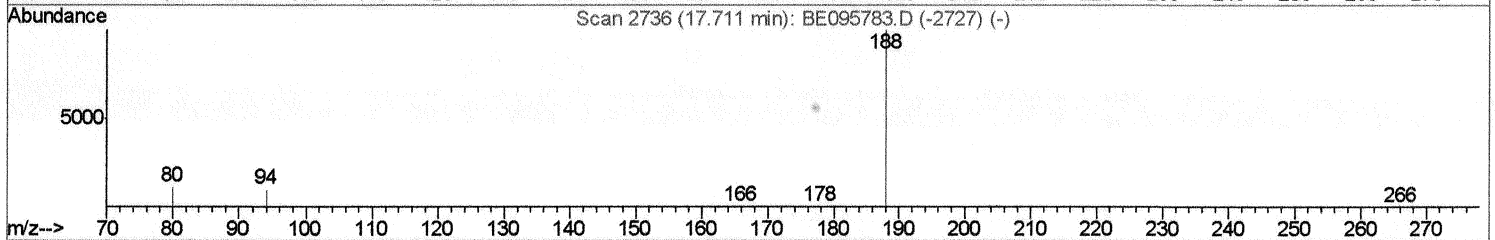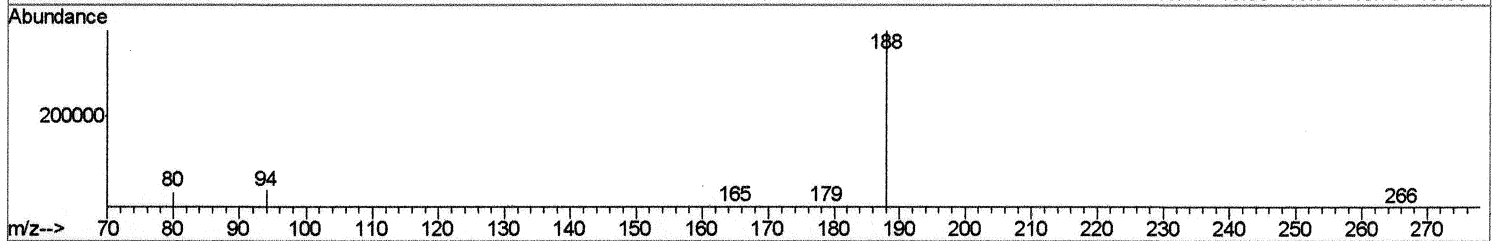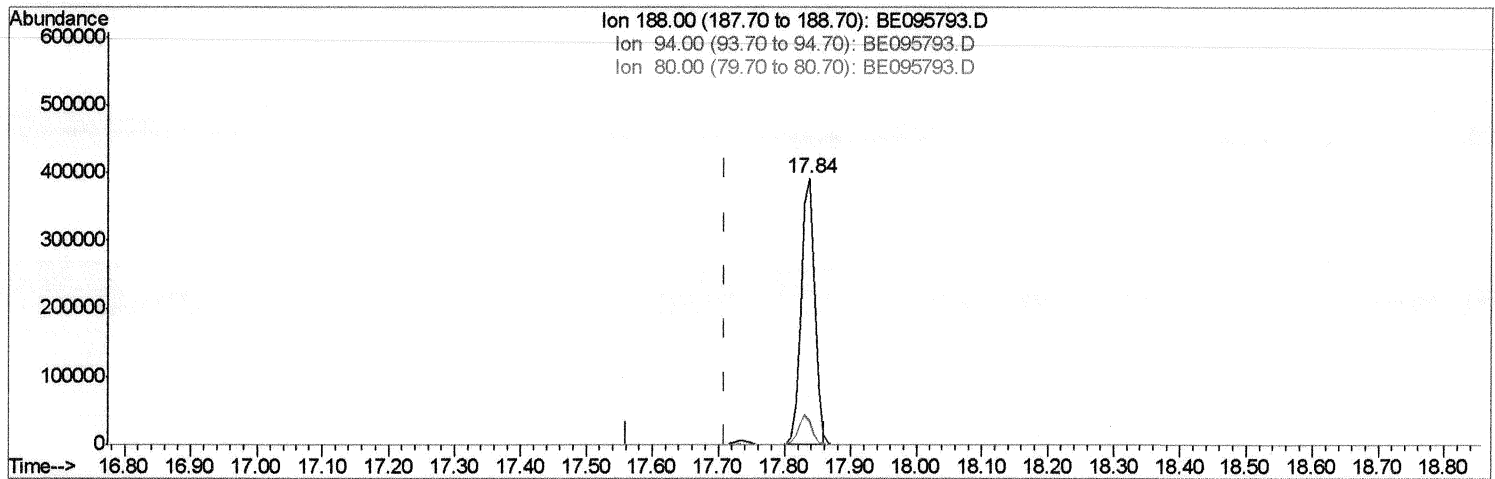

TIC: BE095793.D

(10) Phenanthrene-d10 (I)
 17.838min (+0.126) 0.40ng/ul
 response 565564

Ion	Exp%	Act%
188.00	100	100
94.00	9.33	9.33
80.00	8.55#	8.55#
	0.00	0.00

3/15/2018 6:55:22 PM

Sohil

APPROVED




Manual Integrations

Instrument :
 BNA_E
 ClientSampled :
 F6F36

8.M Thu Mar 15 11:01:37 2018

```
Data Path   : Z:\HPCHEM1\BNA E\DATA\BE031418\  
Data File  : BE095793.D  
Acq On     : 15 Mar 2018      8:34  
Operator   : SJ/JU  
Sample     : J1813-11  
Misc       :  
ALS Vial   : 37      Sample Multiplier: 1
```

Quant Time: Mar 15 10:59:30 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 15 05:35:28 2018
Response via : Initial Calibration

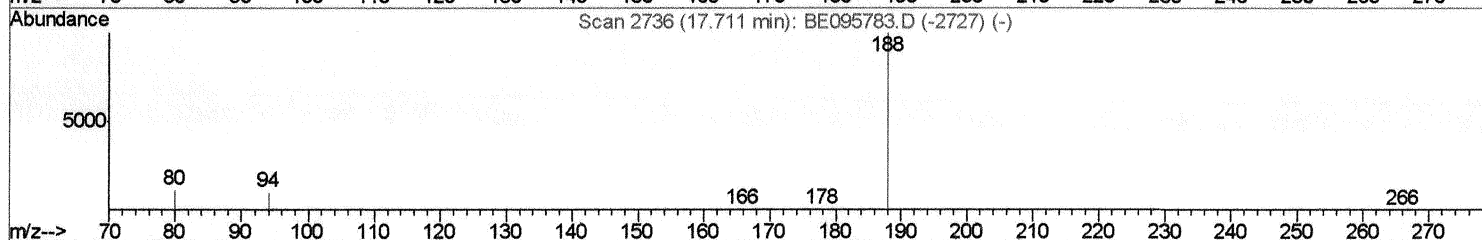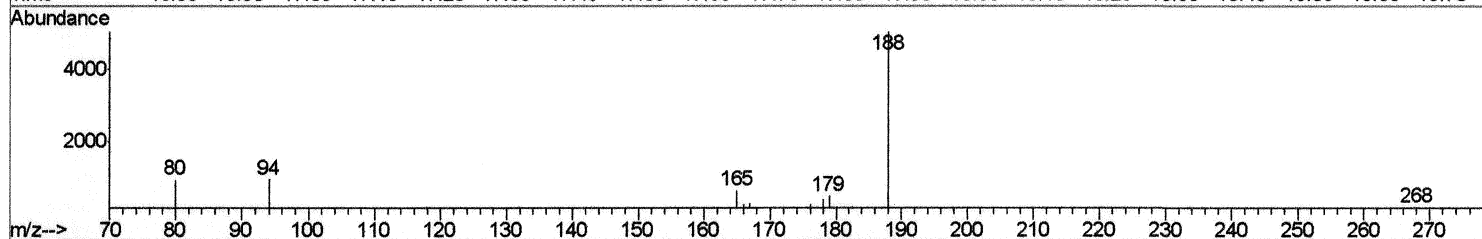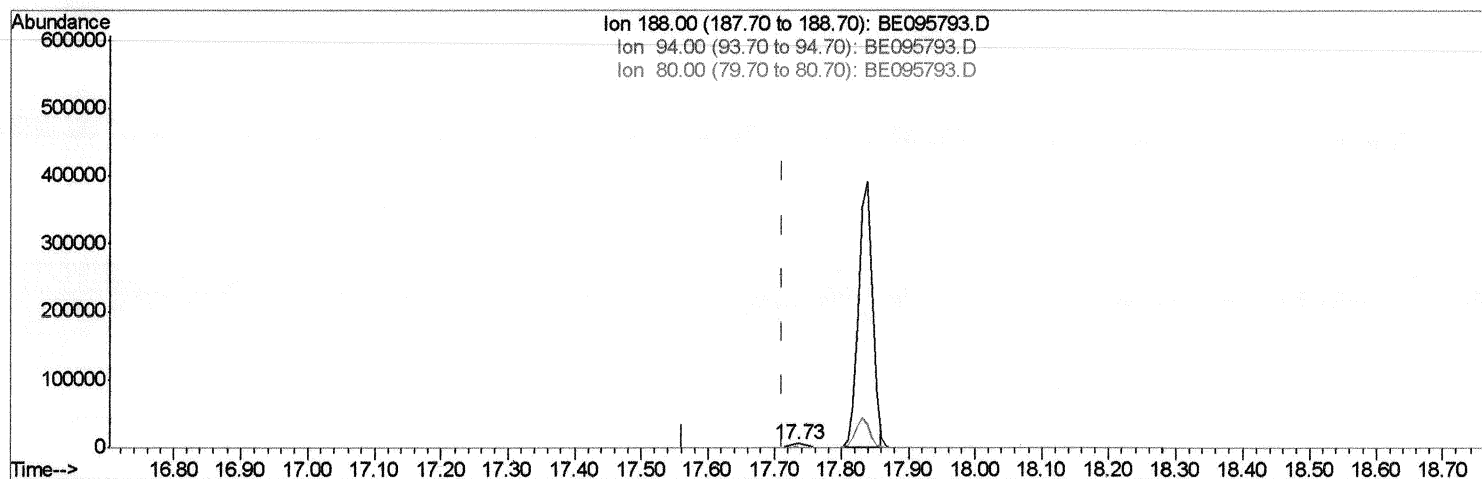

TIC: BE095793.D

(10) Phenanthrene-d10 (I)

17.732min (+0.021) 0.40ng/ul m

response 7811

Ion	Exp%	Act%
-----	------	------

3/15/2018 6:55:22 PM

Sohil

APPROVED

Manual Integrations

ClientSampleId :




Instrument:

8.M Thu Mar 15 11:02:43 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095793.D
 Acq On : 15 Mar 2018 8:34
 Operator : SJ/JU
 Sample : J1813-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Mar 15 10:59:30 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Qlast Update : Thu Mar 15 05:35:28 2018
 Response via : Initial Calibration

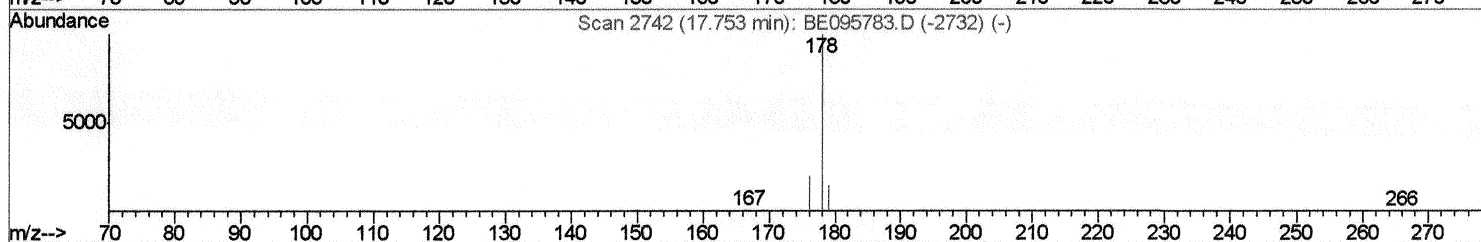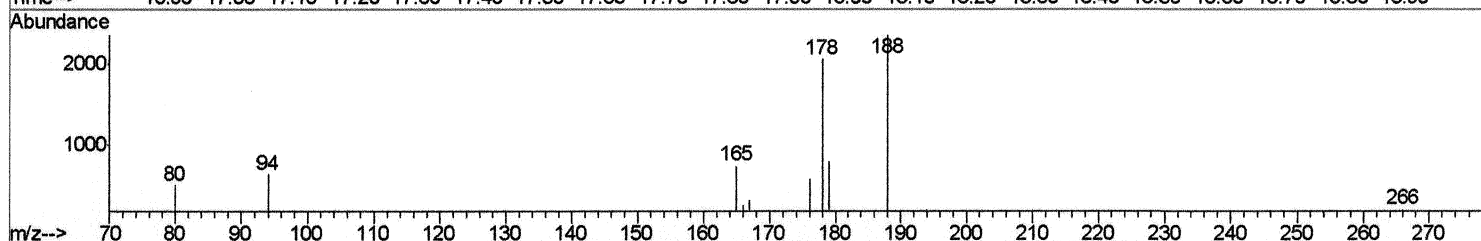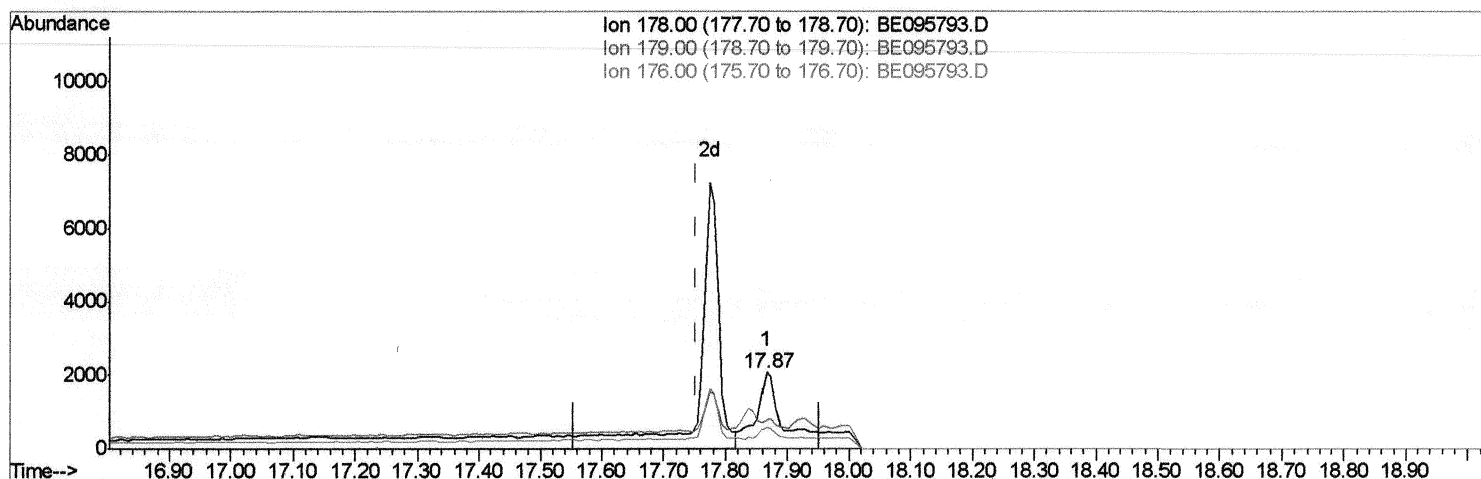

TIC: BE095793.D

(12) Phenanthrene

17.866min (+0.112) 0.35ng/ul

response 8084

Ion	Exp%	Act%
178.00	100	100
179.00	100	38.33#
176.00	100	28.38#
177.00	100	0.00

3/15/2018 6:55:22 PM

Sohil

APPROVED

Manual Integrations

ClientSampled : F6F36

BNA_E




Instrument :

8.M Thu Mar 15 11:03:29 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095793.D
 Acq On : 15 Mar 2018 8:34
 Operator : SJ/JU
 Sample : J1813-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Mar 15 10:59:30 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 15 05:35:28 2018
 Response via : Initial Calibration

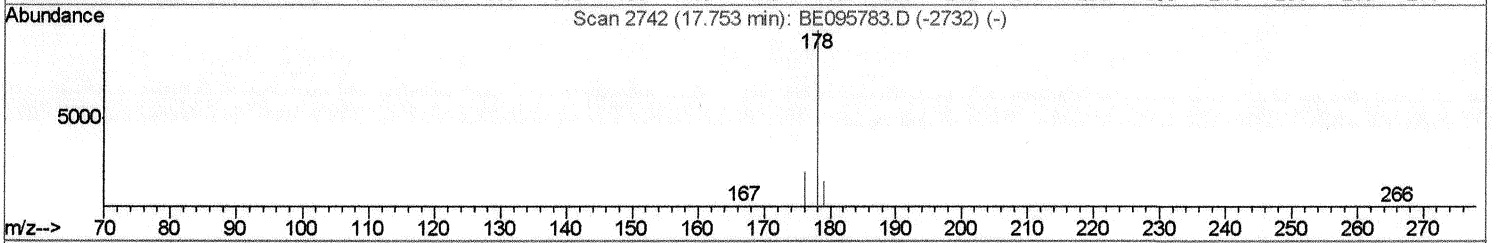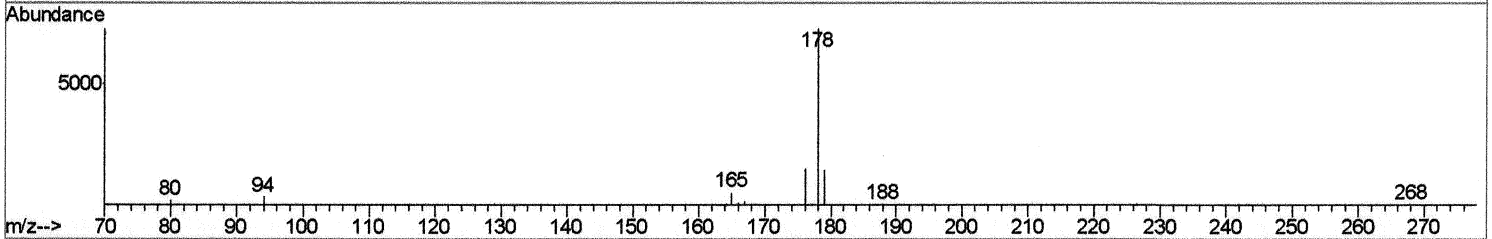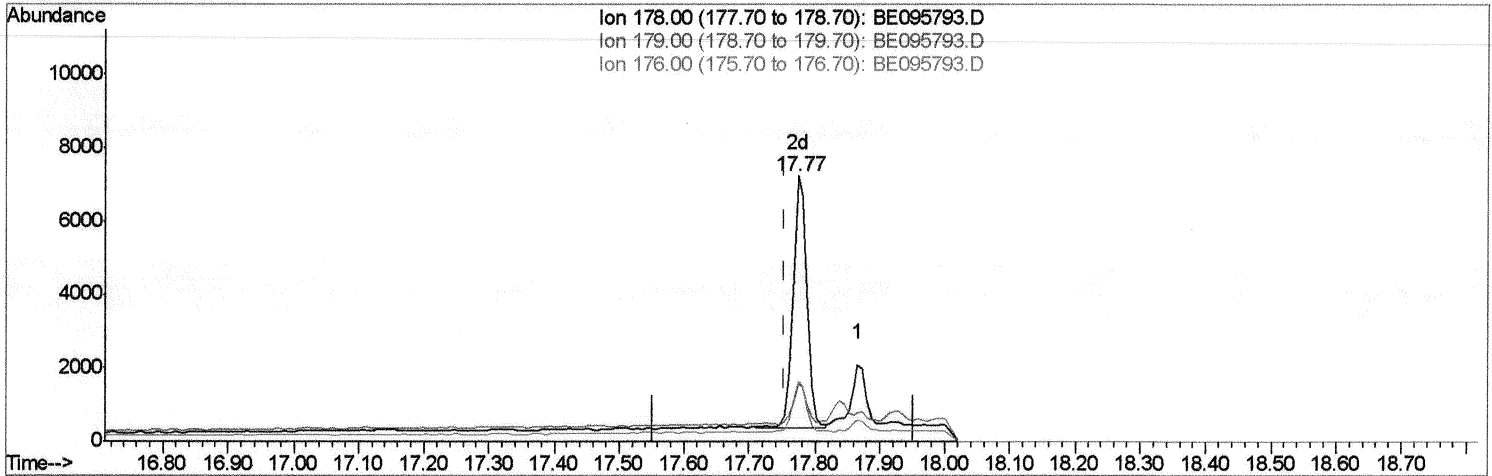

TIC: BE095793.D

(12) Phenanthrene

17.774min (+0.021) 0.45ng/ul > SJ 3/16/18

response 10411

Ion	Exp%	Act%
178.00	100	100
176.00	21.75	22.68
178.00	100	100

3/15/2018 6:55:22 PM

Sohil

APPROVED

Manual Integrations




ClientSampled :
 BNA_E
 Instrument :
 F6F36

18.M Thu Mar 15 11:04:02 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095793.D
 Acq On : 15 Mar 2018 8:34
 Operator : SJ/JU
 Sample : J1813-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Mar 15 11:03:36 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 15 05:35:28 2018
 Response via : Initial Calibration

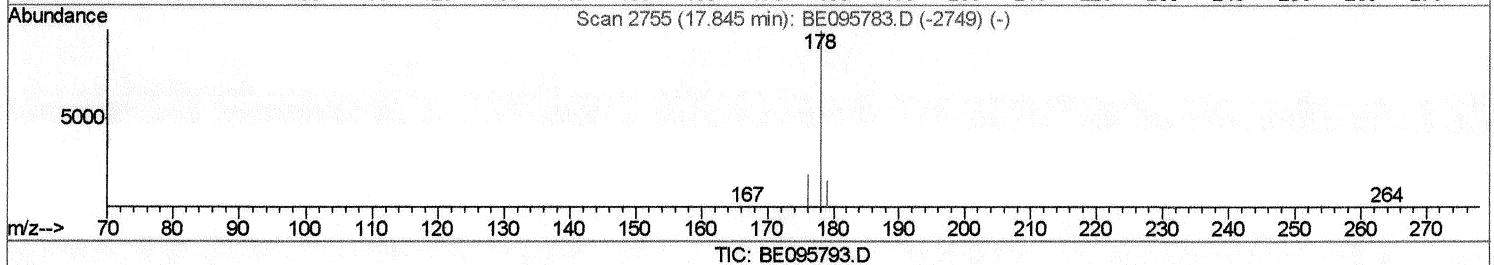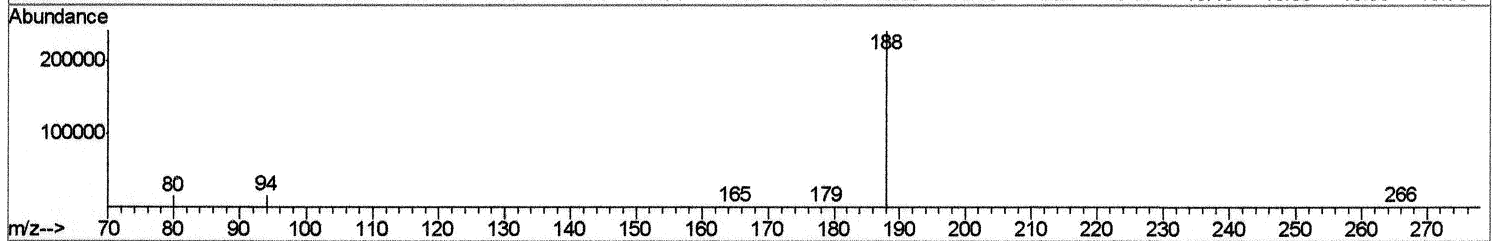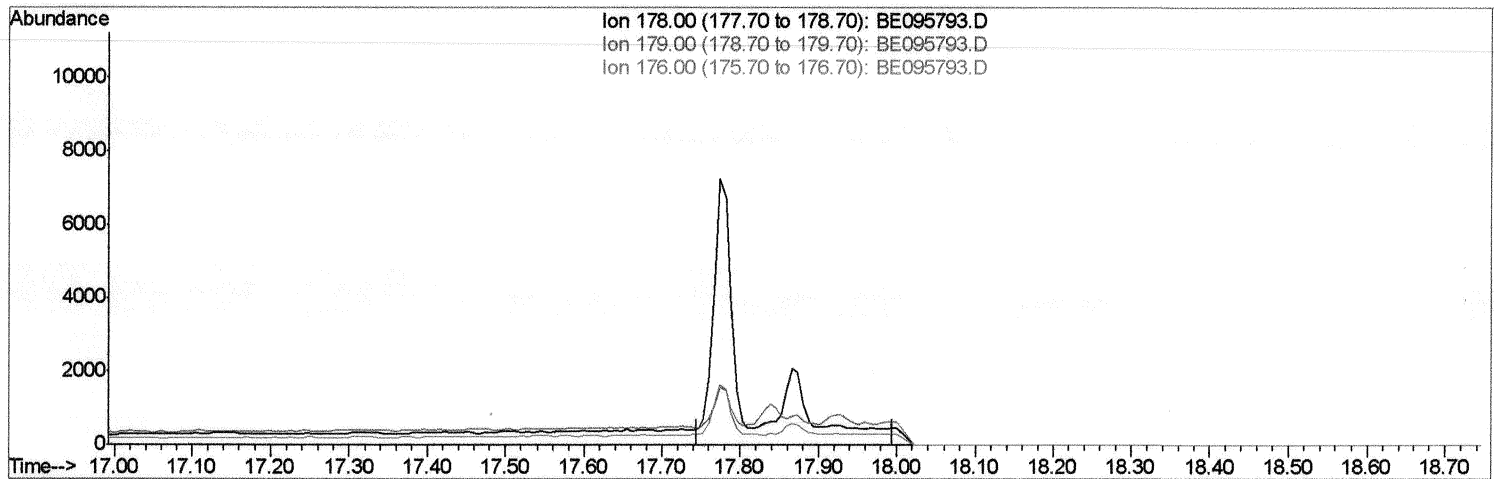

TIC: BE095793.D

(13) Anthracene

17.845min (-17.845) 0.00ng/ui

response 0

Ion	Exp%	Act%
178.00	100	0.00
179.00	100	0.00
176.00	100	0.00

Instrument : BNA_E




ClientSampled : F6F36

8.M Thu Mar 15 11:05:00 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095793.D
 Acq On : 15 Mar 2018 8:34
 Operator : SJ/JU
 Sample : J1813-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Mar 15 11:03:36 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 15 05:35:28 2018
 Response via : Initial Calibration

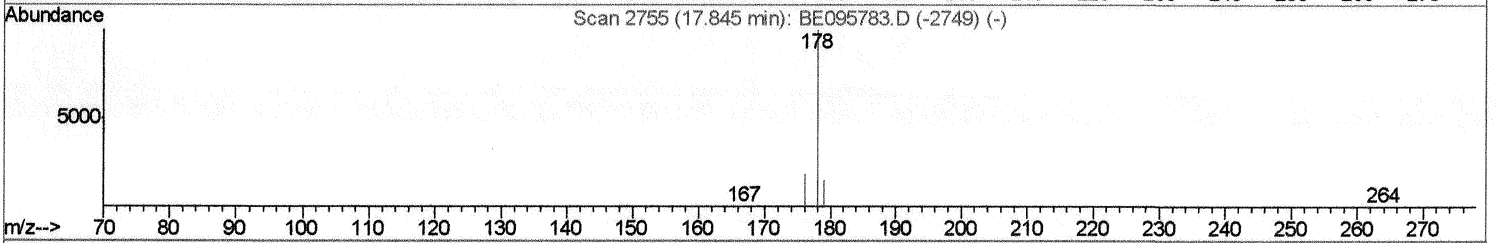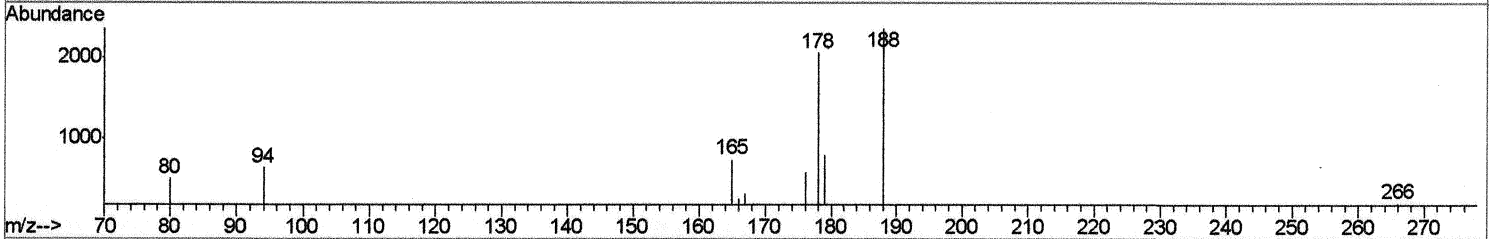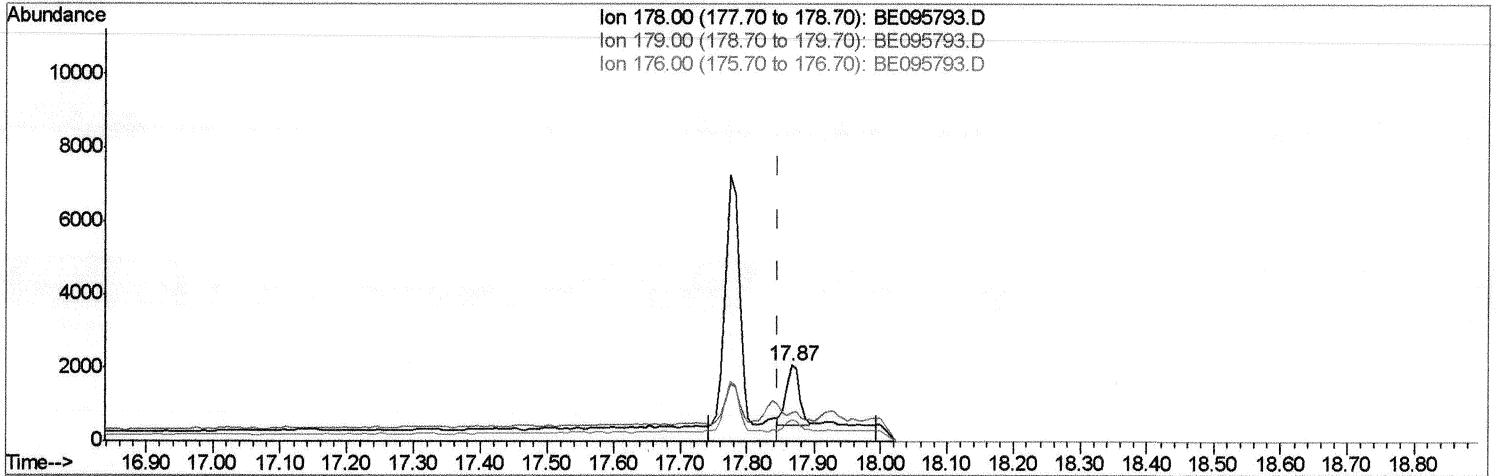

TIC: BE095793.D

(13) Anthracene

17.866min (+0.021) 0.11ng/ul m 2 52 3/16/18

response 2402

Ion Exp% Act%

Ion	Exp%	Act%
178.00	100	100
179.00	38.33	38.33#
176.00	28.38	28.38#
177.00	0.00	0.00

3/15/2018 6:55:22 PM

Sohil

APPROVED

Manual Integrations

F6F36

ClientSampled :

BNA_E




Instrument :

18.M Thu Mar 15 11:05:25 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095793.D
 Acq On : 15 Mar 2018 8:34
 Operator : SJ/JU
 Sample : J1813-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Mar 15 11:03:36 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 15 05:35:28 2018
 Response via : Initial Calibration

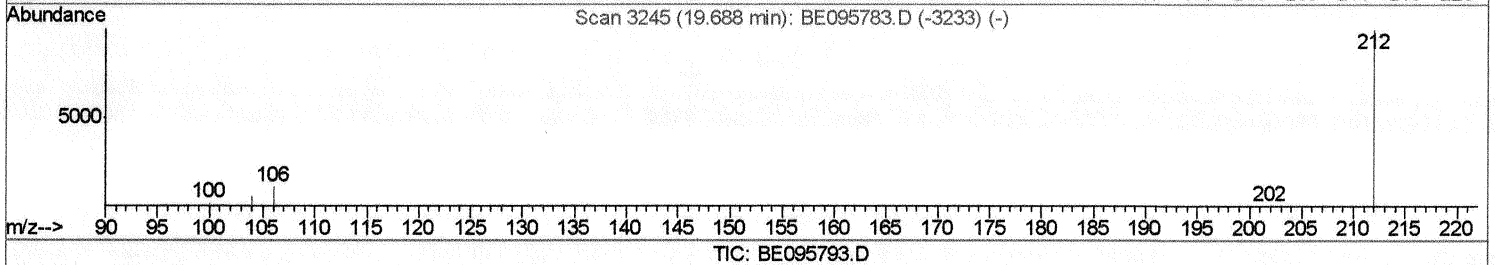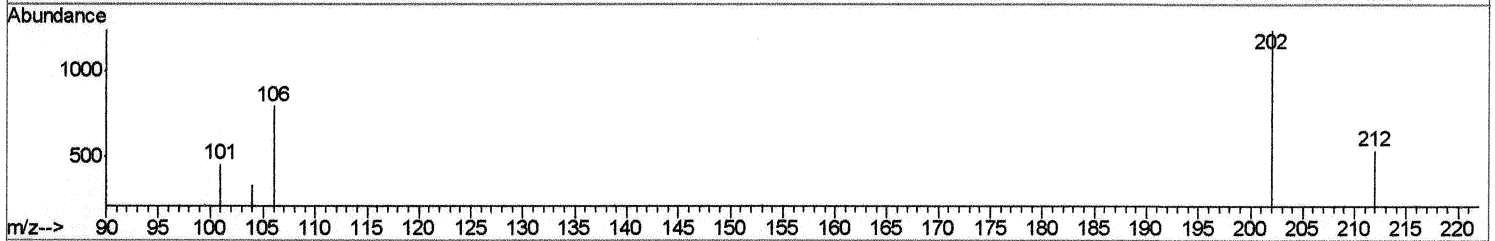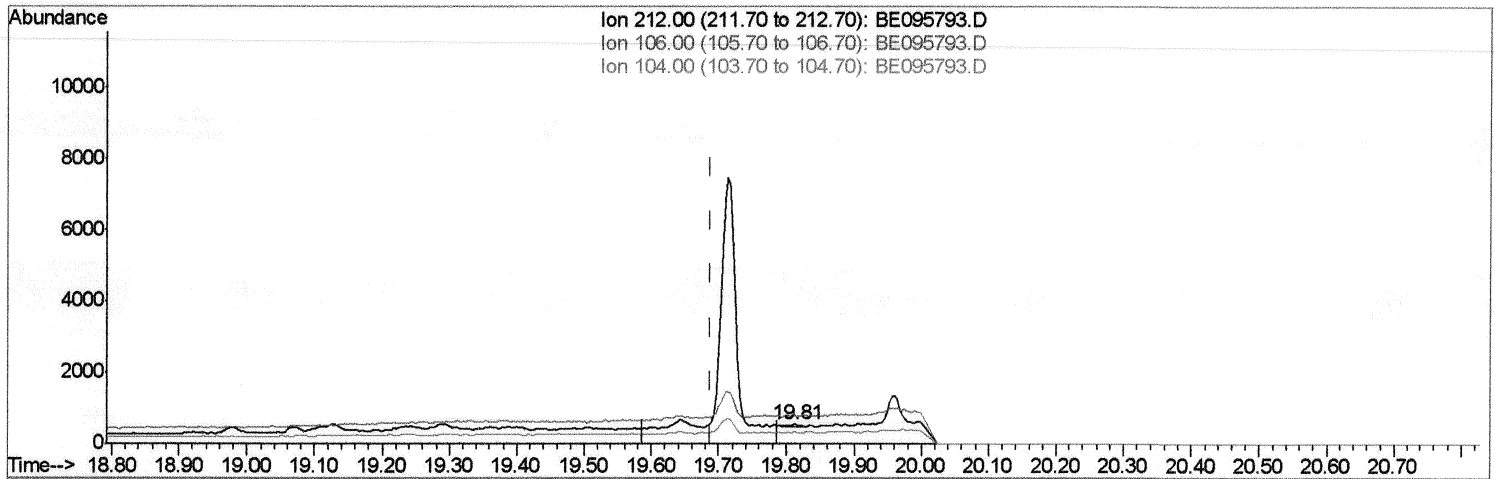

(14) Fluoranthene-d10 (SURR)

19.813min (+0.125) 0.00ng/ui

response 71

Ion	Exp%	Act%
212.00	100	100

3/15/2018 6:55:22 PM

Sohil

APPROVED

Manual Integrations

FF36

ClientSampleId :

BNA_E




Instrument :

8.M Thu Mar 15 11:05:33 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095793.D
 Acq On : 15 Mar 2018 8:34
 Operator : SJ/JU
 Sample : J1813-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Mar 15 11:03:36 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 15 05:35:28 2018
 Response via : Initial Calibration

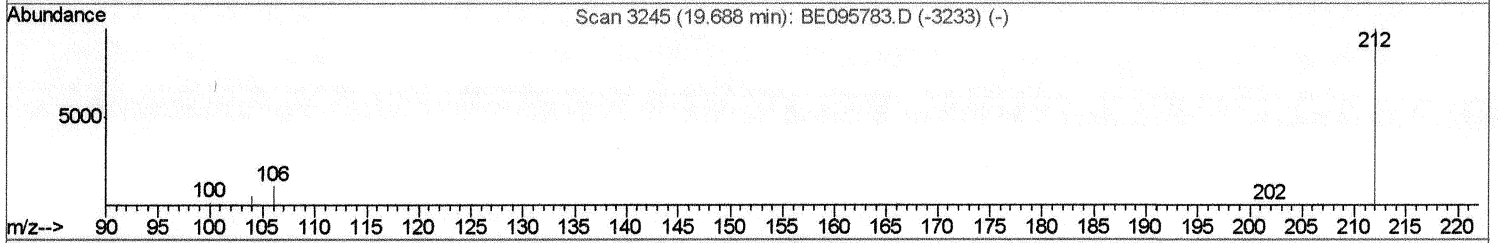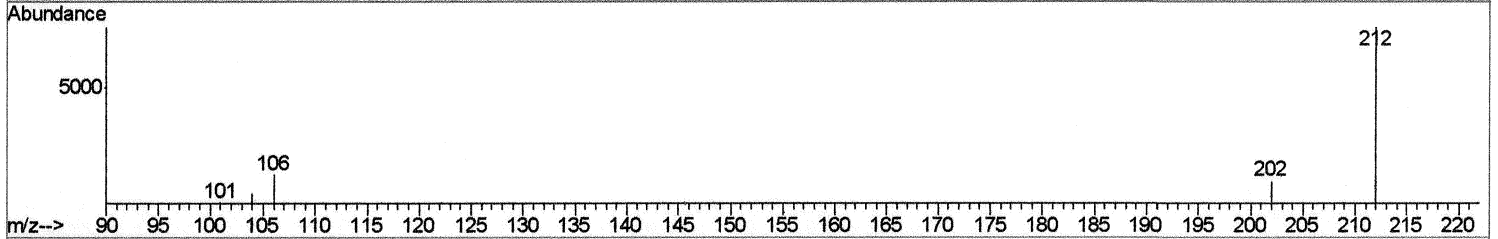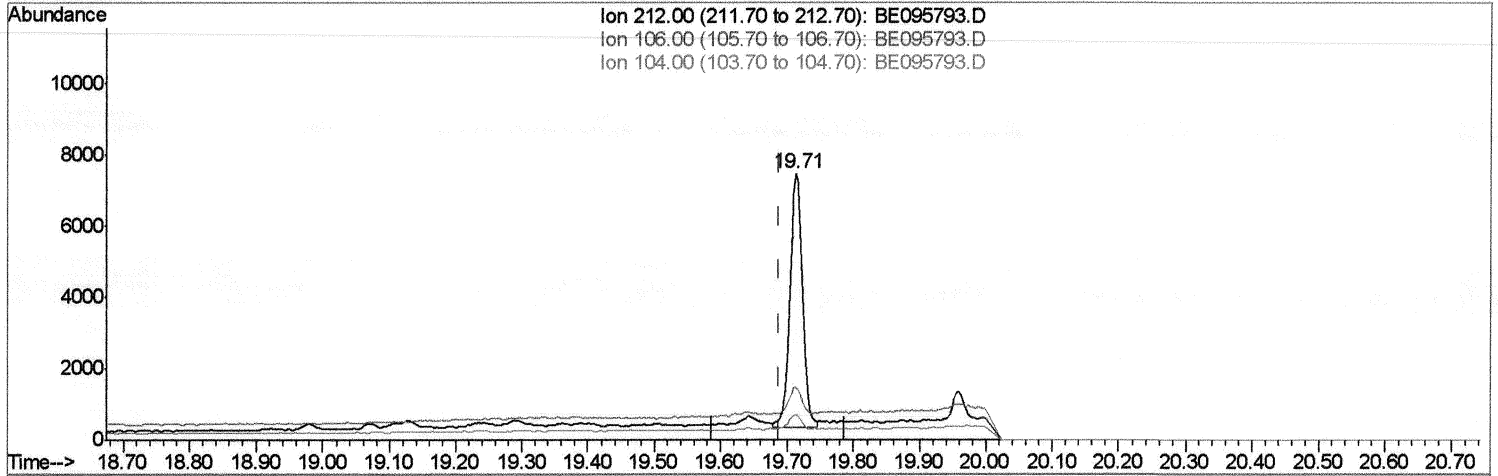

TIC: BE095793.D

(14) Fluoranthene-d10 (SURR)

19.713min (+0.025) 0.40ng/ul m > > 3/16/18

response 9919

Ion	Exp%	Act%
212.00	100	100
106.00	0.54	0.54#
104.00	0.27	0.27#
202.00	0.00	0.00

3/15/2018 6:55:22 PM

Sohil

APPROVED

Manual Integrations

F6F36

ClientSampled :




Instrument :

18.M Thu Mar 15 11:05:59 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095793.D
 Acq On : 15 Mar 2018 8:34
 Operator : SJ/JU
 Sample : J1813-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Mar 15 11:05:33 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 15 05:35:28 2018
 Response via : Initial Calibration

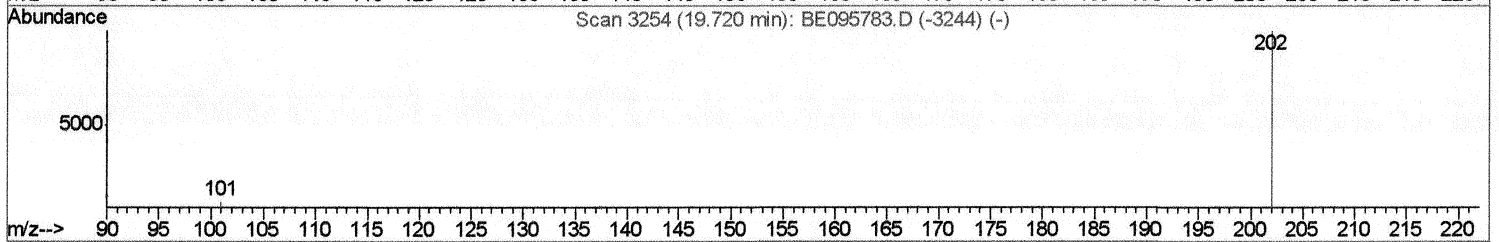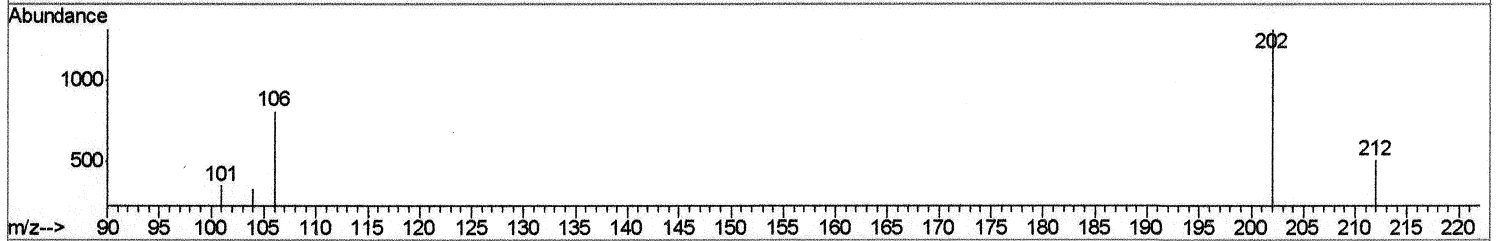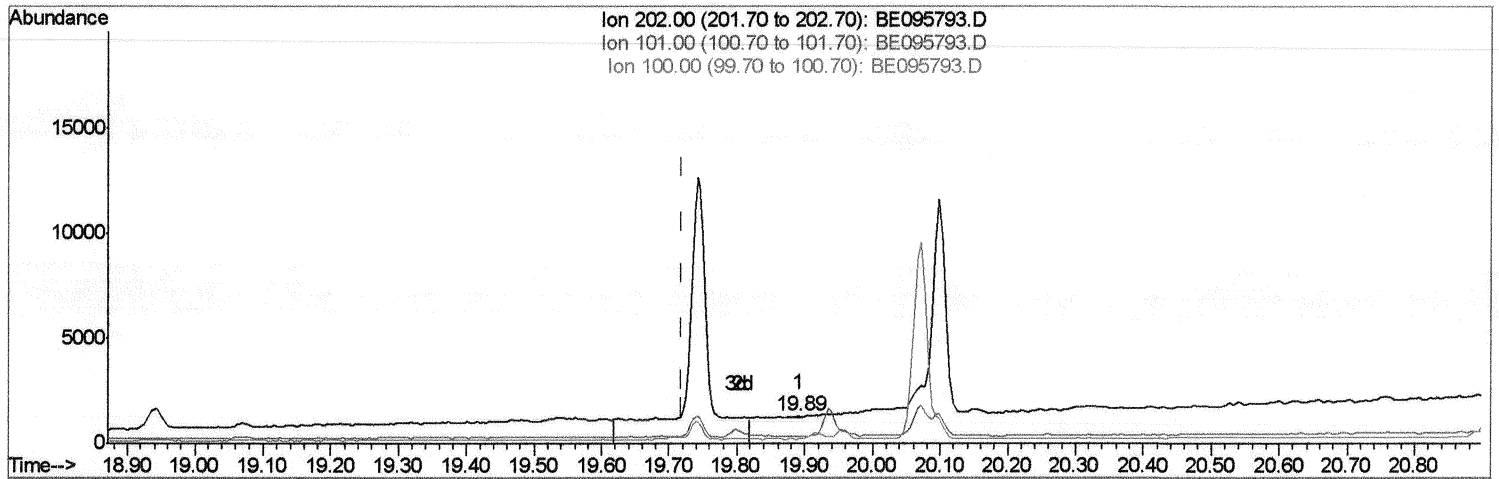

TIC: BE095793.D

(15) Fluoranthene (C)

19.891min (+0.172) 0.00ng/ul

response 96

Ion Exp% Act%

202.00 100 100

3/15/2018 6:55:22 PM

Sohil

APPROVED

Manual Integrations

FF636

ClientSampled :

BNA E




Instrument :

8.M Thu Mar 15 11:06:21 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095793.D
 Acq On : 15 Mar 2018 8:34
 Operator : SJ/JU
 Sample : J1813-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Mar 15 11:05:33 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Qlast Update : Thu Mar 15 05:35:28 2018
 Response via : Initial Calibration

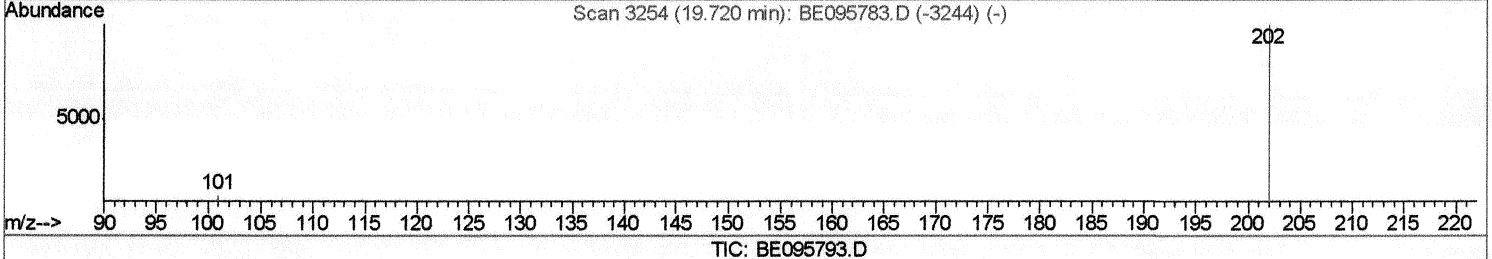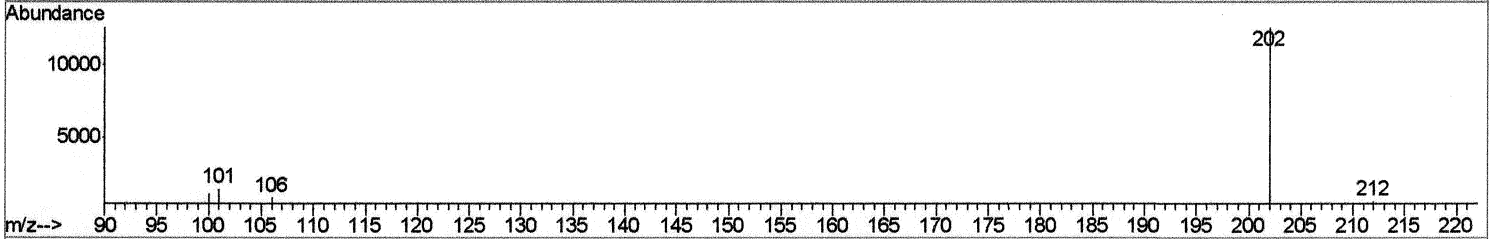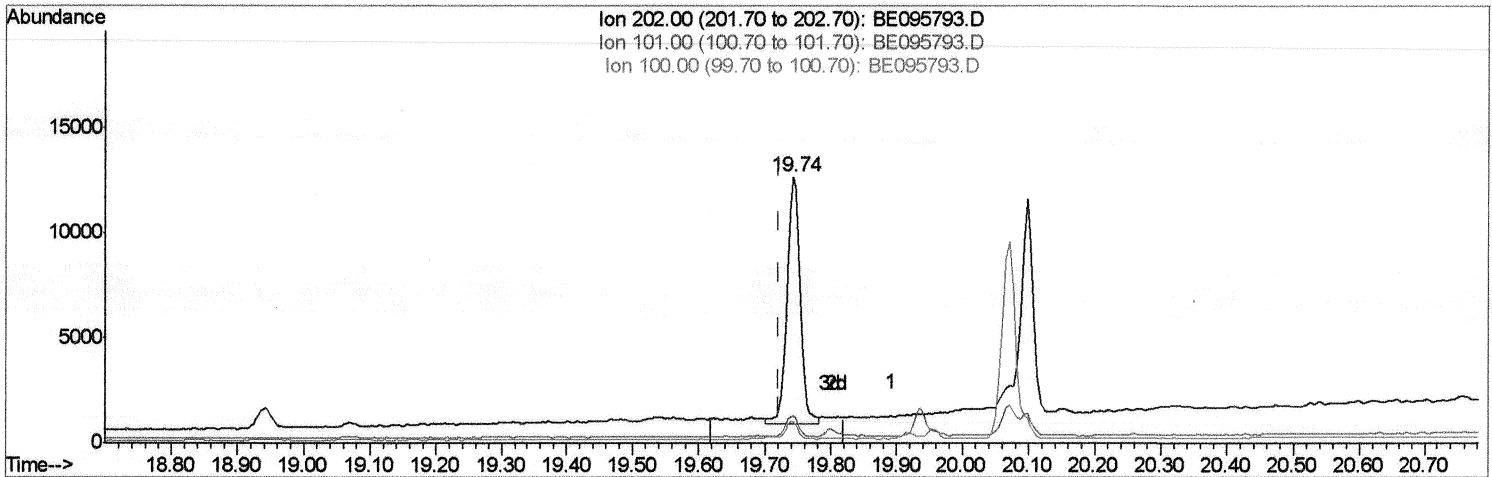

(15) Fluoranthene (C)

19.742min (+0.022) 0.57ng/ul m > 50 3/16/18

response 16222

Ion	Exp%	Act%
202.00	100	100

3/15/2018 6:55:22 PM
 Sohil
 APPROVED
 Manual Integrations




Instrument :
 BNA_E
 ClientSampleId :
 F6F36

8.M Thu Mar 15 11:06:38 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095793.D
 Acq On : 15 Mar 2018 8:34
 Operator : SJ/JU
 Sample : J1813-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Mar 15 11:05:33 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Qlast Update : Thu Mar 15 05:35:28 2018
 Response via : Initial Calibration

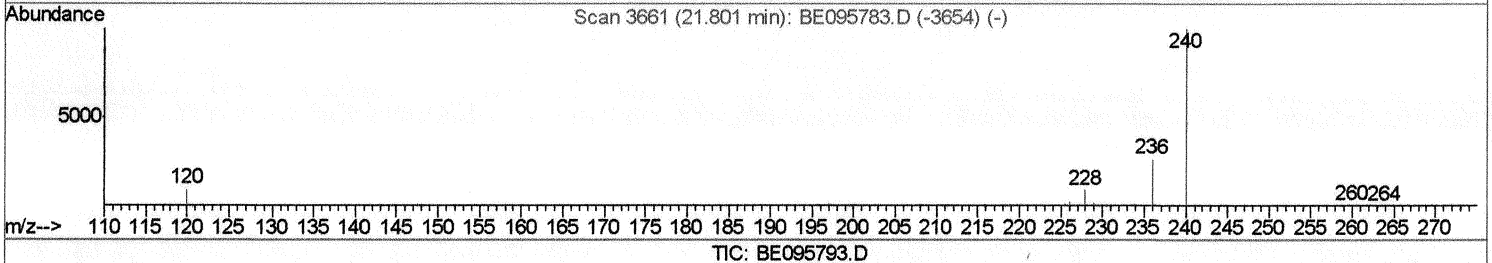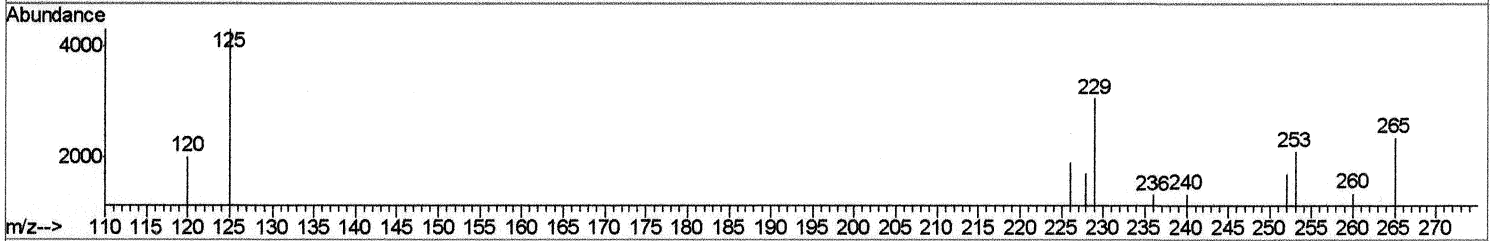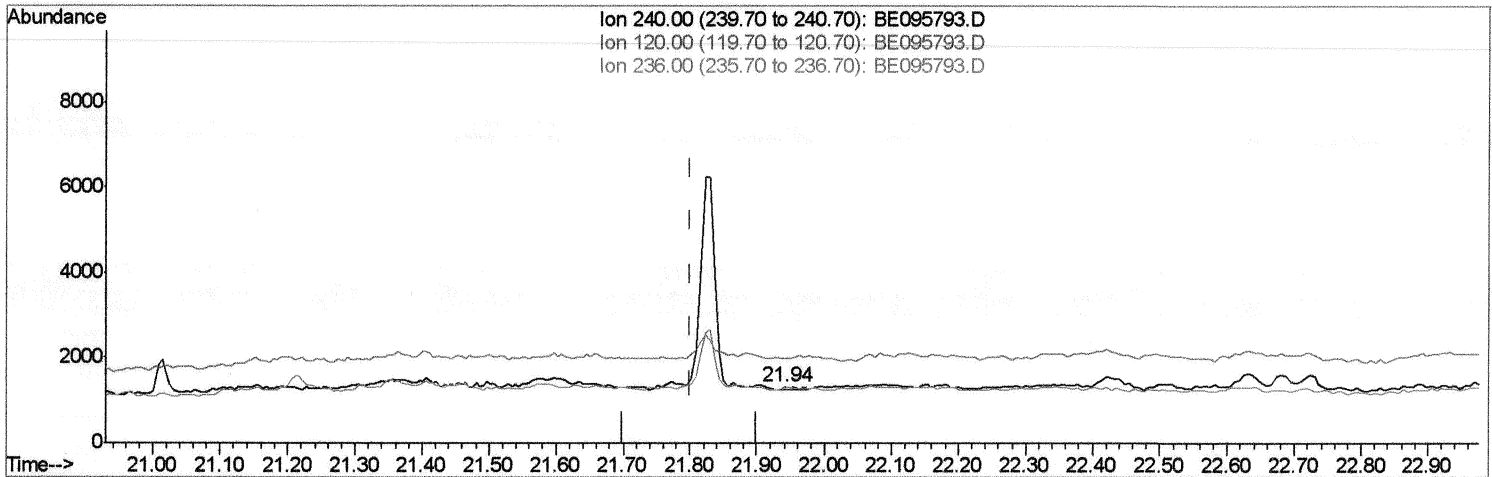

(16) Chrysene-d12 (I)

21.942min (+0.141) 0.40ng/ul

response 116

Ion	Exp%	Act%
240.00	100	100
120.00	100	150.72#
236.00	100	98.64#
260.00	100	100.00

120 236 240 260

3/15/2018 6:55:22 PM

Sohil

APPROVED

Manual Integrations

F6F36

ClientSampled :

BNA_E




Instrument :

8.M Thu Mar 15 11:06:45 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095793.D
 Acq On : 15 Mar 2018 8:34
 Operator : SJ/JU
 Sample : J1813-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Mar 15 11:05:33 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 15 05:35:28 2018
 Response via : Initial Calibration

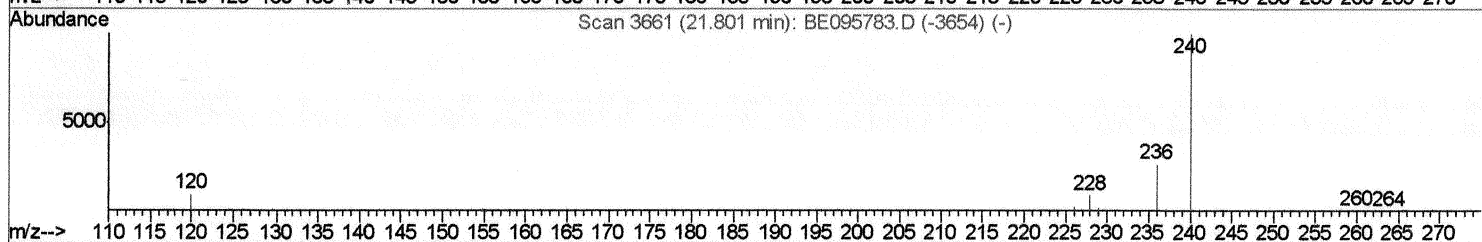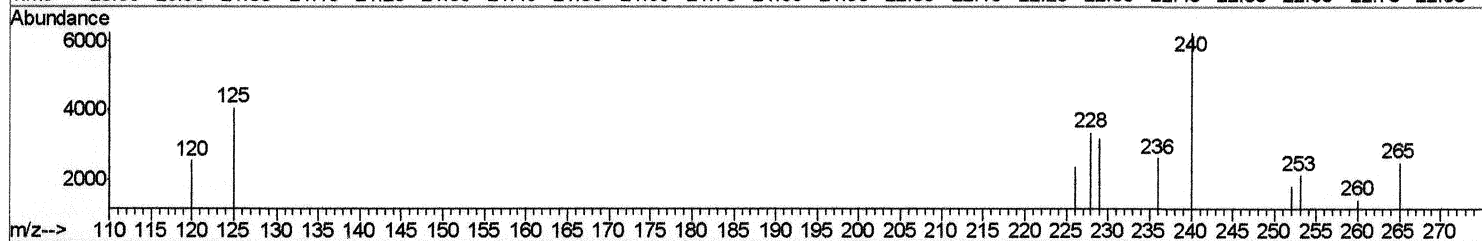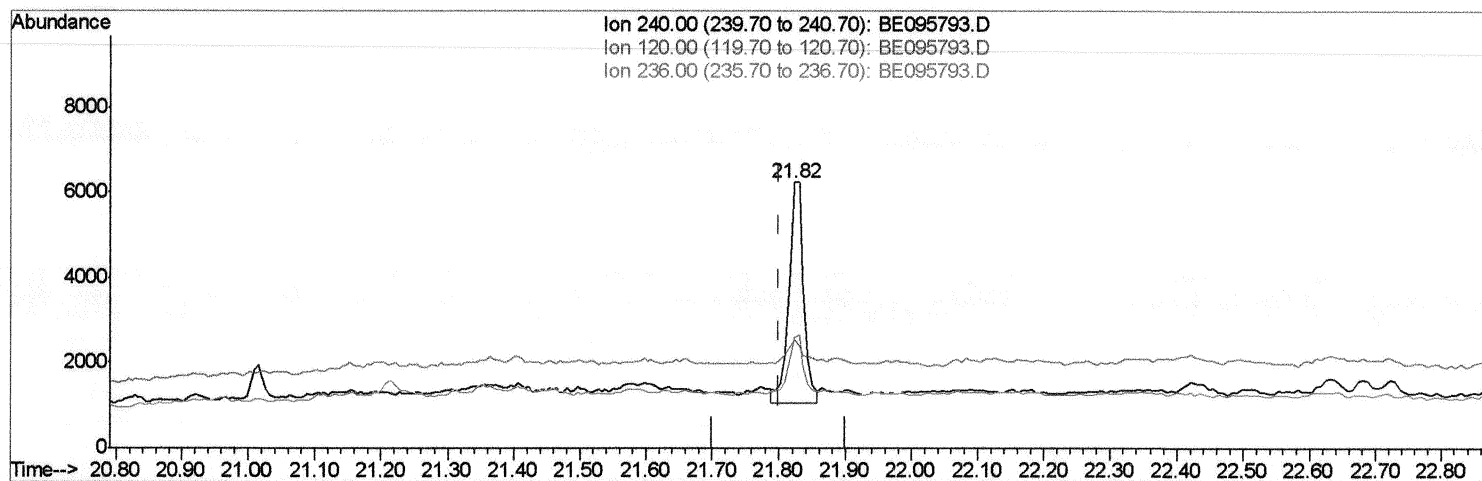

(16) Chrysene-d12 (I)

21.822min (+0.021) 0.40ng/ul m 2 50 3/16/18

response 8264

Ion	Exp%	Act%
240.00	100	100

3/15/2018 6:55:22 PM 40.77#

Sohil

41.91#

APPROVED Manual Integrations 100.00

FF36

ClientSampled :

BNA_E




Instrument :

8.M Thu Mar 15 11:07:03 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095793.D
 Acq On : 15 Mar 2018 8:34
 Operator : SJ/JU
 Sample : J1813-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Mar 15 11:05:33 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 15 05:35:28 2018
 Response via : Initial Calibration

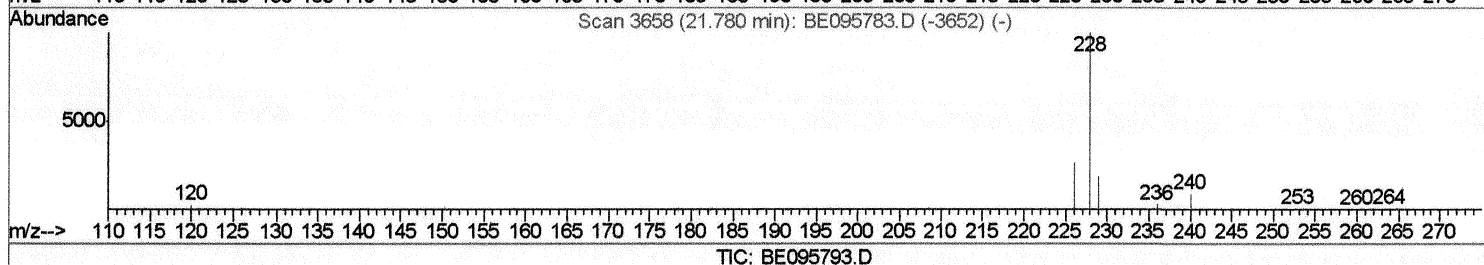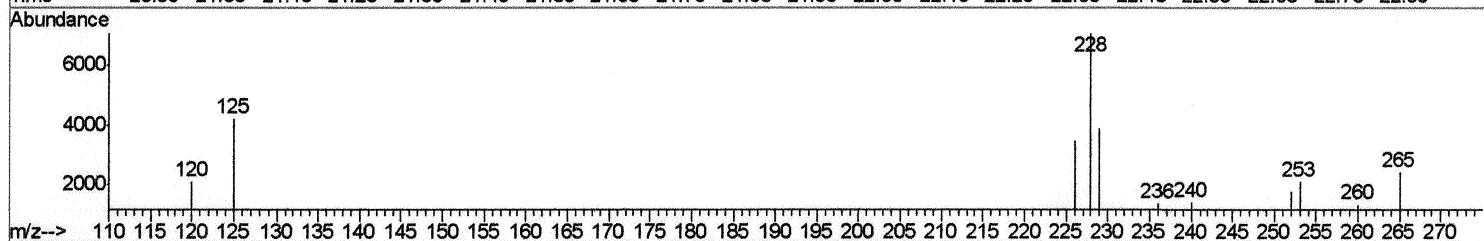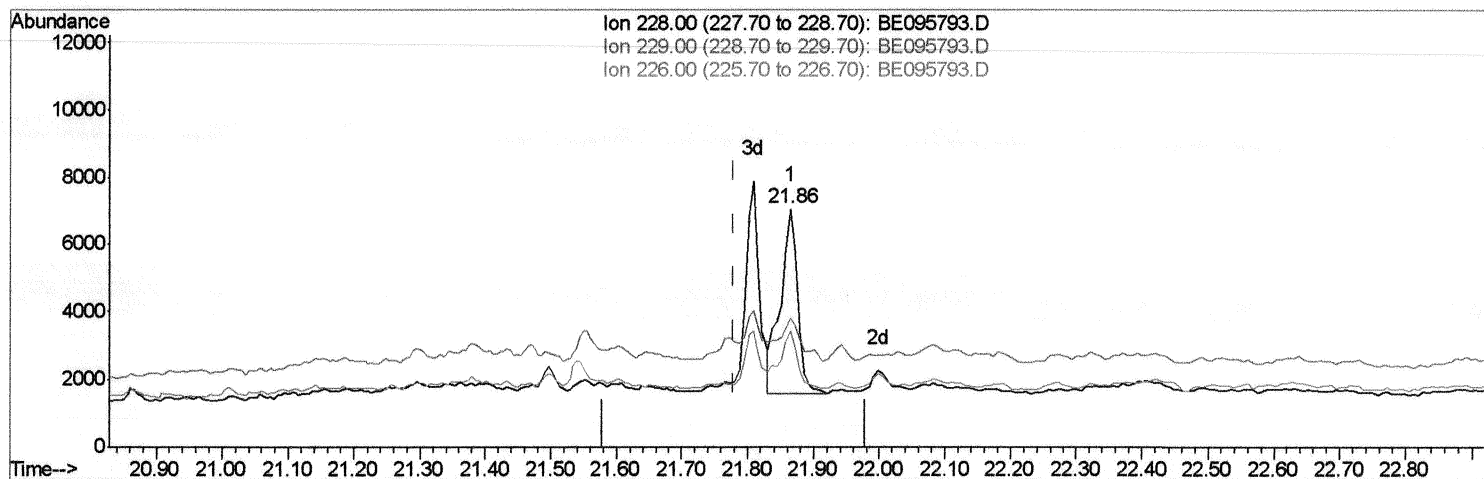

(18) Benzo(a)anthracene

21.864min (+0.085) 0.37ng/ul

response 9879

Ion Exp% Act%

228.00 100 100

3/15/2018 6:55:22 PM 54.46#

Sohil

APPROVED

Manual Integrations 48.70#

100.00

F6F36

ClientSampled :

BNA_E




Instrument :

8.M Thu Mar 15 11:07:17 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095793.D
 Acq On : 15 Mar 2018 8:34
 Operator : SJ/JU
 Sample : J1813-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Mar 15 11:05:33 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 15 05:35:28 2018
 Response via : Initial Calibration

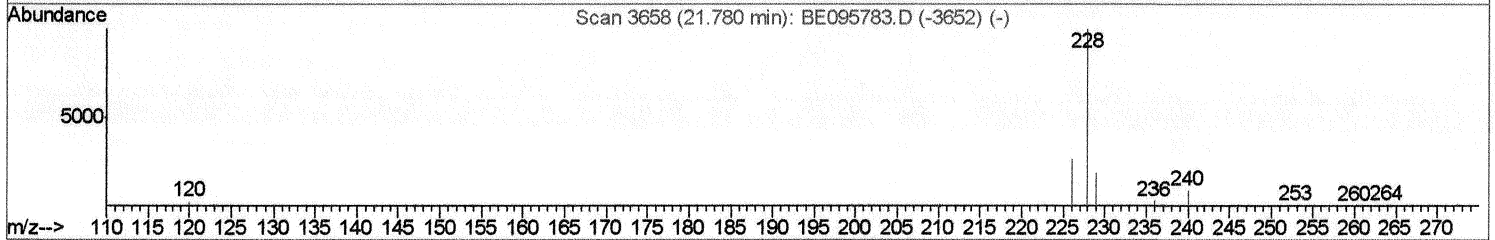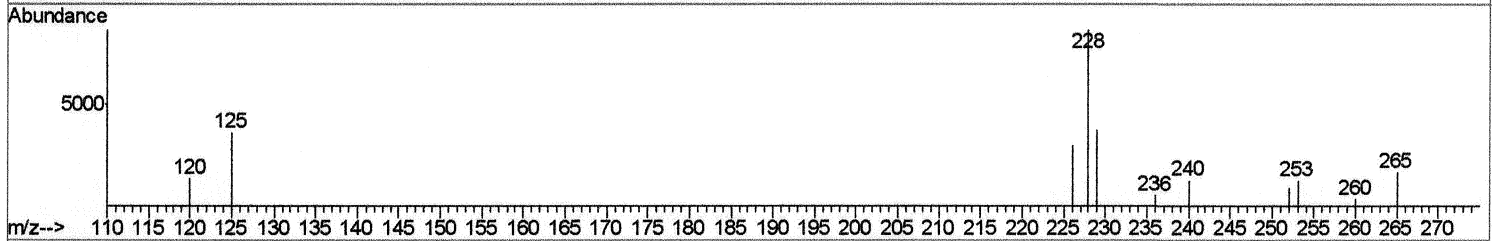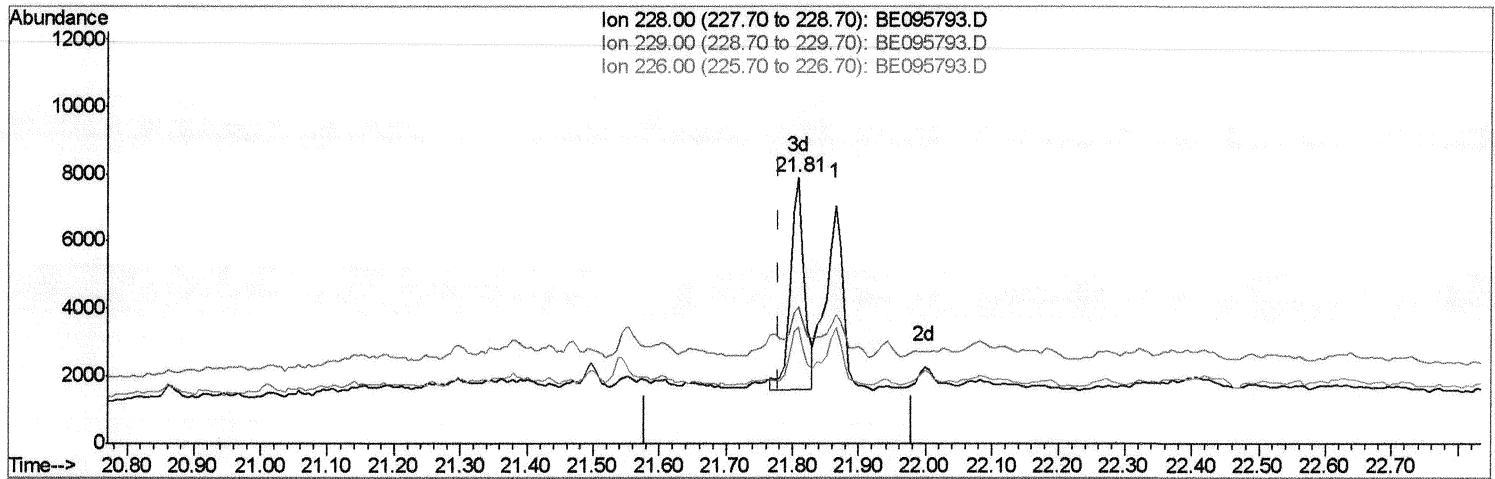

TIC: BE095793.D

(18) Benzo(a)anthracene

21.808min (+0.029) 0.36ng/ul m > ss 3/16/18

response 9468

Ion	Exp%	Act%
228.00	100	100
51.25#		
43.97#		
0.00		

3/15/2018 6:55:22 PM

Sohil

APPROVED

Manual Integrations

F6F36

ClientSampled :

BNA_E




Instrument :

8.M Thu Mar 15 11:07:41 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095793.D
 Acq On : 15 Mar 2018 8:34
 Operator : SJ/JU
 Sample : J1813-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Mar 15 11:05:33 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 15 05:35:28 2018
 Response via : Initial Calibration

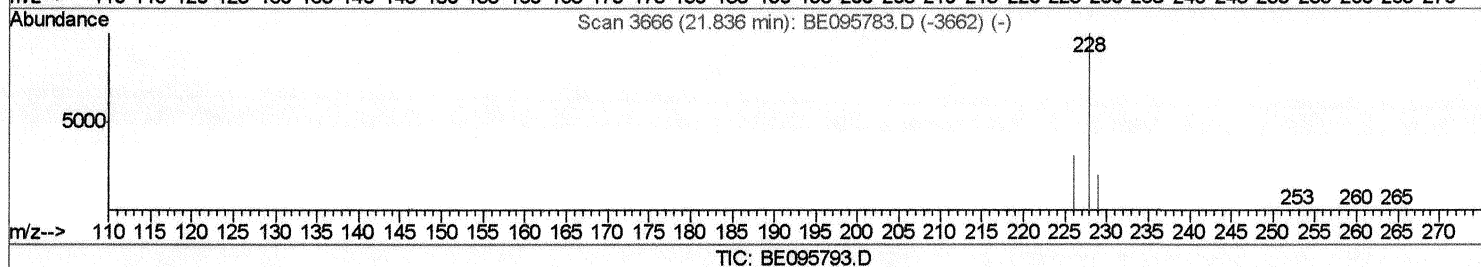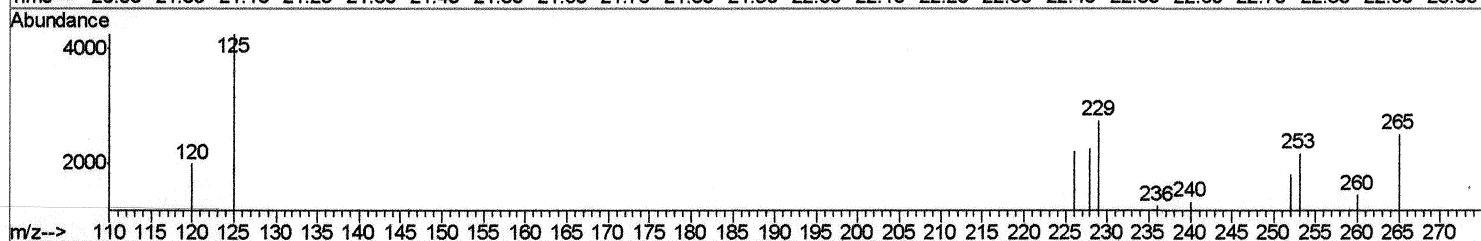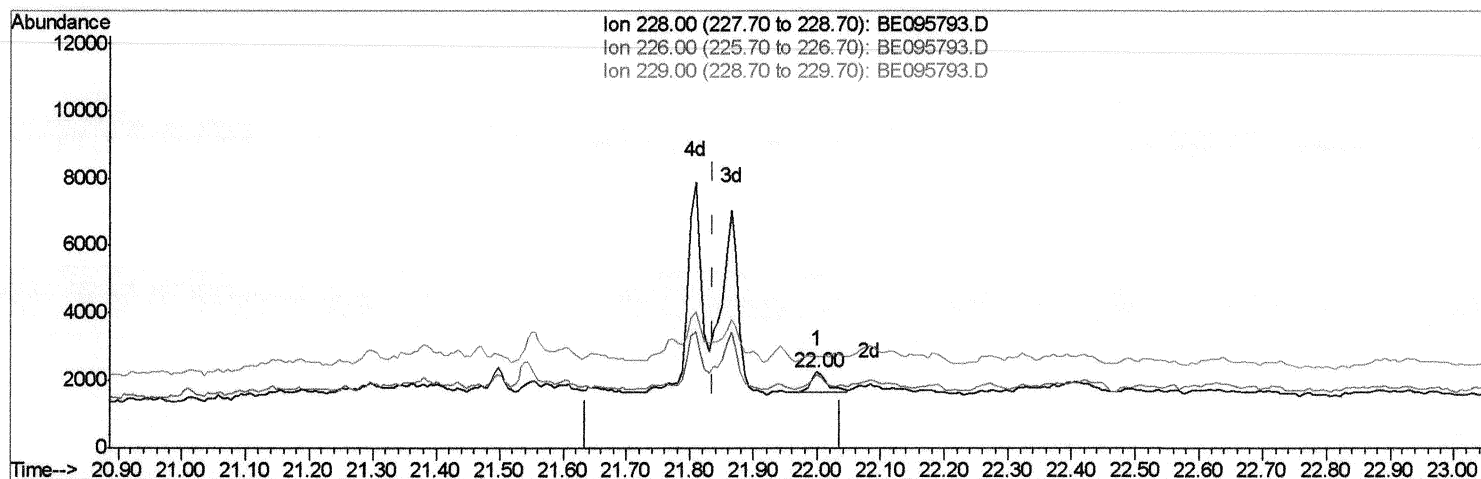

(19) Chrysene

21.998min (+0.162) 0.04ng/ul

response 1124

Ion	Exp%	Act%
228.00	100	100
228.00	100	97.95#
228.00	100	21.75#
228.00	100	100

3/15/2018 6:55:22 PM

APPROVED

Manual Integrations

F6F36

ClientSampled :

BNA_E




Instrument :

8.M Thu Mar 15 11:07:54 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095793.D
 Acq On : 15 Mar 2018 8:34
 Operator : SJ/JU
 Sample : J1813-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Mar 15 11:05:33 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Qlast Update : Thu Mar 15 05:35:28 2018
 Response via : Initial Calibration

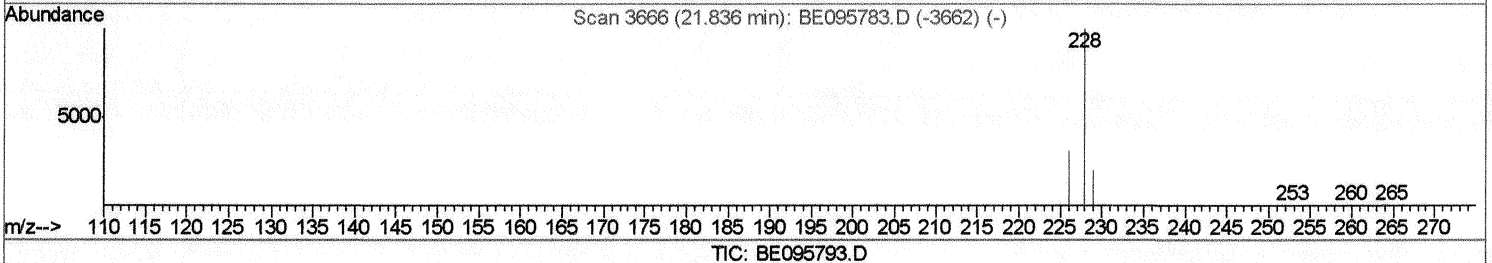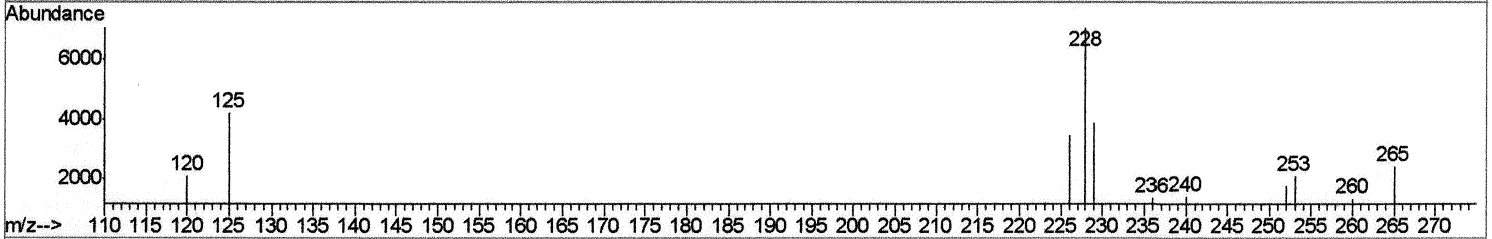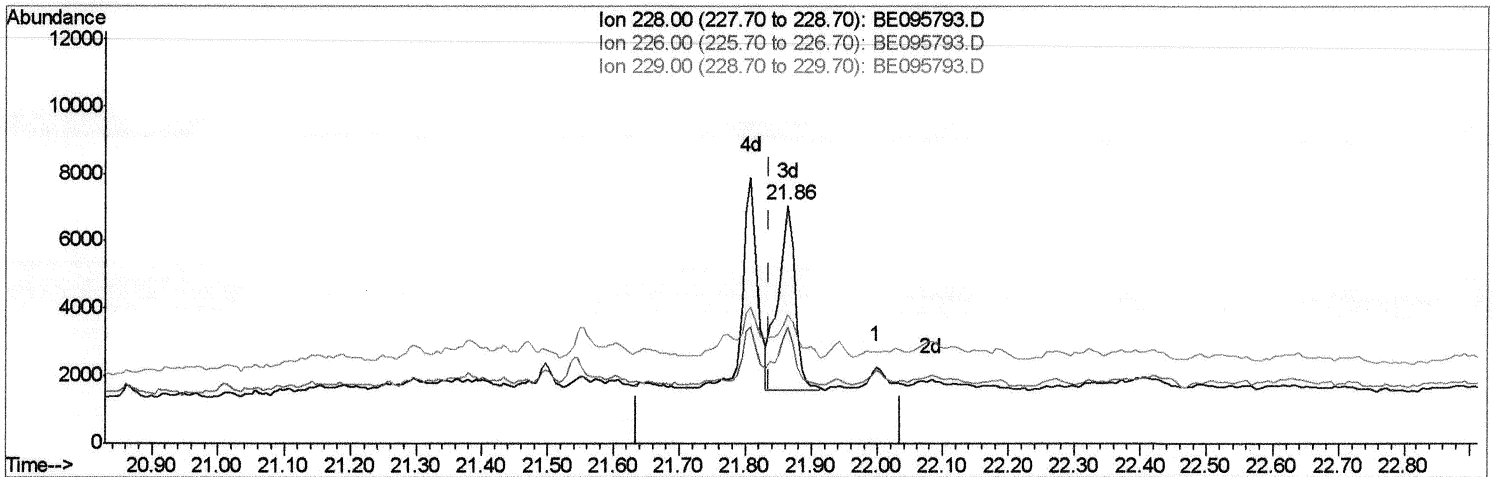

(19) Chrysene

21.864min (+0.029) 0.37ng/ul m > 50 3/16/18

response 10018

Ion	Exp%	Act%
228.00	100	100
226.00	48.70	54.46
229.00	0.00	0.00

Instrument: BNA_E




Client: Sampled

8.M Thu Mar 15 11:08:19 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095793.D
 Acq On : 15 Mar 2018 8:34
 Operator : SJ/JU
 Sample : J1813-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Mar 15 11:05:33 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 15 05:35:28 2018
 Response via : Initial Calibration

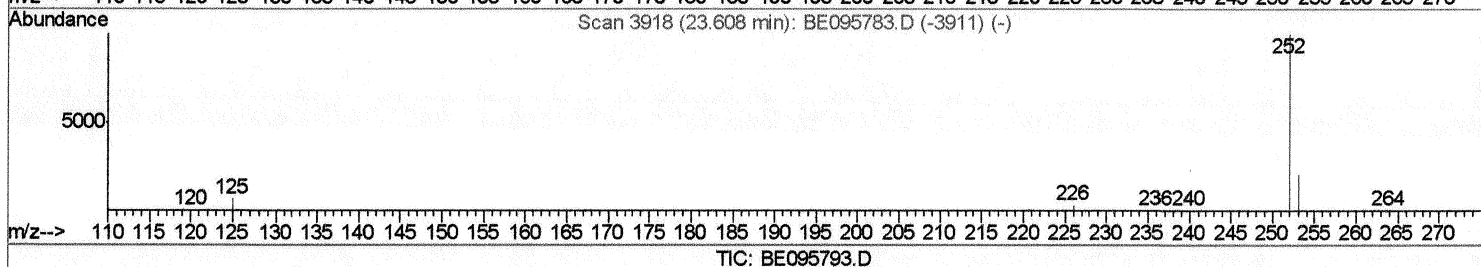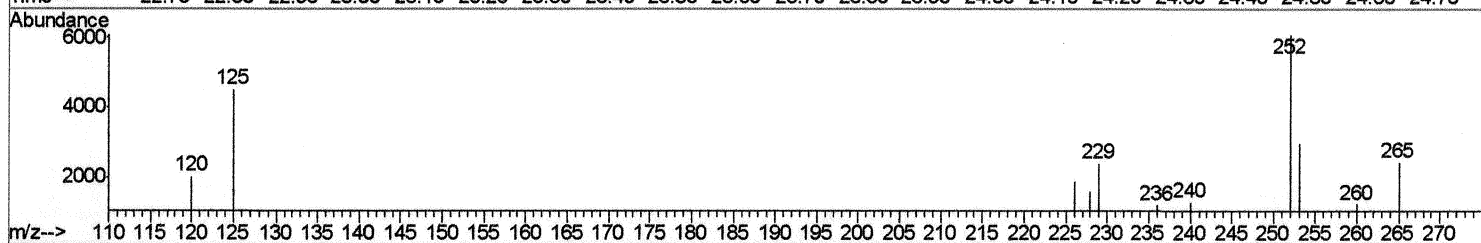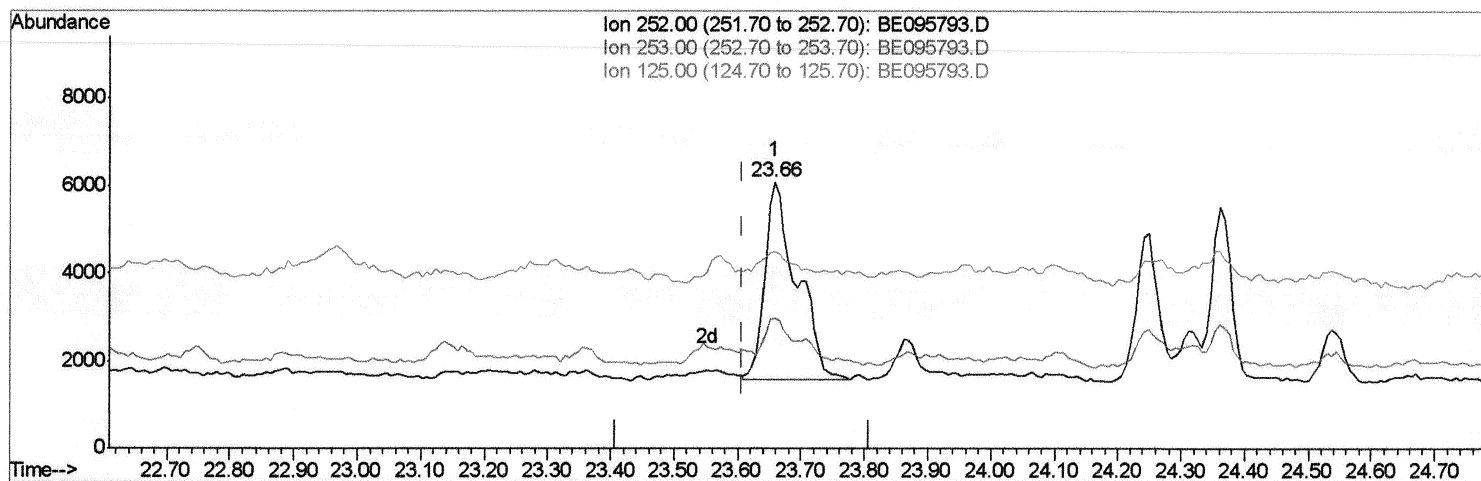

TIC: BE095793.D

(21) Benzo(b)fluoranthene
 23.657min (+0.050) 0.55ng/ul
 response 15633

Ion	Exp%	Act%
252.00	100	100

3/15/2018 6:55:22 PM

Sohil

APPROVED

Manual Integrations

F6F36

Client Sampled :

BNA_E




Instrument :

8.M Thu Mar 15 11:08:43 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095793.D
 Acq On : 15 Mar 2018 8:34
 Operator : SJ/JU
 Sample : J1813-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Mar 15 11:05:33 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 15 05:35:28 2018
 Response via : Initial Calibration

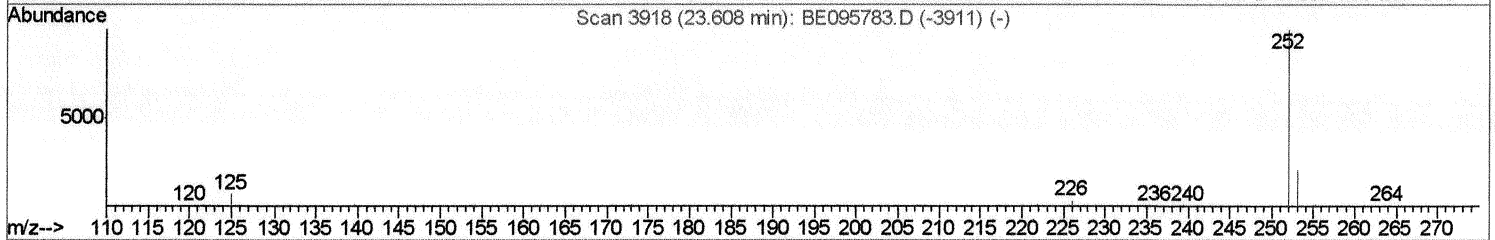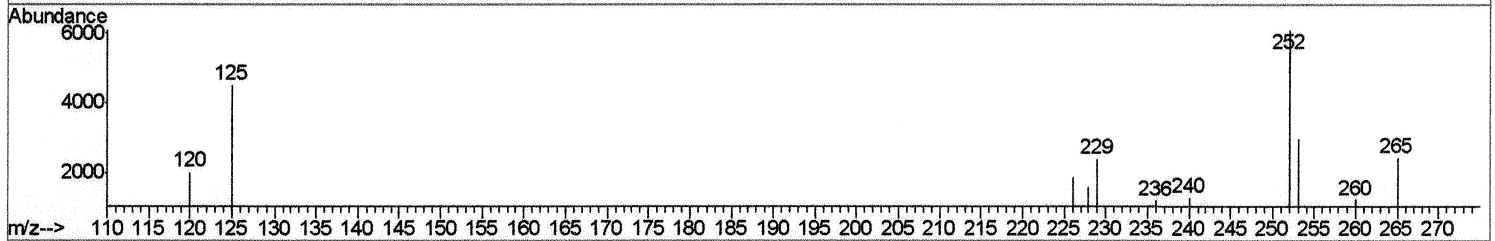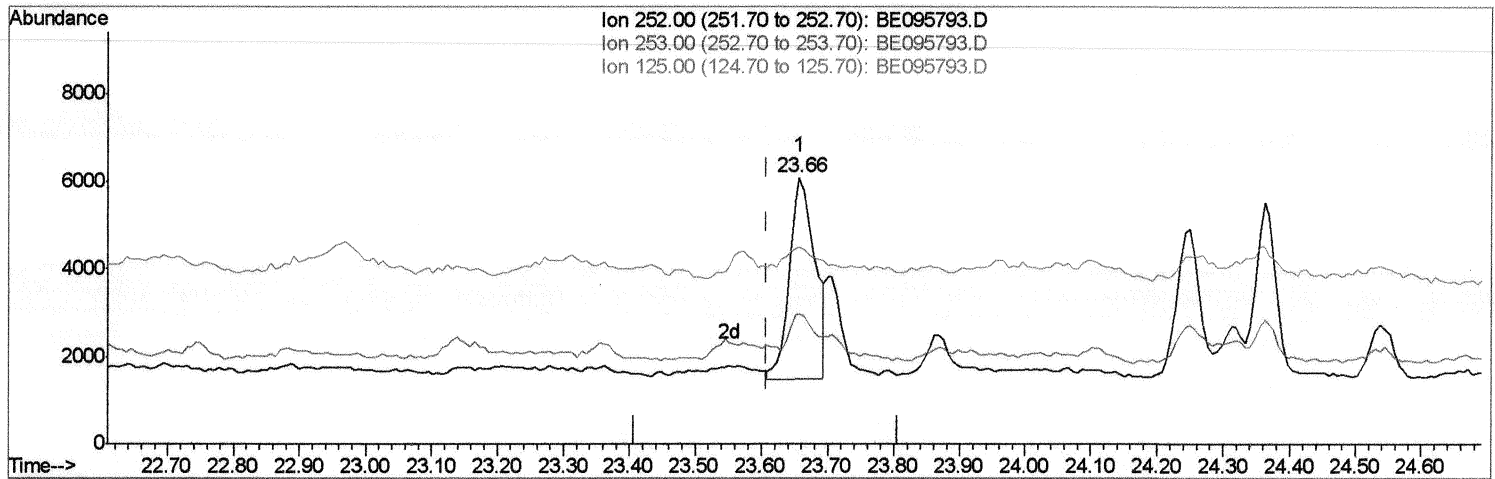

(21) Benzo(b)fluoranthene

23.657min (+0.050) 0.44ng/ul m> 52 3/16/18

response 12429




Ion	Exp%	Act%
252.00	100	100
252.05	48.92	74.18
252.10	0.00	0.00

Instrument : BNA_E
 ClientSampled : 8.M Thu Mar 15 11:09:15 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095793.D
 Acq On : 15 Mar 2018 8:34
 Operator : SJ/JU
 Sample : J1813-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Mar 15 11:05:33 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 15 05:35:28 2018
 Response via : Initial Calibration

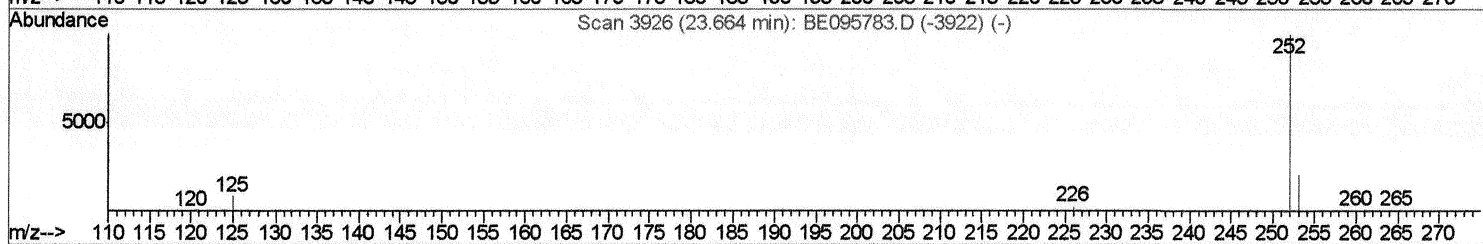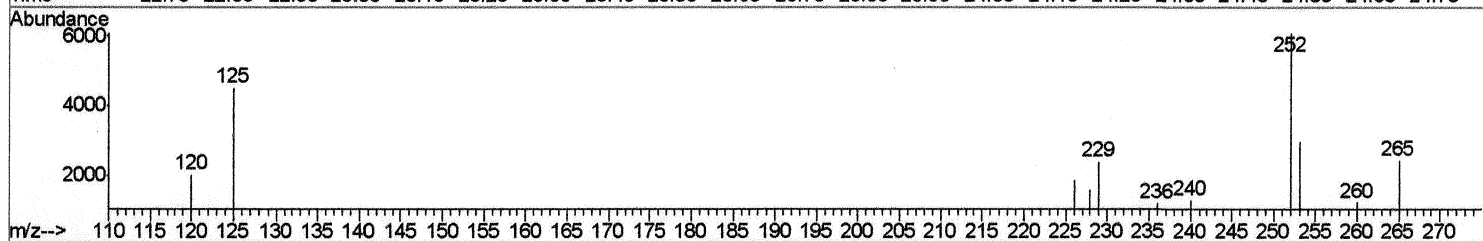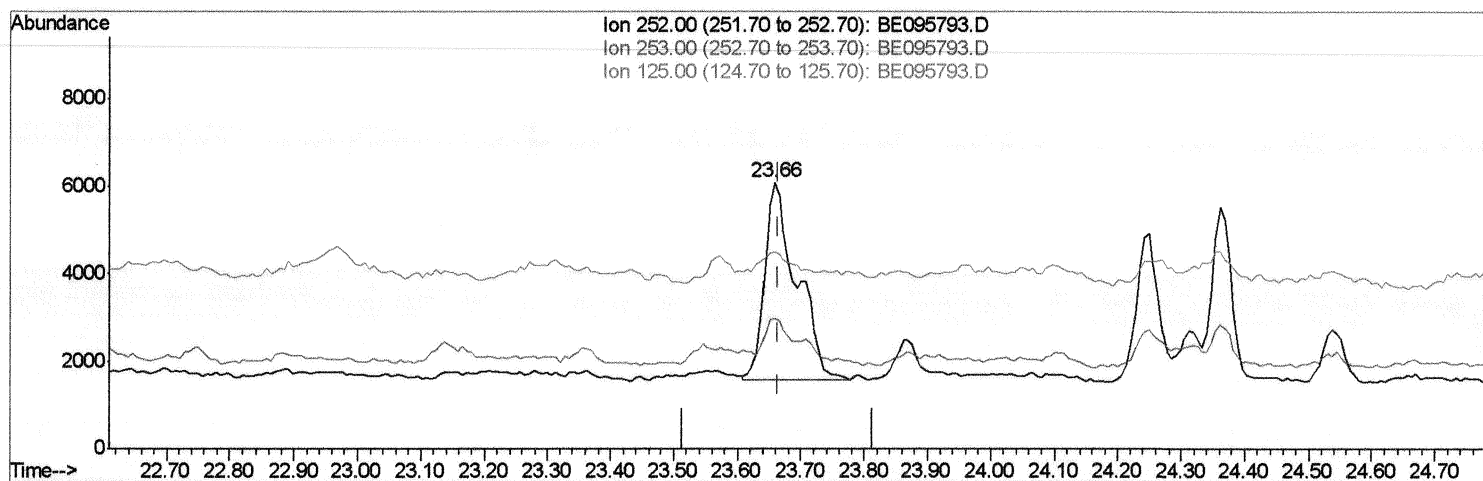

TIC: BE095793.D

(22) Benzo(k)fluoranthene

23.657min (-0.007) 0.58ng/ul

response 15633

Ion Exp% Act%

252.00 100 100

3/15/2018 6:55:22 PM 48.92#

Sohil

APPROVED 74.18#

Manual Integrations 100.00

F6F36

ClientSampled :

BNA_E




Instrument :

8.M Thu Mar 15 11:09:26 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095793.D
 Acq On : 15 Mar 2018 8:34
 Operator : SJ/JU
 Sample : J1813-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Mar 15 11:05:33 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Qlast Update : Thu Mar 15 05:35:28 2018
 Response via : Initial Calibration

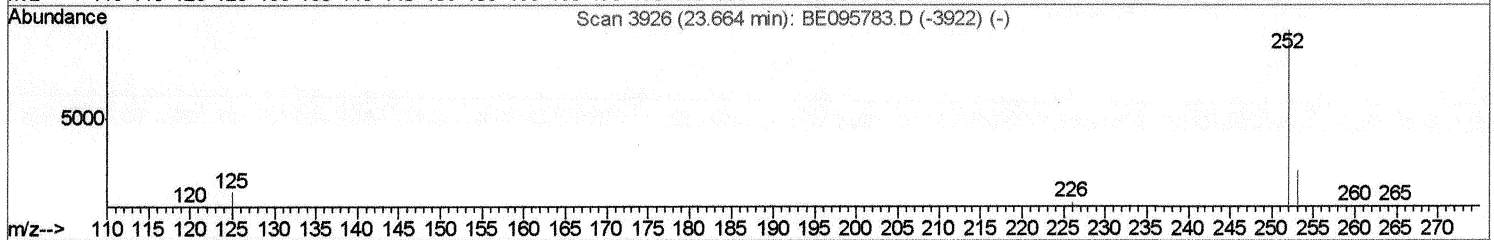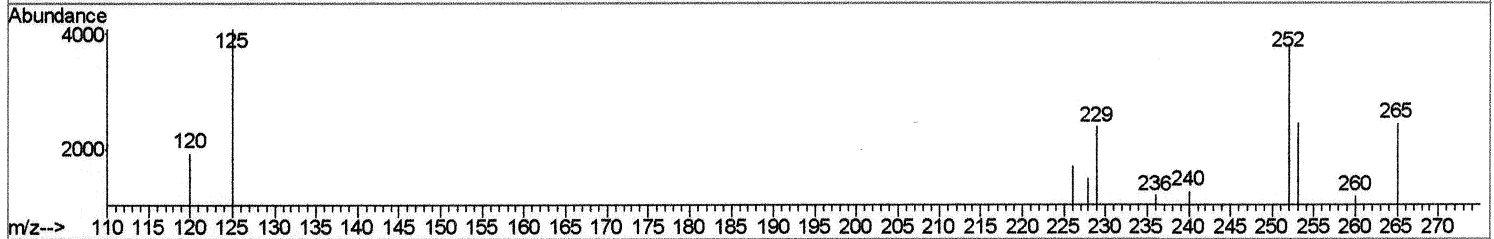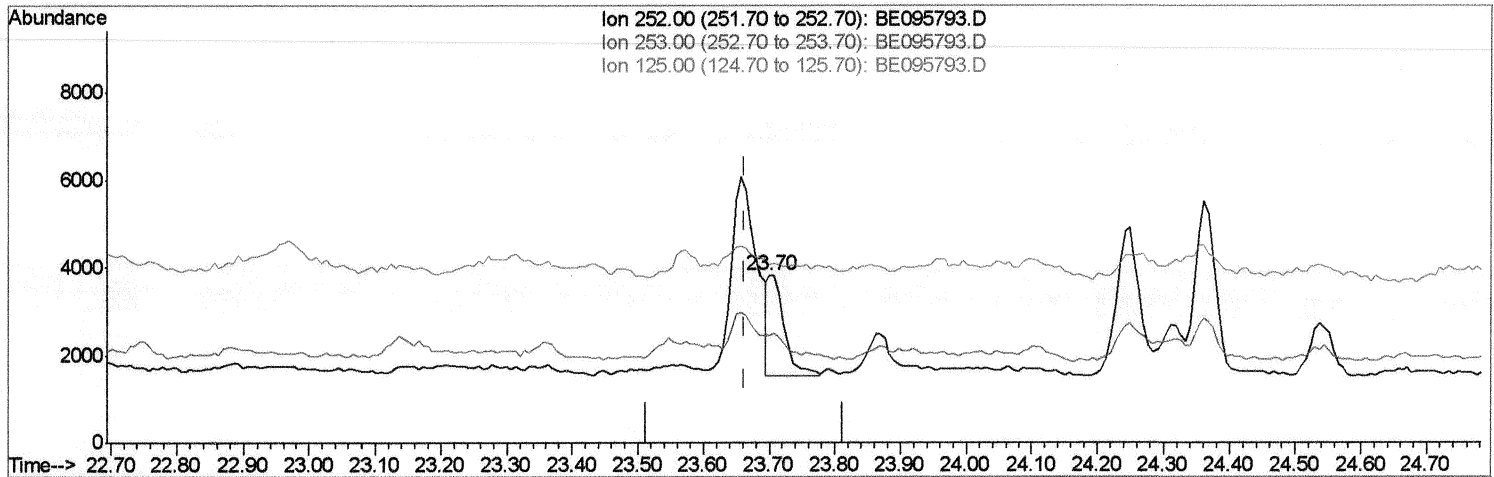

TIC: BE095793.D

(22) Benzo(k)fluoranthene

23.700min (+0.036) 0.15ng/ul m) 50 3/16/18

response 4033

Ion	Exp%	Act%
252.00	100	100
253.00	100	64.66#
125.00	100	106.98#
120.00	100	0.00

3/15/2018 6:55:22 PM

Sohil

APPROVED

Manual Integrations

FF36

Client Sampled :

BNA E

Instrument :

8.M Thu Mar 15 11:09:50 2018

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
 Data File : BE095793.D
 Acq On : 15 Mar 2018 8:34
 Operator : SJ/JU
 Sample : J1813-11
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Mar 15 11:10:44 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 15 05:35:28 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2115	0.40	ng/ul	0.02
2) Naphthalene-d8	11.27	136	6320	0.40	ng/ul	0.02
6) Acenaphthene-d10	15.03	164	3831	0.40	ng/ul	0.02
10) Phenanthrene-d10	17.73	188	7811m	0.40	ng/ul	0.02
16) Chrysene-d12	21.82	240	8264m	0.40	ng/ul	0.02
20) Perylene-d12	24.48	264	8201	0.40	ng/ul	0.05

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.83	152	4141	0.39	ng/ul	0.02
14) Fluoranthene-d10	19.71	212	9919m	0.40	ng/ul	0.03

Target Compounds

Ovalue

3) Naphthalene	11.32	128	1338	0.076	ng/ul#	81
5) 2-Methylnaphthalene	12.90	142	525	0.043	ng/ul	97
8) Acenaphthene	15.09	153	1340	0.092	ng/ul	93
9) Fluorene	16.06	166	859	0.054	ng/ul#	69
11) Pentachlorophenol	17.51	266	36	0.033	ng/ul#	51
12) Phenanthrene	17.77	178	10411m	0.445	ng/ul	
13) Anthracene	17.87	178	2402m	0.110	ng/ul	
15) Fluoranthene	19.74	202	16222m	0.572	ng/ul	
17) Pyrene	20.10	202	14365	0.458	ng/ul#	79
18) Benzo(a)anthracene	21.81	228	9468m	0.355	ng/ul	
19) Chrysene	21.86	228	10018m	0.369	ng/ul	
21) Benzo(b)fluoranthene	23.66	252	12429m	0.438	ng/ul	
22) Benzo(k)fluoranthene	23.70	252	4033m	0.149	ng/ul	
23) Benzo(a)pyrene	24.36	252	8419	0.325	ng/ul#	36
24) Indeno(1,2,3-cd)pyrene	27.32	276	5535	0.192	ng/ul#	67
26) Benzo(a,h,i)perylene	28.22	276	6165	0.250	ng/ul#	40

(#) = qualifier out of range (m) = manual integration (+) = signals summed

3/15/2018 6:55:22 PM

Sohil

Manual Integrations
 APPROVED

Instrument : BNA_E
 Client Sampled : F6F36

M Thu Mar 15 11:11:09 2018