

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE031419\
 Data File : BE098950.D
 Acq On : 14 Mar 2019 19:16
 Operator : JU/SJ
 Sample : K1882-03
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW305S-20190312

Quant Time: Mar 15 05:32:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 06 15:33:24 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	692	0.40	ng	0.01
7) Naphthalene-d8	10.60	136	3228	0.40	ng	0.01
13) Acenaphthene-d10	14.46	164	2355	0.40	ng	0.00
19) Phenanthrene-d10	17.22	188	5623	0.40	ng	0.00
27) Chrysene-d12	21.40	240	6566	0.40	ng	0.00
34) Perylene-d12	23.89	264	6197	0.40	ng	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.41	112	278	0.13	ng	0.02
5) Phenol-d6	7.03	99	191	0.07	ng	0.05
8) Nitrobenzene-d5	9.03	82	953	0.28	ng	0.06
11) 2-Methylnaphthalene-d10	12.21	152	2011	0.34	ng	0.01
14) 2,4,6-Tribromophenol	15.97	330	404	0.34	ng	0.00
15) 2-Fluorobiphenyl	13.09	172	4625	0.47	ng	0.00
25) Fluoranthene-d10	19.24	212	30383	0.34	ng	0.00
29) Terphenyl-d14	19.84	244	7590	0.48	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.28	88	62	Below Cal	#	1
3) n-Nitrosodimethylamine	3.67	42	46	0.026 ng	#	14
22) Pentachlorophenol	16.91	266	10	0.273 ng		93
32) Bis(2-ethylhexyl)phthalate	21.29	149	3348	0.077 ng		99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE031419\
Data File : BE098950.D
Acq On : 14 Mar 2019 19:16
Operator : JU/SJ
Sample : K1882-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BPS1-TT-MW305S-20190312

Quant Time: Mar 15 05:32:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 06 15:33:24 2019
Response via : Initial Calibration

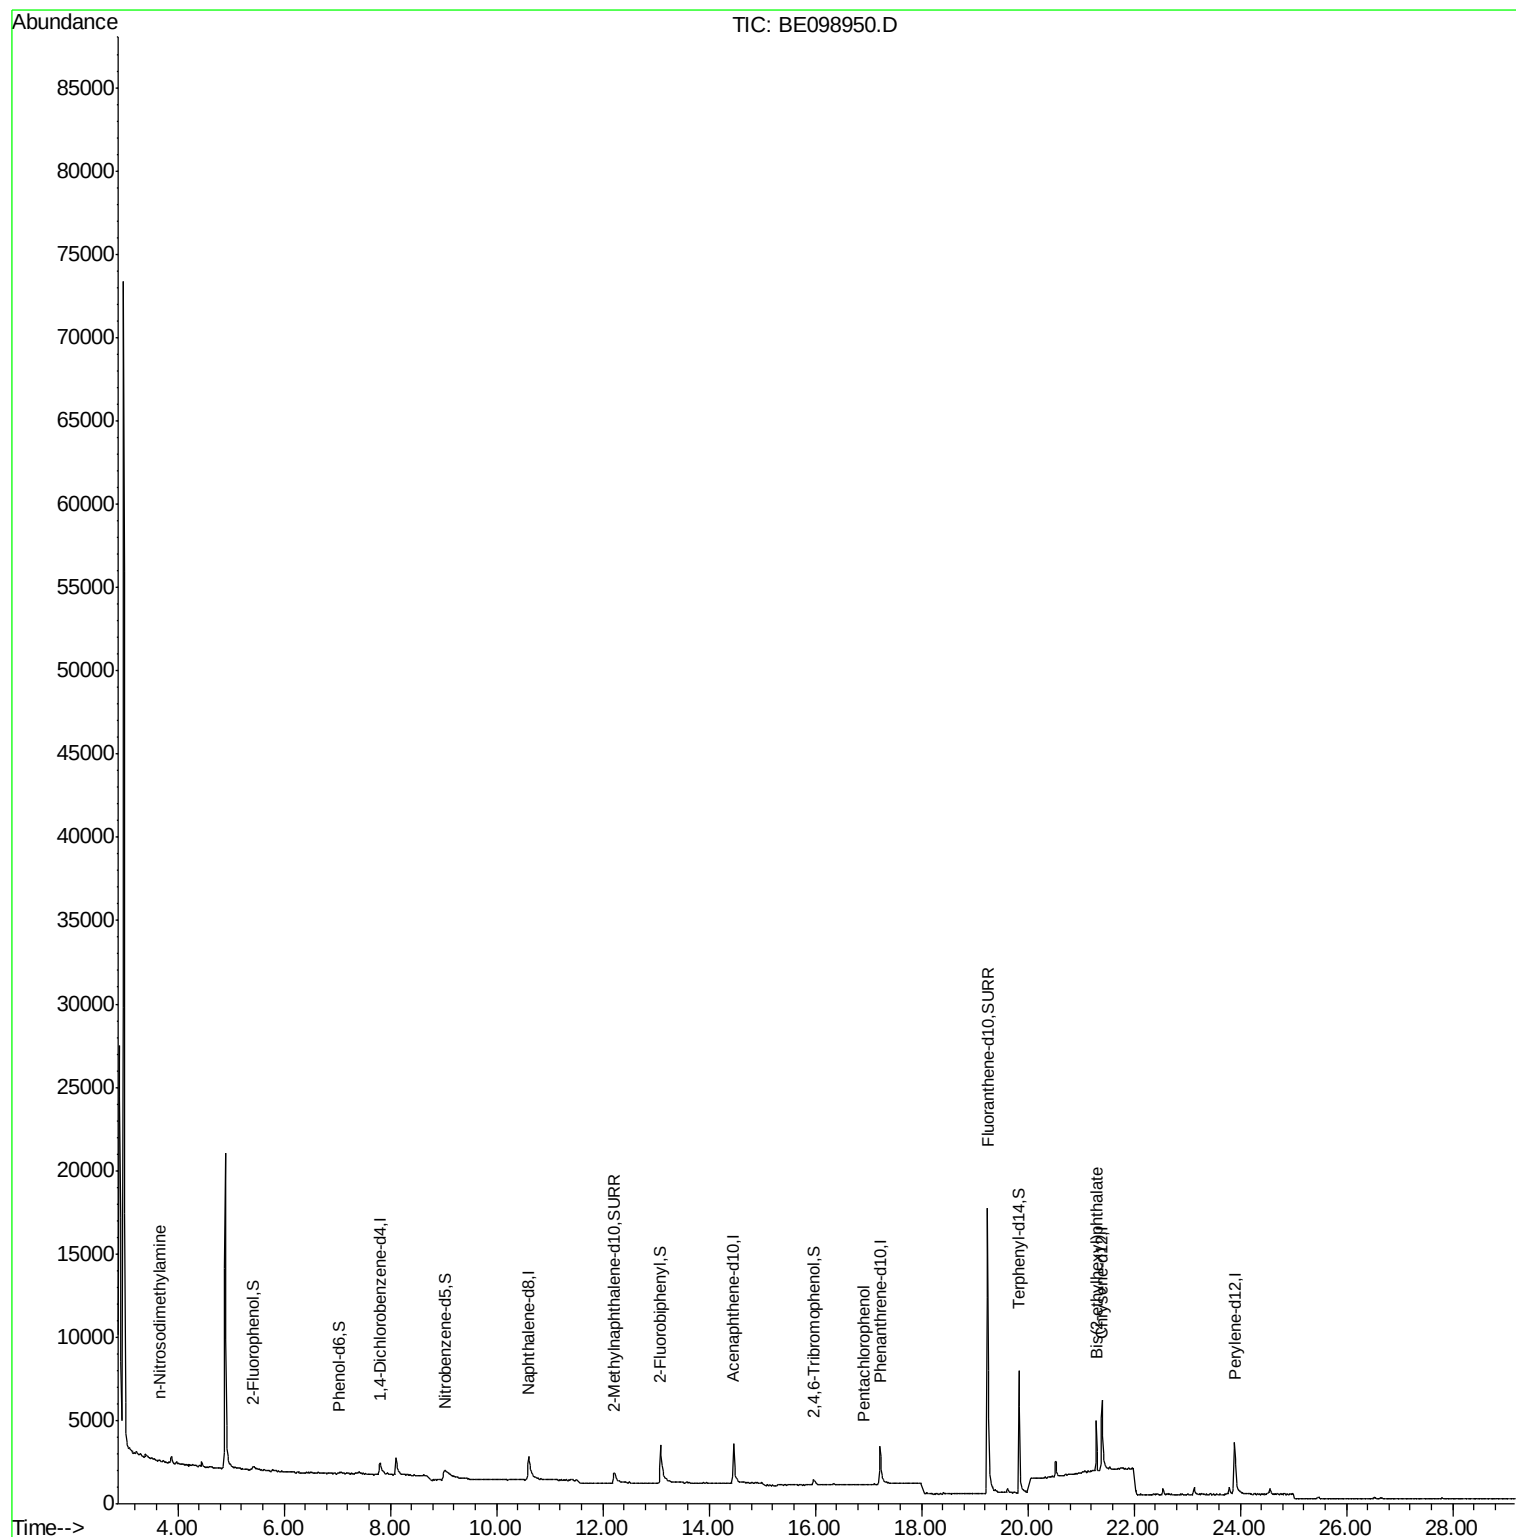




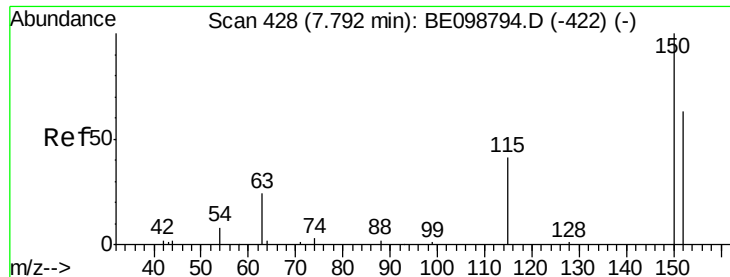


#1

1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.80 min Scan# 429
Delta R.T. 0.01 min
Lab File: BE098950.D
Acq: 14 Mar 2019 19:16

Instrument :
BNA_E
ClientSampleId :
BPS1-TT-MW305S-20190312




Tgt Ion: 152 Resp: 692
Ion Ratio Lower Upper
152 100
150 155.4 122.5 183.7
115 75.8 57.4 86.2

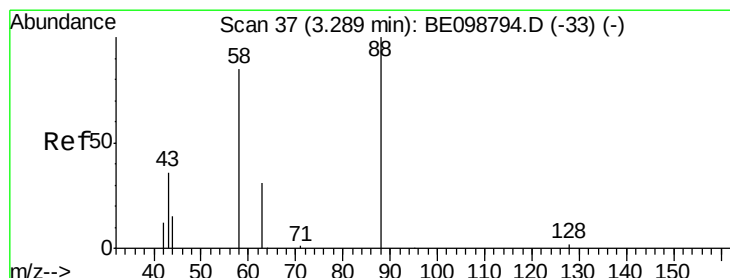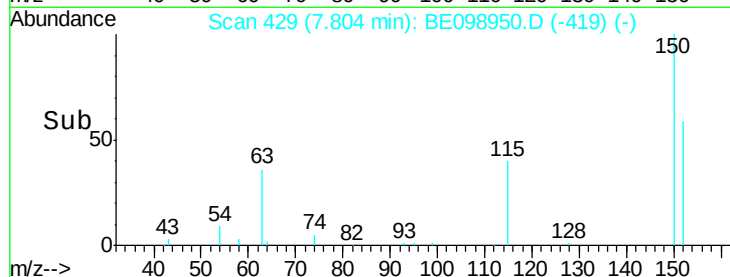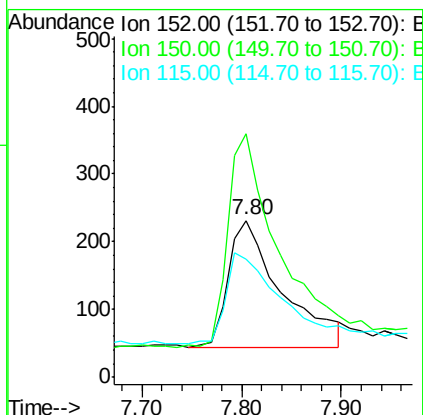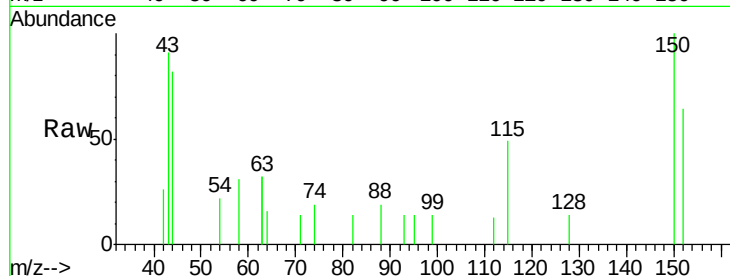


#2

1,4-Dioxane
Concen: Below Cal
RT: 3.28 min Scan# 36
Delta R.T. -0.01 min
Lab File: BE098950.D
Acq: 14 Mar 2019 19:16

Tgt Ion: 88 Resp: 62
Ion Ratio Lower Upper
88 100
58 0.0 75.8 113.6#
43 433.9 41.8 62.8#

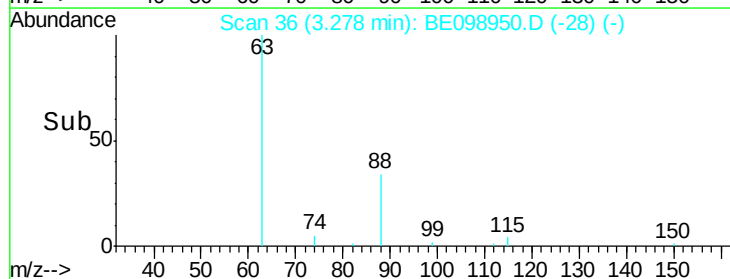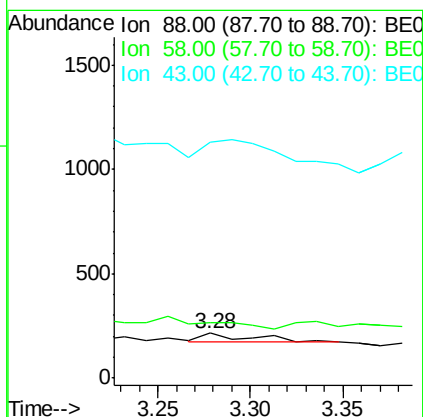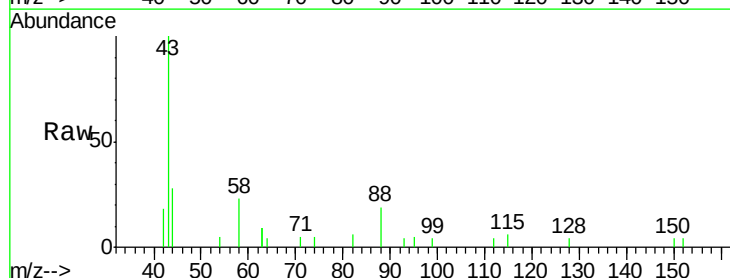

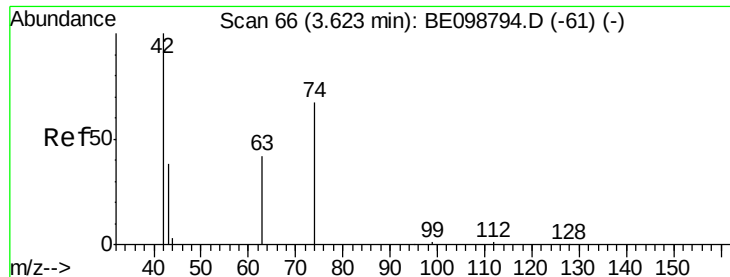

#3

n-Nitrosodimethylamine

Concen: 0.026 ng

RT: 3.67 min Scan# 70

Delta R.T. 0.05 min

Lab File: BE098950.D

Acq: 14 Mar 2019 19:16

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW305S-20190312


Tgt Ion: 42 Resp: 46

Ion Ratio Lower Upper

42 100

74 0.0 57.0 85.4#




44 73.9 0.0 0.0#

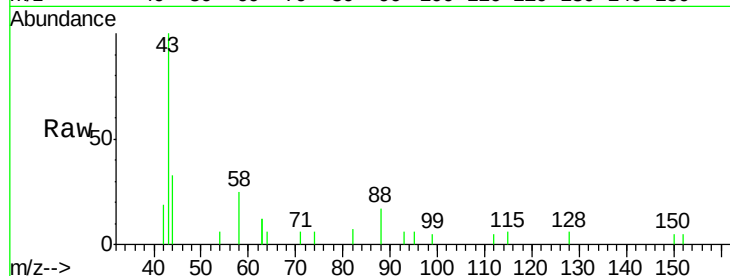

Abundance Ion 42.00 (41.70 to 42.70): BE0

Ion 74.00 (73.70 to 74.70): BE0

Ion 44.00 (43.70 to 44.70): BE0

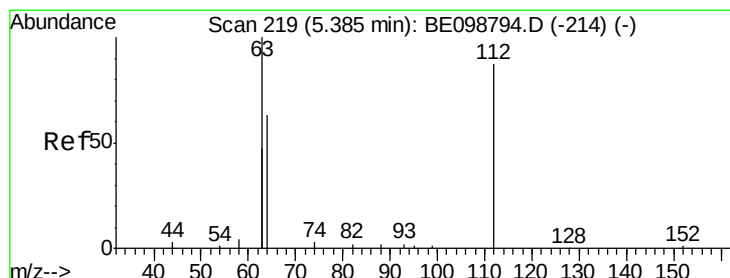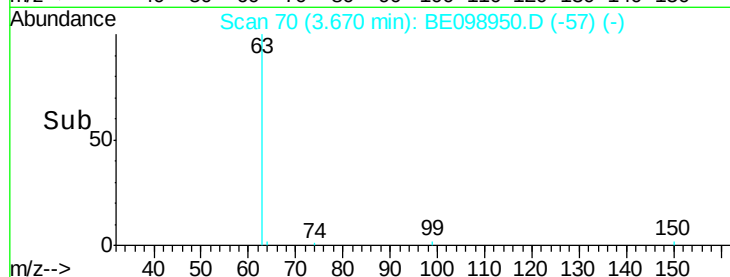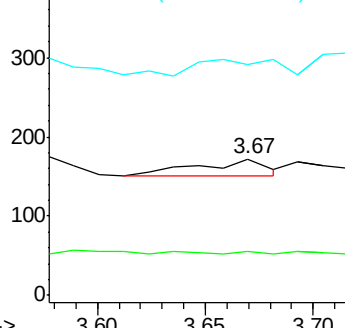

#4

2-Fluorophenol

Concen: 0.134 ng

RT: 5.41 min Scan# 221

Delta R.T. 0.02 min

Lab File: BE098950.D

Acq: 14 Mar 2019 19:16


Tgt Ion: 112 Resp: 278

Ion Ratio Lower Upper

112 100

64 0.0 57.9 86.9#



63 0.0 158.3 237.5#

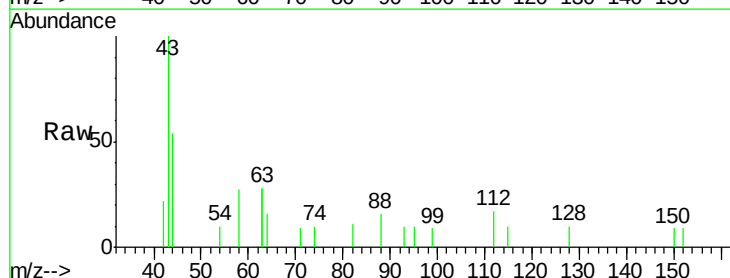


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

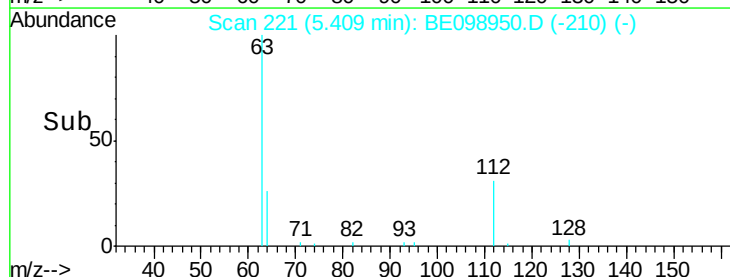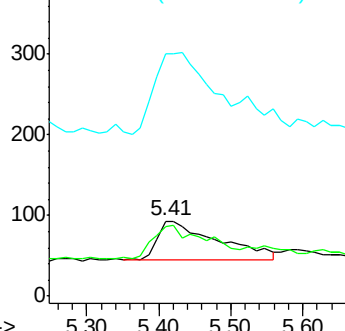



#5

Phenol-d6

Concen: 0.065 ng

RT: 7.03 min Scan# 362

Delta R.T. 0.05 min

Lab File: BE098950.D

Acq: 14 Mar 2019 19:16

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW305S-20190312


Tgt Ion: 99 Resp: 191

Ion Ratio Lower Upper

99 100

42 41.9 24.2 36.2#

71 41.4 35.7 53.5



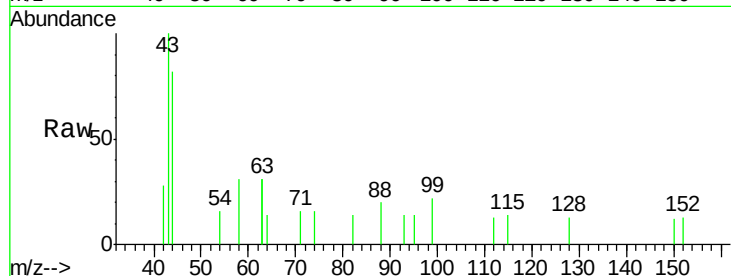


Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

Time-->

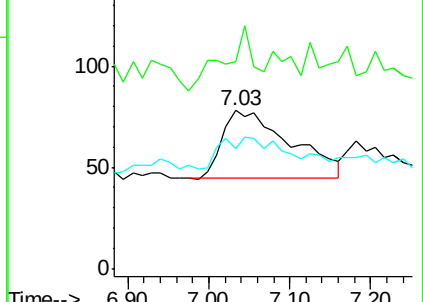

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.60 min Scan# 649

Delta R.T. 0.01 min

Lab File: BE098950.D

Acq: 14 Mar 2019 19:16

Tgt Ion: 136 Resp: 3228


Ion Ratio Lower Upper

136 100

137 15.2 11.4 17.0

54 70.0 39.3 58.9#

68 12.6 6.7 10.1#





Abundance Ion 136.00 (135.70 to 136.70): E


Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

Time-->

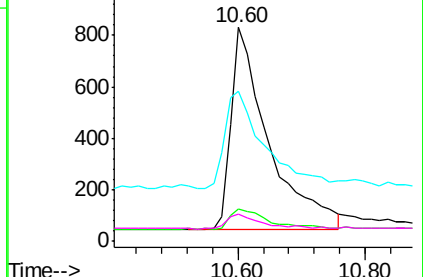



#8

Nitrobenzene-d5

Concen: 0.282 ng

RT: 9.03 min Scan# 528

Delta R.T. 0.06 min

Lab File: BE098950.D

Acq: 14 Mar 2019 19:16





Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW305S-20190312

Tgt Ion	Ratio	Lower	Upper
82	100		
128	196.3	123.8	185.8#
54	309.2	203.4	305.2#

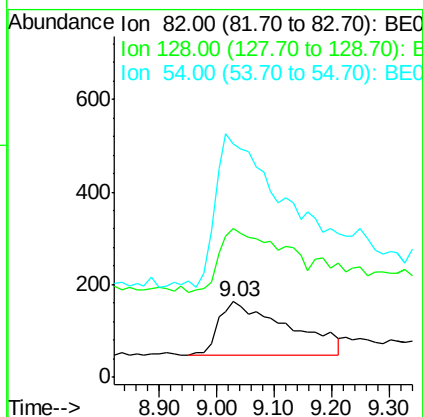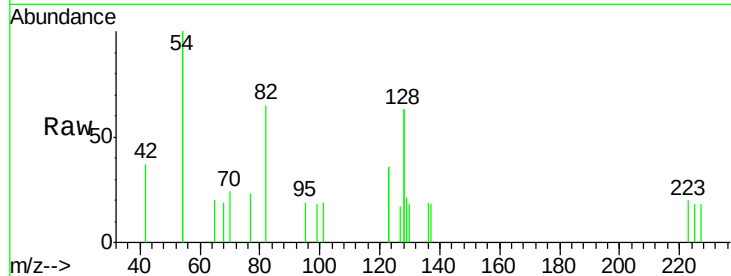

#11

2-Methylnaphthalene-d10

Concen: 0.337 ng




RT: 12.21 min Scan# 763


Delta R.T. 0.01 min

Lab File: BE098950.D

Acq: 14 Mar 2019 19:16

Tgt Ion	Ratio	Lower	Upper
152	100		
151	19.8	16.5	24.7

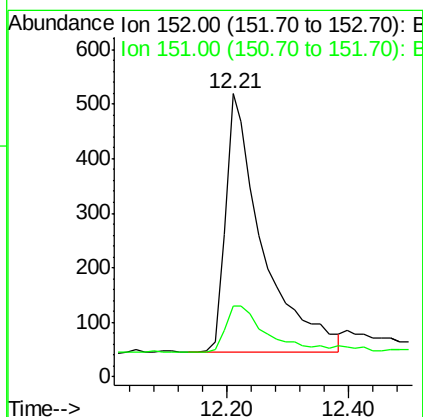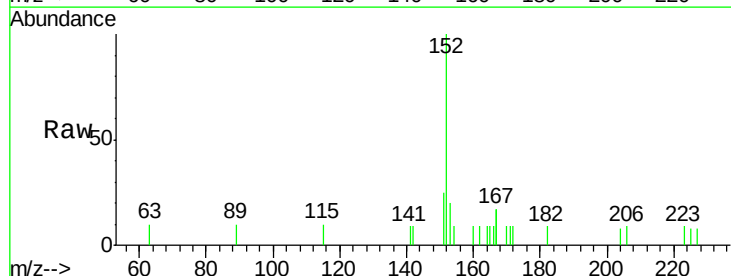

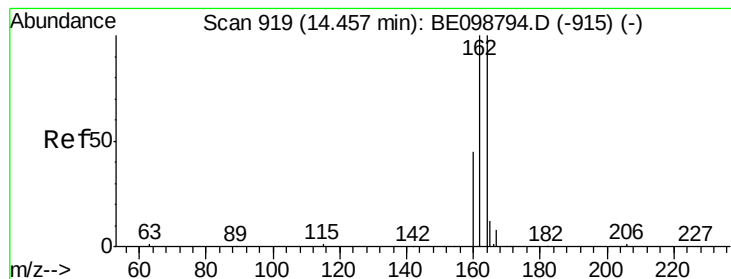

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.46 min Scan# 919

Delta R.T. -0.00 min

Lab File: BE098950.D

Acq: 14 Mar 2019 19:16

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW305S-20190312


Tgt Ion:164 Resp: 2355

Ion Ratio Lower Upper

164 100

162 100.4 80.2 120.2




160 50.0 37.8 56.8



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

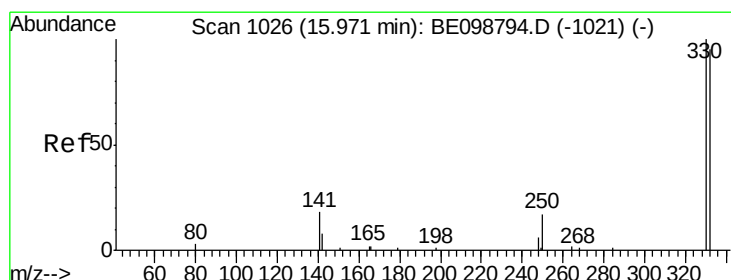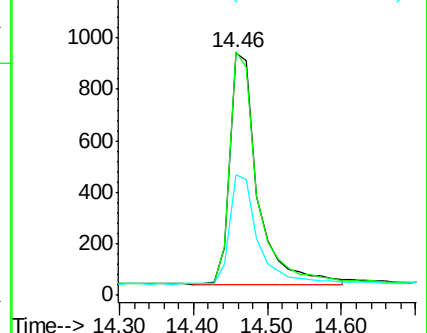

#14

2,4,6-Tribromophenol

Concen: 0.340 ng

RT: 15.97 min Scan# 1026

Delta R.T. -0.00 min

Lab File: BE098950.D

Acq: 14 Mar 2019 19:16


Tgt Ion:330 Resp: 404

Ion Ratio Lower Upper

330 100

332 86.1 77.6 116.4



141 33.2 31.0 46.4




Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E




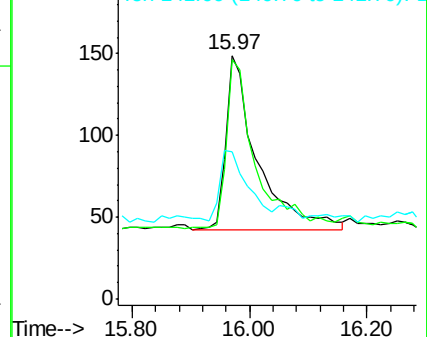


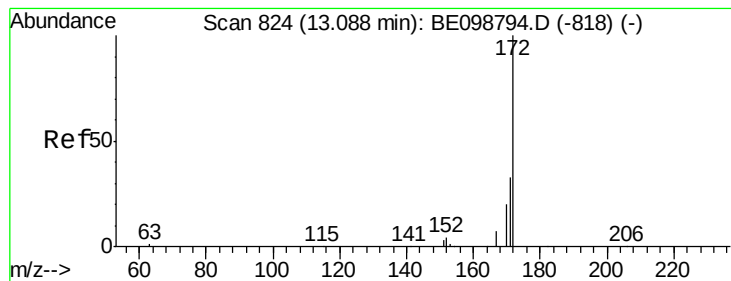

#15
2-Fluorobiphenyl
Concen: 0.474 ng
RT: 13.09 min Scan# 824
Delta R.T. -0.00 min
Lab File: BE098950.D
Acq: 14 Mar 2019 19:16




Instrument :
BNA_E
ClientSampleId :
BPS1-TT-MW305S-20190312


Tgt Ion:172 Resp: 4625
Ion Ratio Lower Upper
172 100
171 35.1 28.0 42.0
170 25.3 17.7 26.5

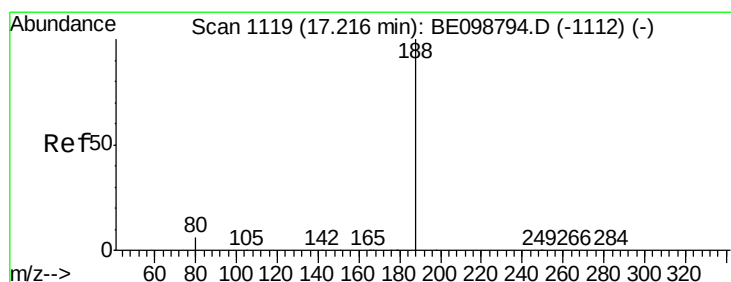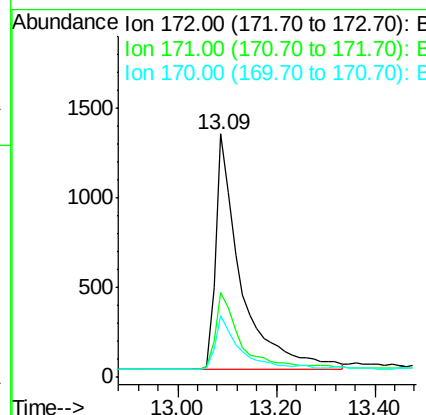

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.22 min Scan# 1119
Delta R.T. -0.00 min
Lab File: BE098950.D
Acq: 14 Mar 2019 19:16

Tgt Ion:188 Resp: 5623
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.3 6.3 9.5#

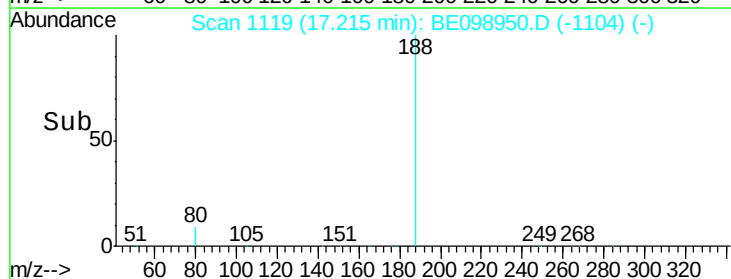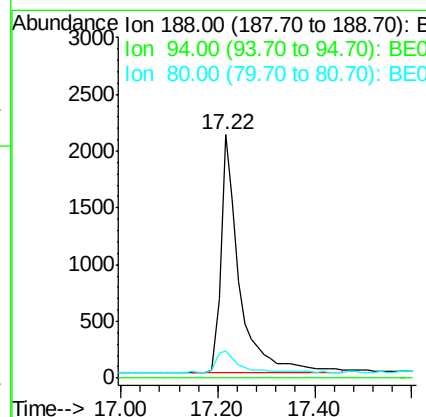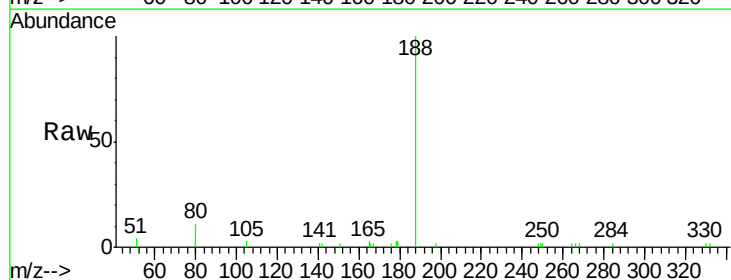

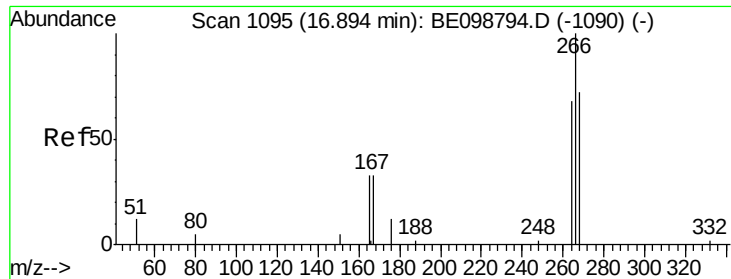

#22

Pentachlorophenol

Concen: 0.273 ng

RT: 16.91 min Scan# 1096

Delta R.T. 0.01 min

Lab File: BE098950.D

Acq: 14 Mar 2019 19:16

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW305S-20190312


Tgt Ion: 266 Resp: 10

Ion Ratio Lower Upper




266 100

264 90.2 66.6 100.0

268 94.1 69.8 104.8

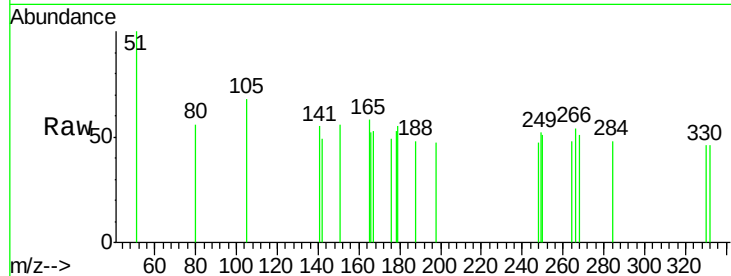

Abundance Ion 266.00 (265.70 to 266.70): E
Ion 264.00 (263.70 to 264.70): E
Ion 268.00 (267.70 to 268.70): E

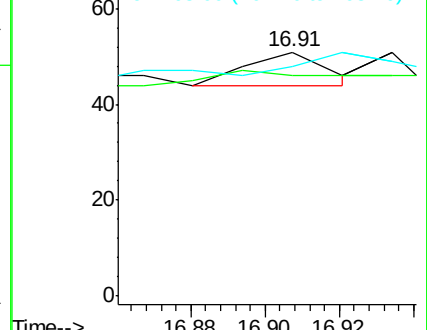

#25

Fluoranthene-d10

Concen: 0.339 ng

RT: 19.24 min Scan# 1388

Delta R.T. -0.00 min

Lab File: BE098950.D

Acq: 14 Mar 2019 19:16


Tgt Ion: 212 Resp: 30383

Ion Ratio Lower Upper



212 100


106 2.3 1.8 2.8

104 1.3 1.0 1.6



Abundance Ion 212.00 (211.70 to 212.70): E
Ion 106.00 (105.70 to 106.70): E
Ion 104.00 (103.70 to 104.70): E

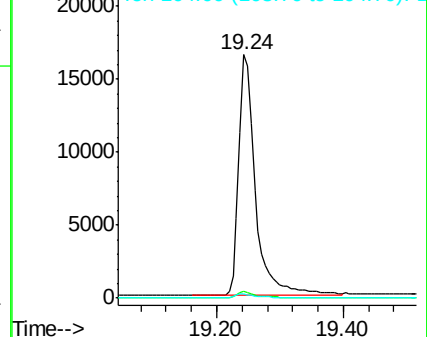



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.40 min Scan# 1632

Delta R.T. -0.00 min

Lab File: BE098950.D

Acq: 14 Mar 2019 19:16

Instrument :

BNA_E

ClientSampleId :

BPS1-TT-MW305S-20190312


Tgt Ion:240 Resp: 6566

Ion Ratio Lower Upper

240 100

120 7.8 5.0 7.4#




236 27.3 22.7 34.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

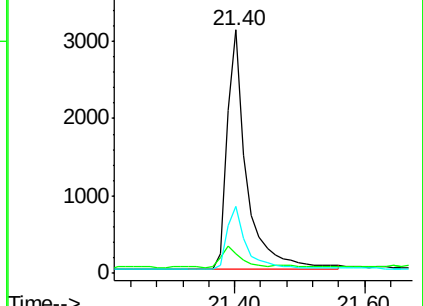

#29

Terphenyl-d14

Concen: 0.476 ng

RT: 19.84 min Scan# 1492

Delta R.T. -0.00 min

Lab File: BE098950.D

Acq: 14 Mar 2019 19:16


Tgt Ion:244 Resp: 7590

Ion Ratio Lower Upper

244 100

212 37.6 29.4 44.2



122 8.9 7.1 10.7




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E




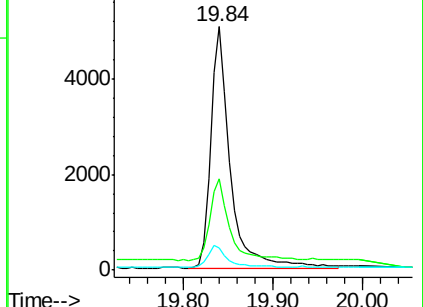




#32
 Bis(2-ethylhexyl)phthalate
 Concen: 0.077 ng
 RT: 21.29 min Scan# 1623
 Delta R.T. -0.01 min
 Lab File: BE098950.D
 Acq: 14 Mar 2019 19:16

Instrument :
 BNA_E
 ClientSampleId :
 BPS1-TT-MW305S-20190312

Tgt Ion:149 Resp: 3348
 Ion Ratio Lower Upper
 149 100
 167 7.1 5.4 8.0
 279 1.1 1.0 1.4

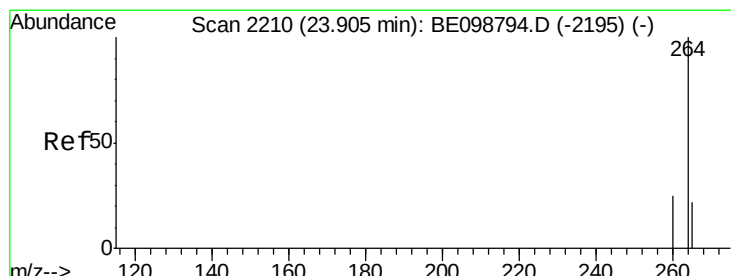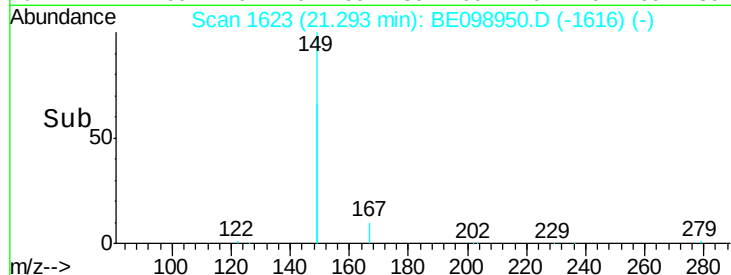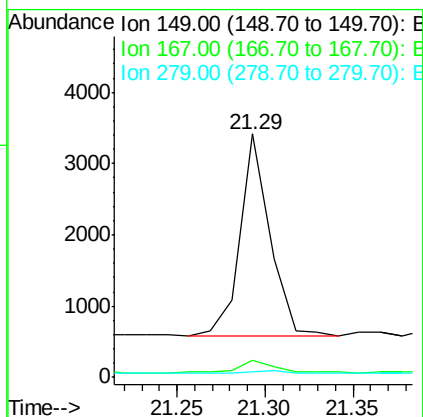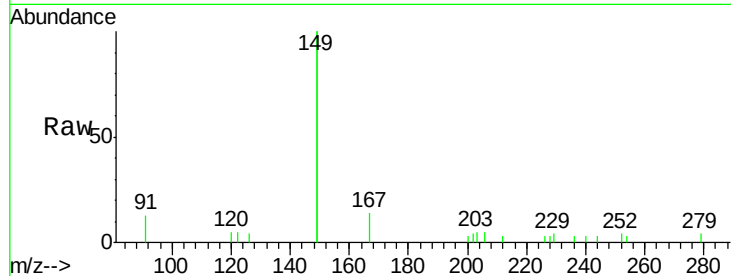

#34
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.89 min Scan# 2206
 Delta R.T. -0.01 min
 Lab File: BE098950.D
 Acq: 14 Mar 2019 19:16

Tgt Ion:264 Resp: 6197
 Ion Ratio Lower Upper
 264 100
 260 27.2 21.2 31.8
 265 29.3 24.6 36.8

