


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE031419\
 Data File : BE098937.D
 Acq On : 14 Mar 2019 9:35
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 15 05:31:33 2019

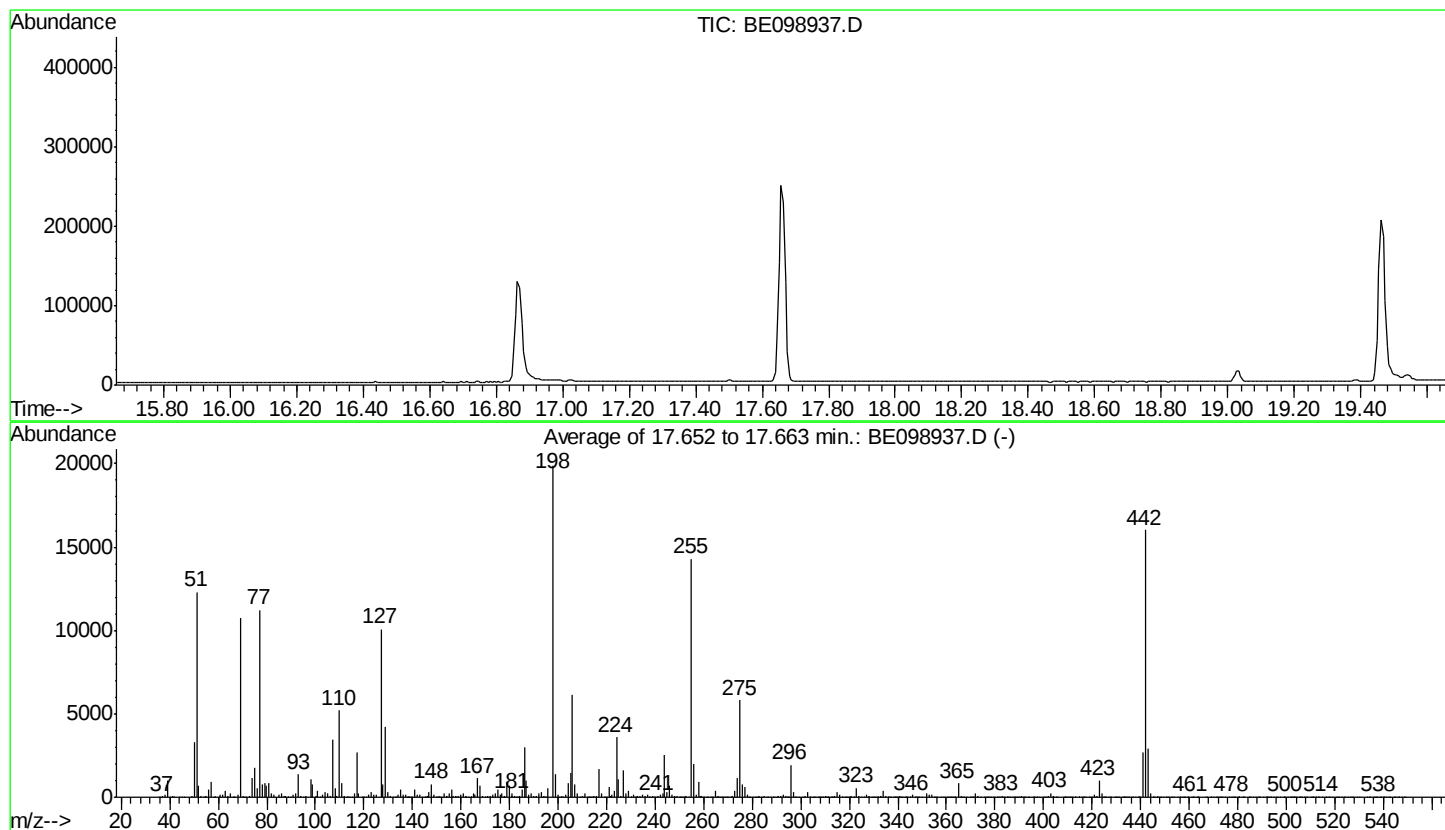

AutoFind: Scans 2564, 2565, 2566; Background Corrected with Scan 2557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.8	12293	PASS
68	69	0.00	2	1.2	131	PASS
69	198	0.00	100	54.2	10771	PASS
70	69	0.00	2	0.5	52	PASS
127	198	10	80	50.6	10062	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19880	PASS
199	198	5	9	6.9	1362	PASS
275	198	10	60	29.3	5824	PASS
365	198	1	100	4.1	816	PASS
441	198	0.01	100	13.6	2712	PASS
442	198	50	100	80.6	16027	PASS
443	442	15	24	18.1	2894	PASS