


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE031616\
 Data File : BE091449.D
 Acq On : 16 Mar 2016 18:46
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-BE031616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 17 15:28:00 2016

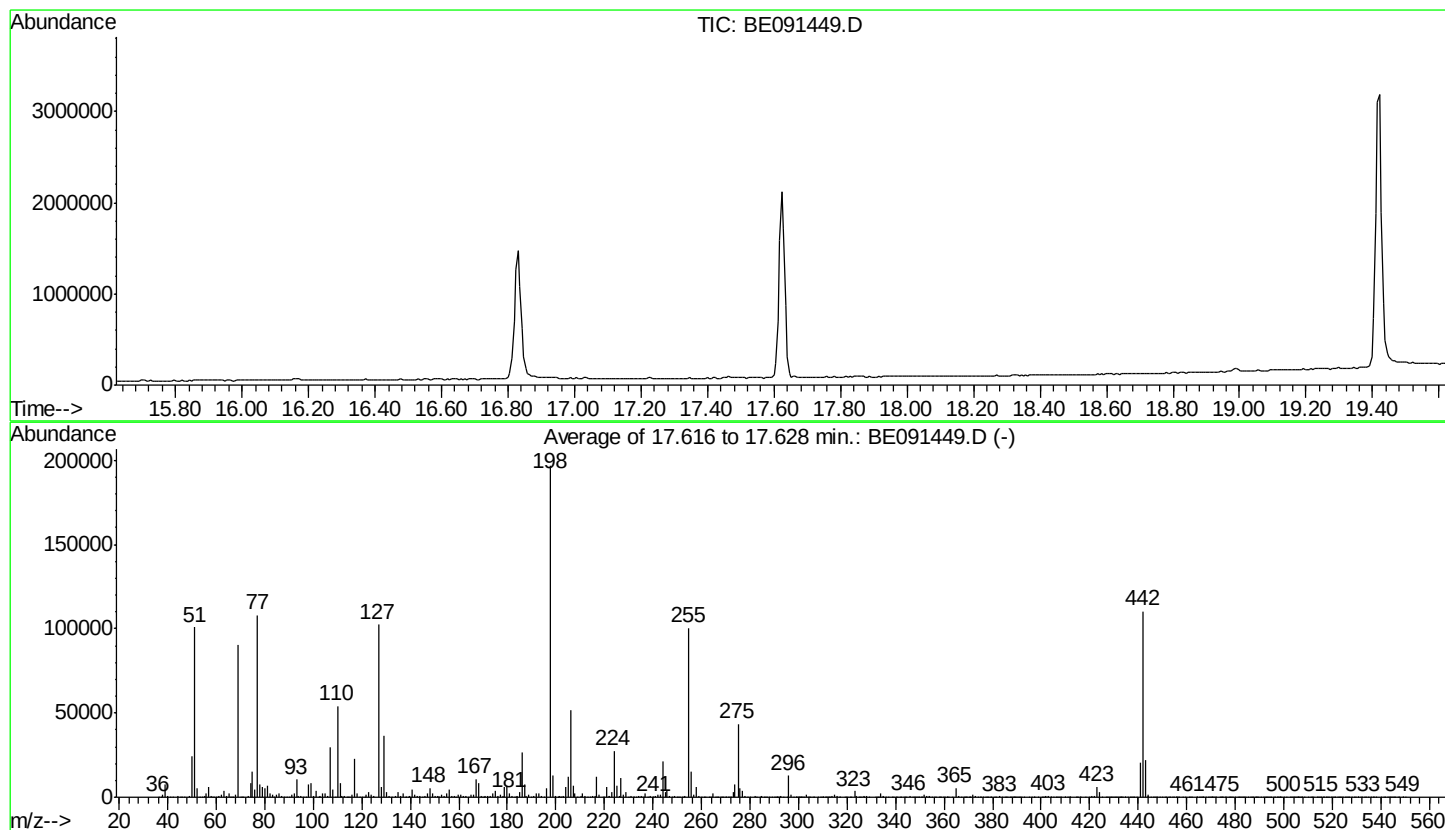

AutoFind: Scans 2558, 2559, 2560; Background Corrected with Scan 2549

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.2	100681	PASS
68	69	0.00	2	1.6	1444	PASS
69	198	0.00	100	45.9	90391	PASS
70	69	0.00	2	0.4	356	PASS
127	198	10	80	52.0	102237	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	196757	PASS
199	198	5	9	6.7	13236	PASS
275	198	10	60	22.0	43381	PASS
365	198	1	100	2.8	5563	PASS
441	442	0.01	24	18.4	20272	PASS
442	198	50	100	56.1	110390	PASS
443	442	15	24	19.7	21721	PASS