


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE031716\
Data File : BE091459.D
Acq On : 17 Mar 2016 9:00
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-BE031616.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 17 15:28:00 2016

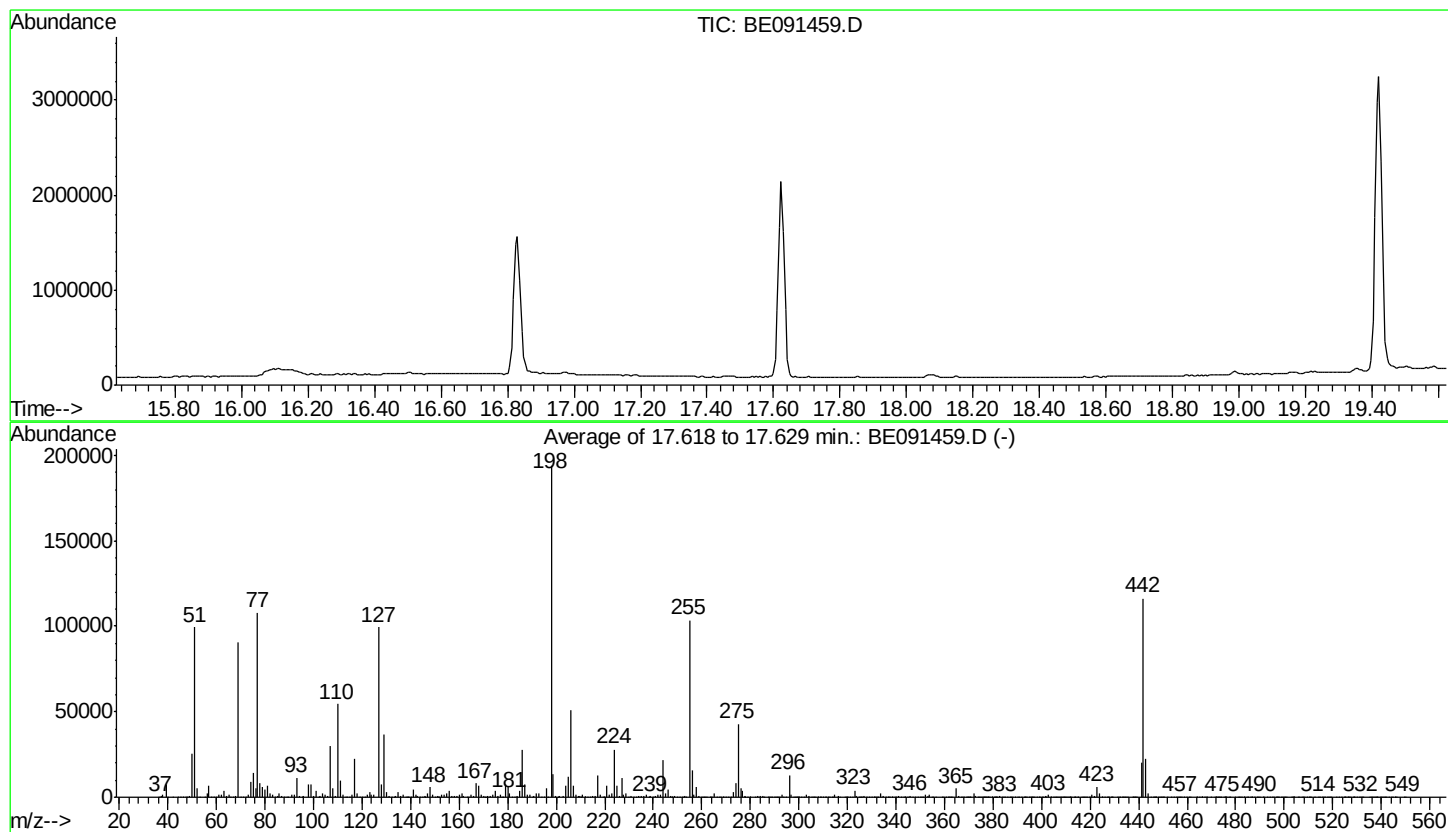

AutoFind: Scans 2558, 2559, 2560; Background Corrected with Scan 2546

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.3	99549	PASS
68	69	0.00	2	1.1	983	PASS
69	198	0.00	100	46.6	90391	PASS
70	69	0.00	2	0.2	206	PASS
127	198	10	80	51.3	99533	PASS
197	198	0.00	2	0.2	314	PASS
198	198	100	100	100.0	193926	PASS
199	198	5	9	7.1	13805	PASS
275	198	10	60	22.2	42994	PASS
365	198	1	100	2.7	5245	PASS
441	442	0.01	24	17.3	20160	PASS
442	198	50	100	60.0	116285	PASS
443	442	15	24	19.4	22545	PASS