

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE031816\
 Data File : BE091474.D
 Acq On : 17 Mar 2016 19:44
 Operator : UM/SJ
 Sample : SSTDICC3.2
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2

Quant Time: Mar 18 02:41:32 2016
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE031816.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 18 02:38:58 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	58739	5.00	ng	0.00
6) Naphthalene-d8	10.61	136	278044	5.00	ng	0.00
10) Acenaphthene-d10	14.45	164	165371	5.00	ng	0.00
16) Phenanthrene-d10	17.18	188	399611	5.00	ng	0.00
22) Chrysene-d12	21.33	240	547153	5.00	ng	0.00
28) Perylene-d12	23.81	264	481306	5.00	ng	0.00

System Monitoring Compounds						
4) 2-Fluorophenol	5.43	112	45119	4.25	ng	0.00
5) Phenol-d6	6.99	99	61251	4.87	ng	0.00
7) Nitrobenzene-d5	8.98	82	43314	3.64	ng	0.00
11) 2,4,6-Tribromophenol	15.93	330	20447	4.64	ng	0.00
12) 2-Fluorobiphenyl	13.07	172	145177	3.15	ng	0.00
24) Terphenyl-d14	19.80	244	227627	3.33	ng	0.00


Target Compounds				Qvalue		
2) 1,4-Dioxane	3.37	88	22347	3.35	ng	96
3) n-Nitrosodimethylamine	3.66	42	37828	7.51	ng	# 90
8) Naphthalene	10.65	128	225669	3.03	ng	99
9) 2-Methylnaphthalene	12.27	142	152031	3.25	ng	99
13) Acenaphthylene	14.16	152	260811	3.19	ng	98
14) Acenaphthene	14.50	154	172077	2.92	ng	99
15) Fluorene	15.49	166	219267	3.22	ng	100
17) Hexachlorobenzene	16.48	284	59294	2.33	ng	99
18) Pentachlorophenol	16.83	266	26572	10.77	ng	93
19) Phenanthrene	17.22	178	378502	3.01	ng	99
20) Anthracene	17.31	178	354058	3.19	ng	100
21) Fluoranthene	19.22	202	447899	3.33	ng	100
23) Pyrene	19.59	202	483585	2.39	ng	99
25) Benzo(a)anthracene	21.31	228	990900	5.47	ng	100
26) Chrysene	21.31	228	997322	5.20	ng	# 87
27) Indeno(1,2,3-cd)pyrene	26.39	276	550173	3.58	ng	99
29) Benzo(b)fluoranthene	23.04	252	502824	2.88	ng	97
30) Benzo(k)fluoranthene	23.09	252	506972	2.93	ng	93
31) Benzo(a)pyrene	23.69	252	466473	3.17	ng	# 95
32) Dibenzo(a,h)anthracene	26.42	278	462325	3.73	ng	97
33) Benzo(g,h,i)perylene	27.18	276	467003	3.33	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE031816\
Data File : BE091474.D
Acq On : 17 Mar 2016 19:44
Operator : UM/SJ
Sample : SSTDICC3.2
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2

Quant Time: Mar 18 02:41:32 2016
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 02:38:58 2016
Response via : Initial Calibration






#1




1,4-Dichlorobenzene-d4
Concen: 5.00 ng
RT: 7.84 min Scan# 302
Delta R.T. 0.00 min
Lab File: BE091474.D
Acq: 17 Mar 2016 19:44

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2

Tgt Ion:152 Resp: 58739
Ion Ratio Lower Upper
152 100
150 150.2 122.2 183.2
115 54.9 45.9 68.9




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E





#2


1,4-Dioxane
Concen: 3.35 ng
RT: 3.37 min Scan# 45
Delta R.T. 0.00 min
Lab File: BE091474.D
Acq: 17 Mar 2016 19:44

Tgt Ion: 88 Resp: 22347
Ion Ratio Lower Upper
88 100
58 80.7 61.0 91.6
43 32.9 25.4 38.2



Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0





#3

n-Nitrosodimethylamine

Concen: 7.51 ng

RT: 3.66 min Scan# 62

Delta R.T. -0.02 min

Lab File: BE091474.D

Acq: 17 Mar 2016 19:44

Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2


Tgt Ion: 42 Resp: 37828

Ion Ratio Lower Upper

42 100

74 95.0 84.3 126.5




44 6.4 6.7 10.1#



Abundance Ion 42.00 (41.70 to 42.70): BE0

Ion 74.00 (73.70 to 74.70): BE0

Ion 44.00 (43.70 to 44.70): BE0



#4

2-Fluorophenol

Concen: 4.25 ng

RT: 5.43 min Scan# 164

Delta R.T. 0.00 min

Lab File: BE091474.D

Acq: 17 Mar 2016 19:44


Tgt Ion: 112 Resp: 45119

Ion Ratio Lower Upper

112 100

64 66.9 53.3 79.9



63 35.6 29.8 44.8




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0





#5

Phenol-d6

Concen: 4.87 ng

RT: 6.99 min Scan# 253

Delta R.T. 0.00 min

Lab File: BE091474.D

Acq: 17 Mar 2016 19:44

Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2


Tgt Ion: 99 Resp: 61251

Ion Ratio Lower Upper




99 100

42 25.6 20.6 30.8

71 35.2 29.0 43.4



Abundance Ion 99.00 (98.70 to 99.70): BE0
Ion 42.00 (41.70 to 42.70): BE0
Ion 71.00 (70.70 to 71.70): BE0



#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.61 min Scan# 513

Delta R.T. -0.00 min

Lab File: BE091474.D

Acq: 17 Mar 2016 19:44

Tgt Ion: 136 Resp: 278044


Ion Ratio Lower Upper

136 100



137 11.0 8.8 13.2


54 6.3 5.2 7.8

68 5.0 4.1 6.1



Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BE0
Ion 68.00 (67.70 to 68.70): BE0





#7

Nitrobenzene-d5

Concen: 3.64 ng

RT: 8.98 min Scan# 394

Delta R.T. 0.00 min

Lab File: BE091474.D

Acq: 17 Mar 2016 19:44

Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2


Tgt Ion: 82 Resp: 43314

Ion Ratio Lower Upper

82 100

128 31.6 23.5 35.3




54 54.9 52.4 78.6



Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0



#8

Naphthalene

Concen: 3.03 ng

RT: 10.65 min Scan# 515

Delta R.T. -0.00 min

Lab File: BE091474.D

Acq: 17 Mar 2016 19:44


Tgt Ion: 128 Resp: 225669

Ion Ratio Lower Upper

128 100

129 10.1 8.2 12.2



127 14.3 11.8 17.8




Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E





#9

2-Methylnaphthalene

Concen: 3.25 ng

RT: 12.27 min Scan# 641

Delta R.T. -0.00 min

Lab File: BE091474.D

Acq: 17 Mar 2016 19:44

Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2


Tgt Ion:142 Resp: 152031

Ion Ratio Lower Upper

142 100

141 82.8 66.9 100.3




115 30.1 25.1 37.7



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E



#10

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.45 min Scan# 822

Delta R.T. 0.00 min

Lab File: BE091474.D

Acq: 17 Mar 2016 19:44


Tgt Ion:164 Resp: 165371

Ion Ratio Lower Upper

164 100

162 105.9 84.4 126.6



160 45.9 37.7 56.5




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E









#11
 2,4,6-Tribromophenol
 Concen: 4.64 ng
 RT: 15.93 min Scan# 942
 Delta R.T. 0.00 min
 Lab File: BE091474.D
 Acq: 17 Mar 2016 19:44

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2

Tgt Ion:330 Resp: 20447
 Ion Ratio Lower Upper
 330 100
 332 96.0 79.2 118.8
 141 40.2 28.1 42.1




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E





#12
 2-Fluorobiphenyl
 Concen: 3.15 ng
 RT: 13.07 min Scan# 710
 Delta R.T. -0.00 min
 Lab File: BE091474.D
 Acq: 17 Mar 2016 19:44

Tgt Ion:172 Resp: 145177
 Ion Ratio Lower Upper
 172 100
 171 36.4 29.8 44.8
 170 25.6 21.4 32.2



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E









#13
Acenaphthylene
Concen: 3.19 ng
RT: 14.16 min Scan# 801
Delta R.T. 0.00 min
Lab File: BE091474.D
Acq: 17 Mar 2016 19:44




Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2


Tgt Ion:152 Resp: 260811
Ion Ratio Lower Upper
152 100
151 19.6 16.3 24.5
153 13.1 11.1 16.7



#14
Acenaphthene
Concen: 2.92 ng
RT: 14.50 min Scan# 826
Delta R.T. 0.00 min
Lab File: BE091474.D
Acq: 17 Mar 2016 19:44

Tgt Ion:154 Resp: 172077
Ion Ratio Lower Upper
154 100
153 109.9 87.3 130.9
152 54.0 42.9 64.3









#15
Fluorene
 Concen: 3.22 ng
 RT: 15.49 min Scan# 904
 Delta R.T. 0.00 min
 Lab File: BE091474.D
 Acq: 17 Mar 2016 19:44




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2


Tgt Ion:166 Resp: 219267
 Ion Ratio Lower Upper
 166 100
 165 99.3 79.2 118.8
 167 13.6 10.8 16.2



#16
Phenanthrene-d10
 Concen: 5.00 ng
 RT: 17.18 min Scan# 1019
 Delta R.T. 0.00 min
 Lab File: BE091474.D
 Acq: 17 Mar 2016 19:44

Tgt Ion:188 Resp: 399611
 Ion Ratio Lower Upper
 188 100
 94 5.7 5.4 8.2
 80 5.1 5.0 7.4









#17
Hexachlorobenzene
Concen: 2.33 ng
RT: 16.48 min Scan# 975
Delta R.T. 0.00 min
Lab File: BE091474.D
Acq: 17 Mar 2016 19:44




Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2


Tgt Ion: 284 Resp: 59294
Ion Ratio Lower Upper
284 100
142 38.8 31.0 46.4
249 31.2 25.8 38.8



#18
Pentachlorophenol
Concen: 10.77 ng
RT: 16.83 min Scan# 995
Delta R.T. 0.00 min
Lab File: BE091474.D
Acq: 17 Mar 2016 19:44

Tgt Ion: 266 Resp: 26572
Ion Ratio Lower Upper
266 100
268 65.7 48.2 72.2
264 59.0 52.1 78.1





#19

Phenanthrene

Concen: 3.01 ng

RT: 17.22 min Scan# 1022

Delta R.T. 0.00 min

Lab File: BE091474.D

Acq: 17 Mar 2016 19:44

Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2


Tgt Ion:178 Resp: 378502

Ion Ratio Lower Upper

178 100

176 19.3 15.5 23.3




179 15.5 13.1 19.7



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E



#20

Anthracene

Concen: 3.19 ng

RT: 17.31 min Scan# 1030

Delta R.T. 0.00 min

Lab File: BE091474.D

Acq: 17 Mar 2016 19:44


Tgt Ion:178 Resp: 354058

Ion Ratio Lower Upper

178 100

176 18.8 14.9 22.3



179 15.4 12.2 18.4




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E





#21

Fluoranthene

Concen: 3.33 ng

RT: 19.22 min Scan# 1152

Delta R.T. -0.00 min

Lab File: BE091474.D

Acq: 17 Mar 2016 19:44

Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2


Tgt Ion: 202 Resp: 447899

Ion Ratio Lower Upper

202 100

101 10.5 8.3 12.5




203 17.2 13.9 20.9



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E



#22

Chrysene-d12

Concen: 5.00 ng

RT: 21.33 min Scan# 1249

Delta R.T. -0.00 min

Lab File: BE091474.D

Acq: 17 Mar 2016 19:44


Tgt Ion: 240 Resp: 547153

Ion Ratio Lower Upper

240 100

120 5.1 4.0 6.0



236 28.6 23.0 34.4




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E









#23
 Pyrene
 Concen: 2.39 ng
 RT: 19.59 min Scan# 1171
 Delta R.T. -0.00 min
 Lab File: BE091474.D
 Acq: 17 Mar 2016 19:44




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2

Tgt Ion: 202 Resp: 483585
 Ion Ratio Lower Upper
 202 100
 200 20.8 16.4 24.6
 203 18.0 14.6 21.8



#24
 Terphenyl-d14
 Concen: 3.33 ng
 RT: 19.80 min Scan# 1182
 Delta R.T. -0.00 min
 Lab File: BE091474.D
 Acq: 17 Mar 2016 19:44

Tgt Ion: 244 Resp: 227627
 Ion Ratio Lower Upper
 244 100
 212 6.9 5.8 8.8
 122 1.2 1.8 2.8#









#25
Benzo(a)anthracene
Concen: 5.47 ng
RT: 21.31 min Scan# 1248
Delta R.T. -0.00 min
Lab File: BE091474.D
Acq: 17 Mar 2016 19:44




Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2


Tgt Ion:228 Resp: 990900
Ion Ratio Lower Upper
228 100
226 29.9 24.0 36.0
229 17.3 13.8 20.6



#26
Chrysene
Concen: 5.20 ng
RT: 21.31 min Scan# 1248
Delta R.T. -0.07 min
Lab File: BE091474.D
Acq: 17 Mar 2016 19:44

Tgt Ion:228 Resp: 997322
Ion Ratio Lower Upper
228 100
226 29.9 18.9 28.3#
229 17.3 19.1 28.7#









#27
 Indeno(1,2,3-cd)pyrene
 Concen: 3.58 ng
 RT: 26.39 min Scan# 1652
 Delta R.T. -0.01 min
 Lab File: BE091474.D
 Acq: 17 Mar 2016 19:44




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2


Tgt Ion: 276 Resp: 550173
 Ion Ratio Lower Upper
 276 100
 138 25.7 20.2 30.4
 277 24.9 19.8 29.8



#28
 Perylene-d12
 Concen: 5.00 ng
 RT: 23.81 min Scan# 1431
 Delta R.T. 0.00 min
 Lab File: BE091474.D
 Acq: 17 Mar 2016 19:44

Tgt Ion: 264 Resp: 481306
 Ion Ratio Lower Upper
 264 100
 260 24.3 20.1 30.1
 265 24.3 18.3 27.5





#29

Benzo(b)fluoranthene

Concen: 2.88 ng

RT: 23.04 min Scan# 1365

Delta R.T. 0.00 min

Lab File: BE091474.D

Acq: 17 Mar 2016 19:44

Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2


Tgt Ion:252 Resp: 502824

Ion Ratio Lower Upper

252 100

253 22.3 18.7 28.1




125 9.9 9.8 14.6



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



#30

Benzo(k)fluoranthene

Concen: 2.93 ng

RT: 23.09 min Scan# 1369

Delta R.T. -0.01 min

Lab File: BE091474.D

Acq: 17 Mar 2016 19:44


Tgt Ion:252 Resp: 506972

Ion Ratio Lower Upper

252 100

253 21.2 20.2 30.4



125 10.5 9.4 14.2




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E





#31

Benzo(a)pyrene

Concen: 3.17 ng

RT: 23.69 min Scan# 1421

Delta R.T. 0.00 min

Lab File: BE091474.D

Acq: 17 Mar 2016 19:44

Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2





Tgt Ion:252 Resp: 466473

Ion Ratio Lower Upper

252 100

253 22.6 19.4 29.0

125 10.6 11.4 17.2#



#32

Dibenzo(a,h)anthracene

Concen: 3.73 ng

RT: 26.42 min Scan# 1655

Delta R.T. 0.00 min

Lab File: BE091474.D

Acq: 17 Mar 2016 19:44




Tgt Ion:278 Resp: 462325


Ion Ratio Lower Upper

278 100

139 15.3 14.2 21.4

279 24.4 19.6 29.4



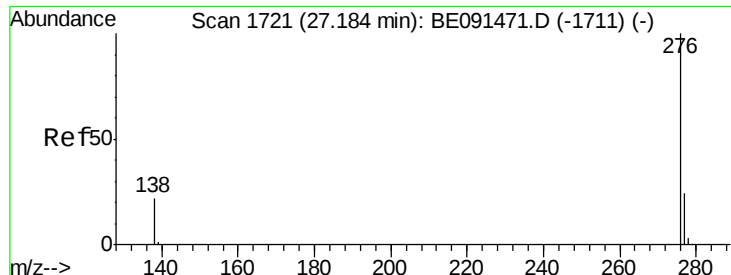

#33

Benzo(g,h,i)perylene

Concen: 3.33 ng

RT: 27.18 min Scan# 1721

Delta R.T. 0.00 min

Lab File: BE091474.D


Acq: 17 Mar 2016 19:44

Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2




Tgt Ion: 276 Resp: 467003

Ion Ratio Lower Upper

276 100

277 23.5 19.4 29.2

138 22.0 18.2 27.4



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

