

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE031816\
 Data File : BE091476.D
 Acq On : 17 Mar 2016 20:59
 Operator : UM/SJ
 Sample : SSTDICC10.0
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC010

Quant Time: Mar 18 02:41:56 2016
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE031816.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 18 02:38:58 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	58217	5.00	ng	0.00
6) Naphthalene-d8	10.61	136	281606	5.00	ng	0.00
10) Acenaphthene-d10	14.45	164	165705	5.00	ng	0.00
16) Phenanthrene-d10	17.18	188	389139	5.00	ng	0.00
22) Chrysene-d12	21.34	240	554894	5.00	ng	0.00
28) Perylene-d12	23.81	264	468385	5.00	ng	0.00

System Monitoring Compounds						
4) 2-Fluorophenol	5.43	112	147018	13.98	ng	0.00
5) Phenol-d6	6.99	99	213444	17.13	ng	0.00
7) Nitrobenzene-d5	8.98	82	160685	13.33	ng	0.00
11) 2,4,6-Tribromophenol	15.92	330	73634	16.68	ng	-0.01
12) 2-Fluorobiphenyl	13.07	172	436799	9.46	ng	0.00
24) Terphenyl-d14	19.80	244	642112	9.25	ng	0.00


Target Compounds				Qvalue		
2) 1,4-Dioxane	3.37	88	66861	10.12	ng	96
3) n-Nitrosodimethylamine	3.66	42	118670	23.78	ng	# 98
8) Naphthalene	10.65	128	683286	9.07	ng	99
9) 2-Methylnaphthalene	12.27	142	472277	9.95	ng	96
13) Acenaphthylene	14.16	152	850634	10.38	ng	99
14) Acenaphthene	14.50	154	533439	9.05	ng	99
15) Fluorene	15.49	166	655182	9.59	ng	99
17) Hexachlorobenzene	16.48	284	175979	7.11	ng	99
18) Pentachlorophenol	16.83	266	101612	42.28	ng	89
19) Phenanthrene	17.22	178	1096865	8.97	ng	99
20) Anthracene	17.31	178	1090780	10.08	ng	99
21) Fluoranthene	19.23	202	1338593	10.23	ng	99
23) Pyrene	19.59	202	1422675	6.93	ng	99
25) Benzo(a)anthracene	21.31	228	2765250	15.05	ng	98
26) Chrysene	21.31	228	2779269	14.30	ng	# 87
27) Indeno(1,2,3-cd)pyrene	26.40	276	1651049	10.60	ng	99
29) Benzo(b)fluoranthene	23.04	252	1464547	8.63	ng	97
30) Benzo(k)fluoranthene	23.09	252	1495888	8.89	ng	94
31) Benzo(a)pyrene	23.69	252	1421172	9.91	ng	# 94
32) Dibenzo(a,h)anthracene	26.42	278	1384410	11.49	ng	98
33) Benzo(g,h,i)perylene	27.20	276	1399634	10.26	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE031816\
Data File : BE091476.D
Acq On : 17 Mar 2016 20:59
Operator : UM/SJ
Sample : SSTDICC10.0
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SSTDICC010

Quant Time: Mar 18 02:41:56 2016
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 18 02:38:58 2016
Response via : Initial Calibration

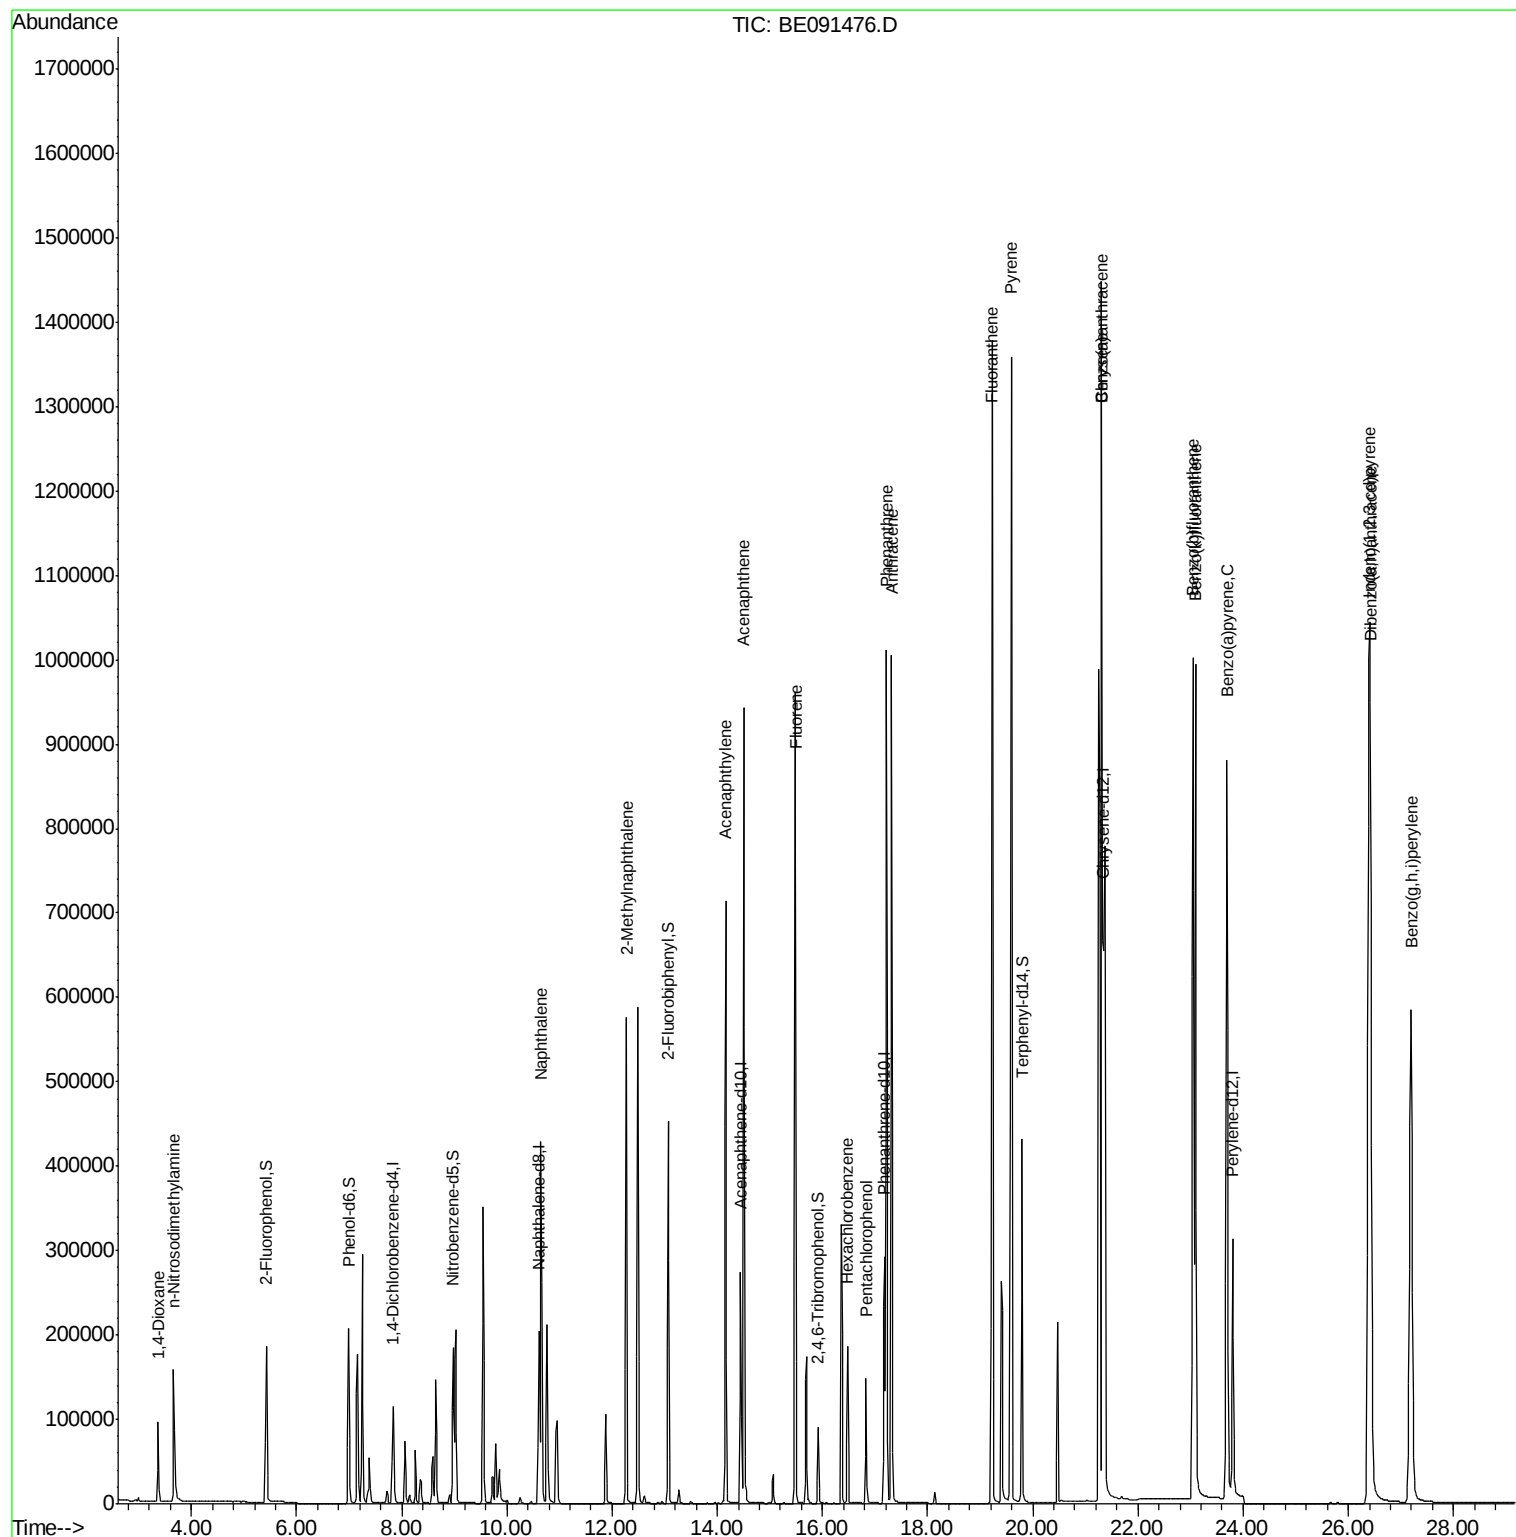



#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.84 min Scan# 302

Delta R.T. 0.00 min

Lab File: BE091476.D

Acq: 17 Mar 2016 20:59

Instrument :

BNA_E

ClientSampleId :

SSTDICC010


Tgt Ion:152 Resp: 58217

Ion Ratio Lower Upper

152 100

150 149.4 122.2 183.2




115 54.5 45.9 68.9

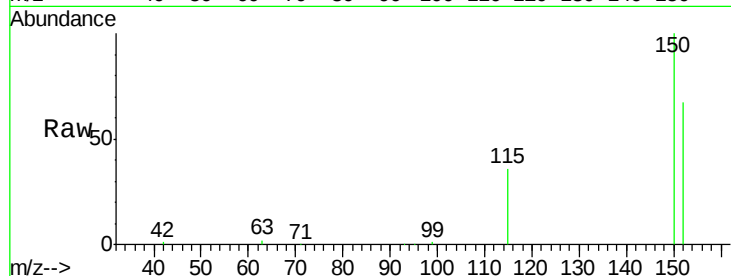

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

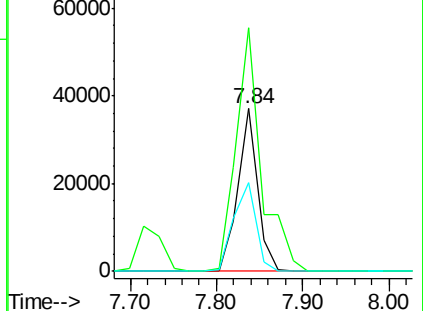

#2

1,4-Dioxane

Concen: 10.12 ng

RT: 3.37 min Scan# 45

Delta R.T. 0.00 min

Lab File: BE091476.D

Acq: 17 Mar 2016 20:59


Tgt Ion: 88 Resp: 66861

Ion Ratio Lower Upper

88 100

58 79.6 61.0 91.6



43 34.1 25.4 38.2



Abundance Ion 88.00 (87.70 to 88.70): BE0

Ion 58.00 (57.70 to 58.70): BE0

Ion 43.00 (42.70 to 43.70): BE0

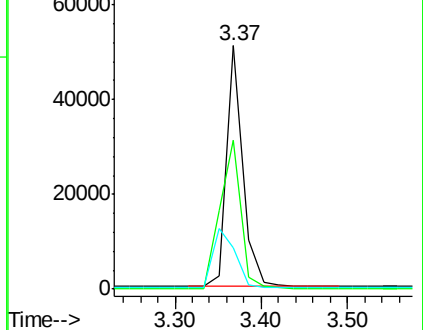



#3

n-Nitrosodimethylamine

Concen: 23.78 ng

RT: 3.66 min Scan# 62

Delta R.T. -0.02 min

Lab File: BE091476.D

Acq: 17 Mar 2016 20:59

Instrument :

BNA_E

ClientSampleId :

SSTDIC010


Tgt Ion: 42 Resp: 118670

Ion Ratio Lower Upper




42 100

74 104.1 84.3 126.5

44 6.4 6.7 10.1#

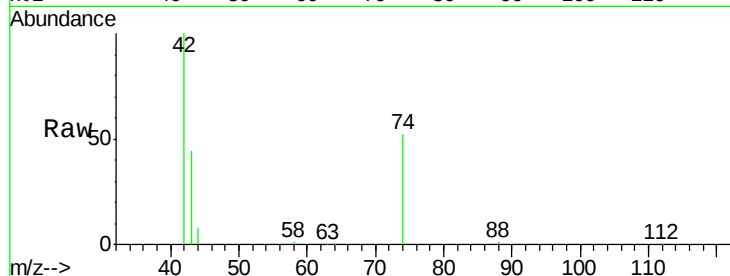

Abundance Ion 42.00 (41.70 to 42.70): BE0
Ion 74.00 (73.70 to 74.70): BE0
Ion 44.00 (43.70 to 44.70): BE0

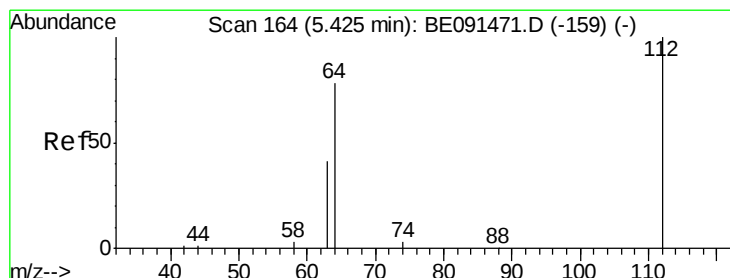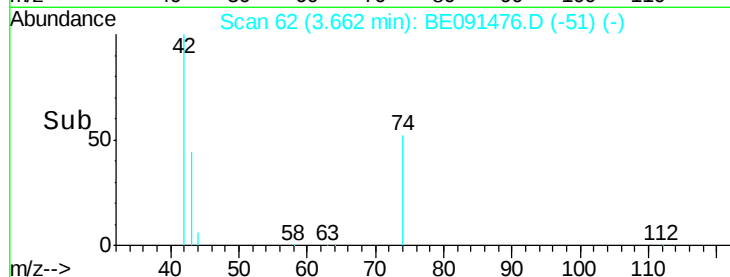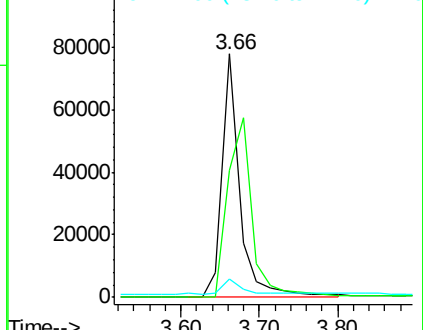

#4

2-Fluorophenol

Concen: 13.98 ng

RT: 5.43 min Scan# 164

Delta R.T. 0.00 min

Lab File: BE091476.D

Acq: 17 Mar 2016 20:59


Tgt Ion: 112 Resp: 147018

Ion Ratio Lower Upper



112 100


64 65.6 53.3 79.9

63 35.2 29.8 44.8

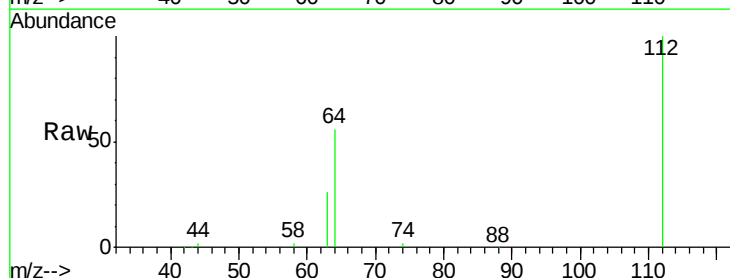

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BE0
Ion 63.00 (62.70 to 63.70): BE0

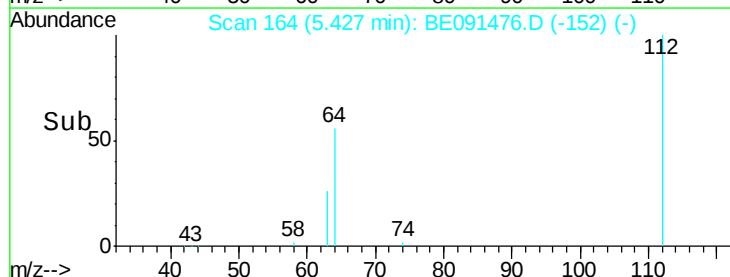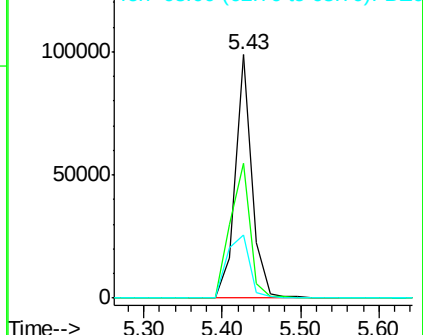

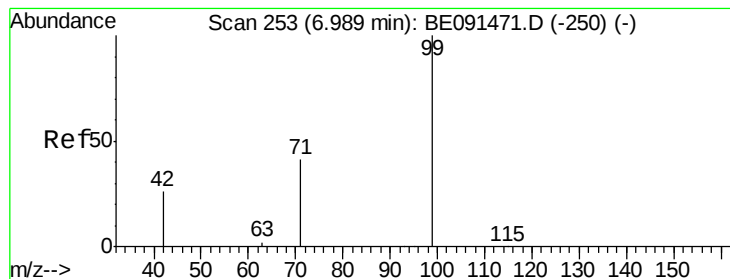

#5

Phenol-d6

Concen: 17.13 ng

RT: 6.99 min Scan# 253

Delta R.T. 0.00 min

Lab File: BE091476.D

Acq: 17 Mar 2016 20:59

Instrument :

BNA_E

ClientSampleId :

SSTDICC010


Tgt Ion: 99 Resp: 213444

Ion Ratio Lower Upper




99 100

42 24.8 20.6 30.8

71 35.0 29.0 43.4

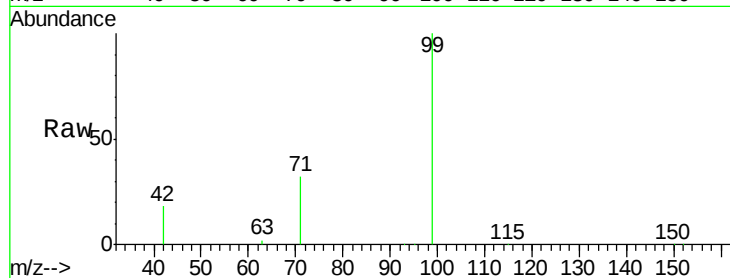

Abundance Ion 99.00 (98.70 to 99.70): BE0
Ion 42.00 (41.70 to 42.70): BE0
Ion 71.00 (70.70 to 71.70): BE0

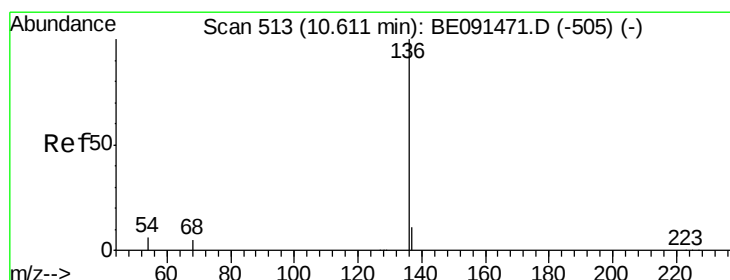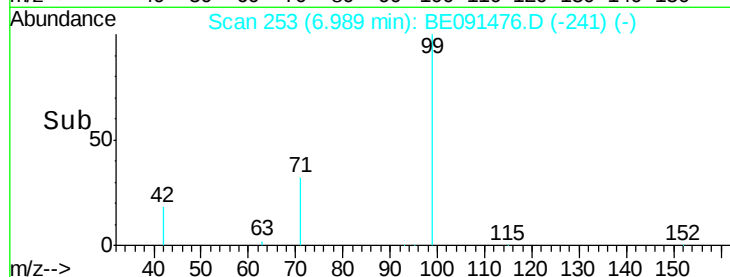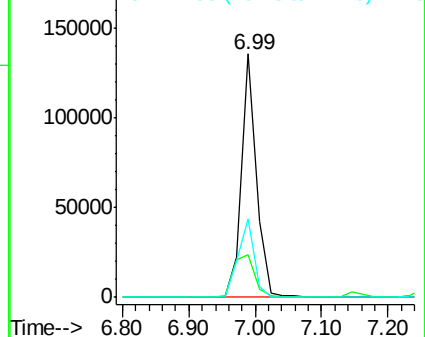

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.61 min Scan# 513

Delta R.T. -0.00 min

Lab File: BE091476.D

Acq: 17 Mar 2016 20:59

Tgt Ion: 136 Resp: 281606


Ion Ratio Lower Upper

136 100



137 11.0 8.8 13.2


54 6.4 5.2 7.8

68 5.0 4.1 6.1

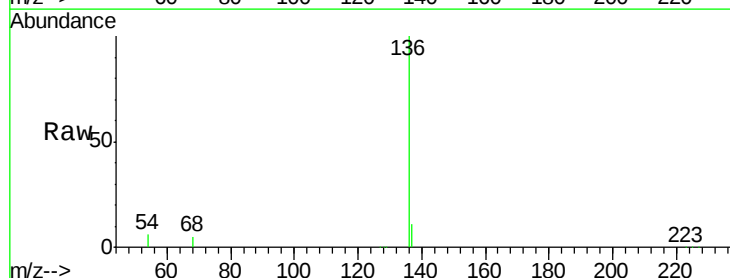

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BE0
Ion 68.00 (67.70 to 68.70): BE0

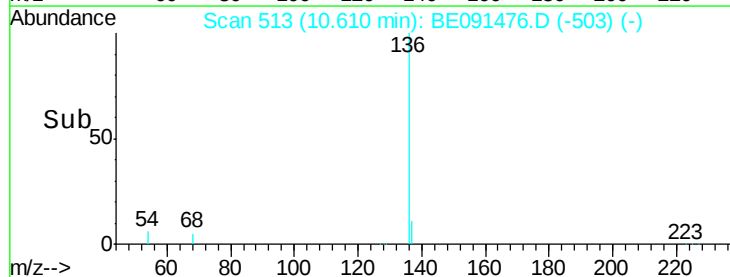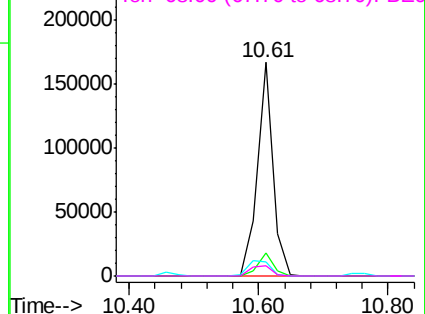



#7

Nitrobenzene-d5

Concen: 13.33 ng

RT: 8.98 min Scan# 394

Delta R.T. 0.00 min

Lab File: BE091476.D

Acq: 17 Mar 2016 20:59

Instrument :

BNA_E

ClientSampleId :

SSTDIC010


Tgt Ion: 82 Resp: 160685

Ion Ratio Lower Upper

82 100

128 34.0 23.5 35.3




54 53.5 52.4 78.6



Abundance Ion 82.00 (81.70 to 82.70): BE091476.D (-377) (-)

Ion 128.00 (127.70 to 128.70): BE091476.D (-377) (-)

Ion 54.00 (53.70 to 54.70): BE091476.D (-377) (-)

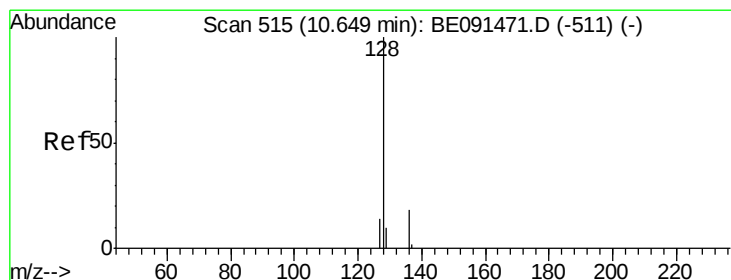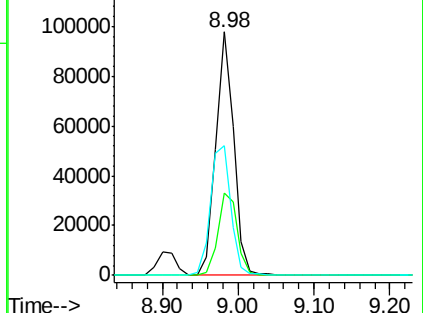

#8

Naphthalene

Concen: 9.07 ng

RT: 10.65 min Scan# 515

Delta R.T. -0.00 min

Lab File: BE091476.D

Acq: 17 Mar 2016 20:59


Tgt Ion: 128 Resp: 683286

Ion Ratio Lower Upper

128 100

129 10.4 8.2 12.2



127 14.4 11.8 17.8




Abundance Ion 128.00 (127.70 to 128.70): BE091476.D (-505) (-)

Ion 129.00 (128.70 to 129.70): BE091476.D (-505) (-)

Ion 127.00 (126.70 to 127.70): BE091476.D (-505) (-)

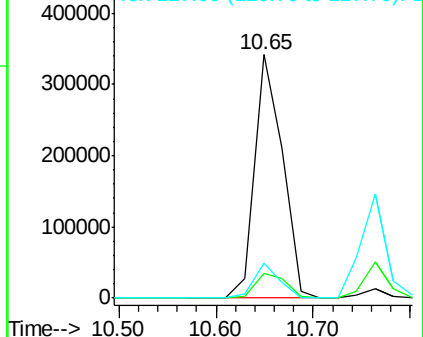

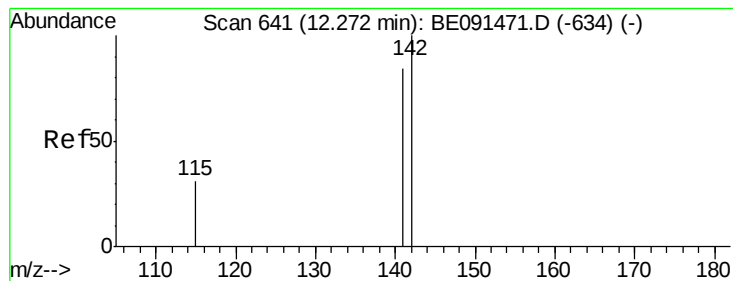

#9

2-Methylnaphthalene

Concen: 9.95 ng

RT: 12.27 min Scan# 641

Delta R.T. -0.00 min

Lab File: BE091476.D

Acq: 17 Mar 2016 20:59

Instrument :

BNA_E

ClientSampleId :

SSTDIC010


Tgt Ion:142 Resp: 472277

Ion Ratio Lower Upper

142 100

141 80.8 66.9 100.3




115 28.6 25.1 37.7

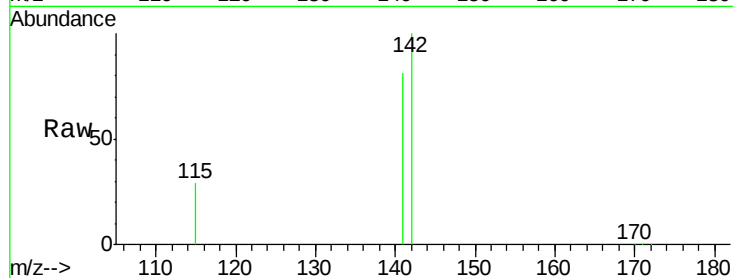

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E

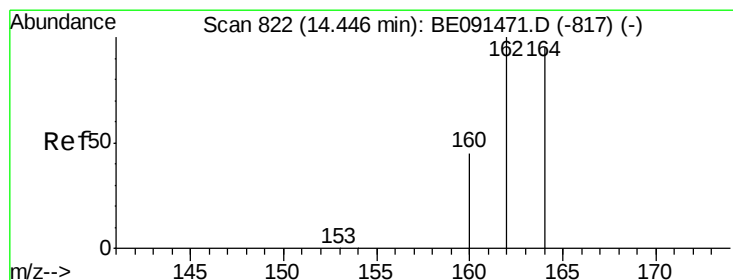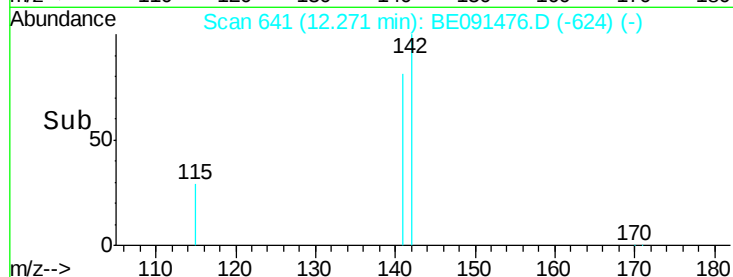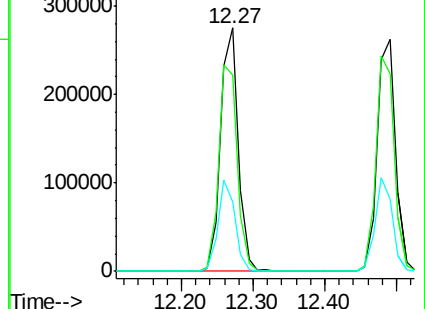

#10

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.45 min Scan# 822

Delta R.T. 0.00 min

Lab File: BE091476.D

Acq: 17 Mar 2016 20:59


Tgt Ion:164 Resp: 165705

Ion Ratio Lower Upper

164 100

162 102.8 84.4 126.6



160 44.2 37.7 56.5

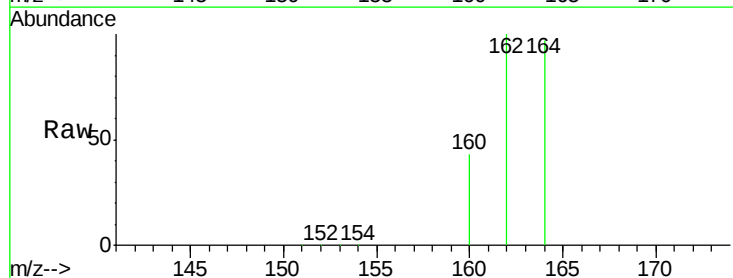


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



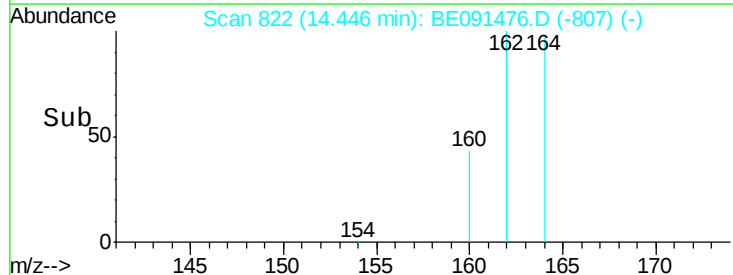
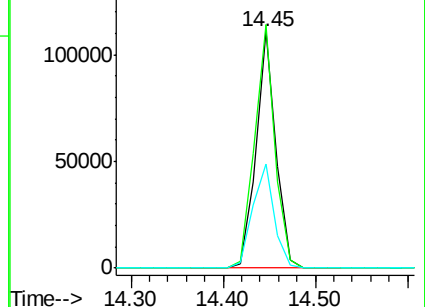




#11
 2,4,6-Tribromophenol
 Concen: 16.68 ng
 RT: 15.92 min Scan# 941
 Delta R.T. -0.01 min
 Lab File: BE091476.D
 Acq: 17 Mar 2016 20:59




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC010


Tgt Ion:330 Resp: 73634
 Ion Ratio Lower Upper
 330 100
 332 96.0 79.2 118.8
 141 40.2 28.1 42.1

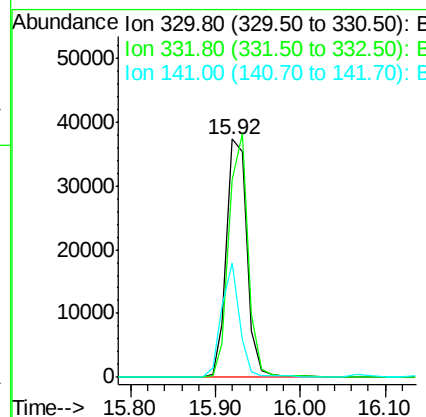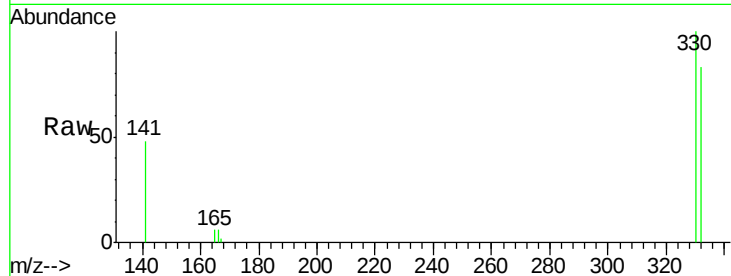

#12
 2-Fluorobiphenyl
 Concen: 9.46 ng
 RT: 13.07 min Scan# 710
 Delta R.T. -0.00 min
 Lab File: BE091476.D
 Acq: 17 Mar 2016 20:59

Tgt Ion:172 Resp: 436799
 Ion Ratio Lower Upper
 172 100
 171 36.1 29.8 44.8
 170 25.0 21.4 32.2



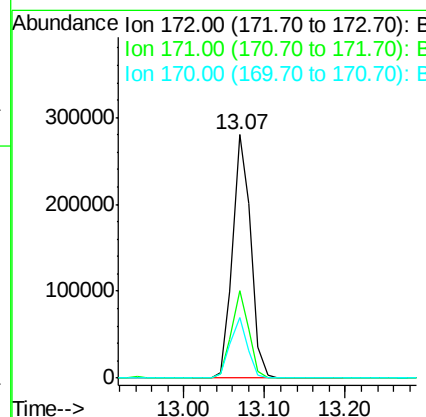





#13
Acenaphthylene
Concen: 10.38 ng
RT: 14.16 min Scan# 801
Delta R.T. 0.00 min
Lab File: BE091476.D
Acq: 17 Mar 2016 20:59




Instrument :
BNA_E
ClientSampleId :
SSTDIC010


Tgt Ion:152 Resp: 850634
Ion Ratio Lower Upper
152 100
151 19.8 16.3 24.5
153 13.2 11.1 16.7

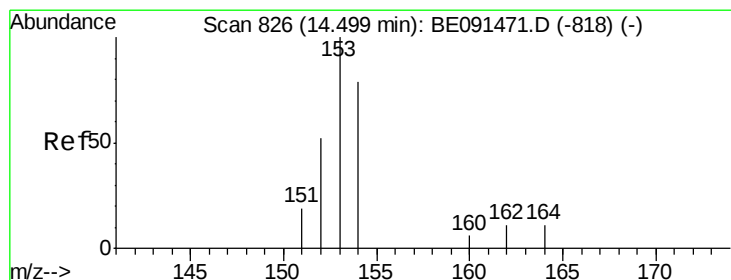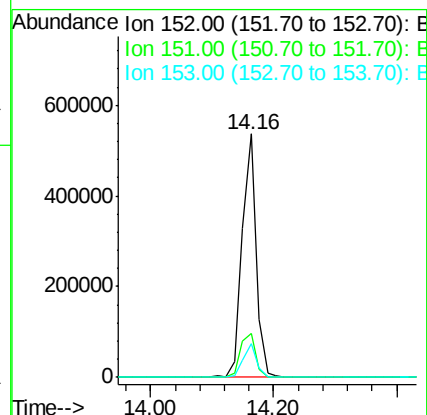

#14
Acenaphthene
Concen: 9.05 ng
RT: 14.50 min Scan# 826
Delta R.T. 0.00 min
Lab File: BE091476.D
Acq: 17 Mar 2016 20:59

Tgt Ion:154 Resp: 533439
Ion Ratio Lower Upper
154 100
153 107.6 87.3 130.9
152 52.5 42.9 64.3

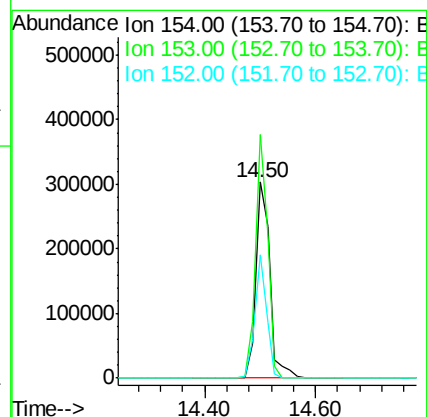



#15

Fluorene

Concen: 9.59 ng

RT: 15.49 min Scan# 904

Delta R.T. 0.00 min

Lab File: BE091476.D

Acq: 17 Mar 2016 20:59

Instrument :

BNA_E

ClientSampleId :

SSTDICC010





Tgt Ion:166 Resp: 655182

Ion Ratio Lower Upper

166 100

165 98.2 79.2 118.8

167 13.7 10.8 16.2

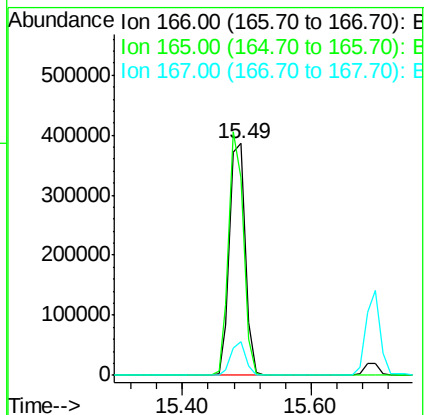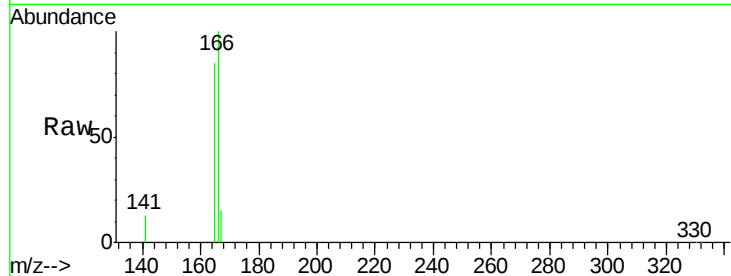

#16

Phenanthrene-d10

Concen: 5.00 ng

RT: 17.18 min Scan# 1019

Delta R.T. 0.00 min

Lab File: BE091476.D

Acq: 17 Mar 2016 20:59




Tgt Ion:188 Resp: 389139


Ion Ratio Lower Upper

188 100

94 5.6 5.4 8.2

80 5.0 5.0 7.4

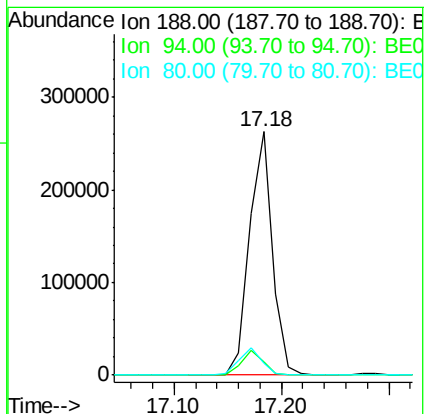







#17
Hexachlorobenzene
Concen: 7.11 ng
RT: 16.48 min Scan# 975
Delta R.T. -0.00 min
Lab File: BE091476.D
Acq: 17 Mar 2016 20:59

Instrument :
BNA_E
ClientSampleId :
SSTDICC010

Tgt Ion: 284 Resp: 175979
Ion Ratio Lower Upper
284 100
142 39.2 31.0 46.4
249 31.4 25.8 38.8




Abundance Ion 283.80 (283.50 to 284.50): E
Ion 142.00 (141.70 to 142.70): E
Ion 249.00 (248.70 to 249.70): E

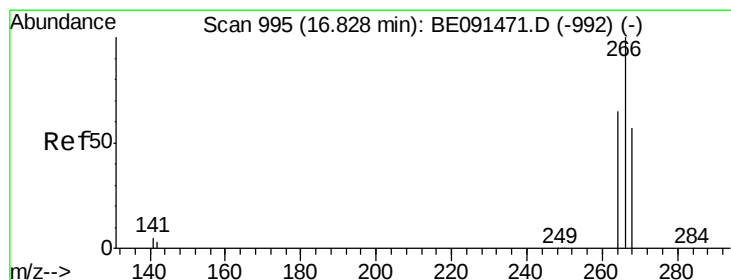
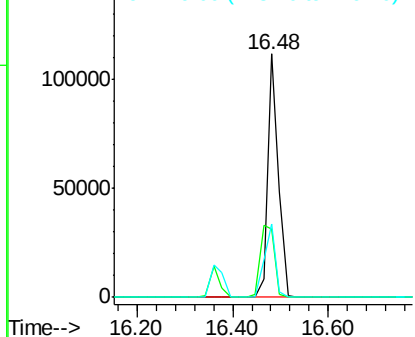



#18
Pentachlorophenol
Concen: 42.28 ng
RT: 16.83 min Scan# 995
Delta R.T. -0.00 min
Lab File: BE091476.D
Acq: 17 Mar 2016 20:59

Tgt Ion: 266 Resp: 101612
Ion Ratio Lower Upper
266 100
268 68.5 48.2 72.2
264 56.9 52.1 78.1

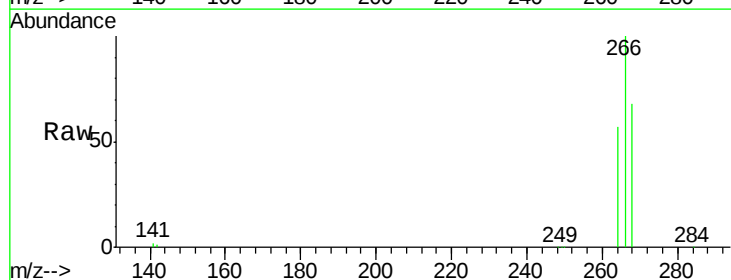

Abundance Ion 265.70 (265.40 to 266.40): E
Ion 268.00 (267.70 to 268.70): E
Ion 264.00 (263.70 to 264.70): E

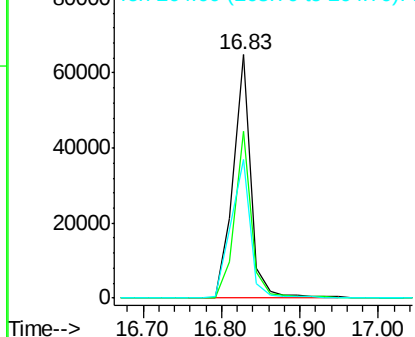

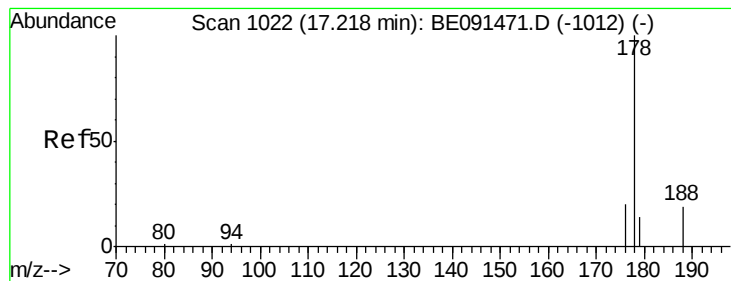

#19

Phenanthrene

Concen: 8.97 ng

RT: 17.22 min Scan# 1022

Delta R.T. 0.00 min

Lab File: BE091476.D

Acq: 17 Mar 2016 20:59

Instrument :

BNA_E

ClientSampleId :

SSTDICC010


Tgt Ion:178 Resp: 1096865

Ion Ratio Lower Upper

178 100

176 19.8 15.5 23.3




179 15.8 13.1 19.7



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

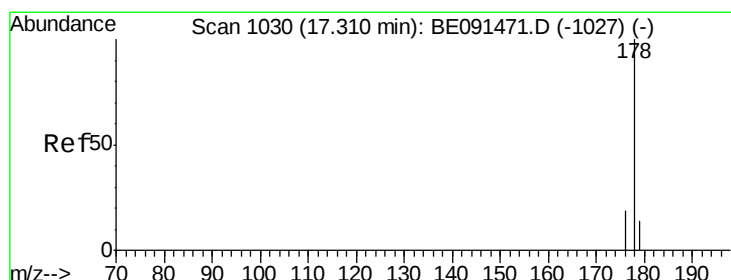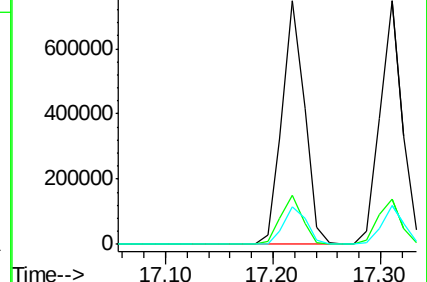

#20

Anthracene

Concen: 10.08 ng

RT: 17.31 min Scan# 1030

Delta R.T. 0.00 min

Lab File: BE091476.D

Acq: 17 Mar 2016 20:59


Tgt Ion:178 Resp: 1090780

Ion Ratio Lower Upper

178 100

176 19.2 14.9 22.3



179 15.7 12.2 18.4




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

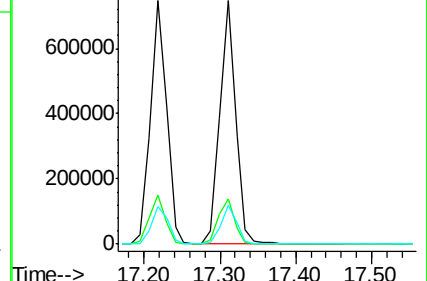

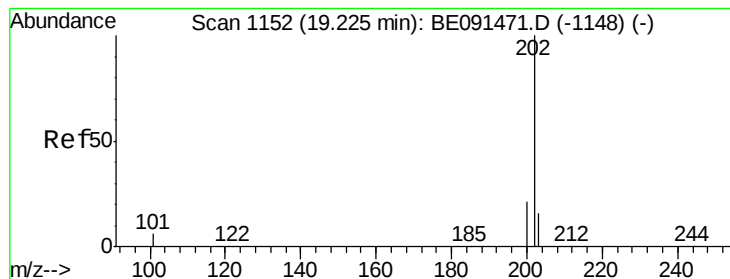

#21

Fluoranthene

Concen: 10.23 ng

RT: 19.23 min Scan# 1152

Delta R.T. 0.00 min

Lab File: BE091476.D

Acq: 17 Mar 2016 20:59

Instrument :

BNA_E

ClientSampleId :

SSTDIC010


Tgt Ion:202 Resp: 1338593

Ion Ratio Lower Upper

202 100

101 10.8 8.3 12.5




203 17.7 13.9 20.9

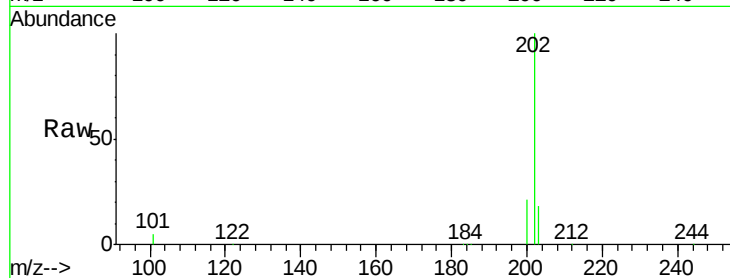

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

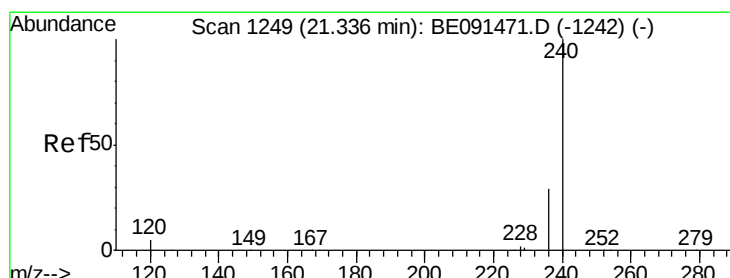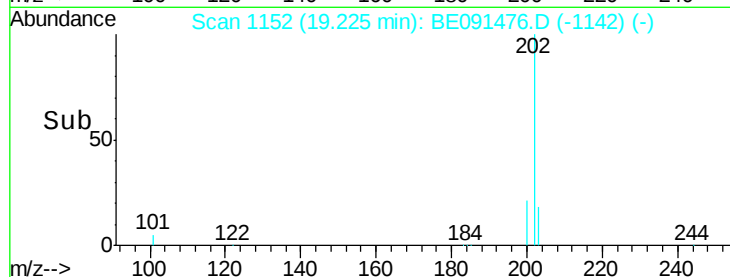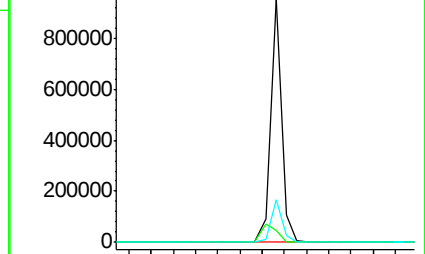

#22

Chrysene-d12

Concen: 5.00 ng

RT: 21.34 min Scan# 1249

Delta R.T. -0.00 min

Lab File: BE091476.D

Acq: 17 Mar 2016 20:59


Tgt Ion:240 Resp: 554894

Ion Ratio Lower Upper

240 100

120 4.5 4.0 6.0



236 29.2 23.0 34.4

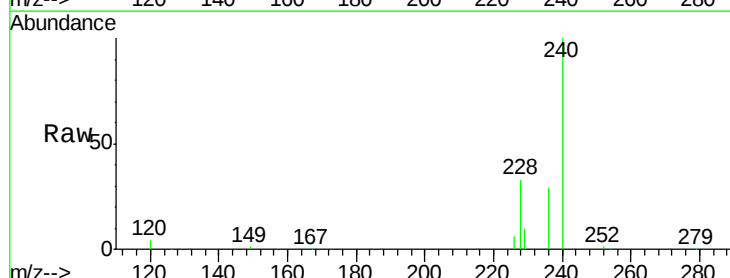


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



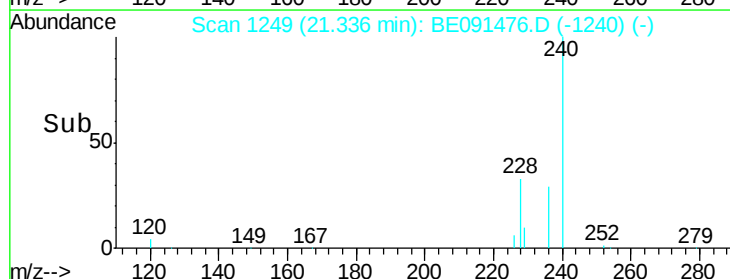
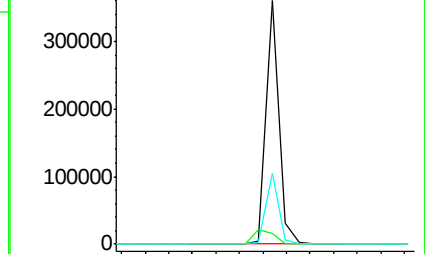




#23
 Pyrene
 Concen: 6.93 ng
 RT: 19.59 min Scan# 1171
 Delta R.T. 0.00 min
 Lab File: BE091476.D
 Acq: 17 Mar 2016 20:59




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC010

Tgt Ion: 202 Resp: 1422675
 Ion Ratio Lower Upper
 202 100
 200 21.3 16.4 24.6
 203 18.2 14.6 21.8

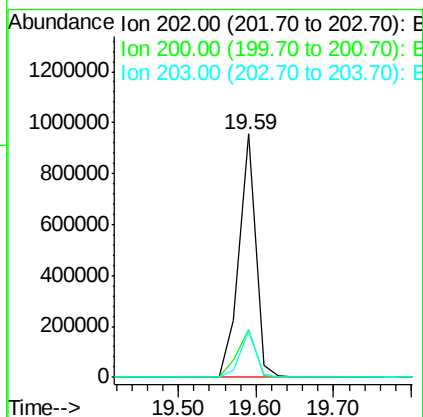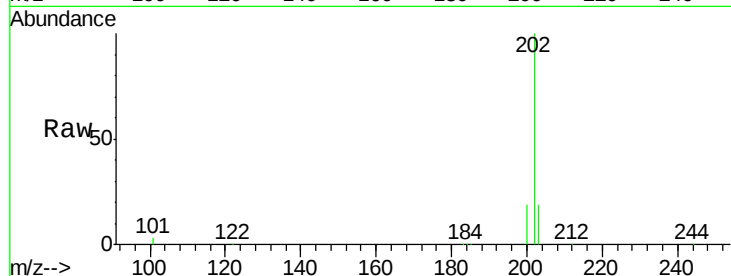

#24
 Terphenyl-d14
 Concen: 9.25 ng
 RT: 19.80 min Scan# 1182
 Delta R.T. 0.00 min
 Lab File: BE091476.D
 Acq: 17 Mar 2016 20:59

Tgt Ion: 244 Resp: 642112
 Ion Ratio Lower Upper
 244 100
 212 6.6 5.8 8.8
 122 0.7 1.8 2.8#



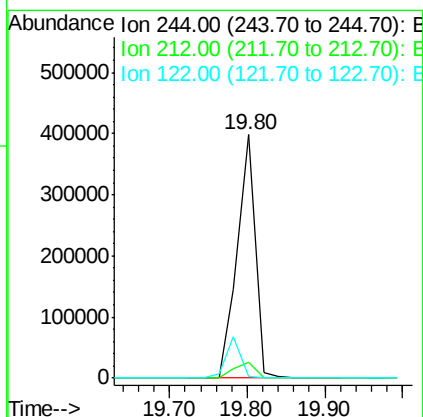





#25
Benzo(a)anthracene
Concen: 15.05 ng
RT: 21.31 min Scan# 1248
Delta R.T. -0.00 min
Lab File: BE091476.D
Acq: 17 Mar 2016 20:59




Instrument :
BNA_E
ClientSampleId :
SSTDICC010


Tgt Ion:228 Resp: 2765250
Ion Ratio Lower Upper
228 100
226 30.7 24.0 36.0
229 18.4 13.8 20.6

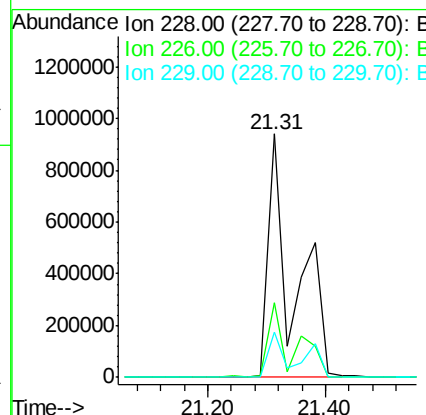

#26
Chrysene
Concen: 14.30 ng
RT: 21.31 min Scan# 1248
Delta R.T. -0.07 min
Lab File: BE091476.D
Acq: 17 Mar 2016 20:59

Tgt Ion:228 Resp: 2779269
Ion Ratio Lower Upper
228 100
226 30.7 18.9 28.3#
229 18.4 19.1 28.7#



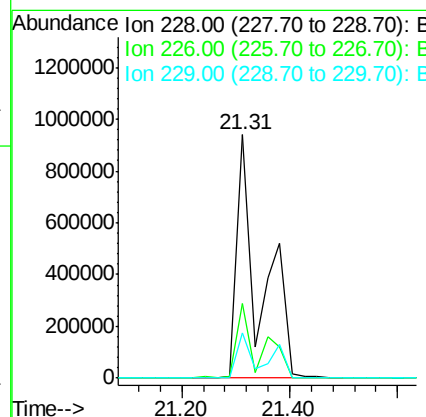





#27
 Indeno(1,2,3-cd)pyrene
 Concen: 10.60 ng
 RT: 26.40 min Scan# 1653
 Delta R.T. 0.00 min
 Lab File: BE091476.D
 Acq: 17 Mar 2016 20:59




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC010


Tgt Ion: 276 Resp: 1651049
 Ion Ratio Lower Upper
 276 100
 138 25.9 20.2 30.4
 277 25.2 19.8 29.8

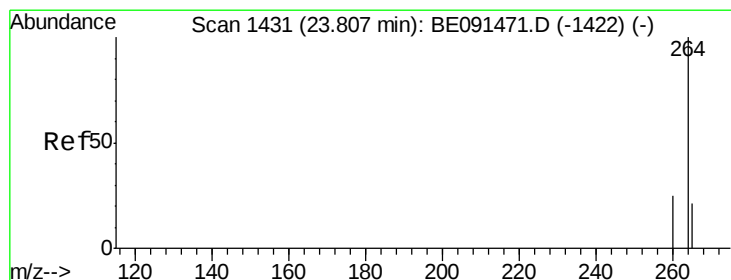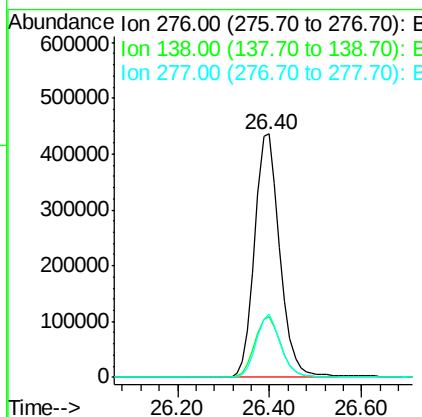

#28
 Perylene-d12
 Concen: 5.00 ng
 RT: 23.81 min Scan# 1431
 Delta R.T. 0.00 min
 Lab File: BE091476.D
 Acq: 17 Mar 2016 20:59

Tgt Ion: 264 Resp: 468385
 Ion Ratio Lower Upper
 264 100
 260 24.8 20.1 30.1
 265 24.0 18.3 27.5

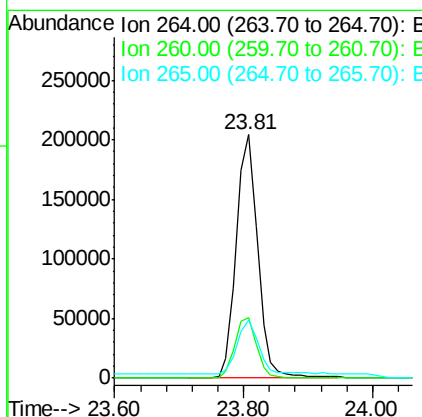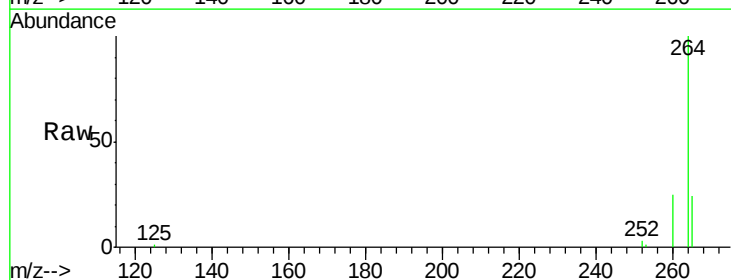

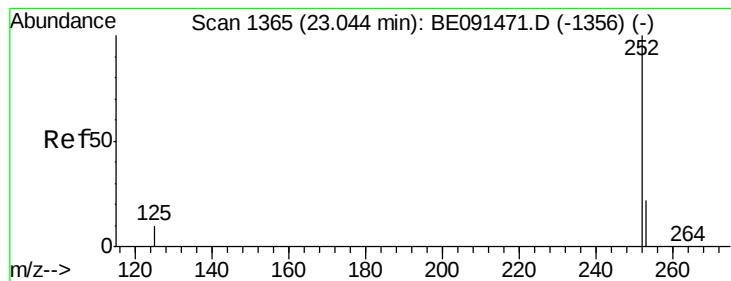

#29

Benzo(b)fluoranthene

Concen: 8.63 ng

RT: 23.04 min Scan# 1365

Delta R.T. 0.00 min

Lab File: BE091476.D

Acq: 17 Mar 2016 20:59

Instrument :

BNA_E

ClientSampleId :

SSTDICC010


Tgt Ion:252 Resp: 1464547

Ion Ratio Lower Upper

252 100

253 22.1 18.7 28.1




125 10.4 9.8 14.6



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

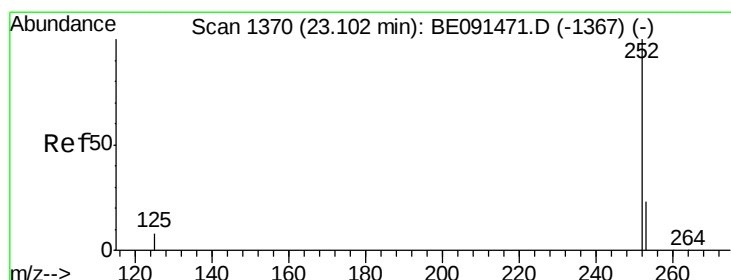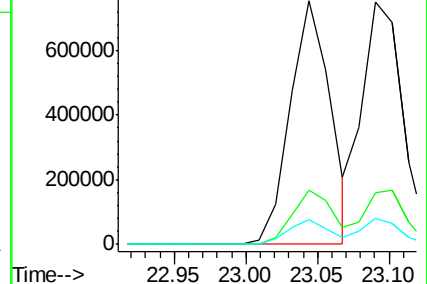

#30

Benzo(k)fluoranthene

Concen: 8.89 ng

RT: 23.09 min Scan# 1369

Delta R.T. -0.01 min

Lab File: BE091476.D

Acq: 17 Mar 2016 20:59


Tgt Ion:252 Resp: 1495888

Ion Ratio Lower Upper

252 100

253 21.3 20.2 30.4



125 10.6 9.4 14.2

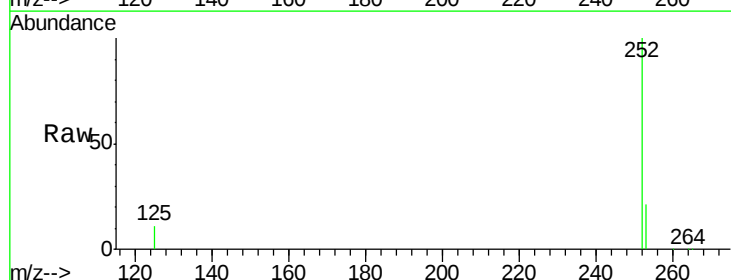


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

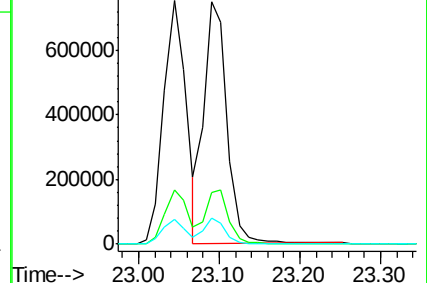

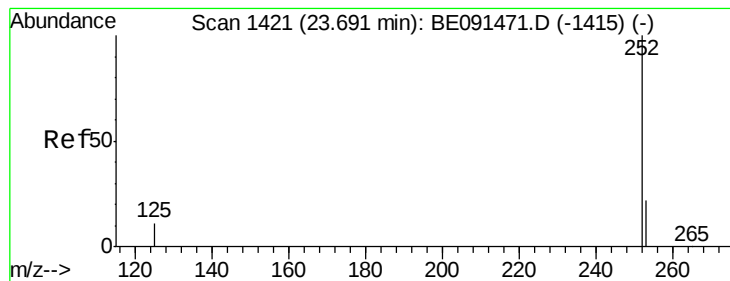

#31

Benzo(a)pyrene

Concen: 9.91 ng

RT: 23.69 min Scan# 1421

Delta R.T. 0.00 min

Lab File: BE091476.D

Acq: 17 Mar 2016 20:59

Instrument :

BNA_E

ClientSampleId :

SSTDICC010


Tgt Ion:252 Resp: 1421172

Ion Ratio Lower Upper




252 100

253 22.2 19.4 29.0

125 10.8 11.4 17.2#

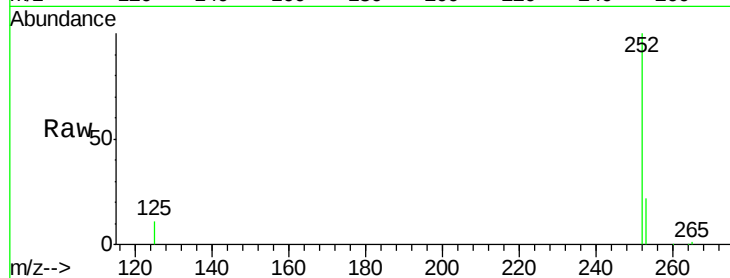

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

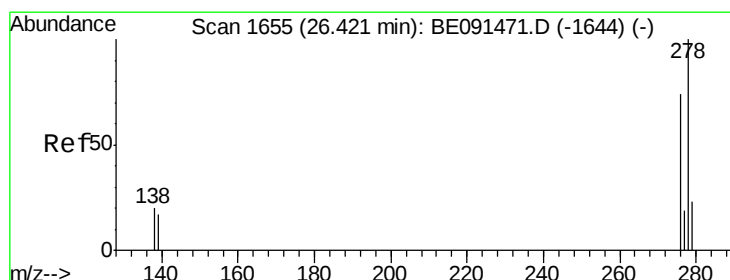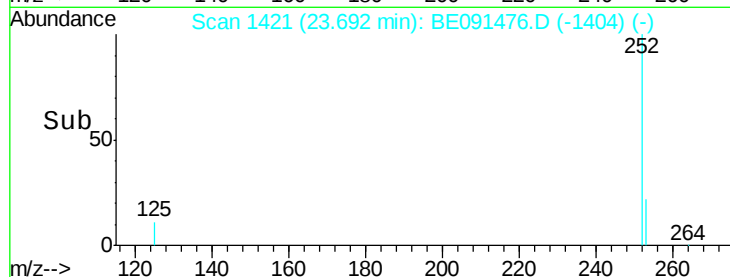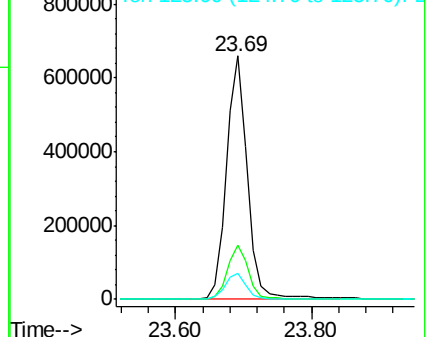

#32

Dibenzo(a,h)anthracene

Concen: 11.49 ng

RT: 26.42 min Scan# 1655

Delta R.T. 0.00 min

Lab File: BE091476.D

Acq: 17 Mar 2016 20:59


Tgt Ion:278 Resp: 1384410

Ion Ratio Lower Upper



278 100


139 16.3 14.2 21.4

279 24.1 19.6 29.4

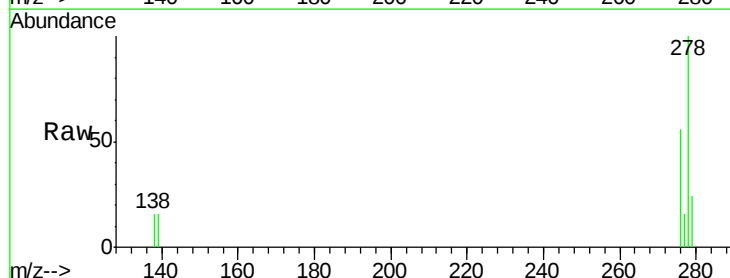

Abundance Ion 278.00 (277.70 to 278.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 279.00 (278.70 to 279.70): E

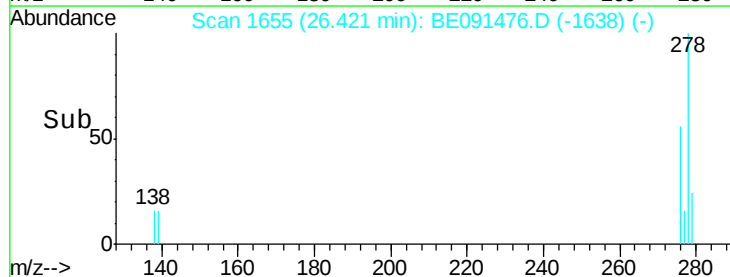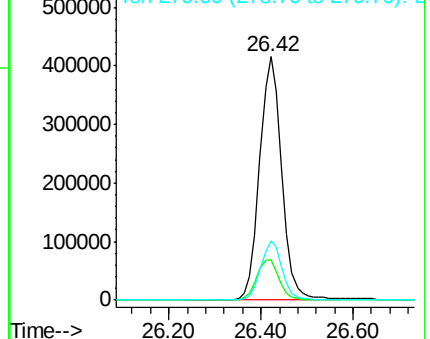

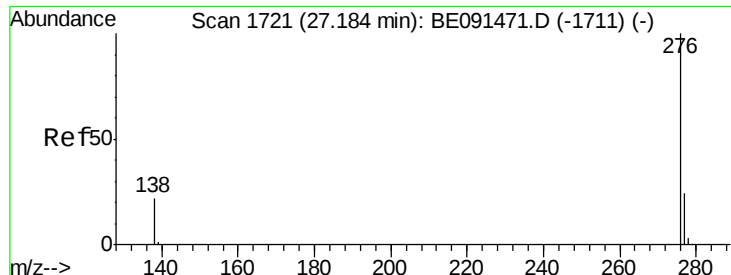

#33

Benzo(g,h,i)perylene

Concen: 10.26 ng

RT: 27.20 min Scan# 1722

Delta R.T. 0.01 min

Lab File: BE091476.D


Acq: 17 Mar 2016 20:59

Instrument :

BNA_E

ClientSampleId :

SSTDIC010

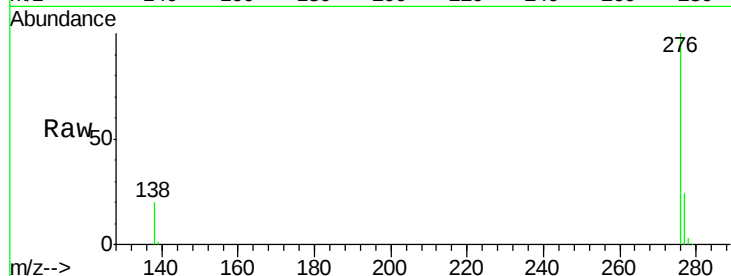


Tgt Ion: 276 Resp: 1399634

Ion Ratio Lower Upper

276 100

277 24.3 19.4 29.2

138 20.1 18.2 27.4



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

