


Data Path : Z:\HPCHEM1\BNA_E\Data\BE031816\
Data File : BE091468.D
Acq On : 17 Mar 2016 16:00
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE031816.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 18 14:14:30 2016

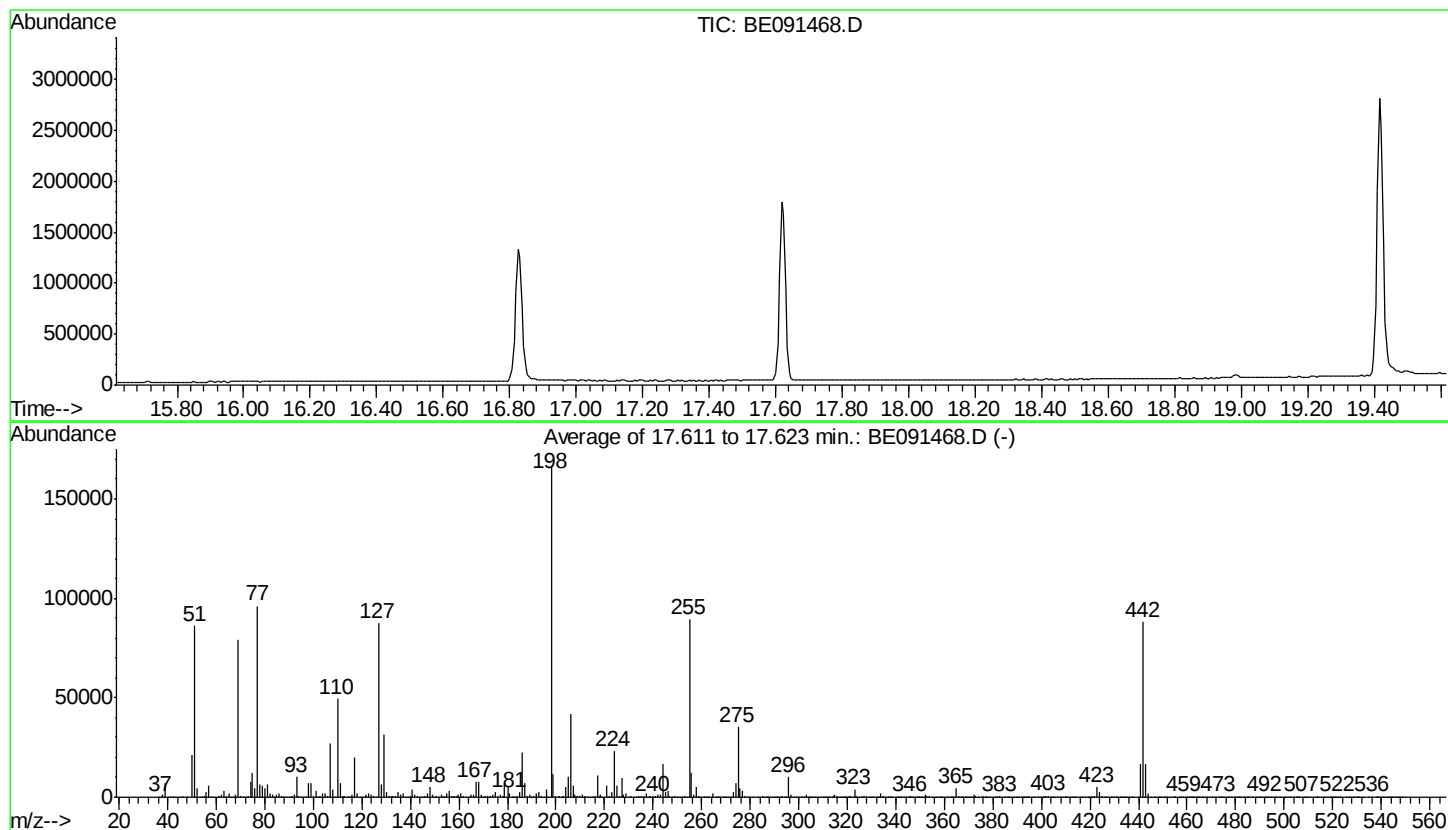

AutoFind: Scans 2557, 2558, 2559; Background Corrected with Scan 2549

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.6	85970	PASS
68	69	0.00	2	2.0	1554	PASS
69	198	0.00	100	47.3	78897	PASS
70	69	0.00	2	0.5	402	PASS
127	198	10	80	52.4	87315	PASS
197	198	0.00	2	0.2	306	PASS
198	198	100	100	100.0	166737	PASS
199	198	5	9	7.1	11768	PASS
275	198	10	60	21.1	35146	PASS
365	198	1	100	2.6	4258	PASS
441	442	0.01	24	18.9	16648	PASS
442	198	50	100	52.8	88062	PASS
443	442	15	24	19.1	16778	PASS