


Data Path : Z:\HPCHEM1\BNA_E\Data\BE031916\
 Data File : BE091478.D
 Acq On : 18 Mar 2016 10:51
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE031816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 18 14:14:30 2016

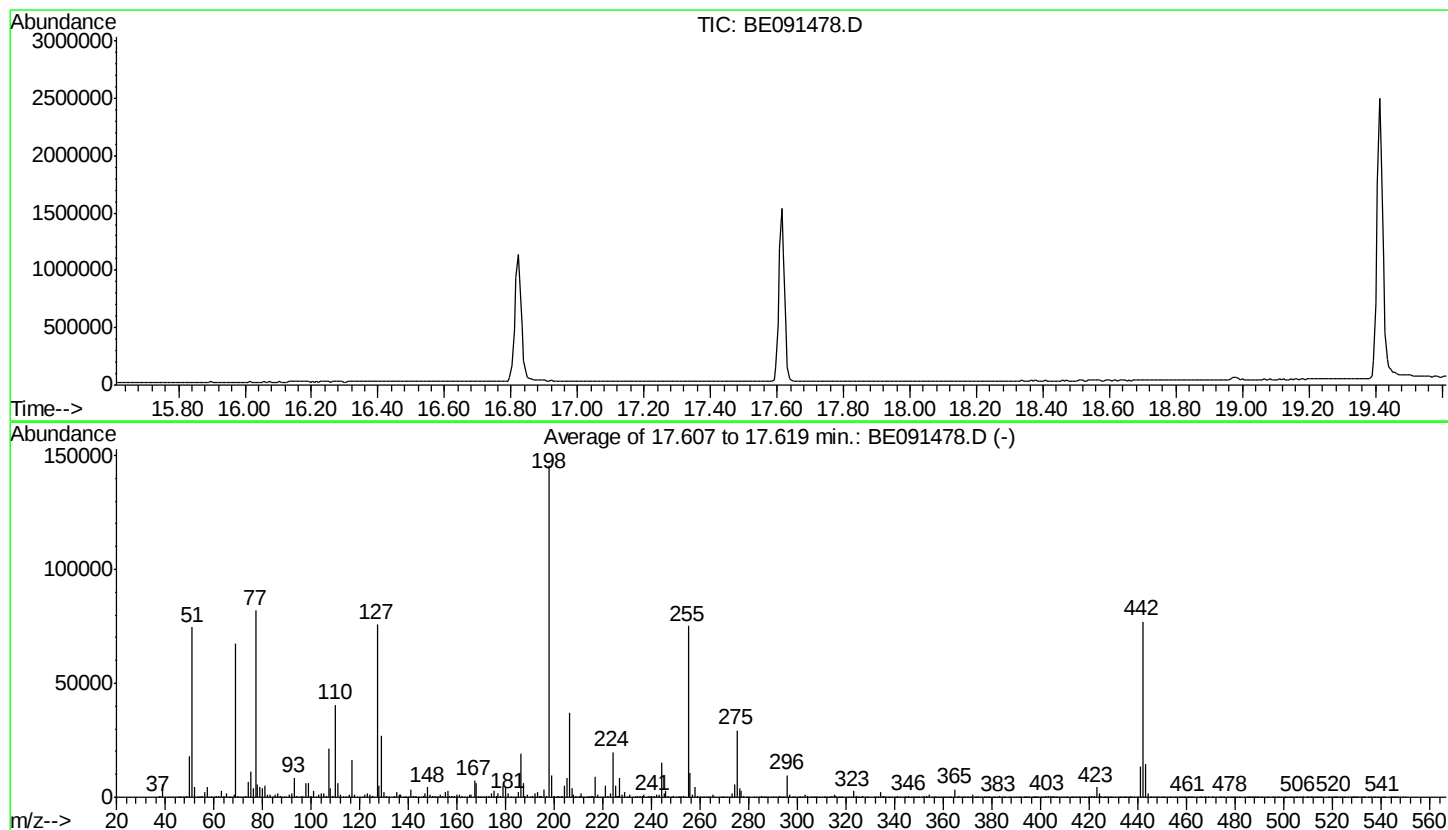

AutoFind: Scans 2556, 2557, 2558; Background Corrected with Scan 2546

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.3	74701	PASS
68	69	0.00	2	1.8	1230	PASS
69	198	0.00	100	46.5	67688	PASS
70	69	0.00	2	0.8	519	PASS
127	198	10	80	52.0	75648	PASS
197	198	0.00	2	0.2	324	PASS
198	198	100	100	100.0	145581	PASS
199	198	5	9	6.5	9516	PASS
275	198	10	60	20.2	29477	PASS
365	198	1	100	2.4	3436	PASS
441	442	0.01	24	17.6	13565	PASS
442	198	50	100	52.9	77016	PASS
443	442	15	24	18.9	14590	PASS