


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE031919\
 Data File : BE099030.D
 Acq On : 19 Mar 2019 10:33
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 15 05:31:33 2019

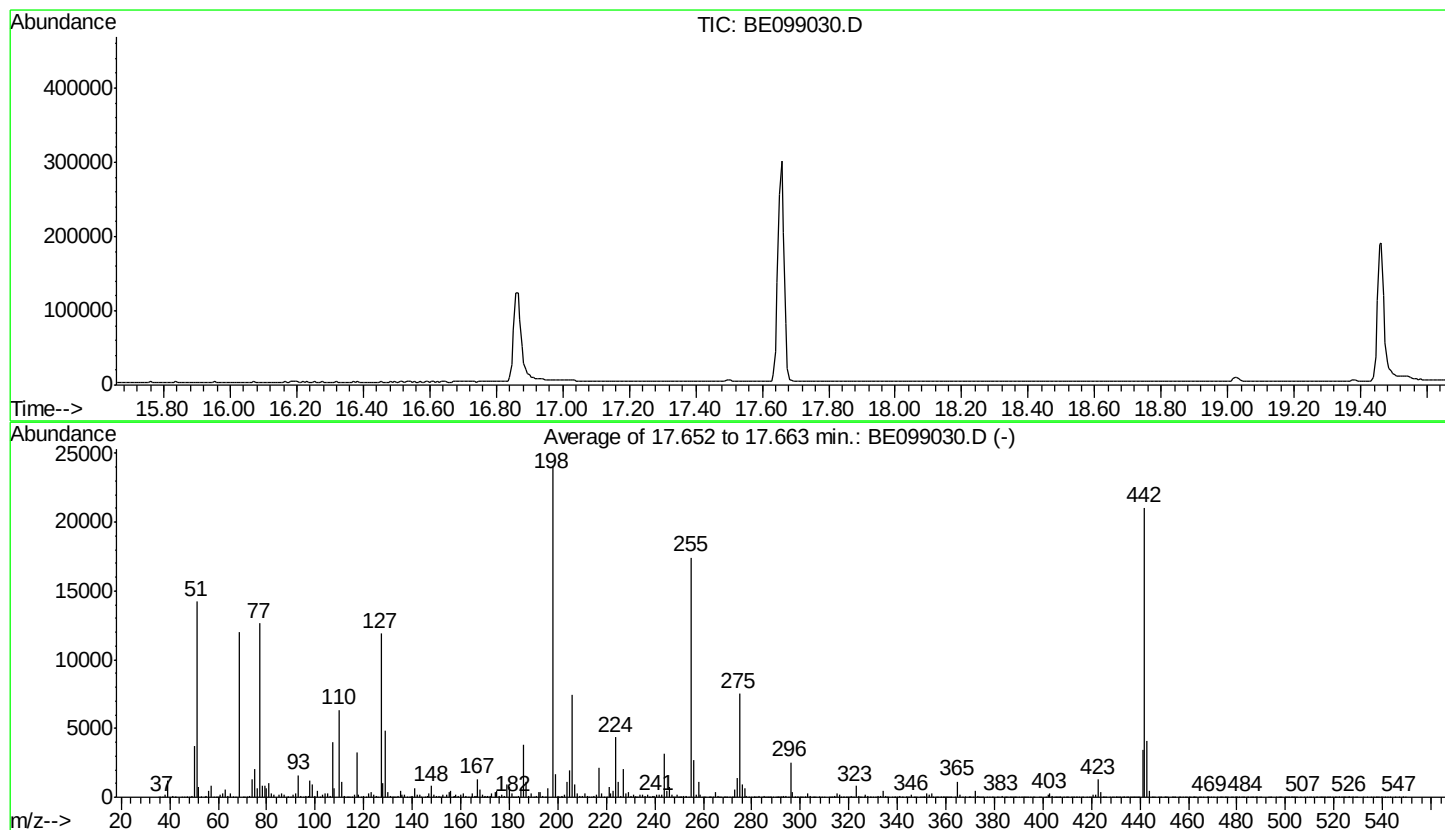

AutoFind: Scans 2564, 2565, 2566; Background Corrected with Scan 2553

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.9	14215	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	50.0	12052	PASS
70	69	0.00	2	0.3	35	PASS
127	198	10	80	49.3	11885	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	24115	PASS
199	198	5	9	7.0	1696	PASS
275	198	10	60	31.3	7537	PASS
365	198	1	100	4.7	1129	PASS
441	198	0.01	100	14.5	3492	PASS
442	198	50	100	87.3	21044	PASS
443	442	15	24	19.5	4106	PASS