


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE031919\
 Data File : BE099047.D
 Acq On : 19 Mar 2019 22:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 15 05:31:33 2019

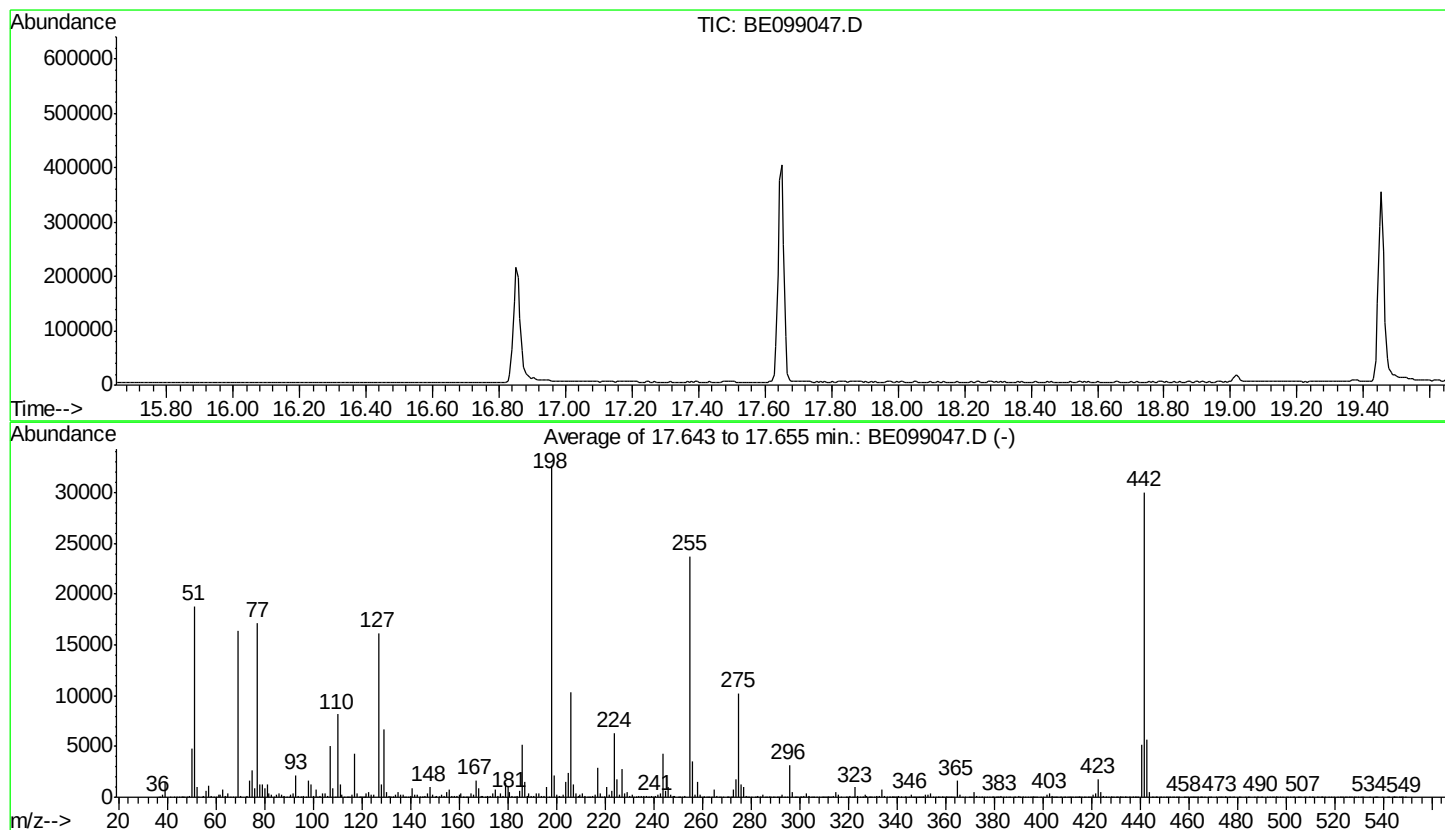

AutoFind: Scans 2562, 2563, 2564; Background Corrected with Scan 2552

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.6	18814	PASS
68	69	0.00	2	0.3	47	PASS
69	198	0.00	100	50.3	16430	PASS
70	69	0.00	2	0.6	91	PASS
127	198	10	80	49.5	16159	PASS
197	198	0.00	2	0.2	57	PASS
198	198	100	100	100.0	32664	PASS
199	198	5	9	6.8	2209	PASS
275	198	10	60	31.3	10219	PASS
365	198	1	100	4.9	1597	PASS
441	198	0.01	100	15.9	5182	PASS
442	198	50	100	92.1	30070	PASS
443	442	15	24	18.7	5624	PASS