


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE032415\
 Data File : BE089825.D
 Acq On : 24 Mar 2015 23:34
 Operator : TP/JJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE032415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 24 18:03:12 2015

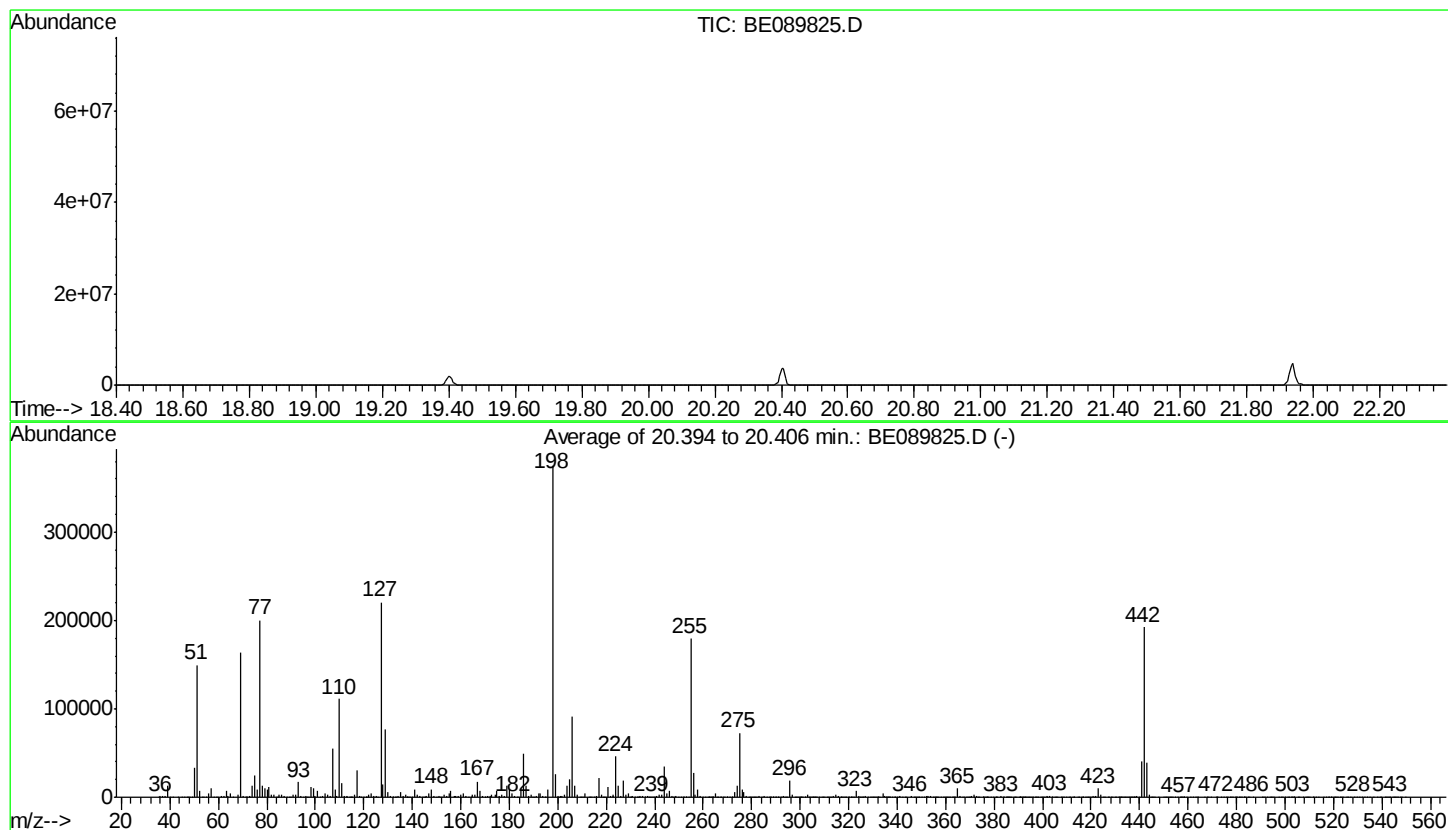

AutoFind: Scans 3235, 3236, 3237; Background Corrected with Scan 3227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	149547	PASS
68	69	0.00	2	1.5	2476	PASS
69	198	0.00	100	43.7	163903	PASS
70	69	0.00	2	0.6	939	PASS
127	198	10	80	58.8	220714	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	375222	PASS
199	198	5	9	6.9	26056	PASS
275	198	10	60	19.4	72625	PASS
365	198	1	100	2.6	9869	PASS
441	442	0.01	24	20.8	40048	PASS
442	198	50	100	51.3	192547	PASS
443	442	15	24	20.1	38709	PASS