


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE032415\
 Data File : BE089810.D
 Acq On : 24 Mar 2015 11:17
 Operator : TP/JJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE032415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 25 16:20:31 2015

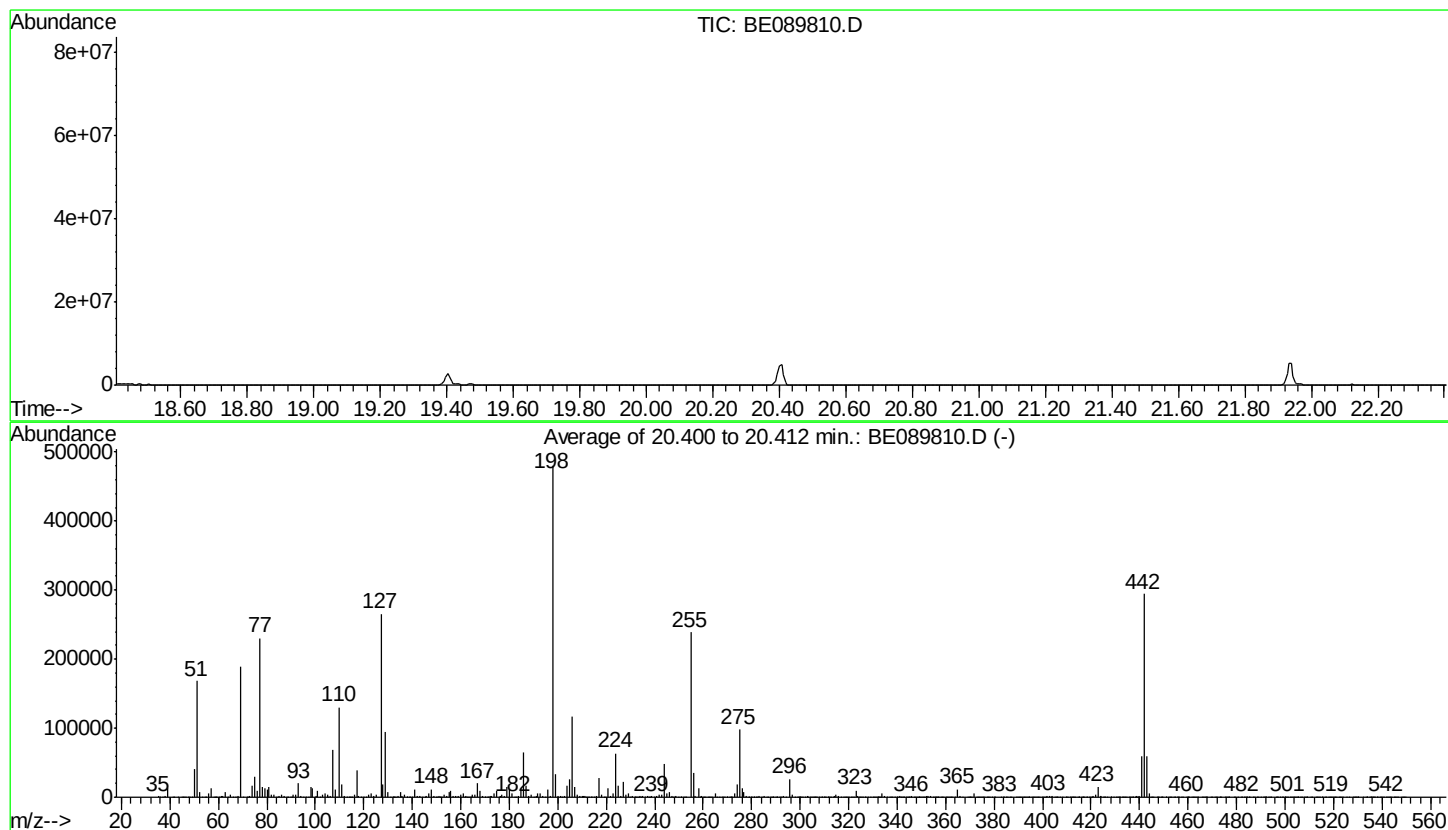

AutoFind: Scans 3236, 3237, 3238; Background Corrected with Scan 3224

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	168270	PASS
68	69	0.00	2	1.3	2383	PASS
69	198	0.00	100	39.5	189925	PASS
70	69	0.00	2	0.3	596	PASS
127	198	10	80	55.3	265578	PASS
197	198	0.00	2	0.3	1265	PASS
198	198	100	100	100.0	480425	PASS
199	198	5	9	7.1	33917	PASS
275	198	10	60	20.5	98288	PASS
365	198	1	100	2.5	12125	PASS
441	442	0.01	24	20.5	60160	PASS
442	198	50	100	61.2	294080	PASS
443	442	15	24	20.2	59486	PASS