


Data Path : Z:\HPCHEM1\BNA_E\Data\BE032515\
 Data File : BE089839.D
 Acq On : 25 Mar 2015 14:50
 Operator : TP/JJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE032415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 25 16:20:31 2015

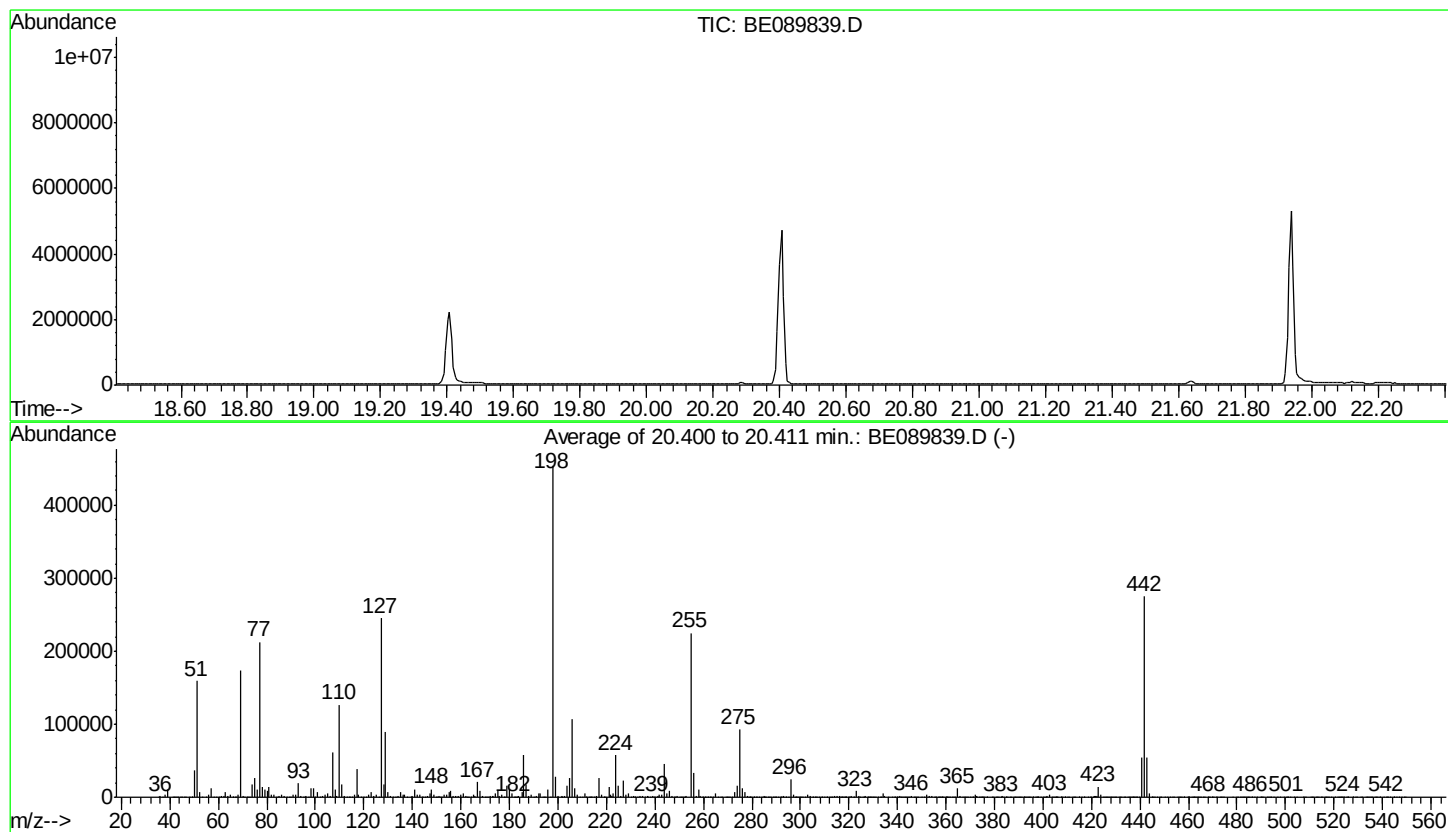

AutoFind: Scans 3236, 3237, 3238; Background Corrected with Scan 3228

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	159317	PASS
68	69	0.00	2	1.7	2887	PASS
69	198	0.00	100	38.2	173272	PASS
70	69	0.00	2	0.7	1184	PASS
127	198	10	80	54.0	245226	PASS
197	198	0.00	2	0.1	445	PASS
198	198	100	100	100.0	454165	PASS
199	198	5	9	6.3	28658	PASS
275	198	10	60	20.3	92133	PASS
365	198	1	100	2.6	11794	PASS
441	442	0.01	24	19.8	54544	PASS
442	198	50	100	60.5	274814	PASS
443	442	15	24	19.9	54810	PASS