

Data Path : Z:\HPCHEM1\BNA E\DATA\BE032516\
 Data File : BE091522.D
 Acq On : 25 Mar 2016 13:28
 Operator : UM/SJ
 Sample : SSTDICC0.2
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Mar 25 15:57:17 2016
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 25 15:55:56 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	39776	5.00	ng	0.00
6) Naphthalene-d8	10.59	136	185198	5.00	ng	0.00
10) Acenaphthene-d10	14.43	164	105509	5.00	ng	0.00
16) Phenanthrene-d10	17.17	188	277654	5.00	ng	0.00
22) Chrysene-d12	21.33	240	268288	5.00	ng	0.00
28) Perylene-d12	23.78	264	287728	5.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.42	112	1419	0.16	ng	0.00
5) Phenol-d6	6.99	99	1869	0.16	ng	0.00
7) Nitrobenzene-d5	8.97	82	1369	0.17	ng	0.00
11) 2,4,6-Tribromophenol	15.91	330	824	0.27	ng	0.00
12) 2-Fluorobiphenyl	13.06	172	5838	0.22	ng	0.00
24) Terphenyl-d14	19.78	244	8334	0.26	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.37	88	1225	0.25	ng	89
3) n-Nitrosodimethylamine	3.68	42	748	0.11	ng	# 94
8) Naphthalene	10.65	128	7404	0.16	ng	# 94
9) 2-Methylnaphthalene	12.26	142	4326	0.15	ng	99
13) Acenaphthylene	14.15	152	7005	0.16	ng	# 86
14) Acenaphthene	14.49	154	5033	0.15	ng	93
15) Fluorene	15.47	166	6030	0.15	ng	99
17) Hexachlorobenzene	16.48	284	1815	0.15	ng	93
18) Pentachlorophenol	16.81	266	412	0.09	ng	89
19) Phenanthrene	17.21	178	12614	0.16	ng	99
20) Anthracene	17.30	178	9261	0.13	ng	100
21) Fluoranthene	19.22	202	10686	0.12	ng	98
23) Pyrene	19.57	202	11532	0.17	ng	98
25) Benzo(a)anthracene	21.36	228	27254	0.37	ng	97
26) Chrysene	21.36	228	27463	0.36	ng	# 90
27) Indeno(1,2,3-cd)pyrene	26.35	276	11480	0.15	ng	100
29) Benzo(b)fluoranthene	23.08	252	9823	0.11	ng	97
30) Benzo(k)fluoranthene	23.08	252	10200	0.11	ng	97
31) Benzo(a)pyrene	23.67	252	8894	0.11	ng	# 96
32) Dibenzo(a,h)anthracene	26.39	278	9673	0.12	ng	97
33) Benzo(g,h,i)perylene	27.15	276	10732	0.13	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE032516\
Data File : BE091522.D
Acq On : 25 Mar 2016 13:28
Operator : UM/SJ
Sample : SSTDICC0.2
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Mar 25 15:57:17 2016
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 25 15:55:56 2016
Response via : Initial Calibration

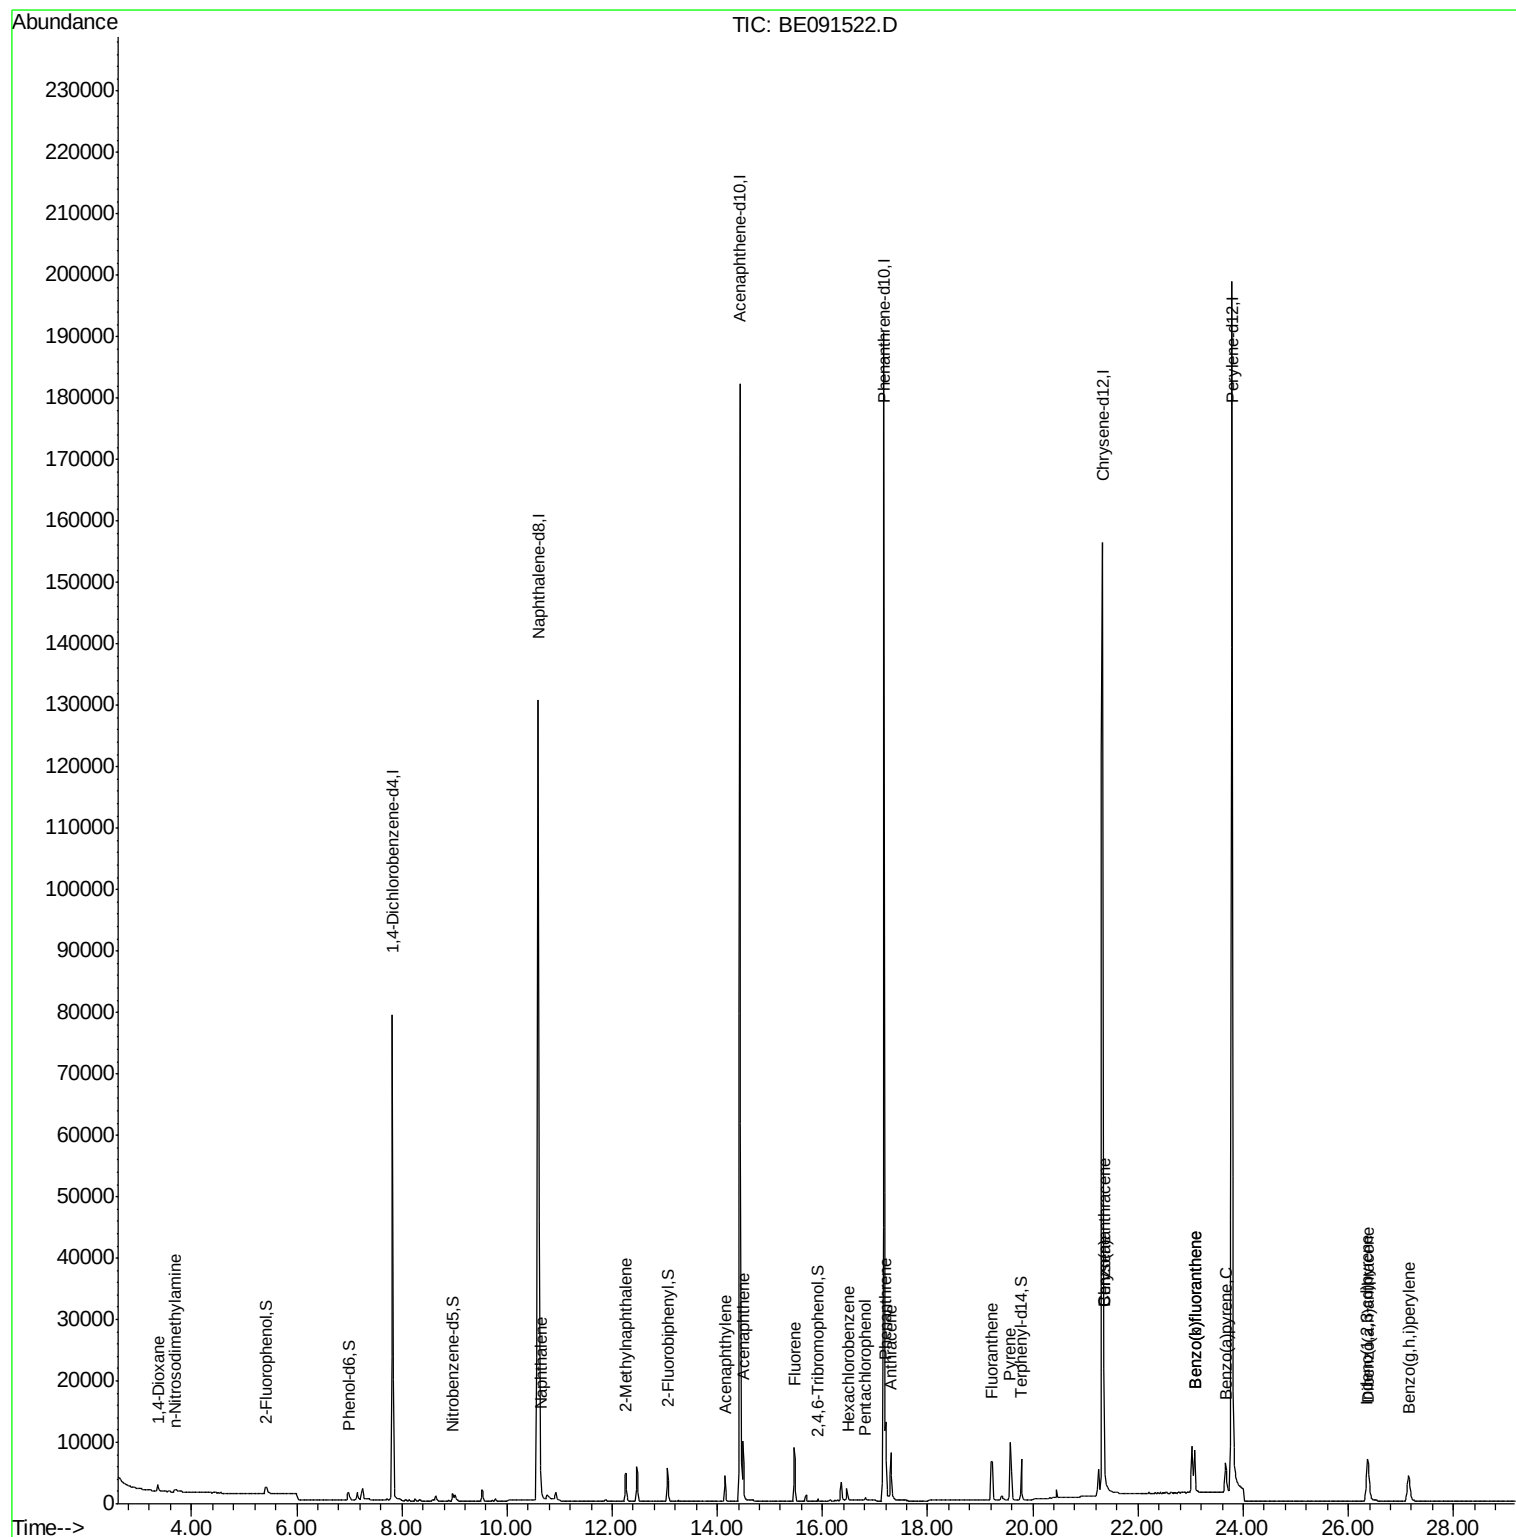




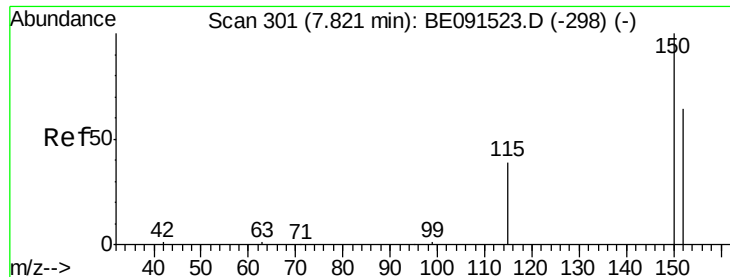


#1

1,4-Dichlorobenzene-d4
Concen: 5.00 ng
RT: 7.82 min Scan# 301
Delta R.T. -0.00 min
Lab File: BE091522.D
Acq: 25 Mar 2016 13:28

Instrument :
BNA_E
ClientSampled :




Tot Ion:152 Resp: 39776
Ion Ratio Lower Upper
152 100
150 155.7 122.2 183.2
115 61.0 45.9 68.9

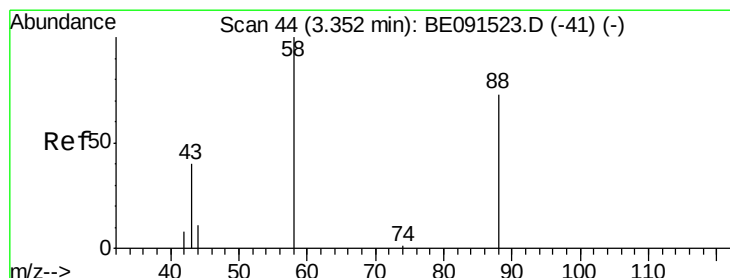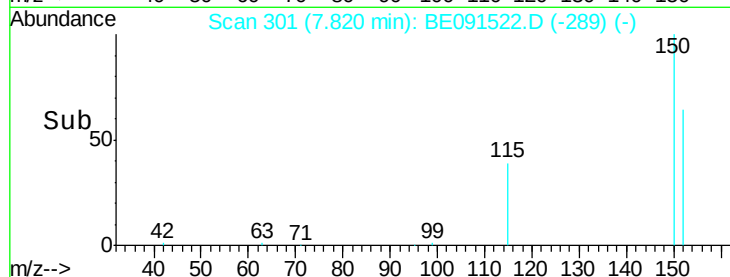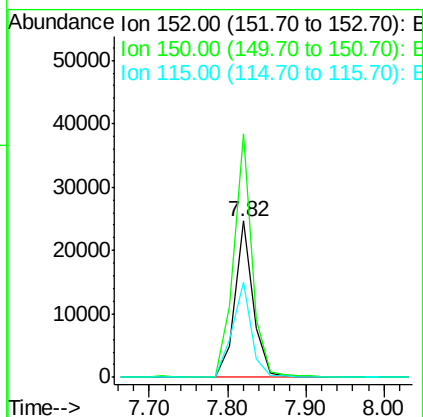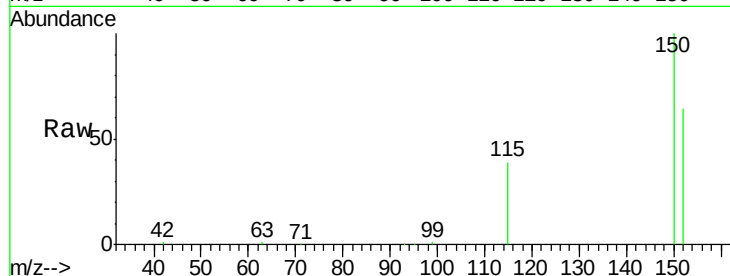


#2

1,4-Dioxane
Concen: 0.25 ng
RT: 3.37 min Scan# 45
Delta R.T. 0.01 min
Lab File: BE091522.D
Acq: 25 Mar 2016 13:28

Tgt Ion: 88 Resp: 1225
Ion Ratio Lower Upper
88 100
58 64.8 61.0 91.6
43 28.4 25.4 38.2

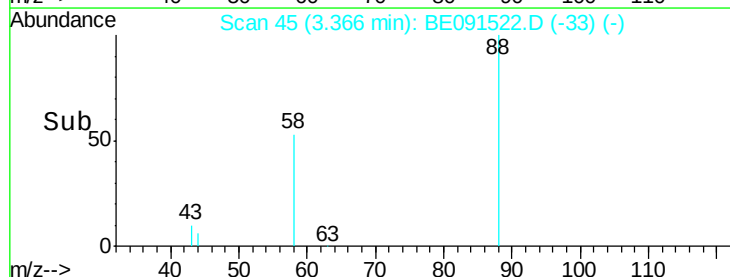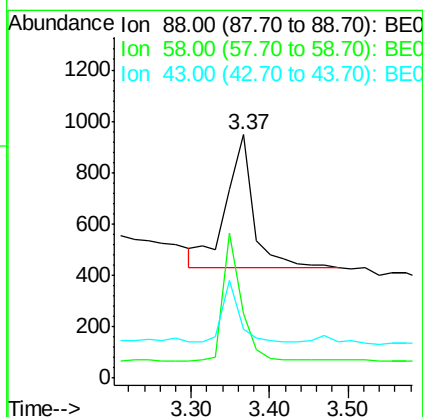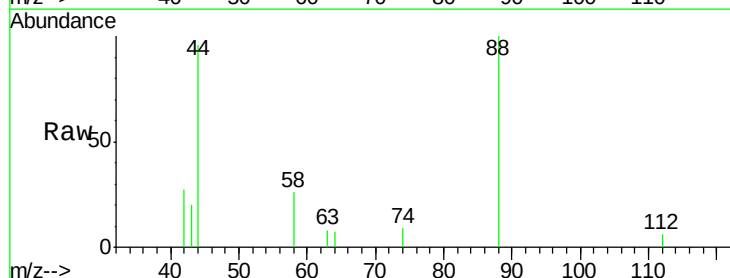

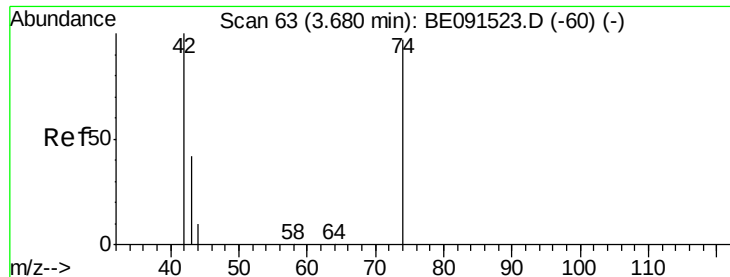

#3

n-Nitrosodimethylamine

Concen: 0.11 ng

RT: 3.68 min Scan# 63

Delta R.T. -0.00 min

Lab File: BE091522.D

Acq: 25 Mar 2016 13:28

Instrument :

BNA_E

ClientSampled :


Tot Ion: 42 Resp: 748

Ion Ratio Lower Upper




42 100

74 100.9 84.3 126.5

44 0.0 6.7 10.1#

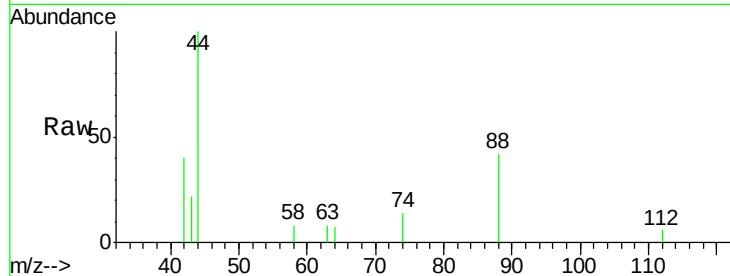

Abundance Ion 42.00 (41.70 to 42.70): BE0
Ion 74.00 (73.70 to 74.70): BE0
Ion 44.00 (43.70 to 44.70): BE0

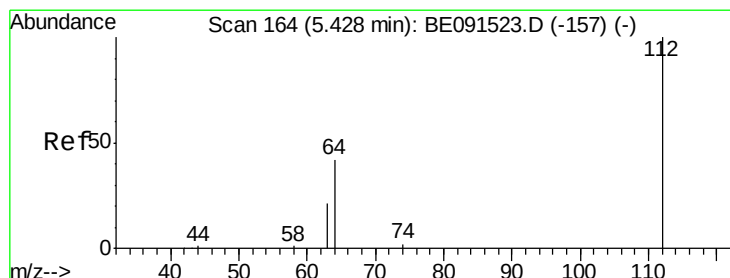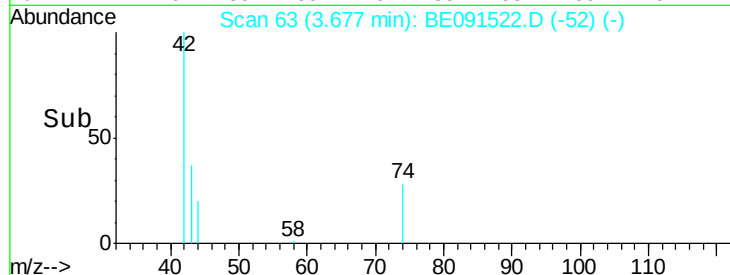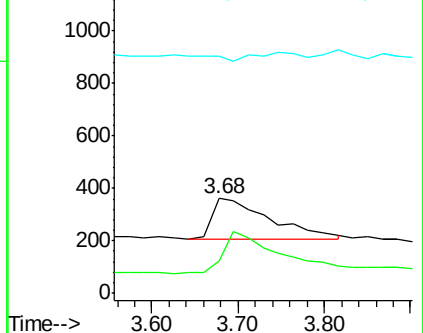

#4

2-Fluorophenol

Concen: 0.16 ng

RT: 5.42 min Scan# 164

Delta R.T. -0.00 min

Lab File: BE091522.D

Acq: 25 Mar 2016 13:28


Tgt Ion: 112 Resp: 1419

Ion Ratio Lower Upper



112 100


64 65.4 53.3 79.9

63 38.3 29.8 44.8

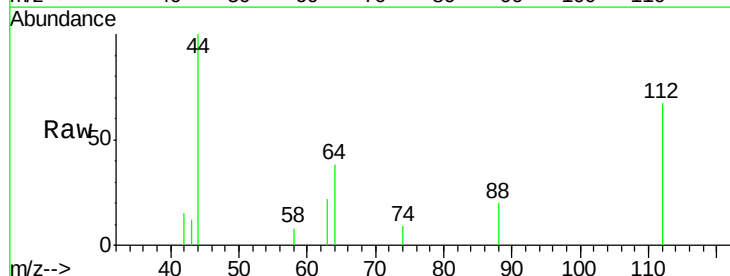

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BE0
Ion 63.00 (62.70 to 63.70): BE0

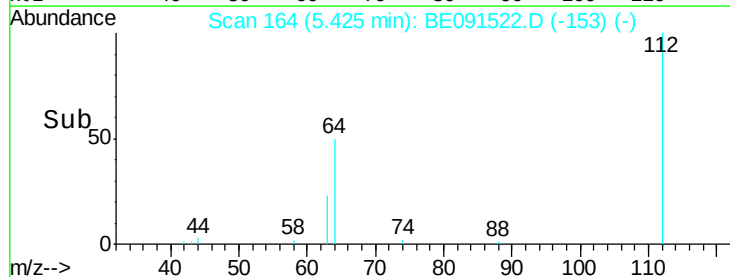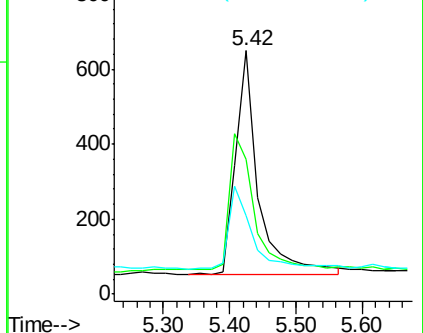



#5

Phenol-d6

Concen: 0.16 ng

RT: 6.99 min Scan# 253

Delta R.T. -0.00 min

Lab File: BE091522.D

Acq: 25 Mar 2016 13:28

Instrument :

BNA_E

ClientSampled :





Tot Ion: 99 Resp: 1869

Ion Ratio Lower Upper

99 100

42 28.0 20.6 30.8

71 36.1 29.0 43.4

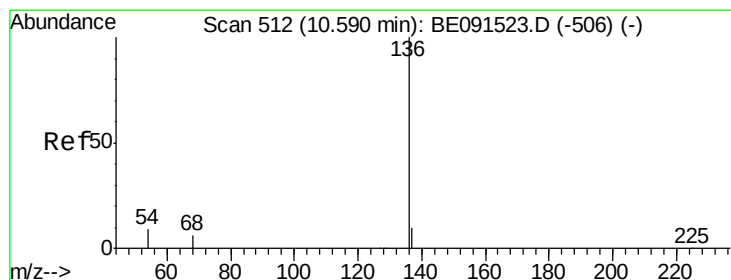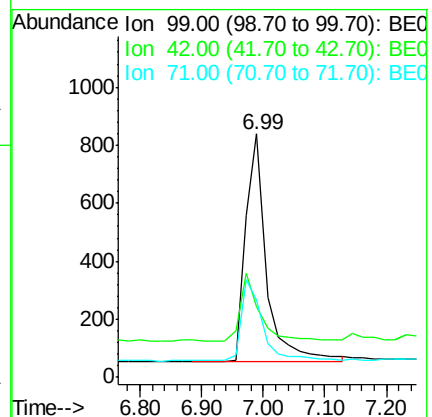

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.59 min Scan# 512

Delta R.T. 0.00 min

Lab File: BE091522.D

Acq: 25 Mar 2016 13:28

Tgt Ion: 136 Resp: 185198




Ion Ratio Lower Upper


136 100

137 10.4 8.8 13.2

54 8.7 5.2 7.8#

68 6.2 4.1 6.1#

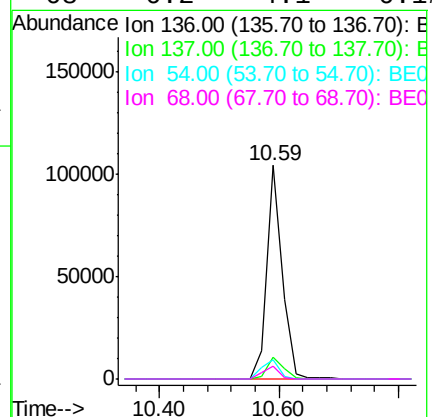



#7

Nitrobenzene-d5

Concen: 0.17 ng

RT: 8.97 min Scan# 393

Delta R.T. 0.00 min

Lab File: BE091522.D

Acq: 25 Mar 2016 13:28

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 82 Resp: 1369

Ion Ratio Lower Upper

82 100

128 31.3 23.5 35.3


54 69.1 52.4 78.6

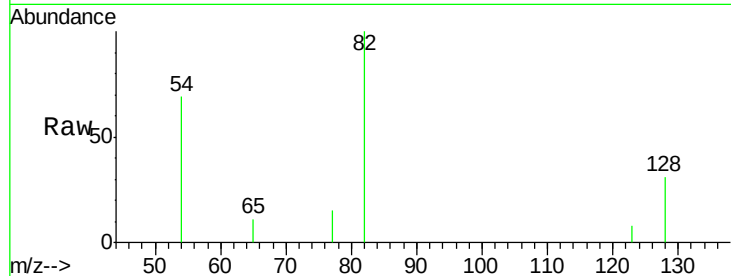



Abundance Ion 82.00 (81.70 to 82.70): BE091523.D (-390) (-)

Ion 128.00 (127.70 to 128.70): BE091523.D (-390) (-)

Ion 54.00 (53.70 to 54.70): BE091523.D (-390) (-)

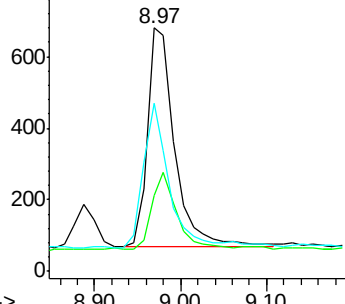

Time-->



#8

Naphthalene

Concen: 0.16 ng

RT: 10.65 min Scan# 515

Delta R.T. 0.00 min

Lab File: BE091522.D

Acq: 25 Mar 2016 13:28


Tgt Ion: 128 Resp: 7404

Ion Ratio Lower Upper

128 100

129 13.2 8.2 12.2#


127 12.6 11.8 17.8




Abundance Ion 128.00 (127.70 to 128.70): BE091523.D (-508) (-)


Ion 129.00 (128.70 to 129.70): BE091523.D (-508) (-)

Ion 127.00 (126.70 to 127.70): BE091523.D (-508) (-)

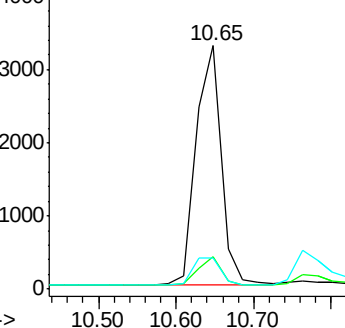

Time-->



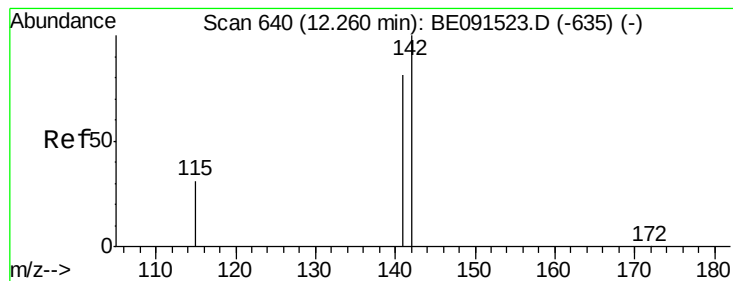

#9

2-Methylnaphthalene

Concen: 0.15 ng

RT: 12.26 min Scan# 640

Delta R.T. -0.00 min

Lab File: BE091522.D

Acq: 25 Mar 2016 13:28

Instrument :

BNA_E

ClientSampleId :


Tot Ion:142 Resp: 4326

Ion Ratio Lower Upper

142 100

141 83.4 66.9 100.3




115 33.9 25.1 37.7

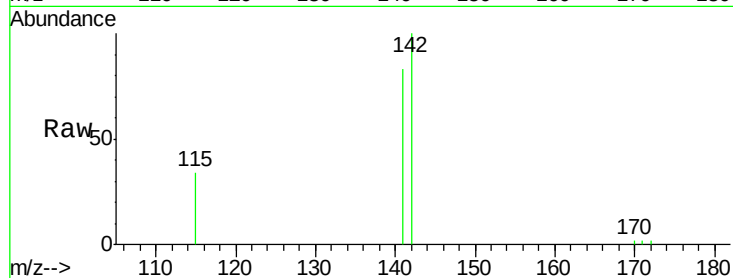

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E

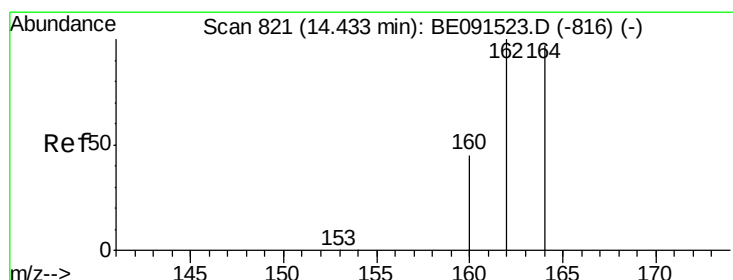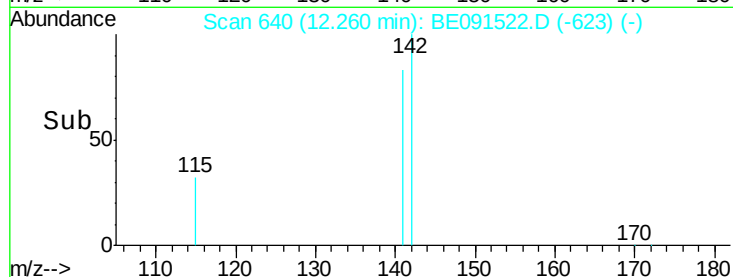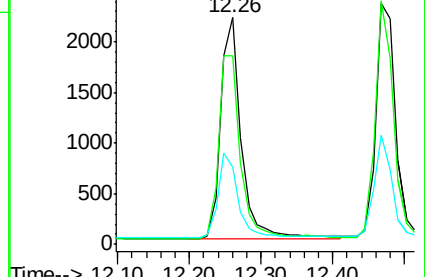

#10

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.43 min Scan# 821

Delta R.T. -0.00 min

Lab File: BE091522.D

Acq: 25 Mar 2016 13:28


Tgt Ion:164 Resp: 105509

Ion Ratio Lower Upper

164 100

162 103.2 84.4 126.6



160 46.3 37.7 56.5

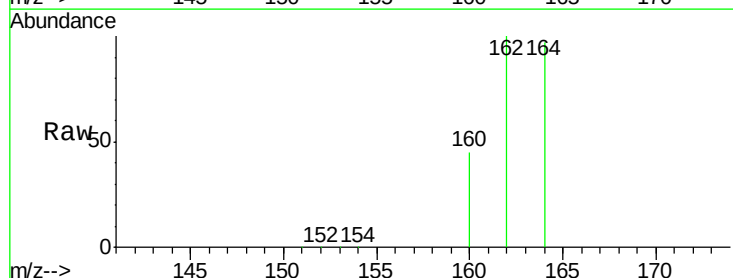


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

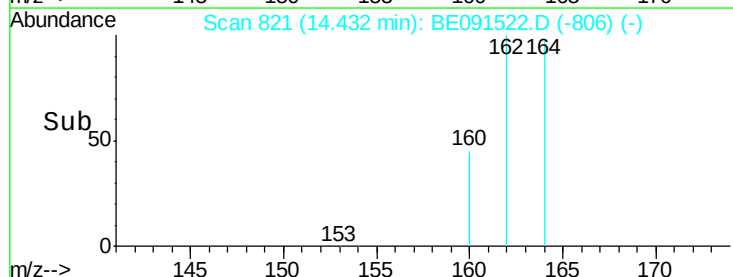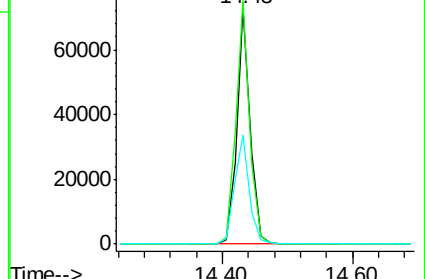


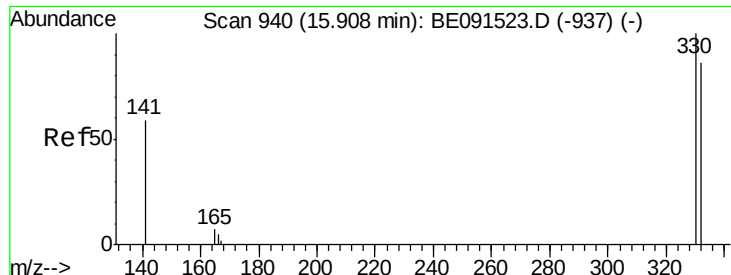




#11
 2,4,6-Tribromophenol
 Concen: 0.27 ng
 RT: 15.91 min Scan# 940
 Delta R.T. 0.00 min
 Lab File: BE091522.D
 Acq: 25 Mar 2016 13:28

Instrument :
 BNA_E
 ClientSampled :

Tot Ion:330 Resp: 824
 Ion Ratio Lower Upper
 330 100
 332 90.5 79.2 118.8
 141 19.8 28.1 42.1#

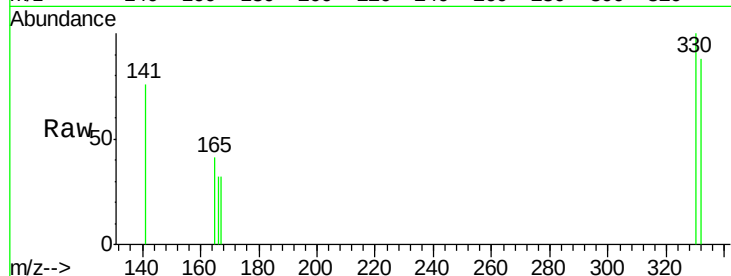


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

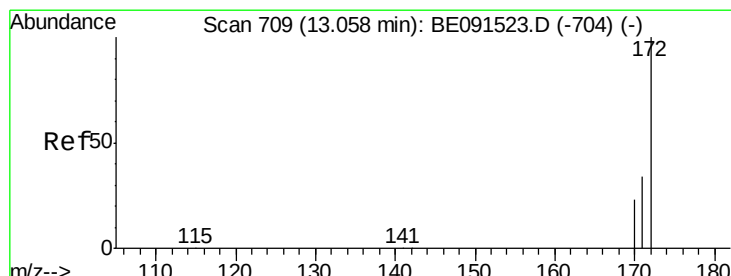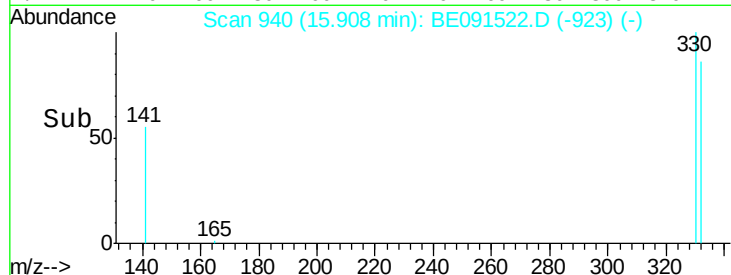
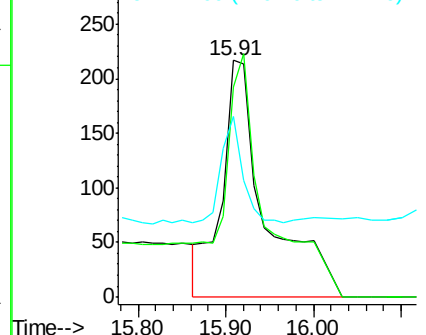



#12
 2-Fluorobiphenyl
 Concen: 0.22 ng
 RT: 13.06 min Scan# 709
 Delta R.T. -0.00 min
 Lab File: BE091522.D
 Acq: 25 Mar 2016 13:28

Tgt Ion:172 Resp: 5838
 Ion Ratio Lower Upper
 172 100
 171 35.7 29.8 44.8
 170 25.0 21.4 32.2

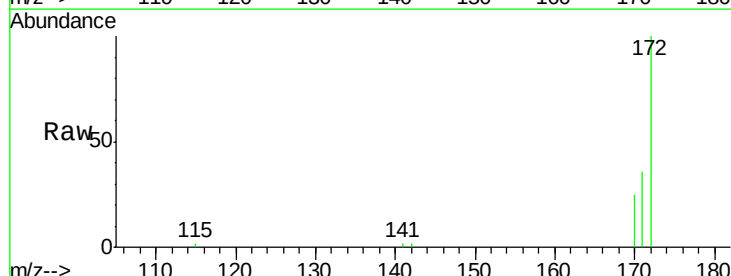

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

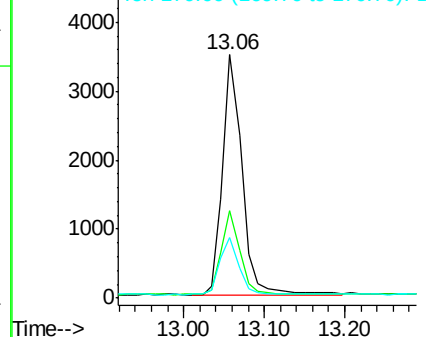

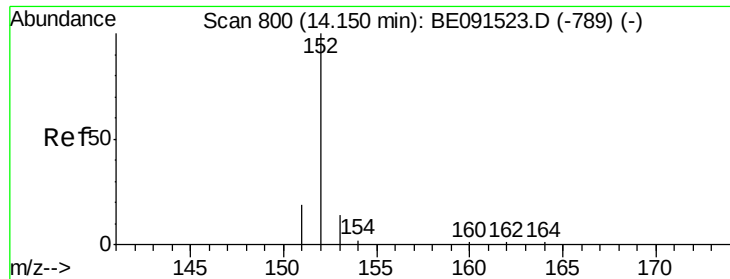

#13

Acenaphthylene

Concen: 0.16 ng

RT: 14.15 min Scan# 800

Delta R.T. -0.00 min

Lab File: BE091522.D

Acq: 25 Mar 2016 13:28

Instrument :

BNA_E

ClientSampleId :





Tot Ion:152 Resp: 7005

Ion Ratio Lower Upper

152 100

151 18.4 16.3 24.5

153 24.8 11.1 16.7#

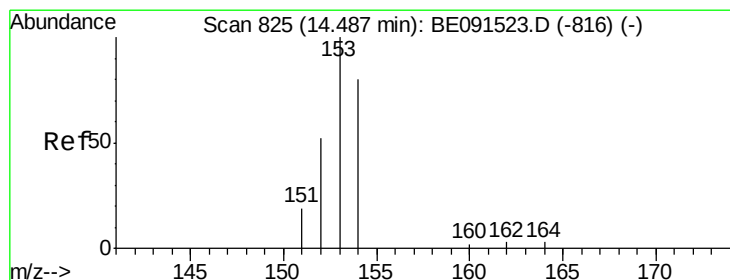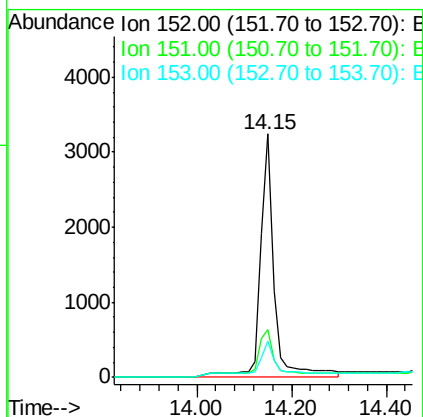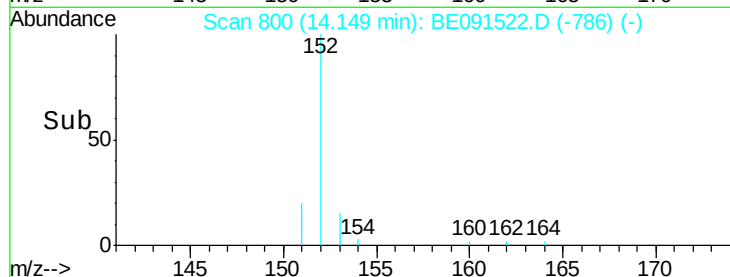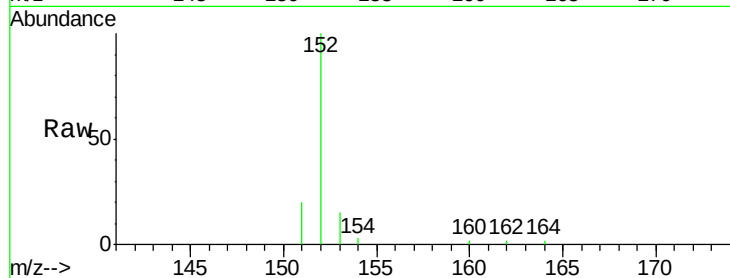

#14

Acenaphthene

Concen: 0.15 ng

RT: 14.49 min Scan# 825

Delta R.T. -0.00 min

Lab File: BE091522.D

Acq: 25 Mar 2016 13:28




Tgt Ion:154 Resp: 5033


Ion Ratio Lower Upper

154 100

153 116.9 87.3 130.9

152 57.8 42.9 64.3

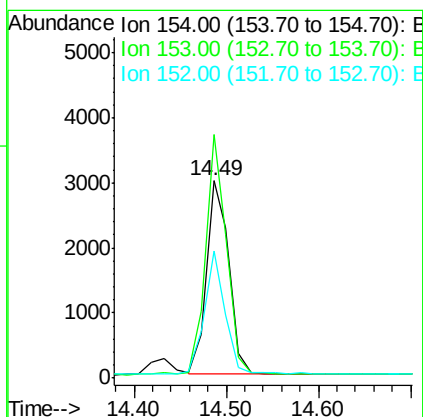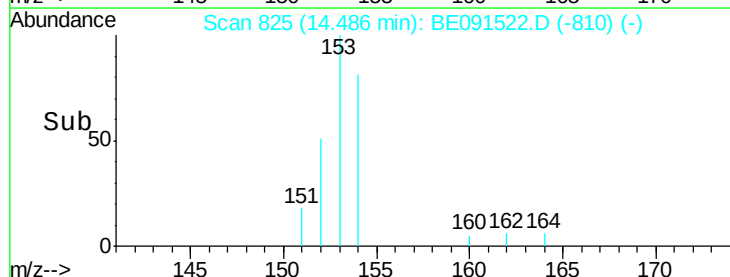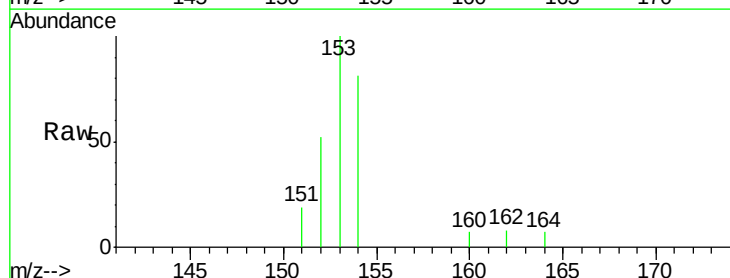



#15

Fluorene

Concen: 0.15 ng

RT: 15.47 min Scan# 902

Delta R.T. 0.00 min

Lab File: BE091522.D

Acq: 25 Mar 2016 13:28

Instrument :

BNA_E

ClientSampleId :


Tot Ion:166 Resp: 6030

Ion Ratio Lower Upper

166 100

165 100.2 79.2 118.8




167 13.5 10.8 16.2

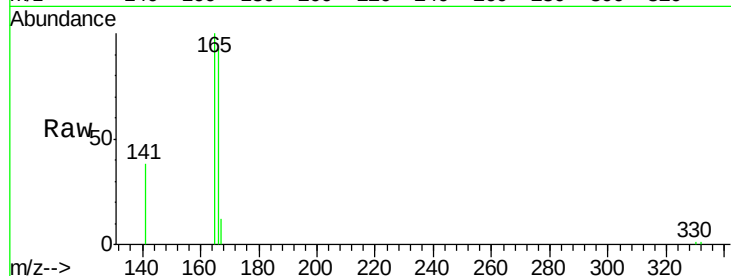

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

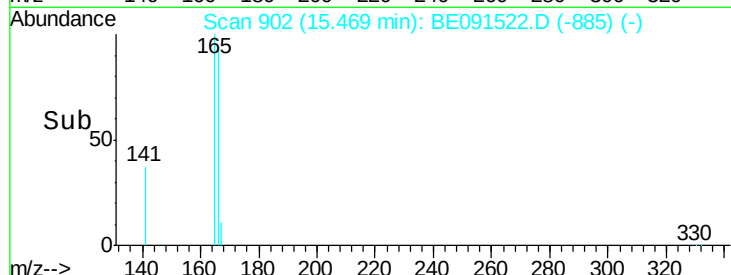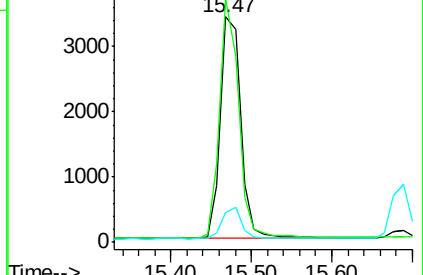

#16

Phenanthrene-d10

Concen: 5.00 ng

RT: 17.17 min Scan# 1018

Delta R.T. 0.00 min

Lab File: BE091522.D

Acq: 25 Mar 2016 13:28


Tgt Ion:188 Resp: 277654

Ion Ratio Lower Upper

188 100

94 5.2 5.4 8.2#



80 4.3 5.0 7.4#




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

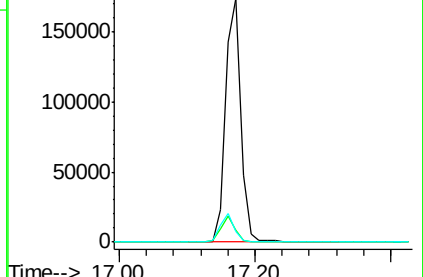







#17
Hexachlorobenzene
Concen: 0.15 ng
RT: 16.48 min Scan# 975
Delta R.T. 0.00 min
Lab File: BE091522.D
Acq: 25 Mar 2016 13:28

Instrument :
BNA_E
ClientSampleId :

Tot Ion:284 Resp: 1815
Ion Ratio Lower Upper
284 100
142 44.7 31.0 46.4
249 34.0 25.8 38.8

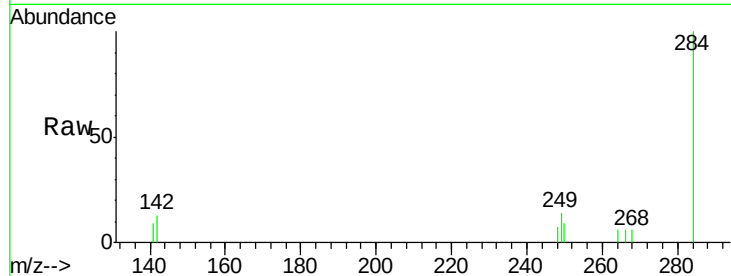


Abundance Ion 283.80 (283.50 to 284.50): E
Ion 142.00 (141.70 to 142.70): E
Ion 249.00 (248.70 to 249.70): E


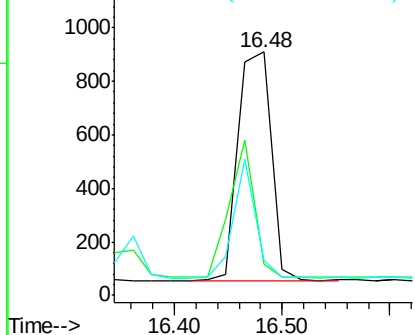



#18
Pentachlorophenol
Concen: 0.09 ng
RT: 16.81 min Scan# 994
Delta R.T. 0.00 min
Lab File: BE091522.D
Acq: 25 Mar 2016 13:28

Tgt Ion:266 Resp: 412
Ion Ratio Lower Upper
266 100
268 67.9 48.2 72.2
264 74.4 52.1 78.1



Abundance Ion 265.70 (265.40 to 266.40): E
Ion 268.00 (267.70 to 268.70): E
Ion 264.00 (263.70 to 264.70): E

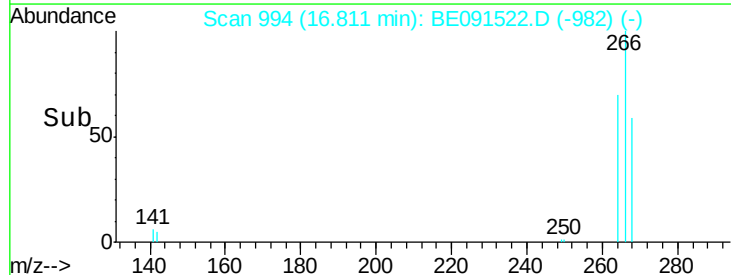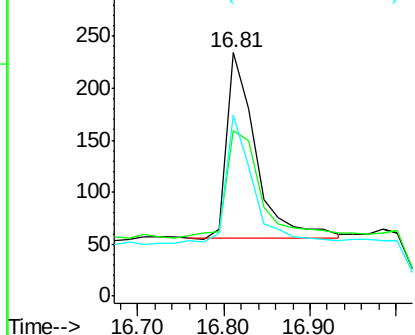



#19

Phenanthrene

Concen: 0.16 ng

RT: 17.21 min Scan# 1021

Delta R.T. 0.00 min

Lab File: BE091522.D

Acq: 25 Mar 2016 13:28

Instrument :

BNA_E

ClientSampleId :


Tot Ion:178 Resp: 12614

Ion Ratio Lower Upper

178 100

176 19.3 15.5 23.3




179 17.1 13.1 19.7



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

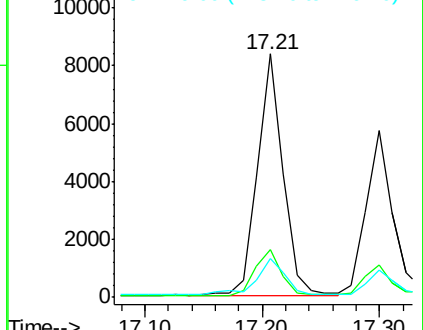

#20

Anthracene

Concen: 0.13 ng

RT: 17.30 min Scan# 1029

Delta R.T. 0.00 min

Lab File: BE091522.D

Acq: 25 Mar 2016 13:28


Tgt Ion:178 Resp: 9261

Ion Ratio Lower Upper

178 100

176 18.8 14.9 22.3



179 15.5 12.2 18.4




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

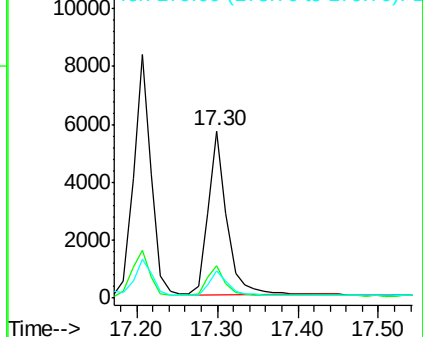



#21

Fluoranthene

Concen: 0.12 ng

RT: 19.22 min Scan# 1152

Delta R.T. -0.00 min

Lab File: BE091522.D

Acq: 25 Mar 2016 13:28

Instrument :

BNA_E

ClientSampleId :


Tot Ion:202 Resp: 10686

Ion Ratio Lower Upper

202 100

101 11.8 8.3 12.5




203 17.8 13.9 20.9



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

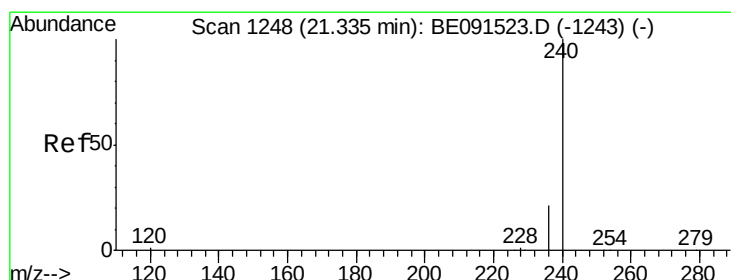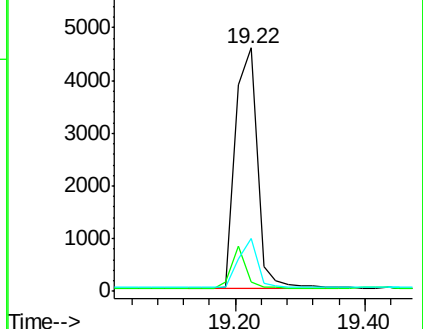

#22

Chrysene-d12

Concen: 5.00 ng

RT: 21.33 min Scan# 1249

Delta R.T. -0.00 min

Lab File: BE091522.D

Acq: 25 Mar 2016 13:28


Tgt Ion:240 Resp: 268288

Ion Ratio Lower Upper

240 100

120 1.0 4.0 6.0#



236 20.7 23.0 34.4#




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



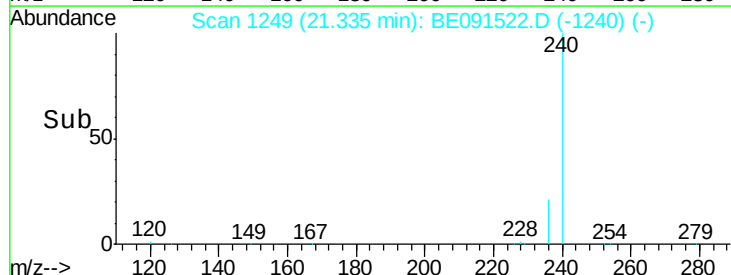
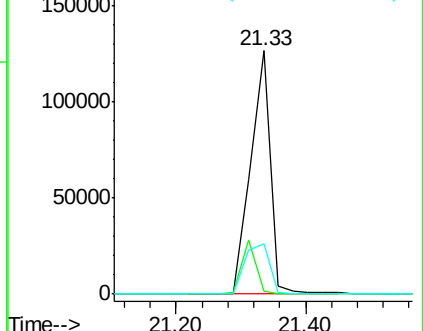




#23
Pvrene
Concen: 0.17 ng
RT: 19.57 min Scan# 1170
Delta R.T. -0.00 min
Lab File: BE091522.D
Acq: 25 Mar 2016 13:28




Instrument :
BNA_E
ClientSampleId :


Tot Ion:202 Resp: 11532
Ion Ratio Lower Upper
202 100
200 21.5 16.4 24.6
203 17.6 14.6 21.8

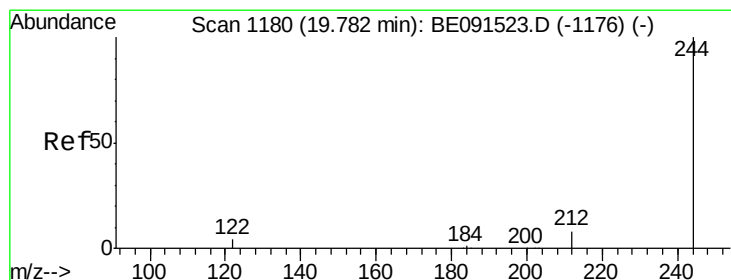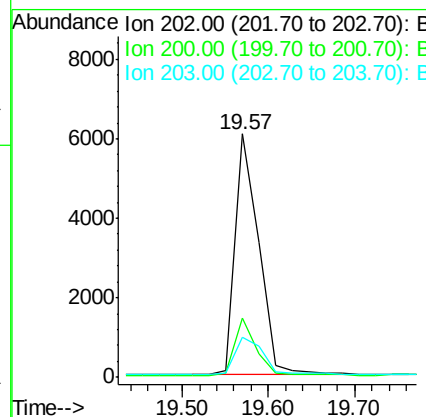

#24
Terphenyl-d14
Concen: 0.26 ng
RT: 19.78 min Scan# 1181
Delta R.T. -0.00 min
Lab File: BE091522.D
Acq: 25 Mar 2016 13:28

Tgt Ion:244 Resp: 8334
Ion Ratio Lower Upper
244 100
212 9.2 5.8 8.8#
122 5.5 1.8 2.8#



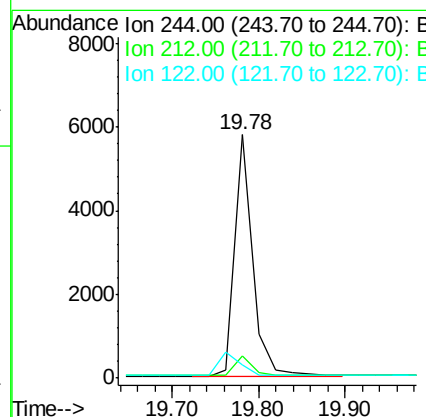
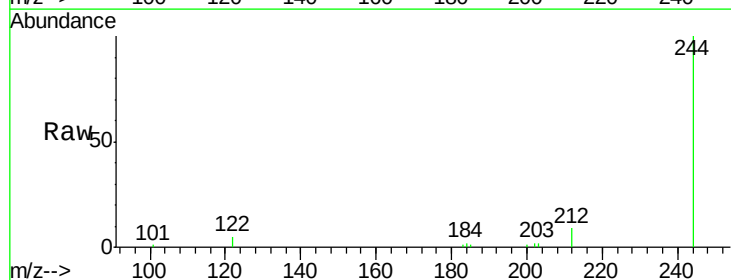


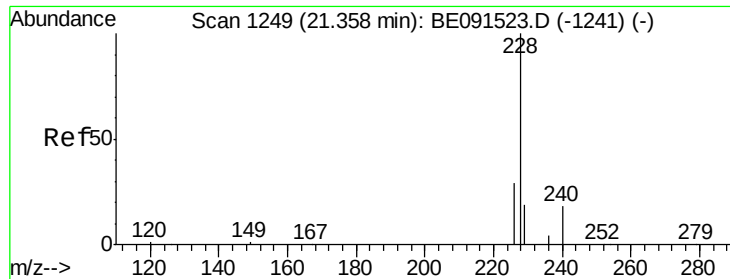

#25
Benzo(a)anthracene
Concen: 0.37 ng
RT: 21.36 min Scan# 1250
Delta R.T. 0.05 min
Lab File: BE091522.D
Acq: 25 Mar 2016 13:28




Instrument :
BNA_E
ClientSampleId :


Tot Ion:228 Resp: 27254
Ion Ratio Lower Upper
228 100
226 29.2 24.0 36.0
229 19.7 13.8 20.6

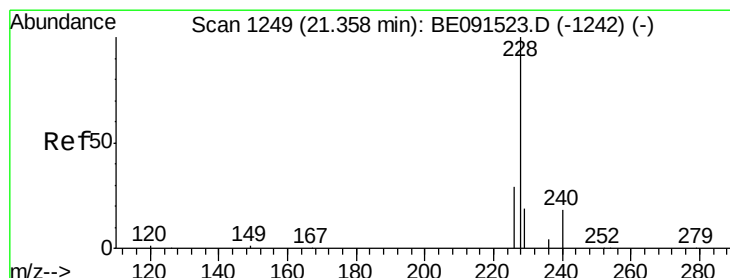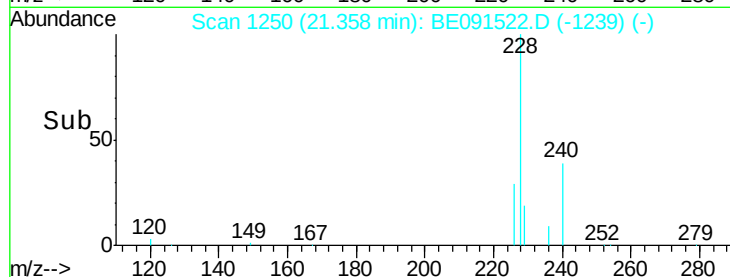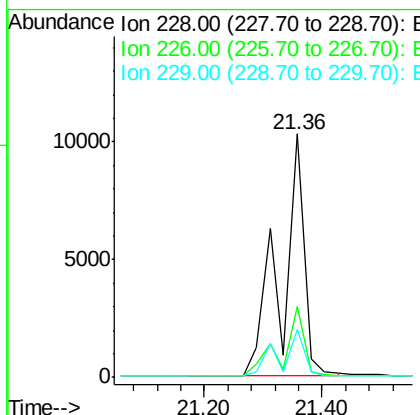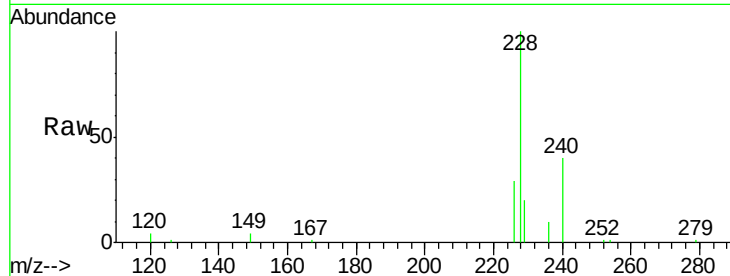

#26
Chrysene
Concen: 0.36 ng
RT: 21.36 min Scan# 1250
Delta R.T. -0.00 min
Lab File: BE091522.D
Acq: 25 Mar 2016 13:28

Tgt Ion:228 Resp: 27463
Ion Ratio Lower Upper
228 100
226 29.2 18.9 28.3#
229 19.7 19.1 28.7

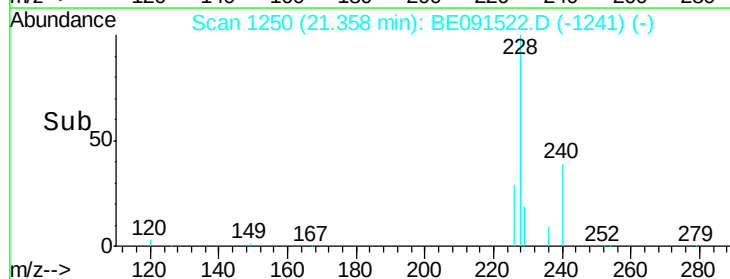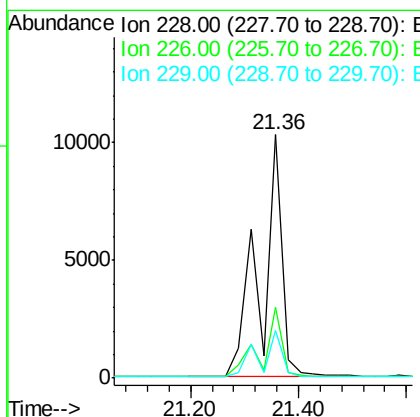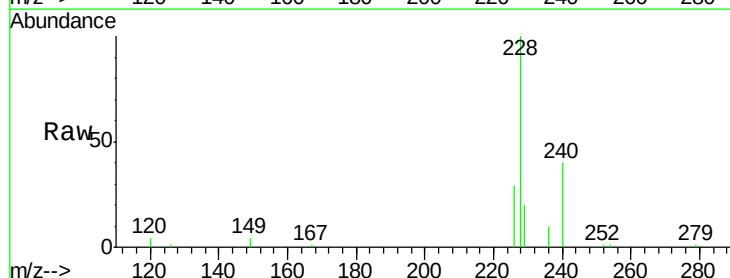







#27
 Indeno(1,2,3-cd)pyrene
 Concen: 0.15 ng
 RT: 26.35 min Scan# 1649
 Delta R.T. -0.00 min
 Lab File: BE091522.D
 Acq: 25 Mar 2016 13:28

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:276 Resp: 11480
 Ion Ratio Lower Upper
 276 100
 138 25.6 20.2 30.4
 277 24.7 19.8 29.8




Abundance Ion 276.00 (275.70 to 276.70): E
 Ion 138.00 (137.70 to 138.70): E
 Ion 277.00 (276.70 to 277.70): E

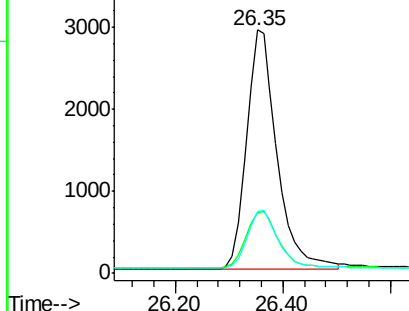




#28
 Perylene-d12
 Concen: 5.00 ng
 RT: 23.78 min Scan# 1429
 Delta R.T. -0.00 min
 Lab File: BE091522.D
 Acq: 25 Mar 2016 13:28

Tgt Ion:264 Resp: 287728
 Ion Ratio Lower Upper
 264 100
 260 25.1 20.1 30.1
 265 21.9 18.3 27.5



Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

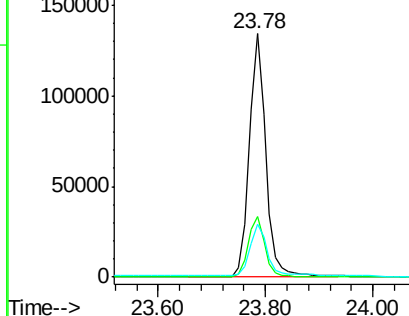



#29

Benzo(b)fluoranthene

Concen: 0.11 ng

RT: 23.08 min Scan# 1368

Delta R.T. 0.06 min

Lab File: BE091522.D

Acq: 25 Mar 2016 13:28

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 9823

Ion Ratio Lower Upper

252 100

253 24.7 18.7 28.1




125 14.0 9.8 14.6



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

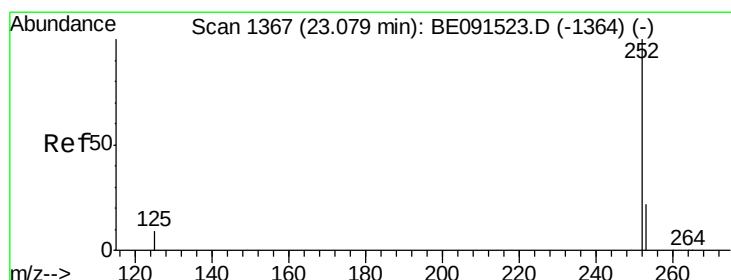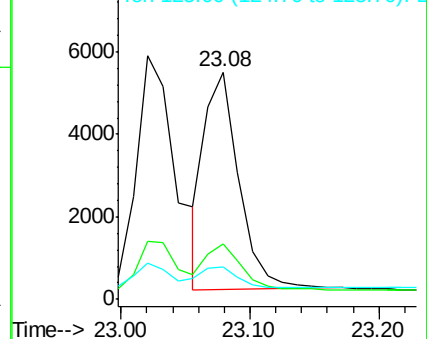

#30

Benzo(k)fluoranthene

Concen: 0.11 ng

RT: 23.08 min Scan# 1368

Delta R.T. -0.00 min

Lab File: BE091522.D

Acq: 25 Mar 2016 13:28


Tgt Ion:252 Resp: 10200

Ion Ratio Lower Upper

252 100

253 24.7 20.2 30.4



125 14.0 9.4 14.2

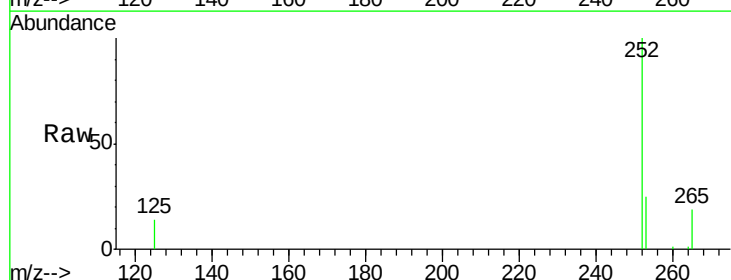


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

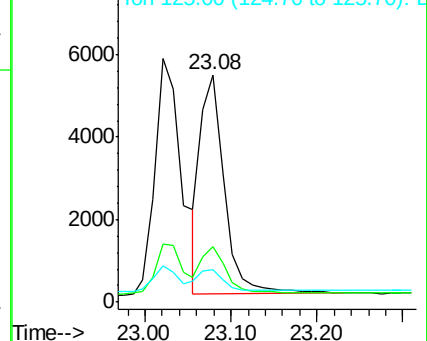



#31

Benzo(a)pyrene

Concen: 0.11 ng

RT: 23.67 min Scan# 1419

Delta R.T. -0.00 min

Lab File: BE091522.D

Acq: 25 Mar 2016 13:28

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 8894

Ion Ratio Lower Upper

252 100

253 25.4 19.4 29.0




125 17.3 11.4 17.2#

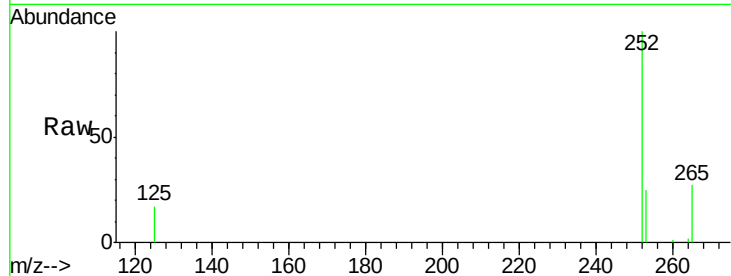

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

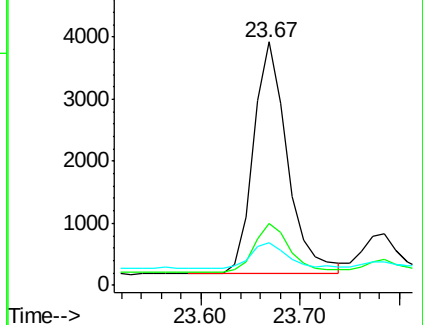

#32

Dibenzo(a,h)anthracene

Concen: 0.12 ng

RT: 26.39 min Scan# 1652

Delta R.T. -0.00 min

Lab File: BE091522.D

Acq: 25 Mar 2016 13:28


Tgt Ion:278 Resp: 9673

Ion Ratio Lower Upper

278 100

139 18.6 14.2 21.4



279 26.3 19.6 29.4




Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

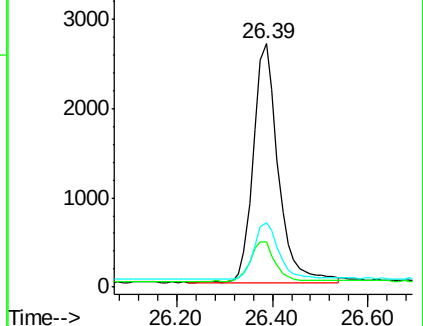

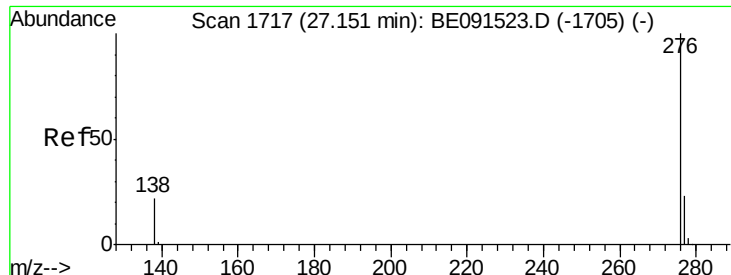

#33

Benzo(a,h,i)perylene

Concen: 0.13 ng

RT: 27.15 min Scan# 1718

Delta R.T. -0.00 min


Lab File: BE091522.D

Acq: 25 Mar 2016 13:28

Instrument :

BNA_E

ClientSampleId :



Tot Ion: 276 Resp: 10732

Ion Ratio Lower Upper

276 100

277 25.0 19.4 29.2

138 24.1 18.2 27.4

Abundance Ion 276.00 (275.70 to 276.70): E
Ion 277.00 (276.70 to 277.70): E
Ion 138.00 (137.70 to 138.70): E

