



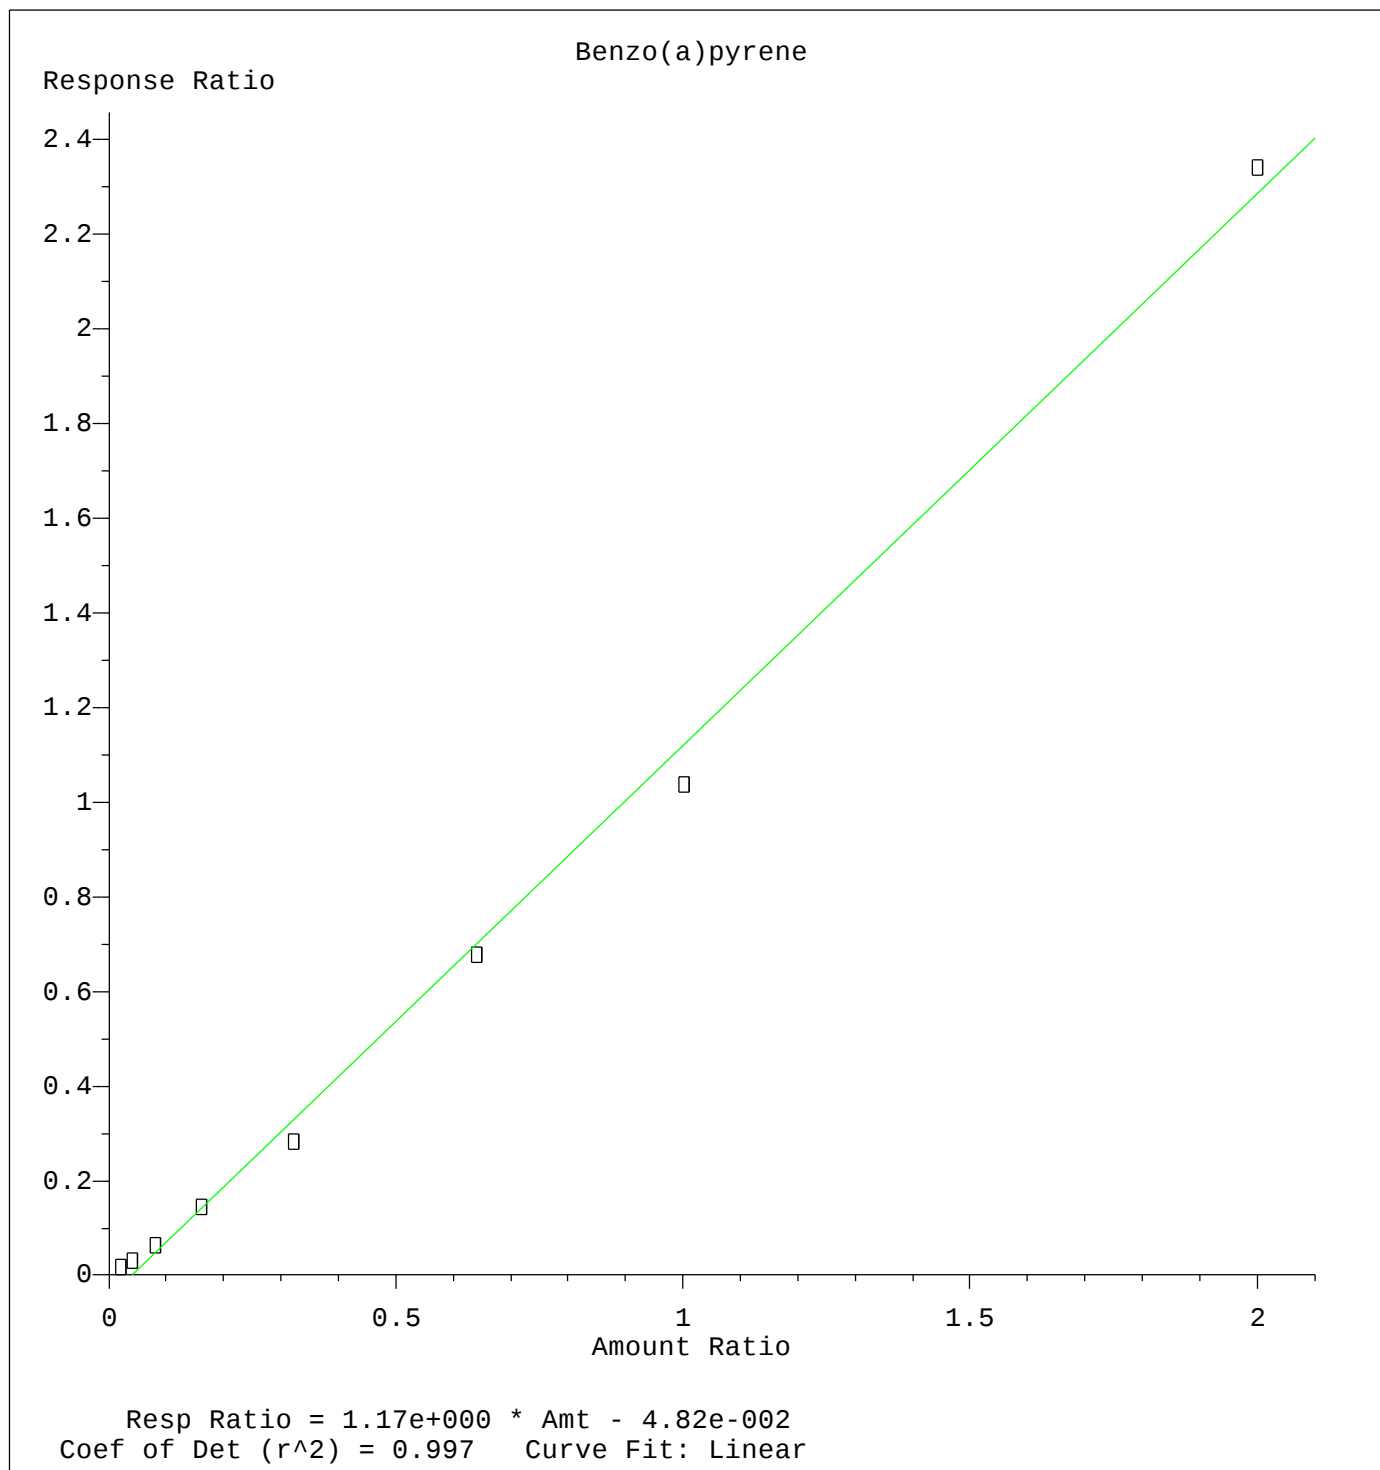

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032516.M
Calibration Table Last Updated: Fri Mar 25 19:00:32 2016


1,4-Dioxane

Response Ratio

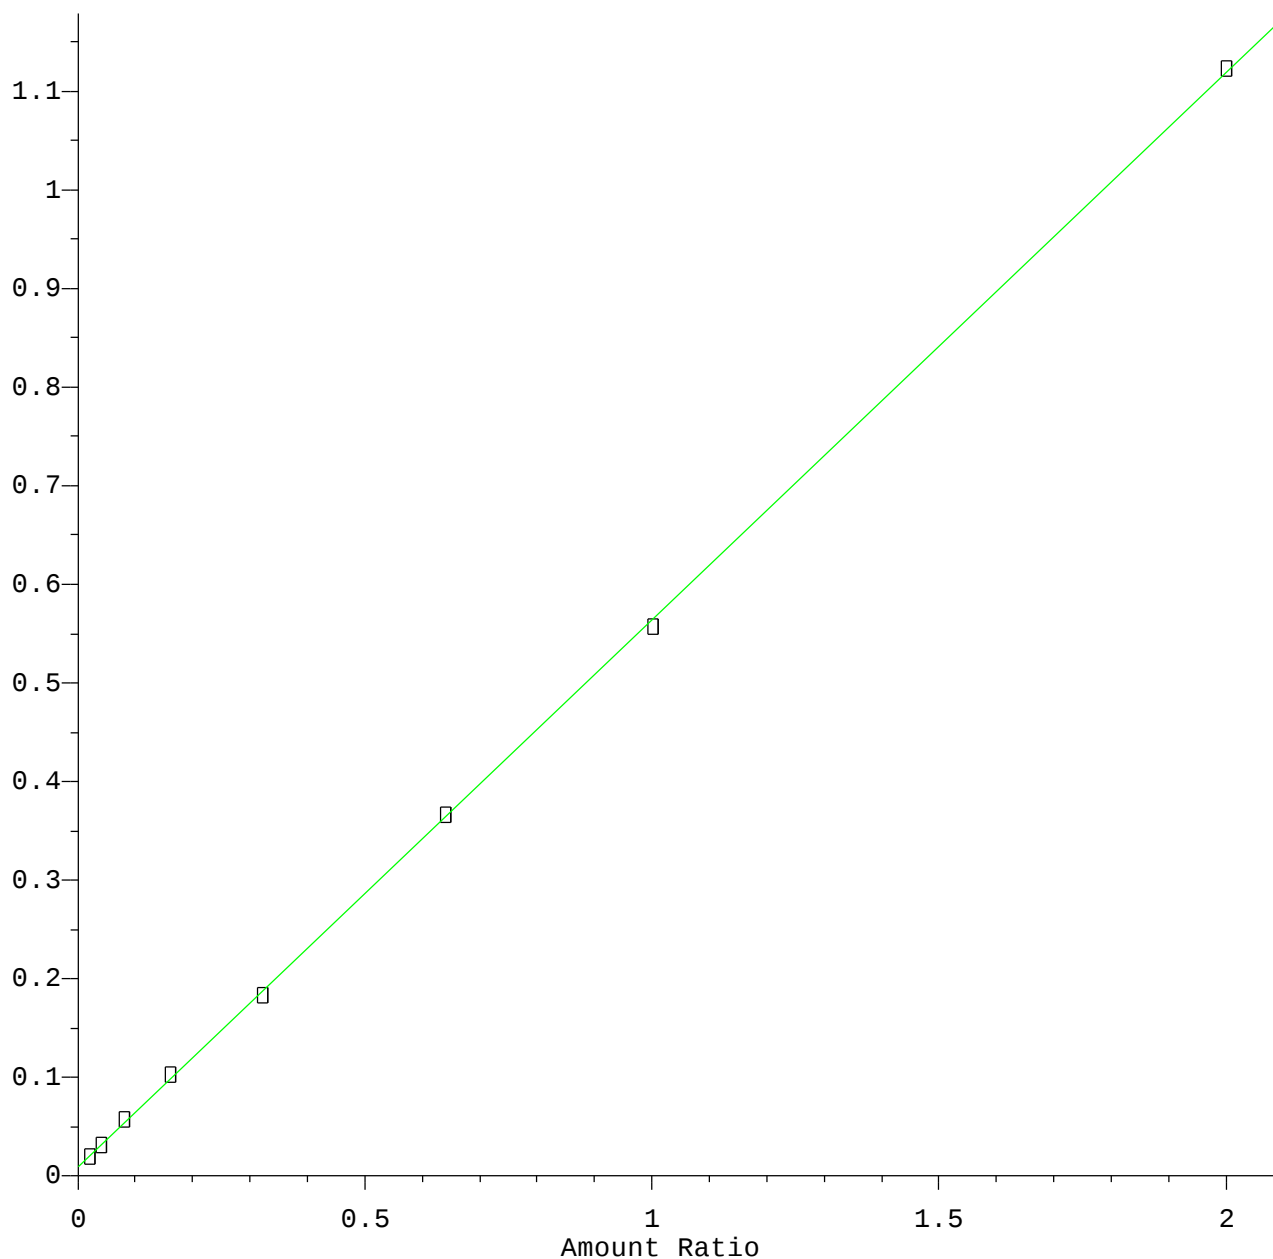


Resp Ratio = $5.55 \times 10^{-1} \times \text{Amt} + 9.04 \times 10^{-3}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032516.M
Calibration Table Last Updated: Fri Mar 25 19:00:32 2016

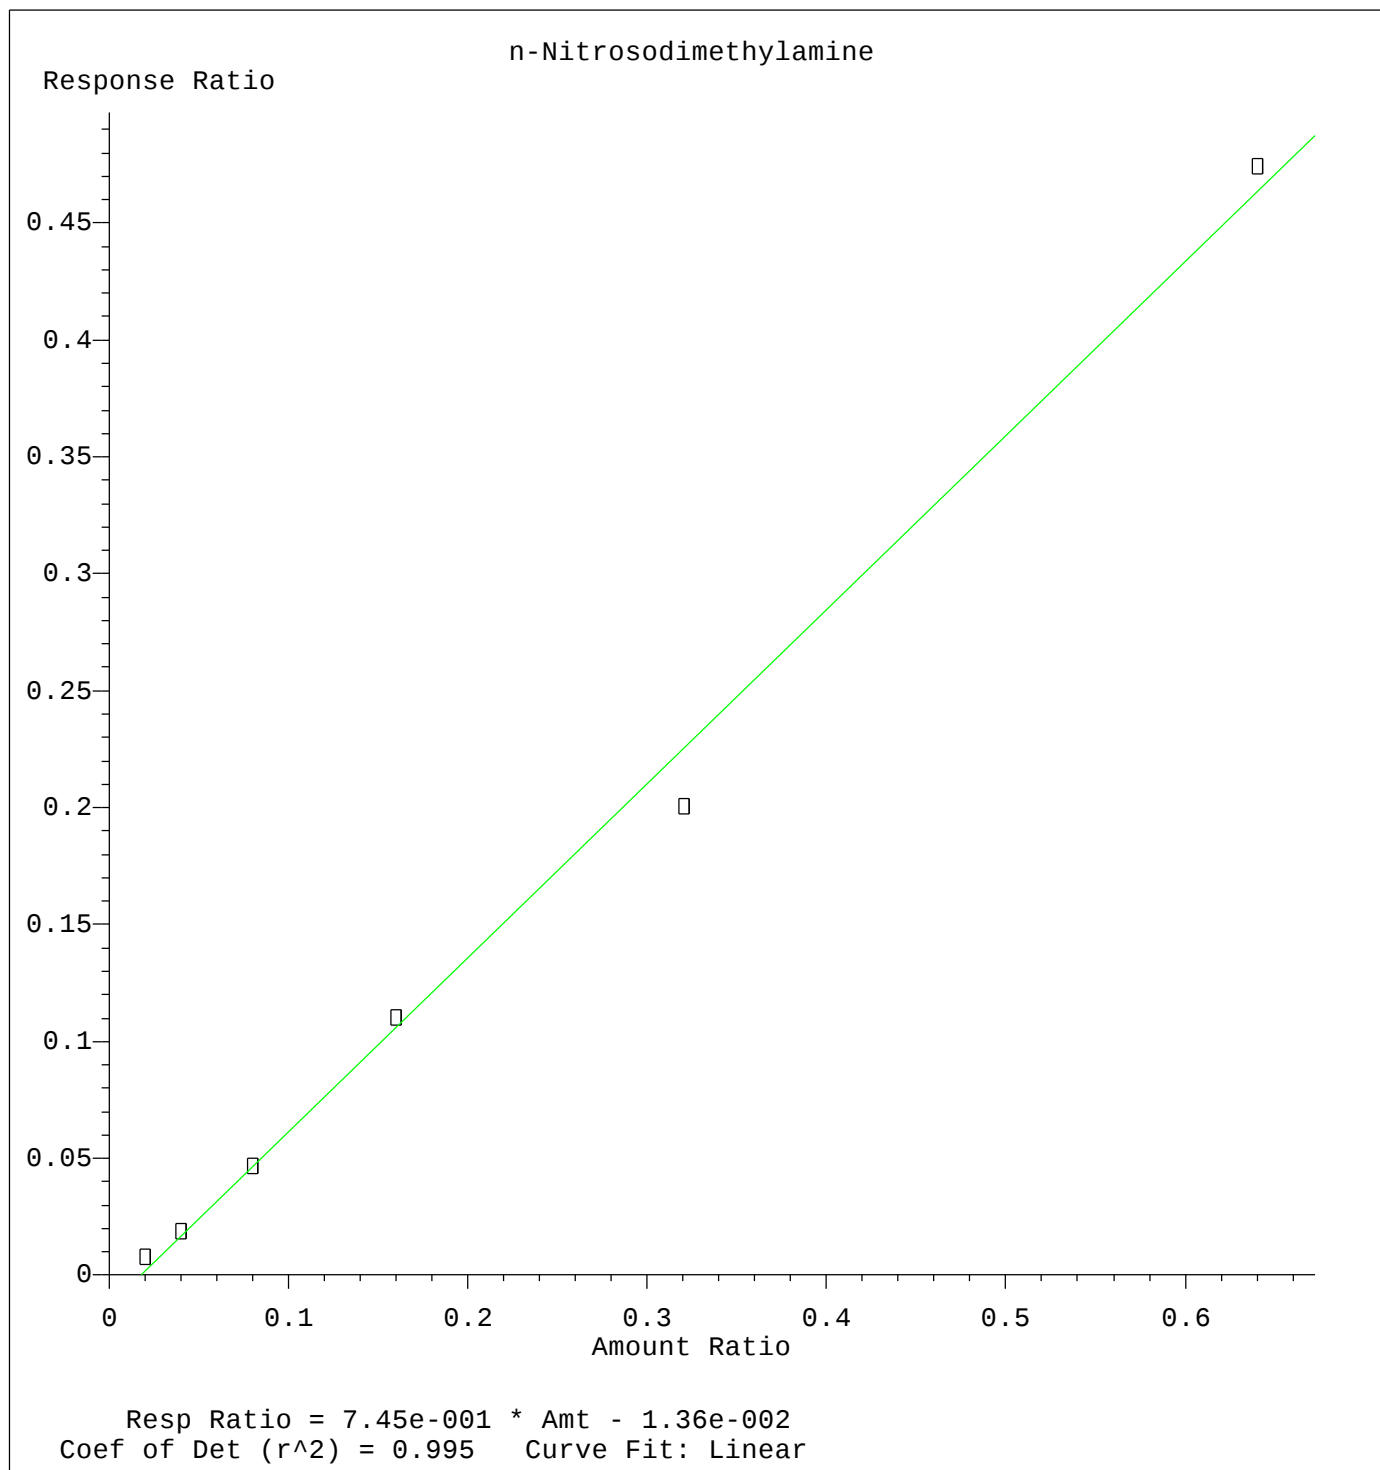

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032516.M
Calibration Table Last Updated: Fri Mar 25 19:00:32 2016

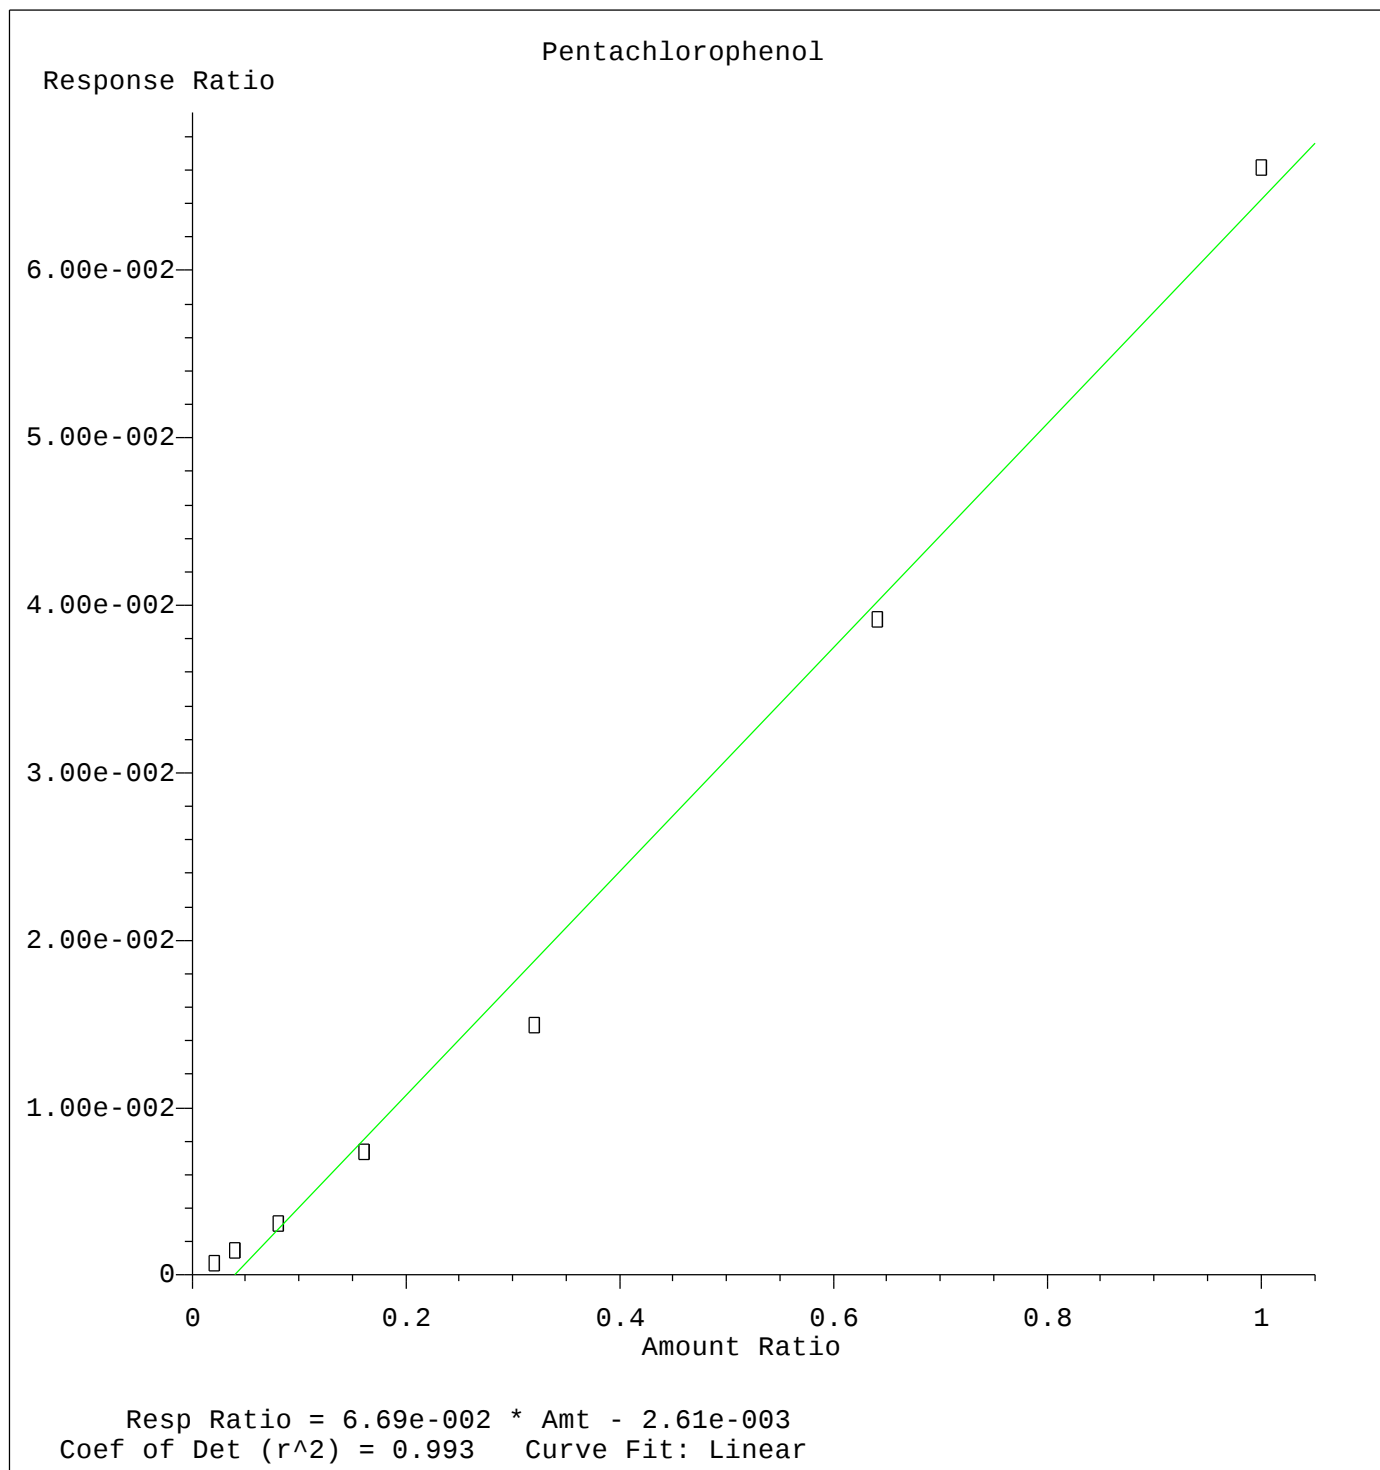

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032516.M
Calibration Table Last Updated: Fri Mar 25 19:00:32 2016