

Data Path : Z:\HPCHEM1\BNA E\DATA\BE032516\
 Data File : BE091526.D
 Acq On : 25 Mar 2016 15:57
 Operator : UM/SJ
 Sample : SSTDICC3.2
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2

Quant Time: Mar 25 17:28:21 2016
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 25 15:19:17 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	38106	5.00	ng	0.00
6) Naphthalene-d8	10.59	136	189463	5.00	ng	0.00
10) Acenaphthene-d10	14.43	164	113213	5.00	ng	-0.01
16) Phenanthrene-d10	17.17	188	272673	5.00	ng	0.00
22) Chrysene-d12	21.34	240	285609	5.00	ng	0.00
28) Perylene-d12	23.78	264	284756	5.00	ng	-0.01

System Monitoring Compounds						
4) 2-Fluorophenol	5.41	112	24971	2.85	ng	-0.02
5) Phenol-d6	6.97	99	34891	3.05	ng	-0.02
7) Nitrobenzene-d5	8.97	82	28004	3.30	ng	-0.01
11) 2,4,6-Tribromophenol	15.91	330	7694m	2.39	ng	-0.01
12) 2-Fluorobiphenyl	13.06	172	105052	3.69	ng	-0.01
24) Terphenyl-d14	19.78	244	158153	4.60	ng	0.00


Target Compounds						Qvalue
2) 1,4-Dioxane	3.35	88	13924	2.93	ng	# 85
3) n-Nitrosodimethylamine	3.66	42	18062	2.67	ng	95
8) Naphthalene	10.65	128	122683	2.65	ng	# 93
9) 2-Methylnaphthalene	12.25	142	80704	2.71	ng	# 87
13) Acenaphthylene	14.15	152	142247	2.94	ng	99
14) Acenaphthene	14.49	154	91841	2.63	ng	98
15) Fluorene	15.47	166	115529	2.62	ng	100
17) Hexachlorobenzene	16.48	284	31682	2.67	ng	94
18) Pentachlorophenol	16.81	266	10674	2.26	ng	99
19) Phenanthrene	17.21	178	203952	2.62	ng	99
20) Anthracene	17.30	178	182488	2.67	ng	99
21) Fluoranthene	19.21	202	204877	2.29	ng	99
23) Pvrene	19.57	202	237095	3.34	ng	97
25) Benzo(a)anthracene	21.31	228	224056	2.85	ng	# 85
26) Chrysene	21.36	228	269657m	3.36	ng	
27) Indeno(1,2,3-cd)pyrene	26.35	276	235735	2.88	ng	99
29) Benzo(b)fluoranthene	23.02	252	212530	2.36	ng	95
30) Benzo(k)fluoranthene	23.08	252	235551	2.56	ng	95
31) Benzo(a)pvrene	23.67	252	192675	2.43	ng	# 94
32) Dibenzo(a,h)anthracene	26.39	278	202134	2.59	ng	98
33) Benzo(g,h,i)perylene	27.15	276	202983	2.50	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE032516\
Data File : BE091526.D
Acq On : 25 Mar 2016 15:57
Operator : UM/SJ
Sample : SSTDICC3.2
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2

Quant Time: Mar 25 17:28:21 2016
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 25 15:19:17 2016
Response via : Initial Calibration



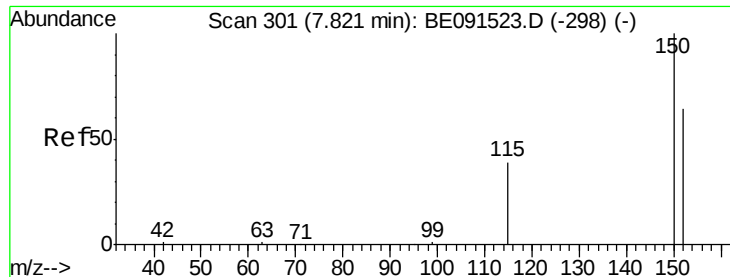


#1




1,4-Dichlorobenzene-d4
Concen: 5.00 ng
RT: 7.82 min Scan# 301
Delta R.T. 0.00 min
Lab File: BE091526.D
Acq: 25 Mar 2016 15:57

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2

Tot Ion:152 Resp: 38106
Ion Ratio Lower Upper
152 100
150 158.3 122.2 183.2
115 63.6 45.9 68.9




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E





#2


1,4-Dioxane
Concen: 2.93 ng
RT: 3.35 min Scan# 44
Delta R.T. -0.02 min
Lab File: BE091526.D
Acq: 25 Mar 2016 15:57

Tgt Ion: 88 Resp: 13924
Ion Ratio Lower Upper
88 100
58 90.1 61.0 91.6
43 38.2 25.4 38.2#



Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0



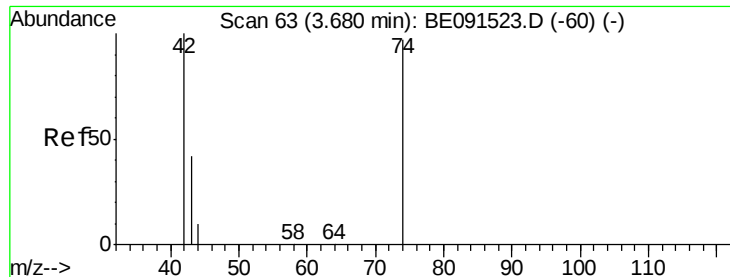


#3




n-Nitrosodimethylamine
 Concen: 2.67 ng
 RT: 3.66 min Scan# 62
 Delta R.T. -0.02 min
 Lab File: BE091526.D
 Acq: 25 Mar 2016 15:57

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2

Tot Ion: 42 Resp: 18062
 Ion Ratio Lower Upper
 42 100
 74 99.9 84.3 126.5
 44 8.3 6.7 10.1




Abundance Ion 42.00 (41.70 to 42.70): BE0
 Ion 74.00 (73.70 to 74.70): BE0
 Ion 44.00 (43.70 to 44.70): BE0





#4


2-Fluorophenol
 Concen: 2.85 ng
 RT: 5.41 min Scan# 163
 Delta R.T. -0.02 min
 Lab File: BE091526.D
 Acq: 25 Mar 2016 15:57

Tgt Ion: 112 Resp: 24971
 Ion Ratio Lower Upper
 112 100
 64 67.7 53.3 79.9
 63 37.5 29.8 44.8



Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BE0
 Ion 63.00 (62.70 to 63.70): BE0





#5

Phenol-d6

Concen: 3.05 ng

RT: 6.97 min Scan# 252

Delta R.T. -0.02 min

Lab File: BE091526.D

Acq: 25 Mar 2016 15:57

Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2


Tot Ion: 99 Resp: 34891

Ion Ratio Lower Upper

99 100

42 28.4 20.6 30.8




71 37.3 29.0 43.4



Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0



#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.59 min Scan# 512

Delta R.T. -0.00 min

Lab File: BE091526.D

Acq: 25 Mar 2016 15:57

Tgt Ion: 136 Resp: 189463


Ion Ratio Lower Upper

136 100

137 10.5 8.8 13.2

54 7.9 5.2 7.8#

68 5.6 4.1 6.1






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0





#7

Nitrobenzene-d5

Concen: 3.30 ng

RT: 8.97 min Scan# 393

Delta R.T. -0.01 min

Lab File: BE091526.D

Acq: 25 Mar 2016 15:57

Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2


Tot Ion: 82 Resp: 28004

Ion Ratio Lower Upper

82 100

128 33.6 23.5 35.3

54 50.6 52.4 78.6#





Abundance Ion 82.00 (81.70 to 82.70): BE091526.D (-377) (-)

Ion 128.00 (127.70 to 128.70): BE091526.D (-377) (-)

Ion 54.00 (53.70 to 54.70): BE091526.D (-377) (-)

Time-->



#8

Naphthalene

Concen: 2.65 ng

RT: 10.65 min Scan# 515

Delta R.T. -0.00 min

Lab File: BE091526.D

Acq: 25 Mar 2016 15:57


Tgt Ion: 128 Resp: 122683

Ion Ratio Lower Upper

128 100

129 12.1 8.2 12.2

127 11.2 11.8 17.8#





Abundance Ion 128.00 (127.70 to 128.70): BE091526.D (-505) (-)

Ion 129.00 (128.70 to 129.70): BE091526.D (-505) (-)

Ion 127.00 (126.70 to 127.70): BE091526.D (-505) (-)

Time-->



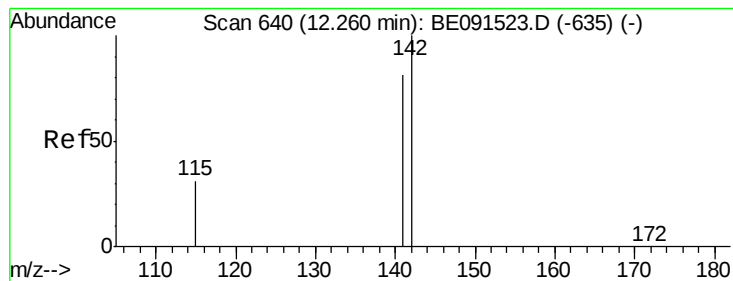

#9

2-Methylnaphthalene

Concen: 2.71 ng

RT: 12.25 min Scan# 639

Delta R.T. -0.01 min

Lab File: BE091526.D

Acq: 25 Mar 2016 15:57

Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2


Tot Ion:142 Resp: 80704

Ion Ratio Lower Upper

142 100

141 94.5 66.9 100.3




115 40.1 25.1 37.7#



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E



#10

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.43 min Scan# 821

Delta R.T. -0.01 min

Lab File: BE091526.D

Acq: 25 Mar 2016 15:57


Tgt Ion:164 Resp: 113213

Ion Ratio Lower Upper

164 100

162 102.8 84.4 126.6



160 45.7 37.7 56.5




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E









#11
 2,4,6-Tribromophenol
 Concen: 2.39 ng/mL
 RT: 15.91 min Scan# 940
 Delta R.T. -0.01 min
 Lab File: BE091526.D
 Acq: 25 Mar 2016 15:57




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2


Tot Ion: 330 Resp: 7694
 Ion Ratio Lower Upper
 330 100
 332 119.9 79.2 118.8#
 141 50.3 28.1 42.1#



#12
 2-Fluorobiphenyl
 Concen: 3.69 ng/mL
 RT: 13.06 min Scan# 709
 Delta R.T. -0.01 min
 Lab File: BE091526.D
 Acq: 25 Mar 2016 15:57

Tgt Ion: 172 Resp: 105052
 Ion Ratio Lower Upper
 172 100
 171 33.5 29.8 44.8
 170 21.7 21.4 32.2





#13

Acenaphthylene

Concen: 2.94 ng

RT: 14.15 min Scan# 800

Delta R.T. 0.00 min

Lab File: BE091526.D

Acq: 25 Mar 2016 15:57

Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2


Tot Ion:152 Resp: 142247

Ion Ratio Lower Upper

152 100

151 20.5 16.3 24.5




153 13.5 11.1 16.7



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E



#14

Acenaphthene

Concen: 2.63 ng

RT: 14.49 min Scan# 825

Delta R.T. -0.01 min

Lab File: BE091526.D

Acq: 25 Mar 2016 15:57


Tgt Ion:154 Resp: 91841

Ion Ratio Lower Upper

154 100

153 111.5 87.3 130.9



152 55.5 42.9 64.3




Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E





#15

Fluorene

Concen: 2.62 ng

RT: 15.47 min Scan# 902

Delta R.T. -0.01 min

Lab File: BE091526.D

Acq: 25 Mar 2016 15:57

Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2


Tot Ion:166 Resp: 115529

Ion Ratio Lower Upper

166 100

165 99.6 79.2 118.8




167 13.5 10.8 16.2



Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E



#16

Phenanthrene-d10

Concen: 5.00 ng

RT: 17.17 min Scan# 1018

Delta R.T. -0.00 min

Lab File: BE091526.D

Acq: 25 Mar 2016 15:57


Tgt Ion:188 Resp: 272673

Ion Ratio Lower Upper

188 100

94 5.4 5.4 8.2#



80 4.7 5.0 7.4#




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0









#17
Hexachlorobenzene
Concen: 2.67 ng
RT: 16.48 min Scan# 975
Delta R.T. -0.00 min
Lab File: BE091526.D
Acq: 25 Mar 2016 15:57




Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2


Tot Ion:284 Resp: 31682
Ion Ratio Lower Upper
284 100
142 44.2 31.0 46.4
249 33.9 25.8 38.8



#18
Pentachlorophenol
Concen: 2.26 ng
RT: 16.81 min Scan# 994
Delta R.T. -0.02 min
Lab File: BE091526.D
Acq: 25 Mar 2016 15:57

Tgt Ion:266 Resp: 10674
Ion Ratio Lower Upper
266 100
268 59.8 48.2 72.2
264 63.4 52.1 78.1









#19
Phenanthrene
Concen: 2.62 ng
RT: 17.21 min Scan# 1021
Delta R.T. -0.00 min
Lab File: BE091526.D
Acq: 25 Mar 2016 15:57




Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2


Tot Ion:178 Resp: 203952
Ion Ratio Lower Upper
178 100
176 19.6 15.5 23.3
179 15.4 13.1 19.7



#20
Anthracene
Concen: 2.67 ng
RT: 17.30 min Scan# 1029
Delta R.T. -0.00 min
Lab File: BE091526.D
Acq: 25 Mar 2016 15:57

Tgt Ion:178 Resp: 182488
Ion Ratio Lower Upper
178 100
176 19.1 14.9 22.3
179 15.3 12.2 18.4





#21

Fluoranthene

Concen: 2.29 ng

RT: 19.21 min Scan# 1151

Delta R.T. -0.02 min

Lab File: BE091526.D

Acq: 25 Mar 2016 15:57

Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2


Tot Ion:202 Resp: 204877

Ion Ratio Lower Upper

202 100

101 11.4 8.3 12.5




203 17.1 13.9 20.9



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E



#22

Chrysene-d12

Concen: 5.00 ng

RT: 21.34 min Scan# 1249

Delta R.T. -0.00 min

Lab File: BE091526.D

Acq: 25 Mar 2016 15:57


Tgt Ion:240 Resp: 285609

Ion Ratio Lower Upper

240 100

120 0.9 4.0 6.0#



236 21.0 23.0 34.4#




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E









#23
Pvrene
Concen: 3.34 ng
RT: 19.57 min Scan# 1170
Delta R.T. 0.00 min
Lab File: BE091526.D
Acq: 25 Mar 2016 15:57




Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2


Tot Ion	Ratio	Lower	Upper
202	100		
200	22.0	16.4	24.6
203	16.9	14.6	21.8



#24
Terphenyl-d14
Concen: 4.60 ng
RT: 19.78 min Scan# 1181
Delta R.T. 0.00 min
Lab File: BE091526.D
Acq: 25 Mar 2016 15:57

Tgt Ion	Ratio	Lower	Upper
244	100		
212	8.5	5.8	8.8
122	2.6	1.8	2.8









#25
Benzo(a)anthracene
Concen: 2.85 ng
RT: 21.31 min Scan# 1248
Delta R.T. -0.00 min
Lab File: BE091526.D
Acq: 25 Mar 2016 15:57




Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2


Tot Ion:228 Resp: 224056
Ion Ratio Lower Upper
228 100
226 21.4 24.0 36.0#
229 23.4 13.8 20.6#



#26
Chrysene
Concen: 3.36 ng m
RT: 21.36 min Scan# 1250
Delta R.T. -0.00 min
Lab File: BE091526.D
Acq: 25 Mar 2016 15:57

Tgt Ion:228 Resp: 269657
Ion Ratio Lower Upper
228 100
226 28.7 18.9 28.3#
229 19.9 19.1 28.7









#27
 Indeno(1,2,3-cd)pyrene
 Concen: 2.88 ng
 RT: 26.35 min Scan# 1649
 Delta R.T. -0.02 min
 Lab File: BE091526.D
 Acq: 25 Mar 2016 15:57




Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2


Tot Ion:276 Resp: 235735
 Ion Ratio Lower Upper
 276 100
 138 26.2 20.2 30.4
 277 24.7 19.8 29.8



#28
 Perylene-d12
 Concen: 5.00 ng
 RT: 23.78 min Scan# 1429
 Delta R.T. -0.01 min
 Lab File: BE091526.D
 Acq: 25 Mar 2016 15:57

Tgt Ion:264 Resp: 284756
 Ion Ratio Lower Upper
 264 100
 260 24.3 20.1 30.1
 265 22.4 18.3 27.5



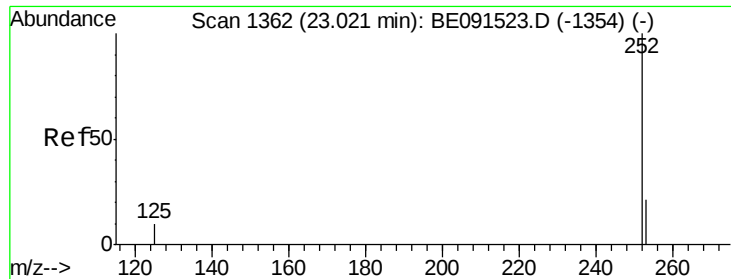

#29

Benzo(b)fluoranthene

Concen: 2.36 ng

RT: 23.02 min Scan# 1363

Delta R.T. -0.01 min

Lab File: BE091526.D

Acq: 25 Mar 2016 15:57

Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2


Tot Ion:252 Resp: 212530

Ion Ratio Lower Upper




252 100

253 20.6 18.7 28.1

125 11.0 9.8 14.6



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E



#30

Benzo(k)fluoranthene

Concen: 2.56 ng

RT: 23.08 min Scan# 1368

Delta R.T. 0.00 min

Lab File: BE091526.D

Acq: 25 Mar 2016 15:57


Tgt Ion:252 Resp: 235551

Ion Ratio Lower Upper



252 100


253 22.9 20.2 30.4

125 9.7 9.4 14.2



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E



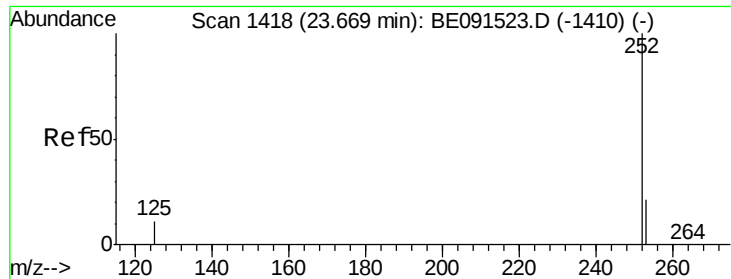

#31

Benzo(a)pyrene

Concen: 2.43 ng

RT: 23.67 min Scan# 1419

Delta R.T. -0.01 min

Lab File: BE091526.D

Acq: 25 Mar 2016 15:57

Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2


Tot Ion:252 Resp: 192675

Ion Ratio Lower Upper

252 100

253 22.1 19.4 29.0




125 11.1 11.4 17.2#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



#32

Dibenzo(a,h)anthracene

Concen: 2.59 ng

RT: 26.39 min Scan# 1652

Delta R.T. -0.01 min

Lab File: BE091526.D

Acq: 25 Mar 2016 15:57


Tgt Ion:278 Resp: 202134

Ion Ratio Lower Upper

278 100

139 15.5 14.2 21.4



279 24.4 19.6 29.4




Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E





#33

Benzo(a,h,i)perylene

Concen: 2.50 ng

RT: 27.15 min Scan# 1718

Delta R.T. -0.01 min

Lab File: BE091526.D

Acq: 25 Mar 2016 15:57

Instrument :

BNA_E

ClientSampleId :

SSTDICC3.2


Tot Ion: 276 Resp: 202983

Ion Ratio Lower Upper

276 100

277 24.2 19.4 29.2

138 22.1 18.2 27.4



Abundance Ion 276.00 (275.70 to 276.70): E
 Ion 277.00 (276.70 to 277.70): E
 Ion 138.00 (137.70 to 138.70): E

