


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032516\
 Data File : BE091520.D
 Acq On : 25 Mar 2016 10:14
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 25 19:00:32 2016

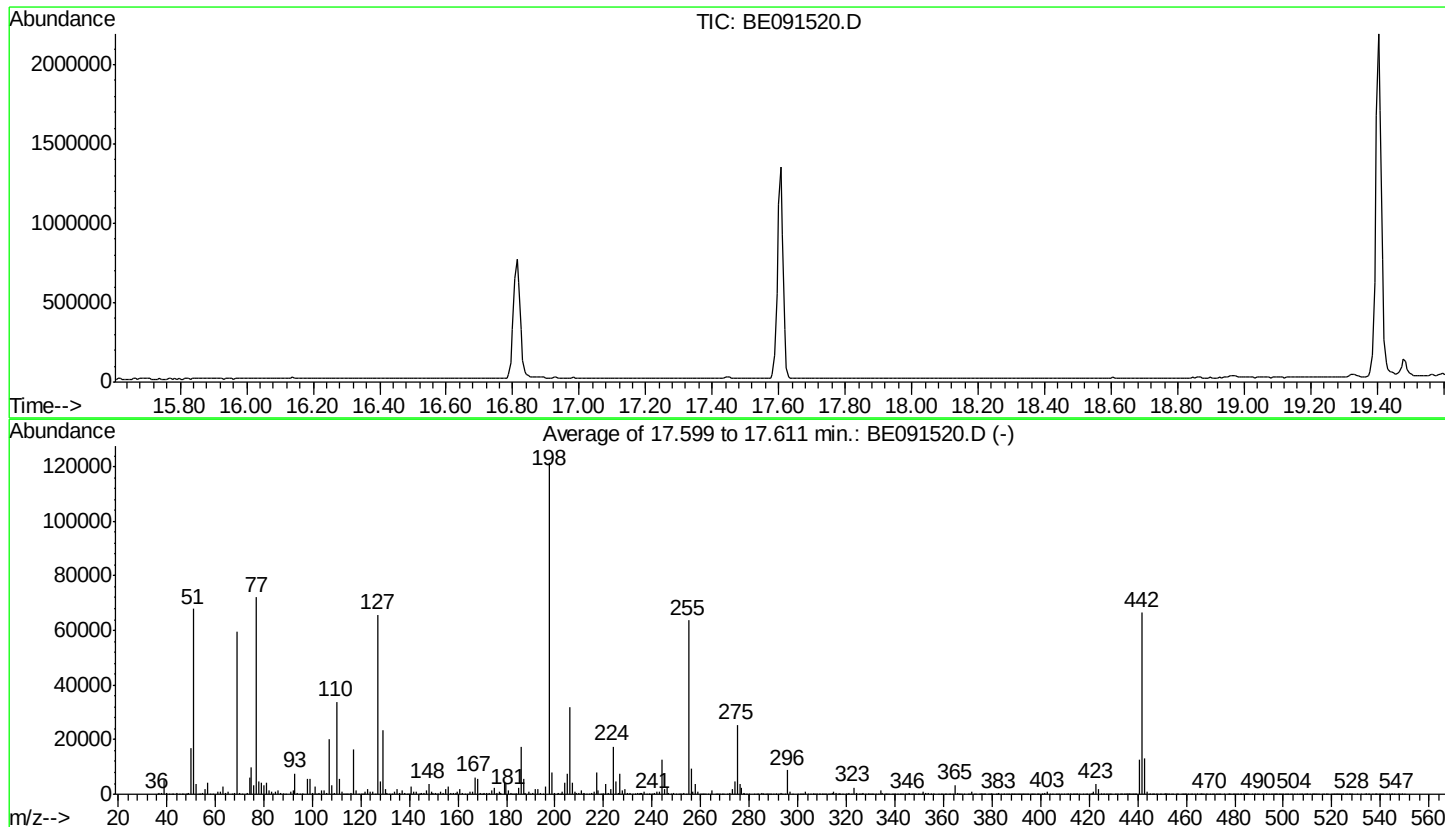

AutoFind: Scans 2555, 2556, 2557; Background Corrected with Scan 2547

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.9	67875	PASS
68	69	0.00	2	1.1	632	PASS
69	198	0.00	100	48.9	59434	PASS
70	69	0.00	2	0.5	280	PASS
127	198	10	80	54.1	65744	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	121467	PASS
199	198	5	9	6.7	8134	PASS
275	198	10	60	21.0	25522	PASS
365	198	1	100	2.9	3478	PASS
441	442	0.01	24	18.8	12487	PASS
442	198	50	100	54.7	66413	PASS
443	442	15	24	19.8	13140	PASS