

Data Path : Z:\HPCHEM1\BNA\_E\DATA\BE032615\  
 Data File : BE089862.D  
 Acq On : 26 Mar 2015 18:09  
 Operator : TP/JJ  
 Sample : SSTDICC0.5  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 SSTDICC0.5

Quant Time: Mar 27 02:13:10 2015  
 Quant Method : Z:\HPCHEM1\BNA\_E\METHODS\SIMPAH-BE032615.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Mar 27 01:45:40 2015  
 Response via : Initial Calibration


| Internal Standards          | R.T.  | QIon | Response | Conc | Units | Dev(Min) |
|-----------------------------|-------|------|----------|------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4   | 7.47  | 152  | 84710    | 5.00 | ng    | 0.00     |
| 4) Naphthalene-d8           | 10.23 | 136  | 369052   | 5.00 | ng    | 0.00     |
| 8) Acenaphthene-d10         | 14.36 | 164  | 200316   | 5.00 | ng    | 0.00     |
| 13) Phenanthrene-d10        | 17.89 | 188  | 383316   | 5.00 | ng    | 0.00     |
| 19) Chrysene-d12            | 24.23 | 240  | 340531   | 5.00 | ng    | 0.00     |
| 25) Perylene-d12            | 27.38 | 264  | 319822   | 5.00 | ng    | 0.00     |
| System Monitoring Compounds |       |      |          |      |       |          |
| 5) Nitrobenzene-d5          | 8.66  | 82   | 9726     | 0.45 | ng    | 0.00     |
| 9) 2-Fluorobiphenyl         | 12.83 | 172  | 23993    | 0.51 | ng    | 0.00     |
| 21) Terphenyl-d14           | 21.83 | 244  | 27083    | 0.54 | ng    | 0.00     |
| Target Compounds            |       |      |          |      |       | Qvalue   |
| 2) 1,4-Dioxane              | 2.47  | 88   | 5121     | 0.44 | ng    | 89       |
| 3) n-Nitrosodimethylamine   | 2.93  | 42   | 6009     | 0.38 | ng    | # 60     |
| 6) Naphthalene              | 10.28 | 128  | 37312    | 0.50 | ng    | 97       |
| 7) 2-Methylnaphthalene      | 11.91 | 142  | 23419    | 0.56 | ng    | 99       |
| 10) Acenaphthylene          | 14.01 | 152  | 140638   | 0.48 | ng    | 99       |
| 11) Acenaphthene            | 14.44 | 154  | 21333    | 0.48 | ng    | 88       |
| 12) Fluorene                | 15.68 | 166  | 27838    | 0.51 | ng    | 93       |
| 14) Hexachlorobenzene       | 16.95 | 284  | 5664     | 0.44 | ng    | 98       |
| 15) Pentachlorophenol       | 17.48 | 266  | 11089    | 2.38 | ng    | 95       |
| 16) Phenanthrene            | 17.95 | 178  | 41198    | 0.48 | ng    | 98       |
| 17) Anthracene              | 18.07 | 178  | 35386    | 0.46 | ng    | 99       |
| 18) Fluoranthene            | 20.79 | 202  | 39517    | 0.51 | ng    | 98       |
| 20) Pyrene                  | 21.31 | 202  | 41962    | 0.49 | ng    | 99       |
| 22) Benzo(a)anthracene      | 24.21 | 228  | 34380    | 0.53 | ng    | 96       |
| 23) Chrysene                | 24.28 | 228  | 35449    | 0.51 | ng    | 99       |
| 24) Indeno(1,2,3-cd)pyrene  | 29.35 | 276  | 31922m   | 0.76 | ng    |          |
| 26) Benzo(b)fluoranthene    | 26.60 | 252  | 53761    | 1.04 | ng    | 98       |
| 27) Benzo(k)fluoranthene    | 26.66 | 252  | 68953m   | 1.00 | ng    |          |
| 28) Benzo(a)pyrene          | 27.26 | 252  | 50550m   | 1.04 | ng    |          |
| 29) Dibenzo(a,h)anthracene  | 29.41 | 278  | 22032    | 0.63 | ng    | # 82     |
| 30) Benzo(g,h,i)perylene    | 29.79 | 276  | 30287    | 0.61 | ng    | # 87     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA\_E\DATA\BE032615\  
Data File : BE089862.D  
Acq On : 26 Mar 2015 18:09  
Operator : TP/JJ  
Sample : SSTDICC0.5  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
SSTDICC0.5

Quant Time: Mar 27 02:13:10 2015  
Quant Method : Z:\HPCHEM1\BNA\_E\METHODS\SIMPAH-BE032615.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Mar 27 01:45:40 2015  
Response via : Initial Calibration

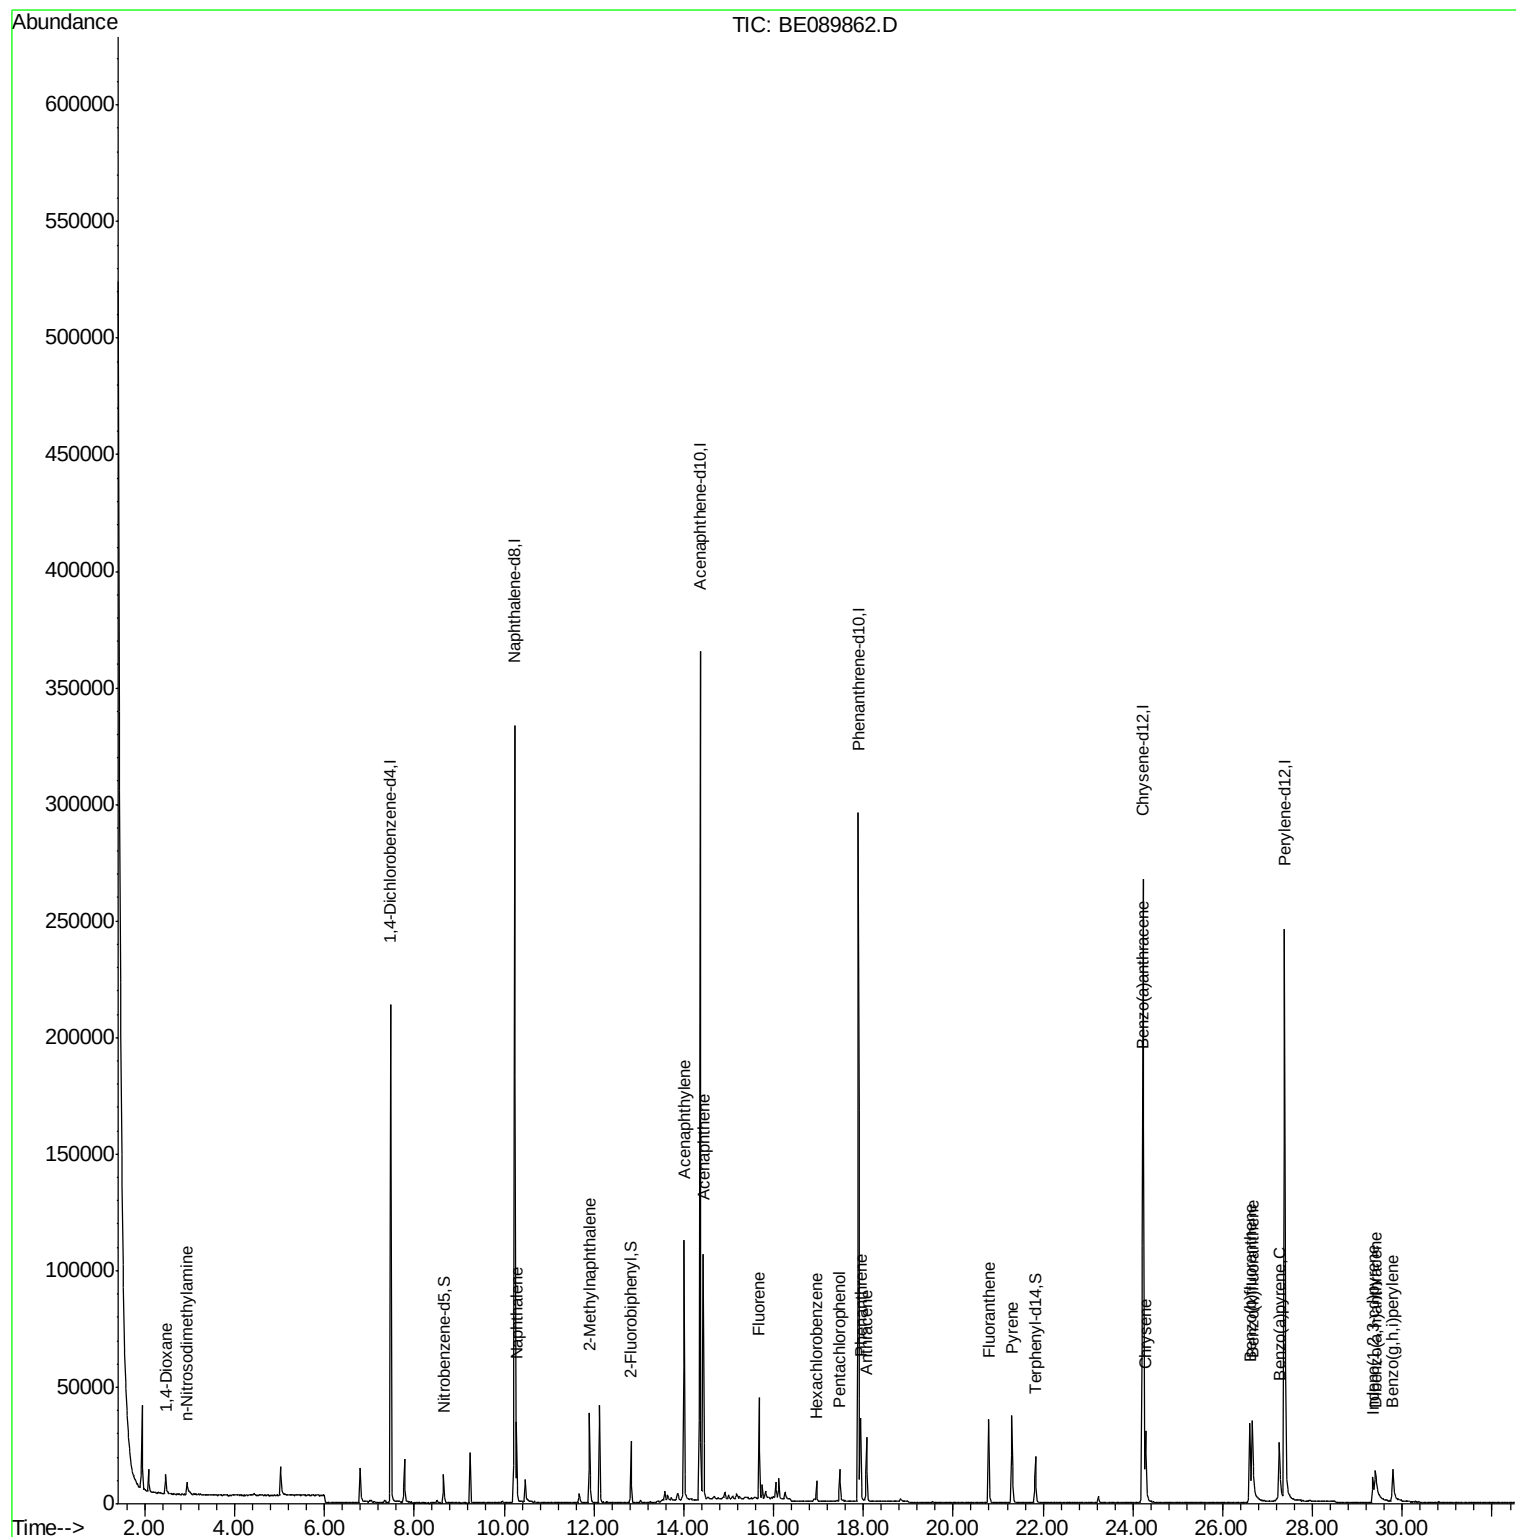

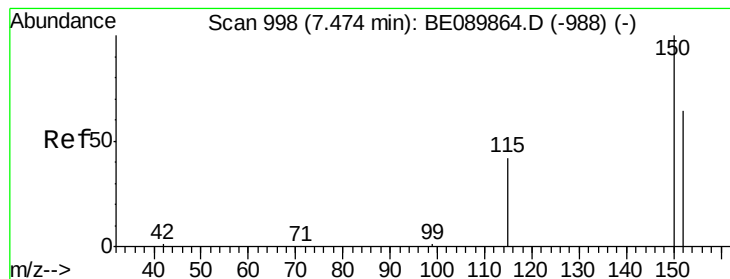

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.47 min Scan# 998

Delta R.T. 0.00 min

Lab File: BE089862.D

Acq: 26 Mar 2015 18:09

Instrument :

BNA\_E

ClientSampleId :

SSTDIC0.5


Tgt Ion:152 Resp: 84710

Ion Ratio Lower Upper

152 100

150 158.8 125.5 188.3




115 68.8 58.0 87.0



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

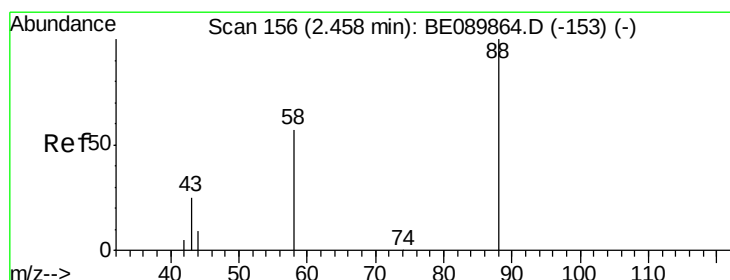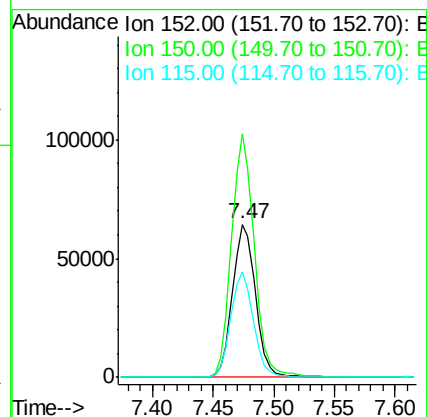

#2

1,4-Dioxane

Concen: 0.44 ng

RT: 2.47 min Scan# 157

Delta R.T. 0.01 min

Lab File: BE089862.D

Acq: 26 Mar 2015 18:09


Tgt Ion: 88 Resp: 5121

Ion Ratio Lower Upper

88 100

58 72.7 48.6 72.8



43 34.4 28.6 43.0




Abundance Ion 88.00 (87.70 to 88.70): BE0

Ion 58.00 (57.70 to 58.70): BE0

Ion 43.00 (42.70 to 43.70): BE0

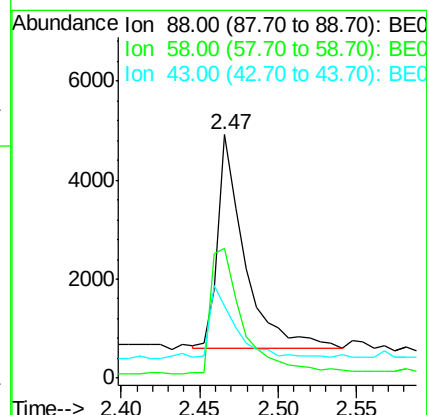

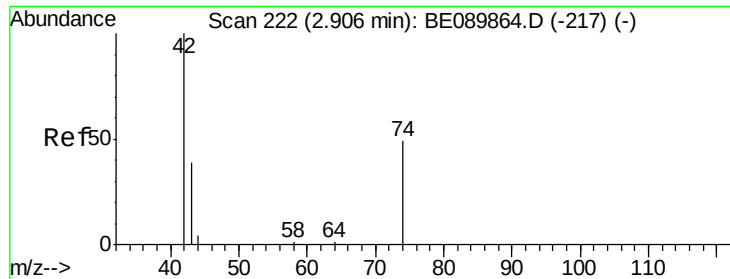

#3

n-Nitrosodimethylamine

Concen: 0.38 ng

RT: 2.93 min Scan# 225

Delta R.T. 0.02 min

Lab File: BE089862.D

Acq: 26 Mar 2015 18:09

Instrument :

BNA\_E

ClientSampleId :

SSTDIC0.5


Tgt Ion: 42 Resp: 6009

Ion Ratio Lower Upper

42 100

74 124.9 68.7 103.1#




44 4.3 6.2 9.4#



Abundance Ion 42.00 (41.70 to 42.70): BE0

Ion 74.00 (73.70 to 74.70): BE0

Ion 44.00 (43.70 to 44.70): BE0

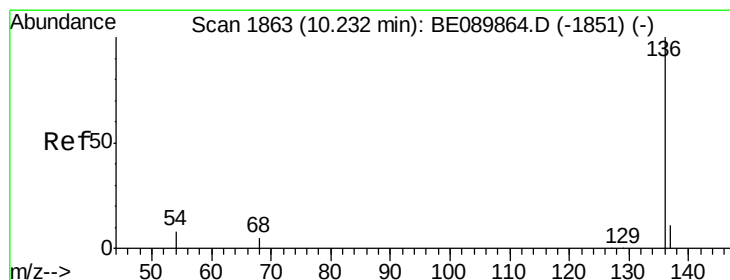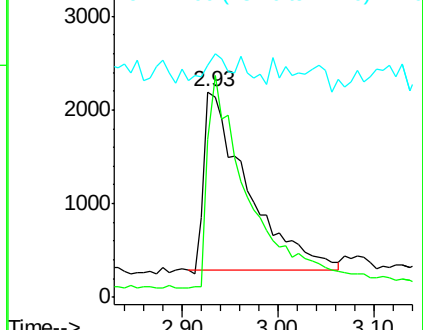

#4

Naphthalene-d8

Concen: 5.00 ng

RT: 10.23 min Scan# 1863

Delta R.T. 0.00 min

Lab File: BE089862.D

Acq: 26 Mar 2015 18:09


Tgt Ion: 136 Resp: 369052

Ion Ratio Lower Upper

136 100

137 11.0 8.8 13.2



54 7.4 7.0 10.4




Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

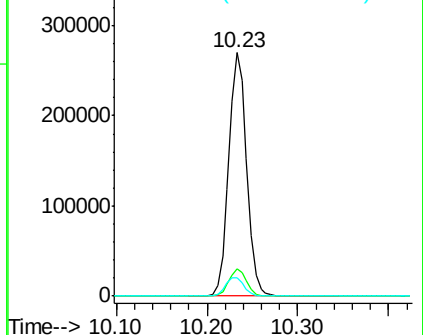

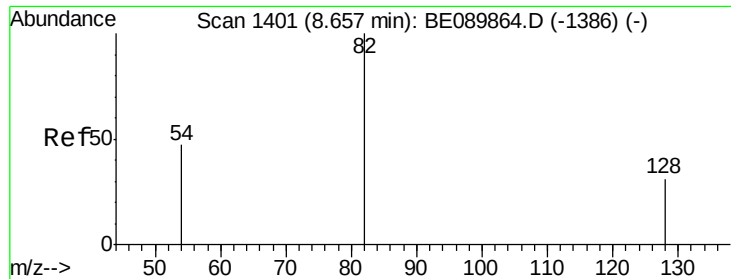

#5

Nitrobenzene-d5

Concen: 0.45 ng

RT: 8.66 min Scan# 1401

Delta R.T. 0.00 min

Lab File: BE089862.D

Acq: 26 Mar 2015 18:09

Instrument :

BNA\_E

ClientSampleId :

SSTDIC0.5


Tgt Ion: 82 Resp: 9726

Ion Ratio Lower Upper

82 100

128 33.4 24.6 37.0

54 53.6 43.0 64.6



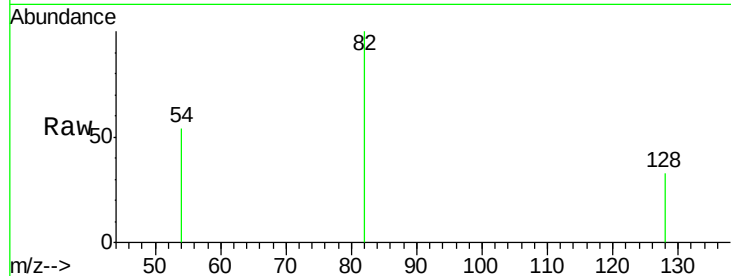


Abundance Ion 82.00 (81.70 to 82.70): BE089862.D (-1277) (-)

Ion 128.00 (127.70 to 128.70): BE089862.D (-1277) (-)

Ion 54.00 (53.70 to 54.70): BE089862.D (-1277) (-)

Time-->

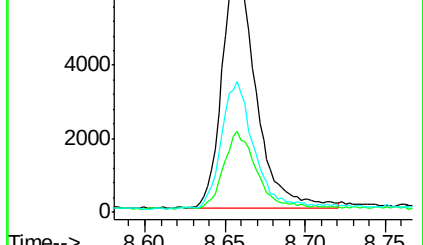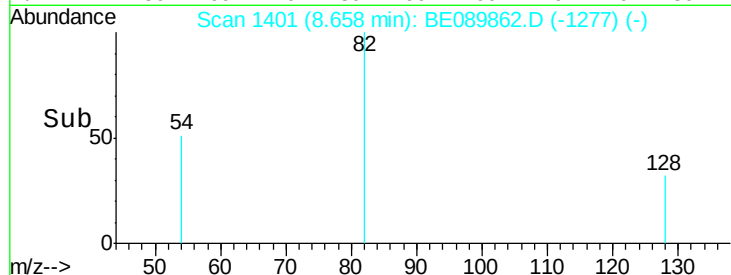

#6

Naphthalene

Concen: 0.50 ng

RT: 10.28 min Scan# 1872

Delta R.T. 0.00 min

Lab File: BE089862.D

Acq: 26 Mar 2015 18:09


Tgt Ion: 128 Resp: 37312

Ion Ratio Lower Upper

128 100

129 11.6 10.0 15.0

127 13.9 12.5 18.7






Abundance Ion 128.00 (127.70 to 128.70): BE089862.D (-1815) (-)

Ion 129.00 (128.70 to 129.70): BE089862.D (-1815) (-)

Ion 127.00 (126.70 to 127.70): BE089862.D (-1815) (-)

Time-->

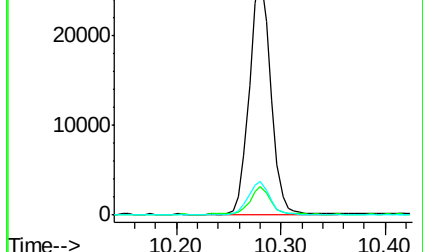

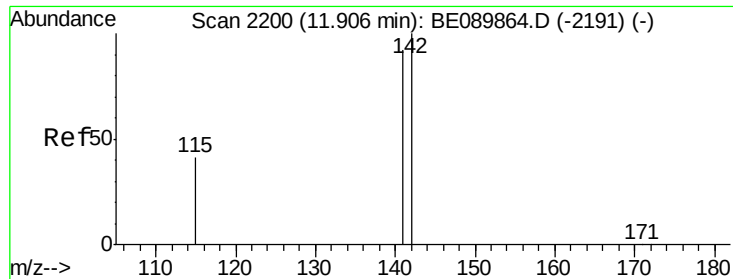

#7

2-Methylnaphthalene

Concen: 0.56 ng

RT: 11.91 min Scan# 2200

Delta R.T. 0.00 min

Lab File: BE089862.D

Acq: 26 Mar 2015 18:09

Instrument :

BNA\_E

ClientSampleId :

SSTDIC0.5


Tgt Ion:142 Resp: 23419

Ion Ratio Lower Upper

142 100

141 91.7 72.8 109.2




115 40.2 32.9 49.3

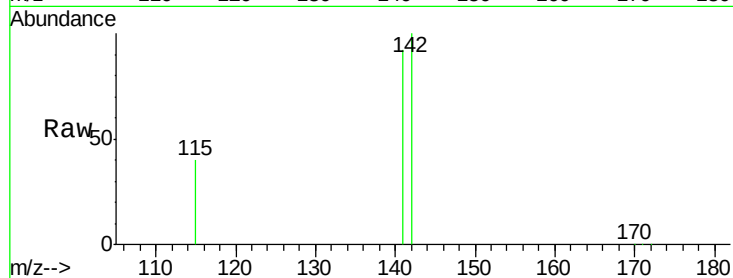

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E

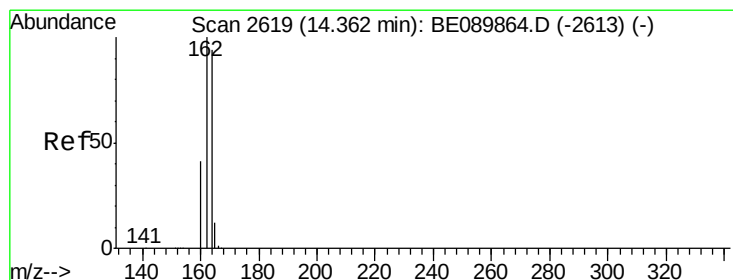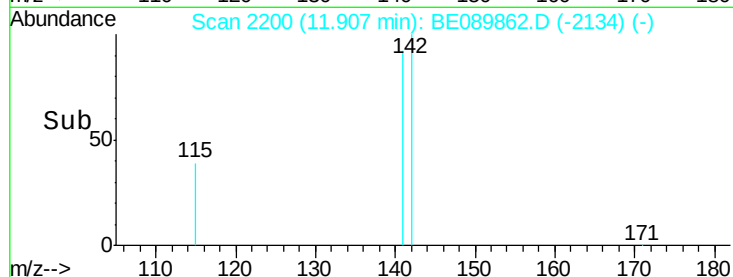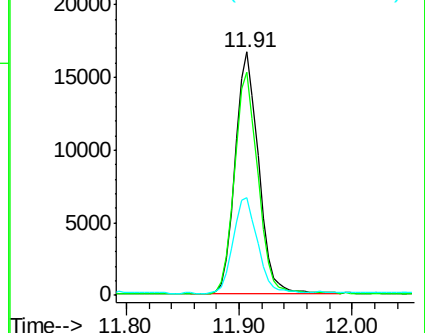

#8

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.36 min Scan# 2619

Delta R.T. 0.00 min

Lab File: BE089862.D

Acq: 26 Mar 2015 18:09


Tgt Ion:164 Resp: 200316

Ion Ratio Lower Upper

164 100

162 105.8 87.6 131.4



160 42.4 36.7 55.1

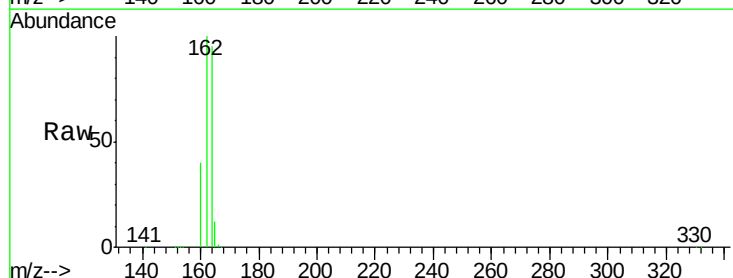


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



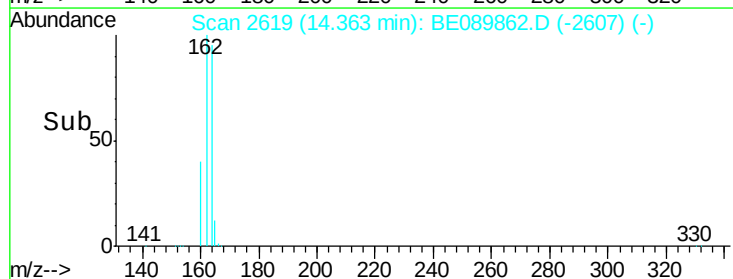
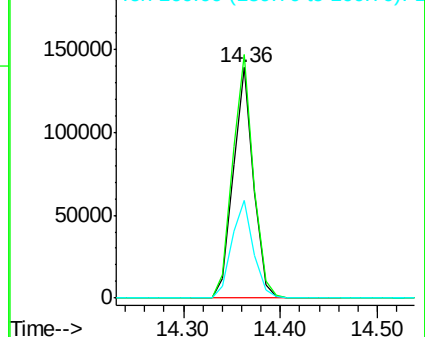


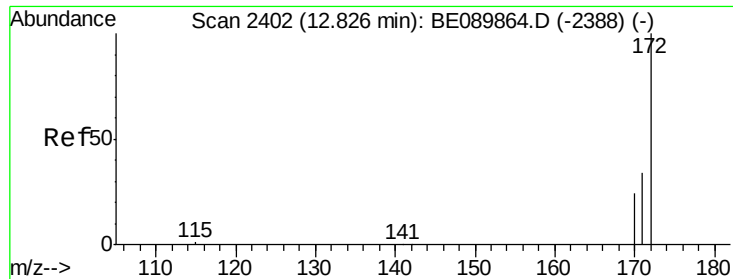

#9  
2-Fluorobiphenyl  
Concen: 0.51 ng  
RT: 12.83 min Scan# 2402  
Delta R.T. 0.00 min  
Lab File: BE089862.D  
Acq: 26 Mar 2015 18:09




Instrument :  
BNA\_E  
ClientSampleId :  
SSTDIC0.5


Tgt Ion:172 Resp: 23993  
Ion Ratio Lower Upper  
172 100  
171 34.3 30.8 46.2  
170 21.5 21.0 31.4

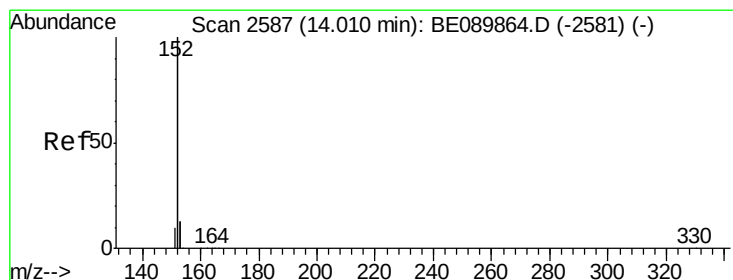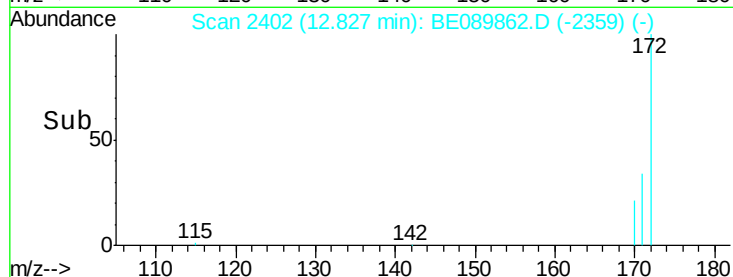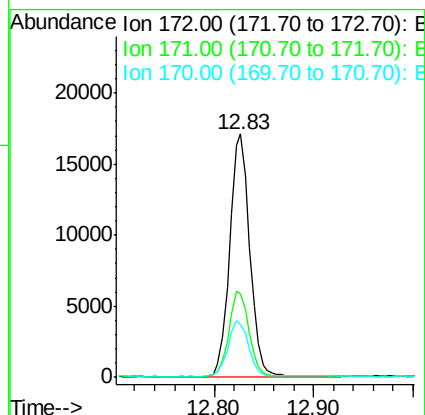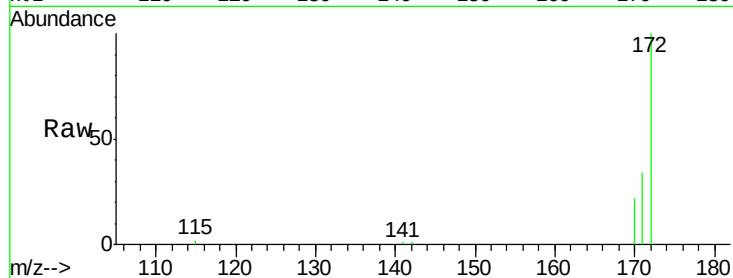

#10  
Acenaphthylene  
Concen: 0.48 ng  
RT: 14.01 min Scan# 2587  
Delta R.T. 0.00 min  
Lab File: BE089862.D  
Acq: 26 Mar 2015 18:09

Tgt Ion:152 Resp: 140638  
Ion Ratio Lower Upper  
152 100  
151 5.1 3.9 5.9  
153 13.2 11.0 16.4

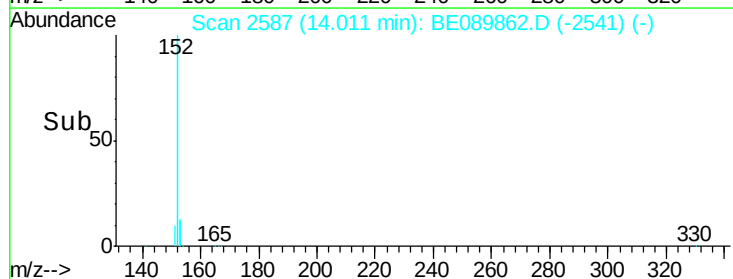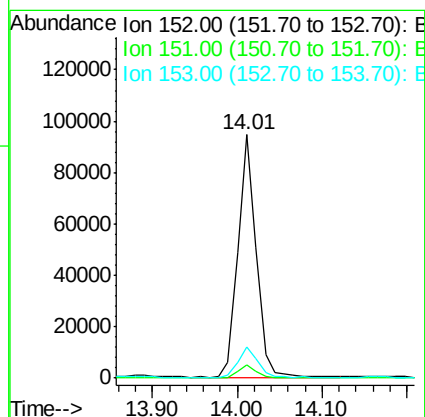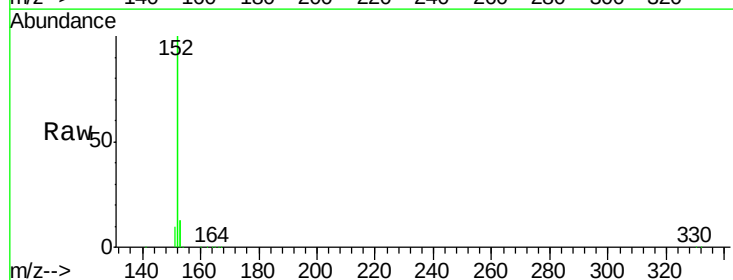



#11

Acenaphthene

Concen: 0.48 ng

RT: 14.44 min Scan# 2626

Delta R.T. 0.00 min

Lab File: BE089862.D

Acq: 26 Mar 2015 18:09

Instrument :

BNA\_E

ClientSampleId :

SSTDIC0.5


Tgt Ion:154 Resp: 21333

Ion Ratio Lower Upper

154 100

153 467.0 401.5 602.3




152 230.3 198.6 298.0

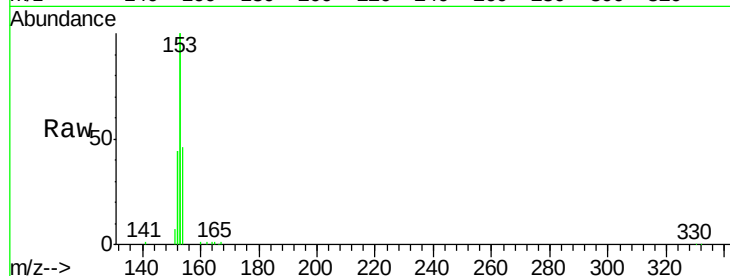

Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

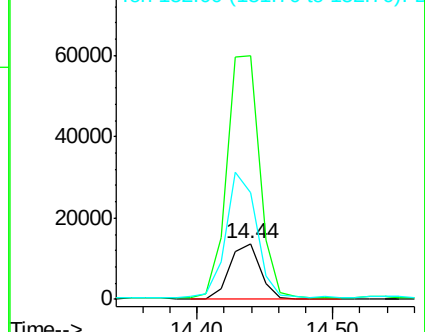

#12

Fluorene

Concen: 0.51 ng

RT: 15.68 min Scan# 2739

Delta R.T. 0.00 min

Lab File: BE089862.D

Acq: 26 Mar 2015 18:09


Tgt Ion:166 Resp: 27838

Ion Ratio Lower Upper

166 100

165 98.6 85.1 127.7



167 13.8 12.2 18.4




Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

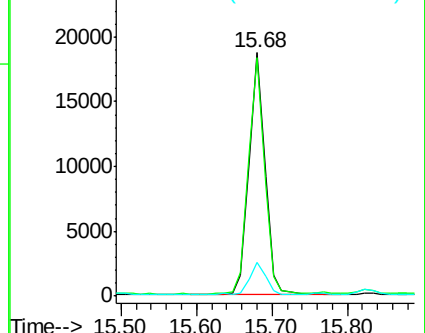





#13

Phenanthrene-d10

Concen: 5.00 ng

RT: 17.89 min Scan# 2969

Delta R.T. 0.00 min

Lab File: BE089862.D

Acq: 26 Mar 2015 18:09

Instrument :

BNA\_E

ClientSampleId :

SSTDIC0.5


Tgt Ion:188 Resp: 383316

Ion Ratio Lower Upper

188 100

94 9.3 8.5 12.7




80 10.8 10.0 15.0

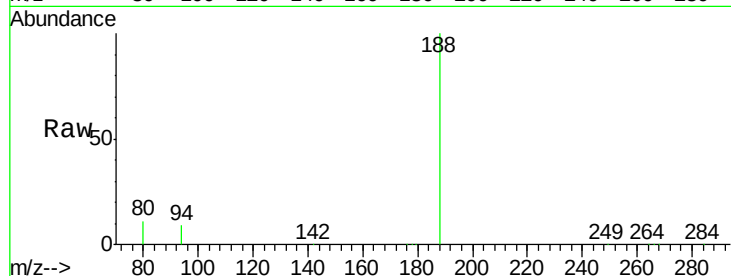

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

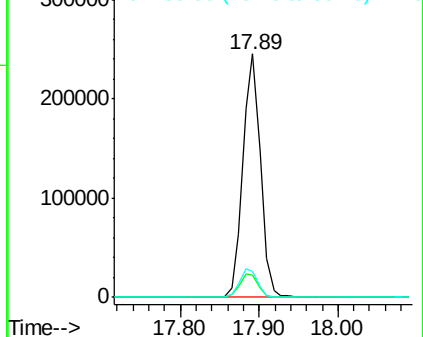

#14

Hexachlorobenzene

Concen: 0.44 ng

RT: 16.95 min Scan# 2865

Delta R.T. 0.00 min

Lab File: BE089862.D

Acq: 26 Mar 2015 18:09


Tgt Ion:284 Resp: 5664

Ion Ratio Lower Upper

284 100

142 68.2 53.3 79.9



249 38.0 31.1 46.7




Abundance Ion 283.80 (283.50 to 284.50): E

Ion 142.00 (141.70 to 142.70): E

Ion 249.00 (248.70 to 249.70): E




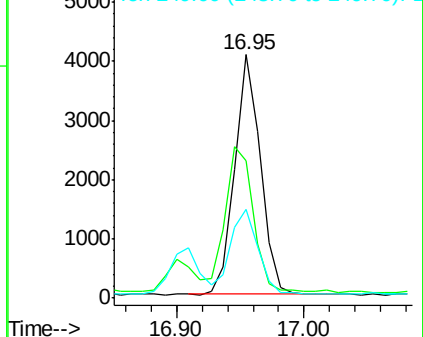




#15  
 Pentachlorophenol  
 Concen: 2.38 ng  
 RT: 17.48 min Scan# 2923  
 Delta R.T. 0.00 min  
 Lab File: BE089862.D  
 Acq: 26 Mar 2015 18:09




Instrument :  
 BNA\_E  
 ClientSampleId :  
 SSTDICC0.5


Tgt Ion: 266 Resp: 11089  
 Ion Ratio Lower Upper  
 266 100  
 268 61.4 51.6 77.4  
 264 67.0 50.2 75.2

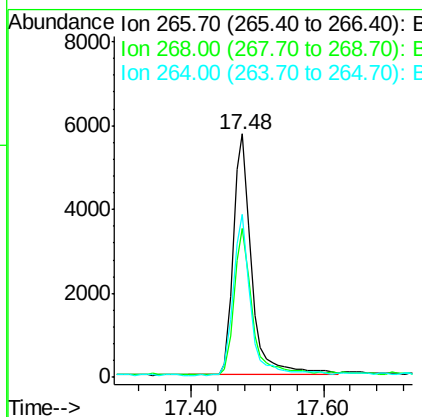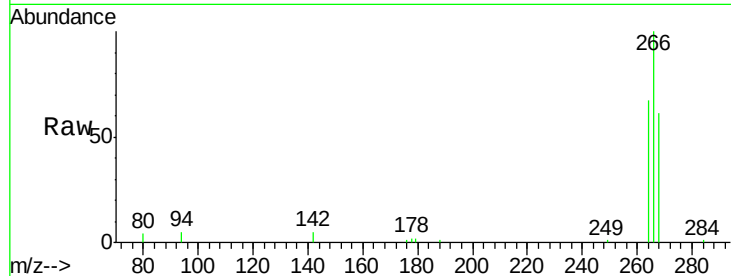

#16  
 Phenanthrene  
 Concen: 0.48 ng  
 RT: 17.95 min Scan# 2975  
 Delta R.T. 0.00 min  
 Lab File: BE089862.D  
 Acq: 26 Mar 2015 18:09

Tgt Ion: 178 Resp: 41198  
 Ion Ratio Lower Upper  
 178 100  
 176 18.7 15.4 23.0  
 179 16.4 12.2 18.4

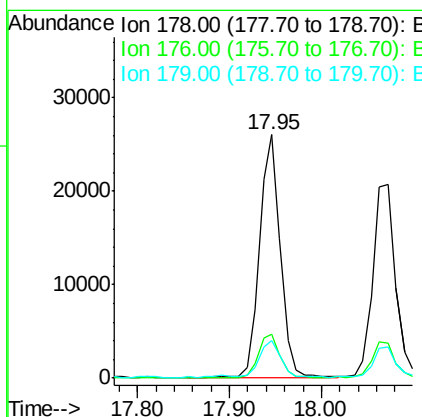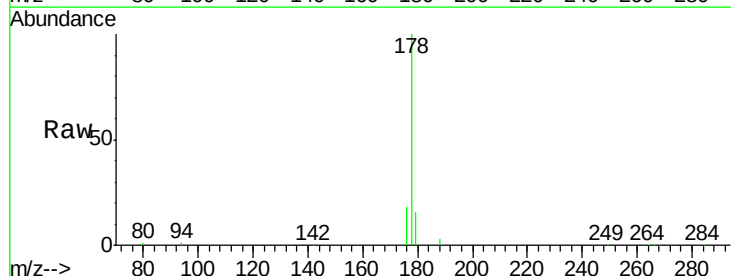



#17

Anthracene

Concen: 0.46 ng

RT: 18.07 min Scan# 2989

Delta R.T. 0.01 min

Lab File: BE089862.D

Acq: 26 Mar 2015 18:09

Instrument :

BNA\_E

ClientSampleId :

SSTDICC0.5


Tgt Ion:178 Resp: 35386

Ion Ratio Lower Upper

178 100

176 18.7 14.6 21.8




179 15.6 12.1 18.1

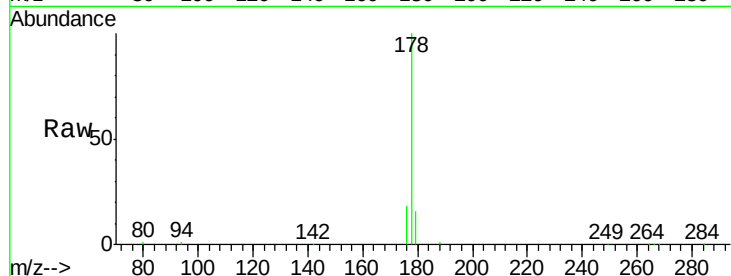

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

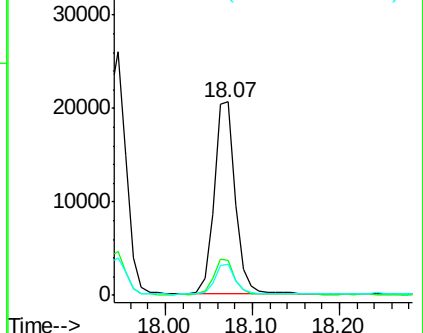

#18

Fluoranthene

Concen: 0.51 ng

RT: 20.79 min Scan# 3426

Delta R.T. -0.00 min

Lab File: BE089862.D

Acq: 26 Mar 2015 18:09


Tgt Ion:202 Resp: 39517

Ion Ratio Lower Upper

202 100

101 10.0 8.2 12.2



203 16.7 14.2 21.4




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

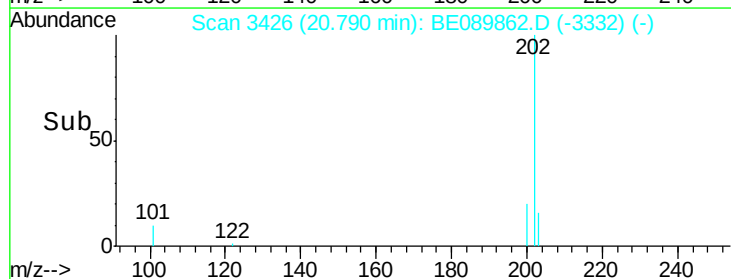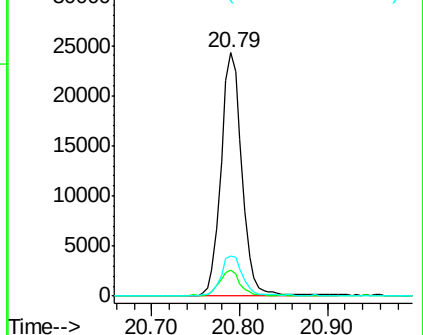

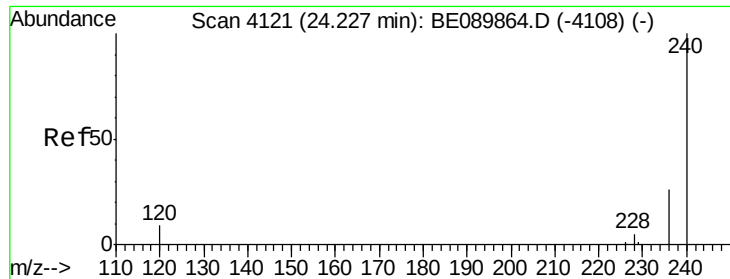

#19

Chrysene-d12

Concen: 5.00 ng

RT: 24.23 min Scan# 4121

Delta R.T. 0.00 min

Lab File: BE089862.D

Acq: 26 Mar 2015 18:09

Instrument :

BNA\_E

ClientSampleId :

SSTDIC0.5


Tgt Ion:240 Resp: 340531

Ion Ratio Lower Upper

240 100

120 8.4 7.5 11.3




236 25.2 20.5 30.7



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

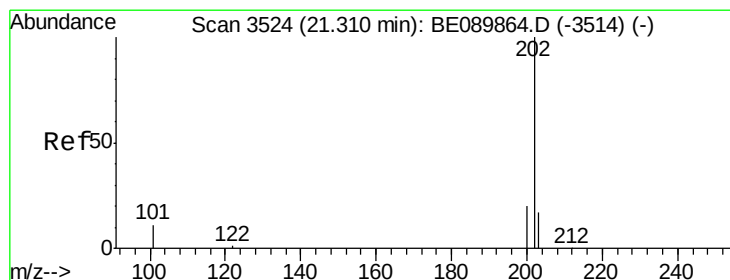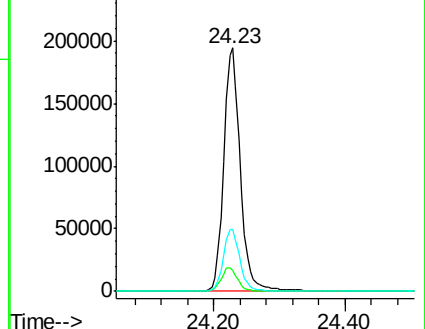

#20

Pyrene

Concen: 0.49 ng

RT: 21.31 min Scan# 3524

Delta R.T. -0.00 min

Lab File: BE089862.D

Acq: 26 Mar 2015 18:09


Tgt Ion:202 Resp: 41962

Ion Ratio Lower Upper

202 100

200 20.9 15.9 23.9



203 17.2 13.6 20.4




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E



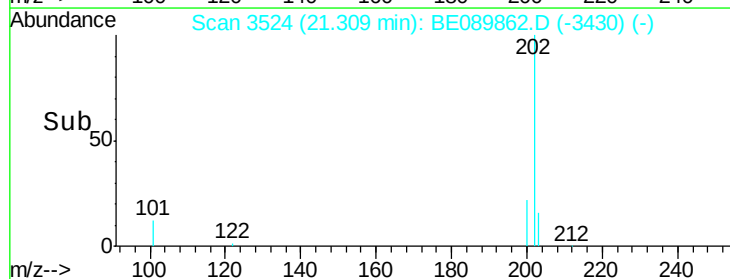
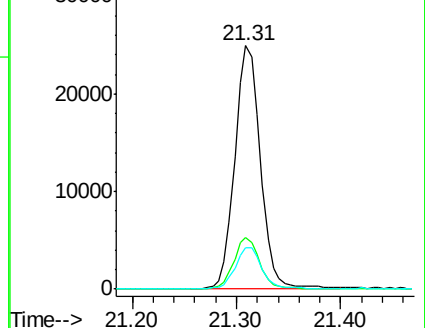




#21  
 Terphenyl-d14  
 Concen: 0.54 ng  
 RT: 21.83 min Scan# 3622  
 Delta R.T. -0.00 min  
 Lab File: BE089862.D  
 Acq: 26 Mar 2015 18:09




Instrument :  
 BNA\_E  
 ClientSampleId :  
 SSTDICC0.5


Tgt Ion: 244 Resp: 27083  
 Ion Ratio Lower Upper  
 244 100  
 212 7.2 7.3 10.9#  
 122 11.5 10.5 15.7

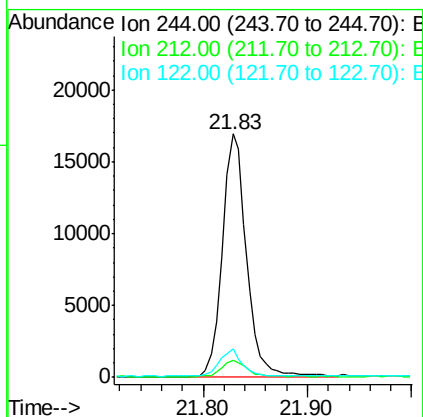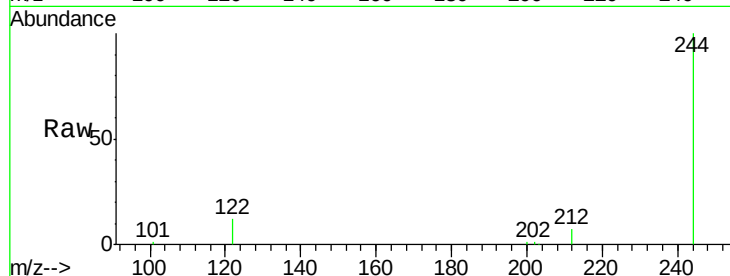

#22  
 Benzo(a)anthracene  
 Concen: 0.53 ng  
 RT: 24.21 min Scan# 4116  
 Delta R.T. -0.00 min  
 Lab File: BE089862.D  
 Acq: 26 Mar 2015 18:09

Tgt Ion: 228 Resp: 34380  
 Ion Ratio Lower Upper  
 228 100  
 226 27.2 19.8 29.8  
 229 18.7 16.3 24.5

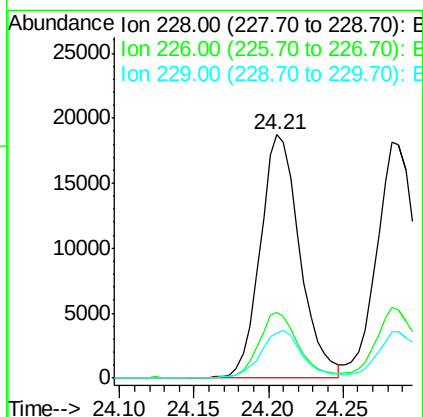

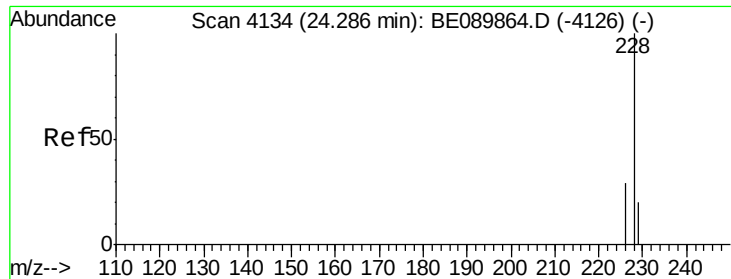

#23

Chrysene

Concen: 0.51 ng

RT: 24.28 min Scan# 4133

Delta R.T. -0.00 min

Lab File: BE089862.D

Acq: 26 Mar 2015 18:09

Instrument :

BNA\_E

ClientSampleId :

SSTDIC0.5





Tgt Ion:228 Resp: 35449

Ion Ratio Lower Upper

228 100

226 29.8 23.0 34.4

229 19.6 15.8 23.6

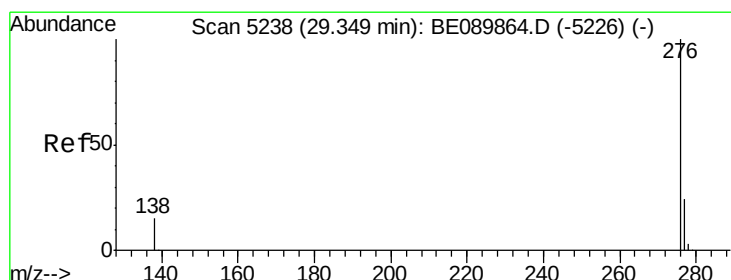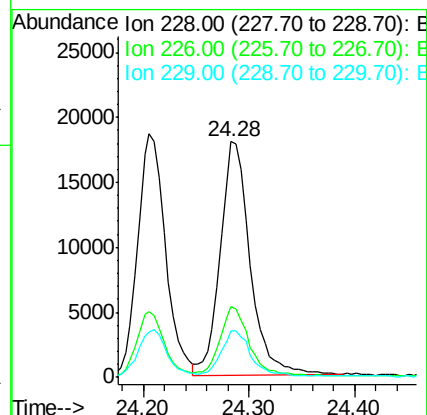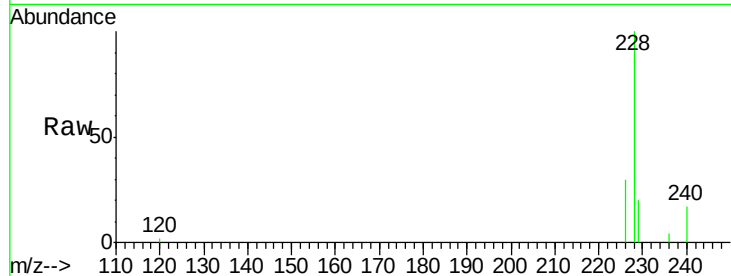

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.76 ng m

RT: 29.35 min Scan# 5238

Delta R.T. -0.00 min

Lab File: BE089862.D

Acq: 26 Mar 2015 18:09




Tgt Ion:276 Resp: 31922


Ion Ratio Lower Upper

276 100

138 8.5 4.3 6.5#

277 12.9 9.0 13.4


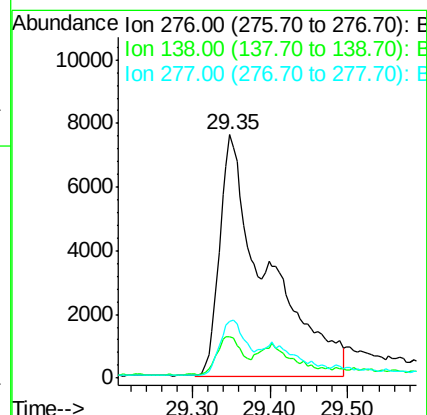




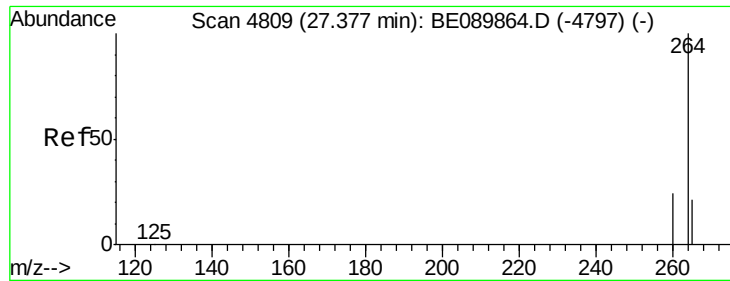

#25  
**Perylene-d12**  
 Concen: 5.00 ng  
 RT: 27.38 min Scan# 4809  
 Delta R.T. 0.00 min  
 Lab File: BE089862.D  
 Acq: 26 Mar 2015 18:09




Instrument :  
 BNA\_E  
 ClientSampleId :  
 SSTDICC0.5


Tgt Ion: 264 Resp: 319822  
 Ion Ratio Lower Upper  
 264 100  
 260 24.0 18.2 27.2  
 265 21.5 17.3 25.9

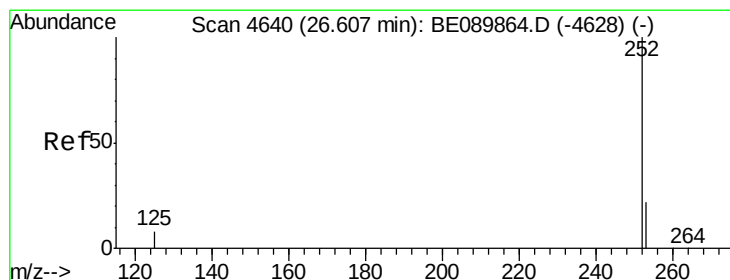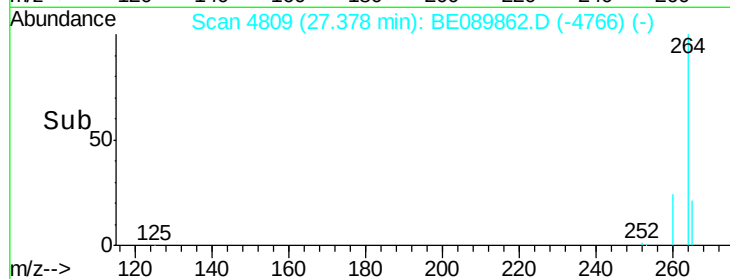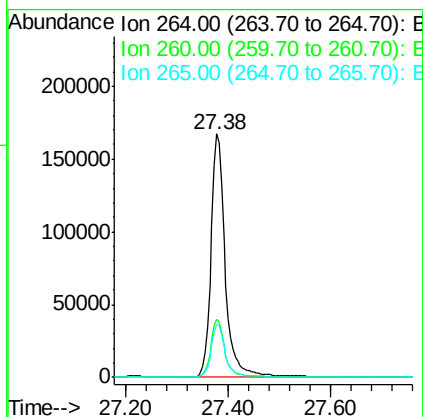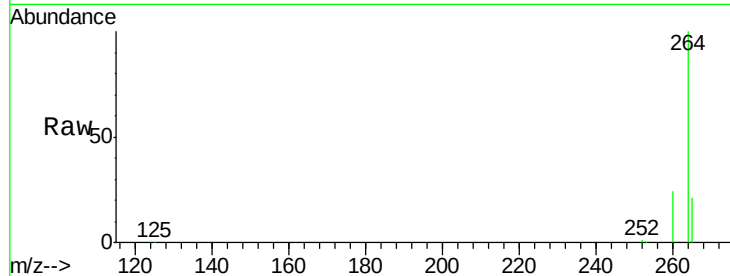

#26  
**Benzo(b)fluoranthene**  
 Concen: 1.04 ng  
 RT: 26.60 min Scan# 4639  
 Delta R.T. -0.00 min  
 Lab File: BE089862.D  
 Acq: 26 Mar 2015 18:09

Tgt Ion: 252 Resp: 53761  
 Ion Ratio Lower Upper  
 252 100  
 253 22.3 17.8 26.6  
 125 9.0 8.7 13.1


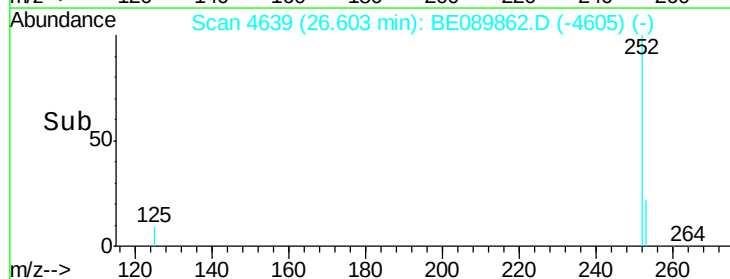
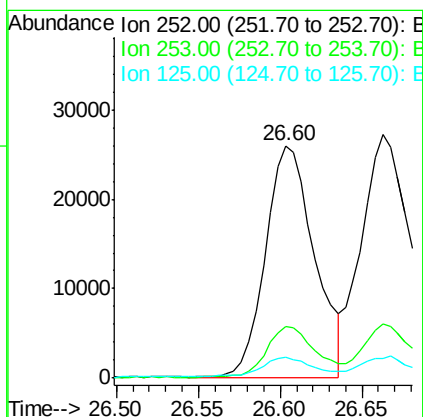
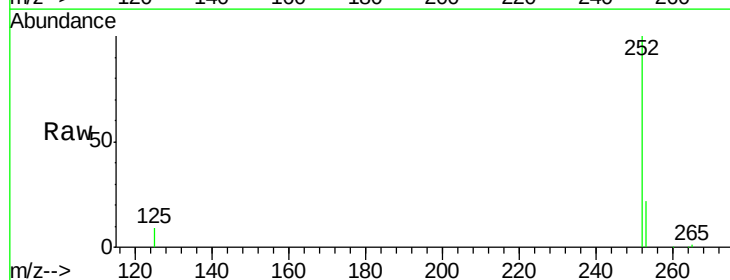


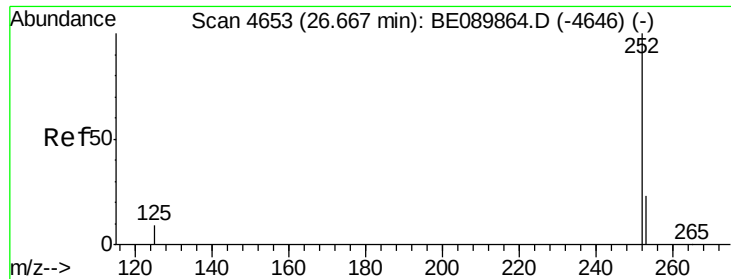

#27  
Benzo(k)fluoranthene  
Concen: 1.00 ng m  
RT: 26.66 min Scan# 4652  
Delta R.T. -0.00 min  
Lab File: BE089862.D  
Acq: 26 Mar 2015 18:09




Instrument :  
BNA\_E  
ClientSampleId :  
SSTDIC0.5

Tgt Ion:252 Resp: 68953  
Ion Ratio Lower Upper  
252 100  
253 22.2 18.6 28.0  
125 8.1 10.8 16.2#

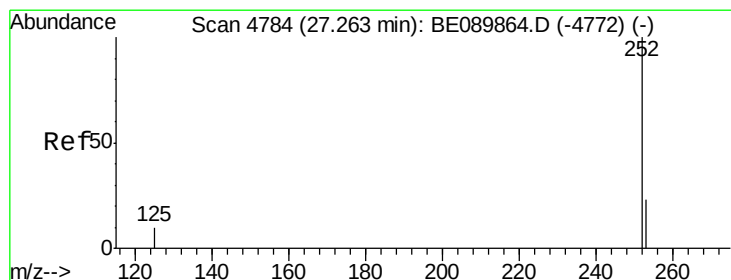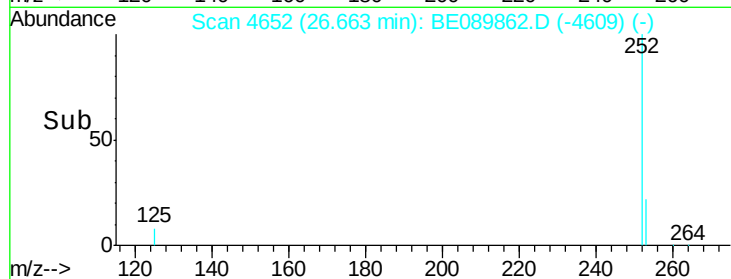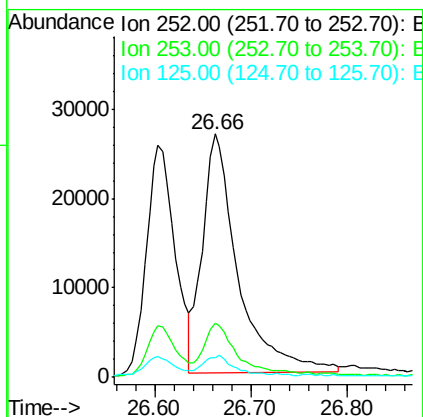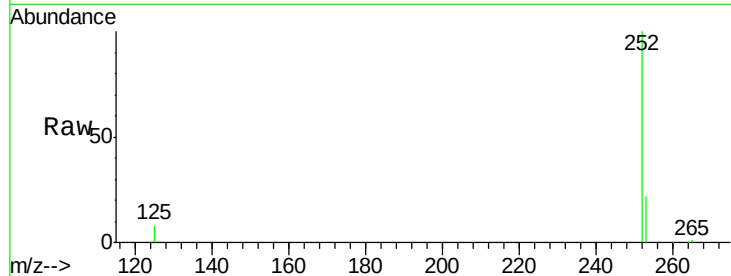


#28  
Benzo(a)pyrene  
Concen: 1.04 ng m  
RT: 27.26 min Scan# 4784  
Delta R.T. 0.00 min  
Lab File: BE089862.D  
Acq: 26 Mar 2015 18:09

Tgt Ion:252 Resp: 50550  
Ion Ratio Lower Upper  
252 100  
253 22.8 21.0 31.4  
125 10.0 13.3 19.9#

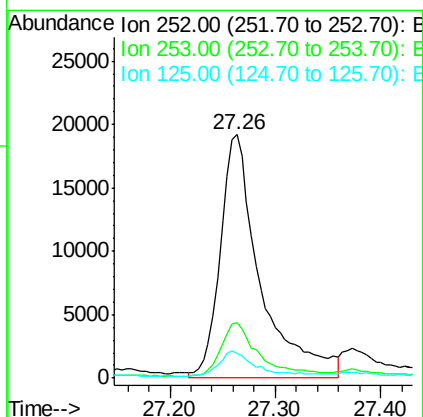





#29

Dibenzo(a,h)anthracene

Concen: 0.63 ng

RT: 29.41 min Scan# 5251

Delta R.T. -0.00 min

Lab File: BE089862.D

Acq: 26 Mar 2015 18:09

Instrument :

BNA\_E

ClientSampleId :

SSTDIC0.5


Tgt Ion: 278 Resp: 22032

Ion Ratio Lower Upper

278 100

139 16.1 20.0 30.0#




279 25.1 28.9 43.3#

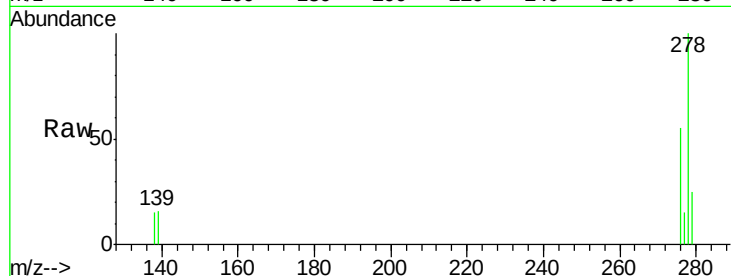

Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

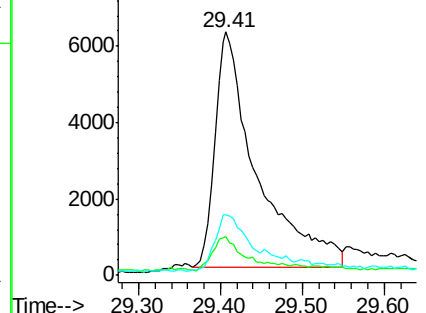

#30

Benzo(g,h,i)perylene

Concen: 0.61 ng

RT: 29.79 min Scan# 5335

Delta R.T. -0.00 min

Lab File: BE089862.D

Acq: 26 Mar 2015 18:09


Tgt Ion: 276 Resp: 30287

Ion Ratio Lower Upper

276 100

277 25.8 19.2 28.8

138 17.3 22.9 34.3#



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

