


Data Path : Z:\HPCHEM1\BNA_E\Data\BE032615\
 Data File : Be089856.d
 Acq On : 26 Mar 2015 10:46
 Operator : TP/JJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE032415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 25 16:20:31 2015

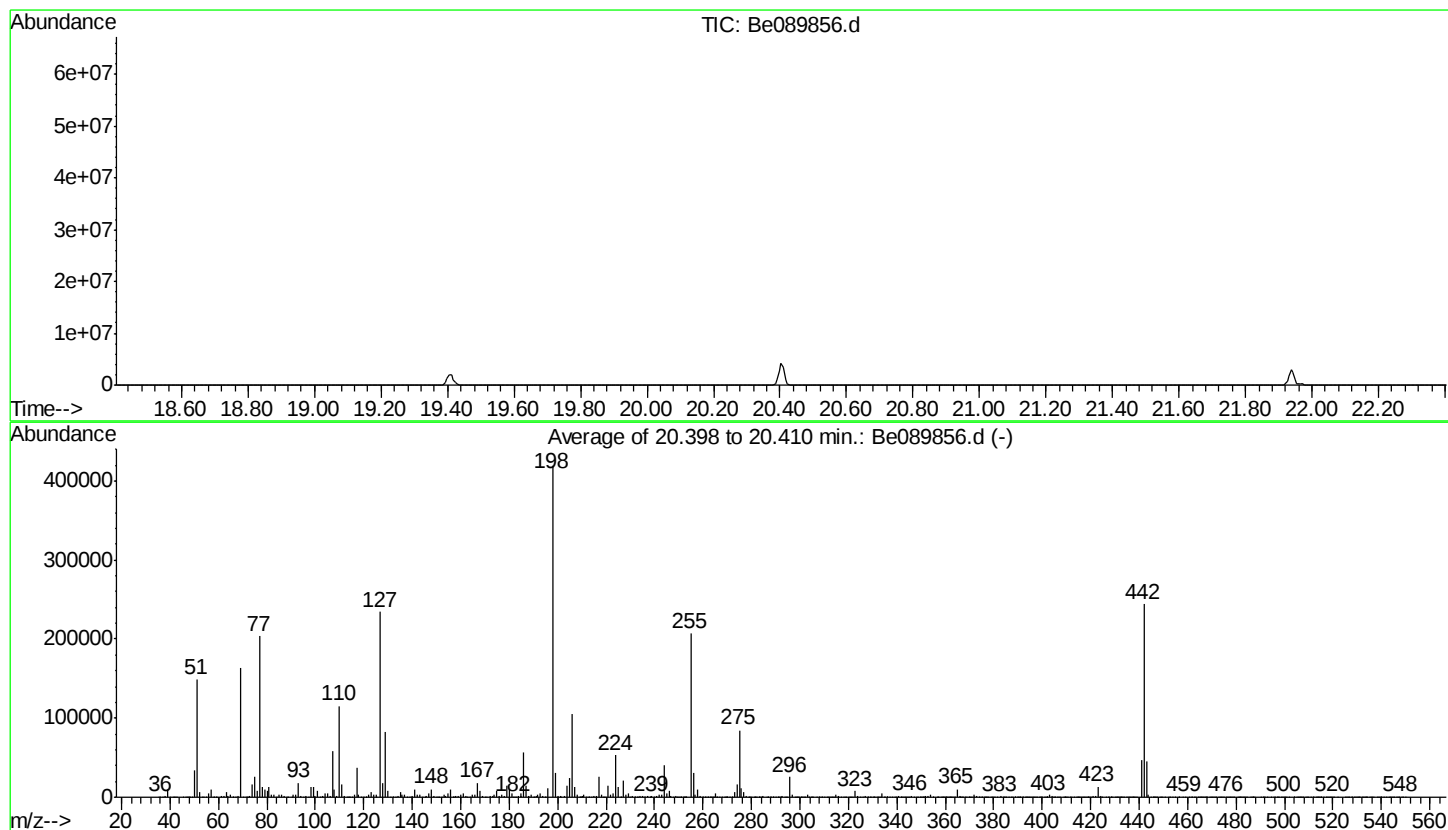

AutoFind: Scans 3235, 3236, 3237; Background Corrected with Scan 3228

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	148501	PASS
68	69	0.00	2	1.4	2338	PASS
69	198	0.00	100	39.1	163853	PASS
70	69	0.00	2	0.5	858	PASS
127	198	10	80	55.8	234084	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	419378	PASS
199	198	5	9	7.2	30217	PASS
275	198	10	60	20.1	84439	PASS
365	198	1	100	2.4	10248	PASS
441	442	0.01	24	19.5	47650	PASS
442	198	50	100	58.1	243794	PASS
443	442	15	24	18.9	45973	PASS