


Data Path : Z:\HPCHEM1\BNA E\Data\BE032618\  
 Data File : BE095831.D  
 Acq On : 26 Mar 2018 8:27  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE032318.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Mar 23 12:41:11 2018

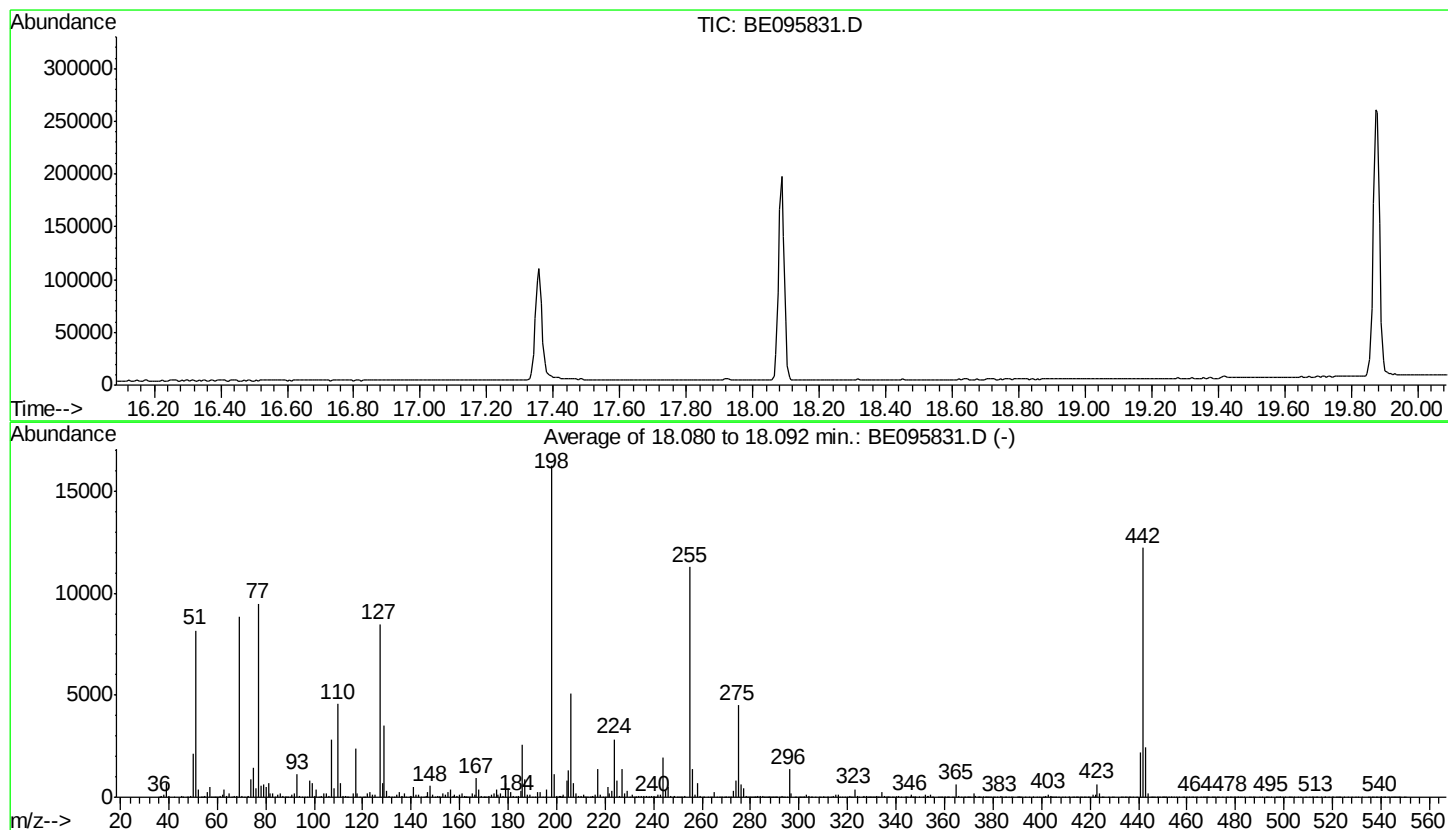

AutoFind: Scans 2637, 2638, 2639; Background Corrected with Scan 2629

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 50.2      | 8164    | PASS             |
| 68          | 69           | 0.00         | 2            | 1.0       | 89      | PASS             |
| 69          | 198          | 0.00         | 100          | 54.3      | 8823    | PASS             |
| 70          | 69           | 0.00         | 2            | 0.4       | 39      | PASS             |
| 127         | 198          | 10           | 80           | 52.1      | 8462    | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 16252   | PASS             |
| 199         | 198          | 5            | 9            | 6.9       | 1118    | PASS             |
| 275         | 198          | 10           | 60           | 27.8      | 4517    | PASS             |
| 365         | 198          | 1            | 100          | 3.7       | 601     | PASS             |
| 441         | 443          | 0.01         | 100          | 90.6      | 2213    | PASS             |
| 442         | 198          | 50           | 100          | 75.1      | 12208   | PASS             |
| 443         | 442          | 15           | 24           | 20.0      | 2443    | PASS             |