


Data Path : Z:\HPCHEM1\BNA E\Data\BE032618\
 Data File : BE095847.D
 Acq On : 26 Mar 2018 19:13
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 23 12:41:11 2018

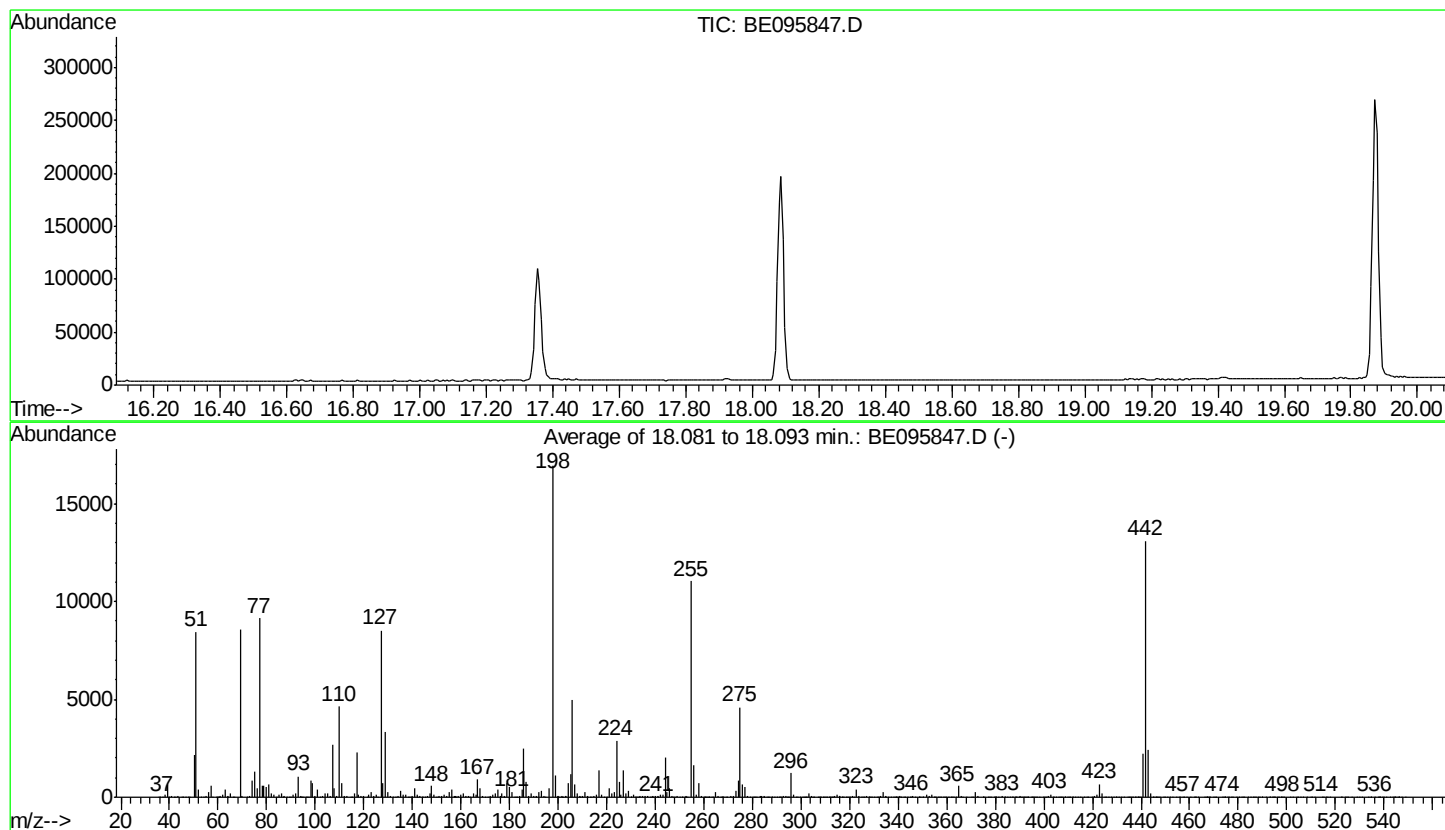

AutoFind: Scans 2637, 2638, 2639; Background Corrected with Scan 2629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.9	8454	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	50.7	8589	PASS
70	69	0.00	2	0.4	37	PASS
127	198	10	80	50.3	8529	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	16941	PASS
199	198	5	9	6.7	1142	PASS
275	198	10	60	27.2	4600	PASS
365	198	1	100	3.3	564	PASS
441	443	0.01	100	91.4	2224	PASS
442	198	50	100	77.3	13092	PASS
443	442	15	24	18.6	2433	PASS