


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032718\
 Data File : BE095865.D
 Acq On : 27 Mar 2018 9:06
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 23 12:41:11 2018

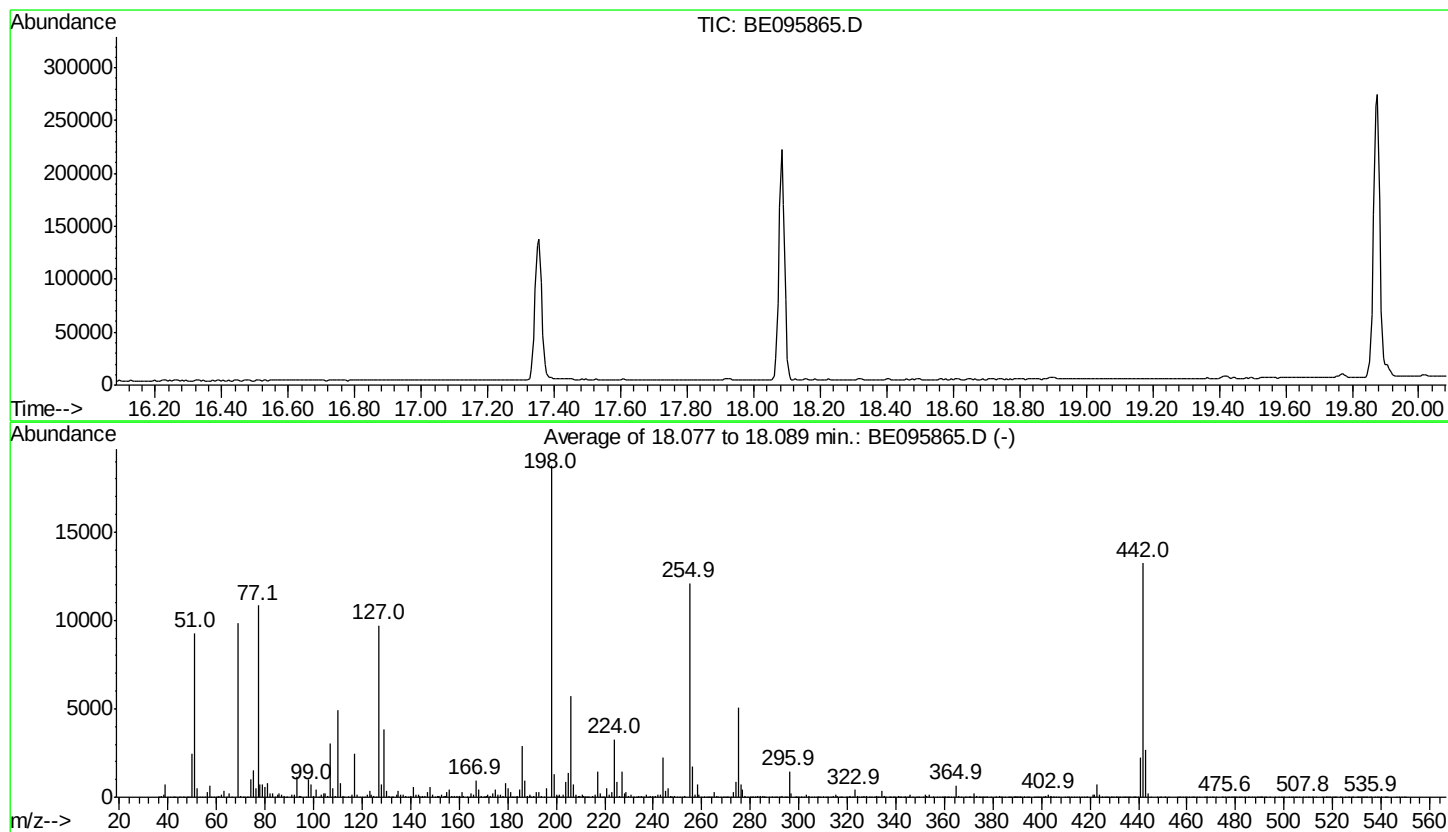

AutoFind: Scans 2636, 2637, 2638; Background Corrected with Scan 2624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.5	9273	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	52.6	9859	PASS
70	69	0.00	2	0.5	53	PASS
127	198	10	80	51.9	9733	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	18749	PASS
199	198	5	9	6.8	1279	PASS
275	198	10	60	26.9	5050	PASS
365	198	1	100	3.7	689	PASS
441	443	0.01	100	84.2	2233	PASS
442	198	50	100	70.8	13266	PASS
443	442	15	24	20.0	2651	PASS