

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE032816\
 Data File : BE091549.D
 Acq On : 28 Mar 2016 22:16
 Operator : UM/SJ
 Sample : H1855-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SB-5A

Quant Time: Mar 29 01:07:57 2016
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 25 19:00:32 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	42058	5.00	ng	0.00
6) Naphthalene-d8	10.59	136	221015	5.00	ng	0.00
10) Acenaphthene-d10	14.43	164	135663	5.00	ng	-0.01
16) Phenanthrene-d10	17.17	188	325893	5.00	ng	0.00
22) Chrysene-d12	21.34	240	321878	5.00	ng	0.00
28) Perylene-d12	23.78	264	368941	5.00	ng	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.41	112	63874	7.79	ng	-0.02
5) Phenol-d6	6.97	99	100195	8.95	ng	-0.02
7) Nitrobenzene-d5	8.97	82	40940	4.26	ng	-0.01
11) 2,4,6-Tribromophenol	15.91	330	28376	12.30	ng	-0.01
12) 2-Fluorobiphenyl	13.06	172	135583	3.55	ng	-0.01
24) Terphenyl-d14	19.78	244	216333	4.09	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) n-Nitrosodimethylamine	3.66	42	258	0.13	ng	# 4
8) Naphthalene	10.63	128	6391	0.14	ng	# 87
9) 2-Methylnaphthalene	12.25	142	5727	0.21	ng	# 91
13) Acenaphthylene	14.15	152	19127	0.40	ng	# 89
14) Acenaphthene	14.49	154	4684	0.14	ng	90
15) Fluorene	15.47	166	6082	0.15	ng	# 94
18) Pentachlorophenol	16.81	266	1321	0.50	ng	95
19) Phenanthrene	17.20	178	190238	2.55	ng	99
20) Anthracene	17.30	178	36083	0.58	ng	99
21) Fluoranthene	19.20	202	561960	8.05	ng	99
23) Pyrene	19.57	202	542969	7.14	ng	95
25) Benzo(a)anthracene	21.36	228	552660	7.44	ng	# 94
26) Chrysene	21.36	228	552510	5.66	ng	# 93
27) Indeno(1,2,3-cd)pyrene	26.35	276	169036	2.23	ng	95
29) Benzo(b)fluoranthene	23.02	252	504593	6.16	ng	97
30) Benzo(k)fluoranthene	23.02	252	504593	6.18	ng	95
31) Benzo(a)pyrene	23.55	252	181343	2.31	ng	96
32) Dibenzo(a,h)anthracene	26.36	278	39474	0.54	ng	98
33) Benzo(g,h,i)perylene	27.15	276	171410	2.26	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE032816\
Data File : BE091549.D
Acq On : 28 Mar 2016 22:16
Operator : UM/SJ
Sample : H1855-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SB-5A

Quant Time: Mar 29 01:07:57 2016
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 25 19:00:32 2016
Response via : Initial Calibration



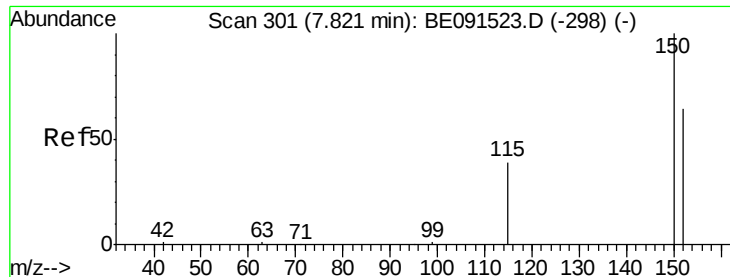

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.82 min Scan# 301

Delta R.T. 0.00 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16

Instrument :

BNA_E

ClientSampleId :

SB-5A


Tgt Ion:152 Resp: 42058

Ion Ratio Lower Upper

152 100

150 145.9 122.2 183.2




115 54.6 45.9 68.9



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E



#3

n-Nitrosodimethylamine

Concen: 0.13 ng

RT: 3.66 min Scan# 62

Delta R.T. -0.02 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16


Tgt Ion: 42 Resp: 258

Ion Ratio Lower Upper

42 100

74 0.0 84.3 126.5#



44 0.0 6.7 10.1#




Abundance Ion 42.00 (41.70 to 42.70): BE0

Ion 74.00 (73.70 to 74.70): BE0

Ion 44.00 (43.70 to 44.70): BE0





#4

2-Fluorophenol

Concen: 7.79 ng

RT: 5.41 min Scan# 163

Delta R.T. -0.02 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16

Instrument :

BNA_E

ClientSampleId :

SB-5A


Tgt Ion: 112 Resp: 63874

Ion Ratio Lower Upper

112 100

64 66.9 53.3 79.9




63 36.6 29.8 44.8



Abundance Ion 112.00 (111.70 to 112.70): BE091523.D (-157) (-)

Ion 64.00 (63.70 to 64.70): BE091523.D (-157) (-)

Ion 63.00 (62.70 to 63.70): BE091523.D (-157) (-)



#5

Phenol-d6

Concen: 8.95 ng

RT: 6.97 min Scan# 252

Delta R.T. -0.02 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16


Tgt Ion: 99 Resp: 100195

Ion Ratio Lower Upper

99 100

42 28.4 20.6 30.8



71 50.4 29.0 43.4#




Abundance Ion 99.00 (98.70 to 99.70): BE091523.D (-249) (-)

Ion 42.00 (41.70 to 42.70): BE091523.D (-249) (-)

Ion 71.00 (70.70 to 71.70): BE091523.D (-249) (-)





#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.59 min Scan# 512

Delta R.T. -0.00 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16

Instrument :

BNA_E

ClientSampleId :

SB-5A

Tgt Ion: 136 Resp: 221015


Ion Ratio Lower Upper

136 100

137 10.9 8.8 13.2

54 7.1 5.2 7.8

68 5.3 4.1 6.1






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0



#7

Nitrobenzene-d5

Concen: 4.26 ng

RT: 8.97 min Scan# 393

Delta R.T. -0.01 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16


Tgt Ion: 82 Resp: 40940

Ion Ratio Lower Upper

82 100

128 37.4 23.5 35.3#



54 43.7 52.4 78.6#




Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0





#8

Naphthalene

Concen: 0.14 ng

RT: 10.63 min Scan# 514

Delta R.T. -0.02 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16

Instrument :

BNA_E

ClientSampleId :

SB-5A


Tgt Ion:128 Resp: 6391

Ion Ratio Lower Upper

128 100

129 17.6 8.2 12.2#




127 18.0 11.8 17.8#



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E



#9

2-Methylnaphthalene

Concen: 0.21 ng

RT: 12.25 min Scan# 639

Delta R.T. -0.01 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16


Tgt Ion:142 Resp: 5727

Ion Ratio Lower Upper

142 100

141 90.1 66.9 100.3



115 39.6 25.1 37.7#




Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E





#10

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.43 min Scan# 821

Delta R.T. -0.01 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16

Instrument :

BNA_E

ClientSampleId :

SB-5A


Tgt Ion:164 Resp: 135663

Ion Ratio Lower Upper

164 100

162 97.3 84.4 126.6




160 41.2 37.7 56.5



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



#11

2,4,6-Tribromophenol

Concen: 12.30 ng

RT: 15.91 min Scan# 940

Delta R.T. -0.01 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16


Tgt Ion:330 Resp: 28376

Ion Ratio Lower Upper

330 100

332 97.1 79.2 118.8



141 41.5 28.1 42.1




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E









#12
2-Fluorobiphenyl
Concen: 3.55 ng
RT: 13.06 min Scan# 709
Delta R.T. -0.01 min
Lab File: BE091549.D
Acq: 28 Mar 2016 22:16




Instrument :
BNA_E
ClientSampleId :
SB-5A


Tgt Ion:172 Resp: 135583
Ion Ratio Lower Upper
172 100
171 30.5 29.8 44.8
170 18.2 21.4 32.2#



#13
Acenaphthylene
Concen: 0.40 ng
RT: 14.15 min Scan# 800
Delta R.T. 0.00 min
Lab File: BE091549.D
Acq: 28 Mar 2016 22:16

Tgt Ion:152 Resp: 19127
Ion Ratio Lower Upper
152 100
151 28.1 16.3 24.5#
153 15.2 11.1 16.7





#14

Acenaphthene

Concen: 0.14 ng

RT: 14.49 min Scan# 825

Delta R.T. -0.01 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16

Instrument :

BNA_E

ClientSampleId :

SB-5A


Tgt Ion:154 Resp: 4684

Ion Ratio Lower Upper

154 100

153 117.4 87.3 130.9


152 63.7 42.9 64.3





Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E



Time--> 14.40 14.50 14.60



#15

Fluorene

Concen: 0.15 ng

RT: 15.47 min Scan# 902

Delta R.T. -0.01 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16


Tgt Ion:166 Resp: 6082

Ion Ratio Lower Upper

166 100

165 104.0 79.2 118.8


167 18.3 10.8 16.2#




Abundance Ion 166.00 (165.70 to 166.70): E


Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E



Time--> 15.40 15.50









#16
Phenanthrene-d10
Concen: 5.00 ng
RT: 17.17 min Scan# 1017
Delta R.T. -0.00 min
Lab File: BE091549.D
Acq: 28 Mar 2016 22:16




Instrument :
BNA_E
ClientSampleId :
SB-5A


Tgt Ion:188 Resp: 325893
Ion Ratio Lower Upper
188 100
94 4.8 5.4 8.2#
80 4.1 5.0 7.4#



#18
Pentachlorophenol
Concen: 0.50 ng
RT: 16.81 min Scan# 994
Delta R.T. -0.02 min
Lab File: BE091549.D
Acq: 28 Mar 2016 22:16

Tgt Ion:266 Resp: 1321
Ion Ratio Lower Upper
266 100
268 66.7 48.2 72.2
264 64.4 52.1 78.1





#19

Phenanthrene

Concen: 2.55 ng

RT: 17.20 min Scan# 1020

Delta R.T. -0.00 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16

Instrument :

BNA_E

ClientSampleId :

SB-5A


Tgt Ion:178 Resp: 190238

Ion Ratio Lower Upper




178 100

176 19.5 15.5 23.3

179 15.7 13.1 19.7



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E



#20

Anthracene

Concen: 0.58 ng

RT: 17.30 min Scan# 1028

Delta R.T. -0.00 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16


Tgt Ion:178 Resp: 36083

Ion Ratio Lower Upper



178 100


176 18.0 14.9 22.3

179 15.7 12.2 18.4



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E





#21

Fluoranthene

Concen: 8.05 ng

RT: 19.20 min Scan# 1150

Delta R.T. -0.02 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16

Instrument :

BNA_E

ClientSampleId :

SB-5A


Tgt Ion: 202 Resp: 561960

Ion Ratio Lower Upper

202 100

101 10.7 8.3 12.5




203 17.1 13.9 20.9



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E



#22

Chrysene-d12

Concen: 5.00 ng

RT: 21.34 min Scan# 1248

Delta R.T. -0.00 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16


Tgt Ion: 240 Resp: 321878

Ion Ratio Lower Upper

240 100

120 0.9 4.0 6.0#



236 20.1 23.0 34.4#




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E





#23

Pyrene

Concen: 7.14 ng

RT: 19.57 min Scan# 1169

Delta R.T. -0.00 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16

Instrument :

BNA_E

ClientSampleId :

SB-5A


Tgt Ion:202 Resp: 542969

Ion Ratio Lower Upper

202 100

200 21.6 16.4 24.6




203 21.6 14.6 21.8



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E



#24

Terphenyl-d14

Concen: 4.09 ng

RT: 19.78 min Scan# 1180

Delta R.T. -0.00 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16


Tgt Ion:244 Resp: 216333

Ion Ratio Lower Upper

244 100

212 7.9 5.8 8.8



122 1.6 1.8 2.8#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E









#25
Benzo(a)anthracene
Concen: 7.44 ng
RT: 21.36 min Scan# 1249
Delta R.T. 0.05 min
Lab File: BE091549.D
Acq: 28 Mar 2016 22:16




Instrument :
BNA_E
ClientSampleId :
SB-5A


Tgt Ion:228 Resp: 552660
Ion Ratio Lower Upper
228 100
226 28.6 24.0 36.0
229 22.5 13.8 20.6#



#26
Chrysene
Concen: 5.66 ng
RT: 21.36 min Scan# 1249
Delta R.T. -0.00 min
Lab File: BE091549.D
Acq: 28 Mar 2016 22:16

Tgt Ion:228 Resp: 552510
Ion Ratio Lower Upper
228 100
226 28.6 18.9 28.3#
229 22.5 19.1 28.7









#27
 Indeno(1,2,3-cd)pyrene
 Concen: 2.23 ng
 RT: 26.35 min Scan# 1648
 Delta R.T. -0.02 min
 Lab File: BE091549.D
 Acq: 28 Mar 2016 22:16




Instrument :
 BNA_E
 ClientSampleId :
 SB-5A


Tgt Ion: 276 Resp: 169036
 Ion Ratio Lower Upper
 276 100
 138 20.9 20.2 30.4
 277 24.1 19.8 29.8



#28
 Perylene-d12
 Concen: 5.00 ng
 RT: 23.78 min Scan# 1428
 Delta R.T. -0.01 min
 Lab File: BE091549.D
 Acq: 28 Mar 2016 22:16

Tgt Ion: 264 Resp: 368941
 Ion Ratio Lower Upper
 264 100
 260 25.0 20.1 30.1
 265 22.9 18.3 27.5





#29

Benzo(b)fluoranthene

Concen: 6.16 ng

RT: 23.02 min Scan# 1362

Delta R.T. -0.01 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16

Instrument :

BNA_E

ClientSampleId :

SB-5A


Tgt Ion:252 Resp: 504593

Ion Ratio Lower Upper

252 100

253 21.8 18.7 28.1




125 11.2 9.8 14.6



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



#30

Benzo(k)fluoranthene

Concen: 6.18 ng

RT: 23.02 min Scan# 1362

Delta R.T. -0.06 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16


Tgt Ion:252 Resp: 504593

Ion Ratio Lower Upper

252 100

253 21.8 20.2 30.4



125 11.2 9.4 14.2




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E





#31

Benzo(a)pyrene

Concen: 2.31 ng

RT: 23.55 min Scan# 1408

Delta R.T. -0.13 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16

Instrument :

BNA_E

ClientSampleId :

SB-5A


Tgt Ion:252 Resp: 181343

Ion Ratio Lower Upper

252 100

253 21.5 19.4 29.0




125 15.1 11.4 17.2



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



#32

Dibenzo(a,h)anthracene

Concen: 0.54 ng

RT: 26.36 min Scan# 1649

Delta R.T. -0.03 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16


Tgt Ion:278 Resp: 39474

Ion Ratio Lower Upper

278 100

139 18.9 14.2 21.4



279 25.2 19.6 29.4




Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E





#33

Benzo(g,h,i)perylene

Concen: 2.26 ng

RT: 27.15 min Scan# 1717

Delta R.T. -0.01 min

Lab File: BE091549.D

Acq: 28 Mar 2016 22:16

Instrument :

BNA_E

ClientSampleId :

SB-5A


Tgt Ion: 276 Resp: 171410

Ion Ratio Lower Upper

276 100

277 24.7 19.4 29.2

138 20.8 18.2 27.4



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

