

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE032816\
 Data File : BE091541.D
 Acq On : 28 Mar 2016 15:57
 Operator : UM/SJ
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC0.4EC

Manual Integrations
 APPROVED

Sohil
 3/29/2016 5:05:46 PM

Quant Time: Mar 29 01:17:19 2016
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 25 19:00:32 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	33073	5.00	ng	0.00
6) Naphthalene-d8	10.59	136	157726	5.00	ng	0.00
10) Acenaphthene-d10	14.43	164	90173	5.00	ng	-0.01
16) Phenanthrene-d10	17.17	188	237725	5.00	ng	0.00
22) Chrysene-d12	21.34	240	238198	5.00	ng	0.00
28) Perylene-d12	23.78	264	259341	5.00	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.41	112	2553	0.40	ng	-0.02
5) Phenol-d6	6.97	99	3357	0.38	ng	-0.02
7) Nitrobenzene-d5	8.97	82	2702	0.39	ng	-0.01
11) 2,4,6-Tribromophenol	15.91	330	624m	0.41	ng	-0.01
12) 2-Fluorobiphenyl	13.06	172	10102	0.40	ng	-0.01
24) Terphenyl-d14	19.78	244	16067	0.41	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.37	88	1814	0.41	ng	# 96
3) n-Nitrosodimethylamine	3.68	42	1562	0.41	ng	# 94
8) Naphthalene	10.65	128	12797	0.40	ng	# 93
9) 2-Methylnaphthalene	12.25	142	7566	0.38	ng	# 88
13) Acenaphthylene	14.15	152	11972	0.38	ng	97
14) Acenaphthene	14.49	154	9127	0.41	ng	99
15) Fluorene	15.47	166	10649	0.39	ng	100
17) Hexachlorobenzene	16.48	284	3242m	0.39	ng	
18) Pentachlorophenol	16.81	266	828	0.46	ng	98
19) Phenanthrene	17.21	178	21673	0.40	ng	100
20) Anthracene	17.30	178	17061	0.38	ng	100
21) Fluoranthene	19.21	202	19613	0.39	ng	99
23) Pyrene	19.57	202	21790	0.39	ng	97
25) Benzo(a)anthracene	21.31	228	21632m	0.39	ng	
26) Chrysene	21.36	228	30050m	0.42	ng	
27) Indeno(1,2,3-cd)pyrene	26.36	276	22234	0.40	ng	99
29) Benzo(b)fluoranthene	23.02	252	23703	0.41	ng	98
30) Benzo(k)fluoranthene	23.08	252	20006	0.35	ng	98
31) Benzo(a)pyrene	23.67	252	17371	0.49	ng	98
32) Dibenzo(a,h)anthracene	26.39	278	18932	0.37	ng	98
33) Benzo(g,h,i)perylene	27.15	276	19745	0.37	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE032816\
Data File : BE091541.D
Acq On : 28 Mar 2016 15:57
Operator : UM/SJ
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4EC

Manual Integrations
APPROVED

Sohil
3/29/2016 5:05:46 PM

Quant Time: Mar 29 01:17:19 2016
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 25 19:00:32 2016
Response via : Initial Calibration

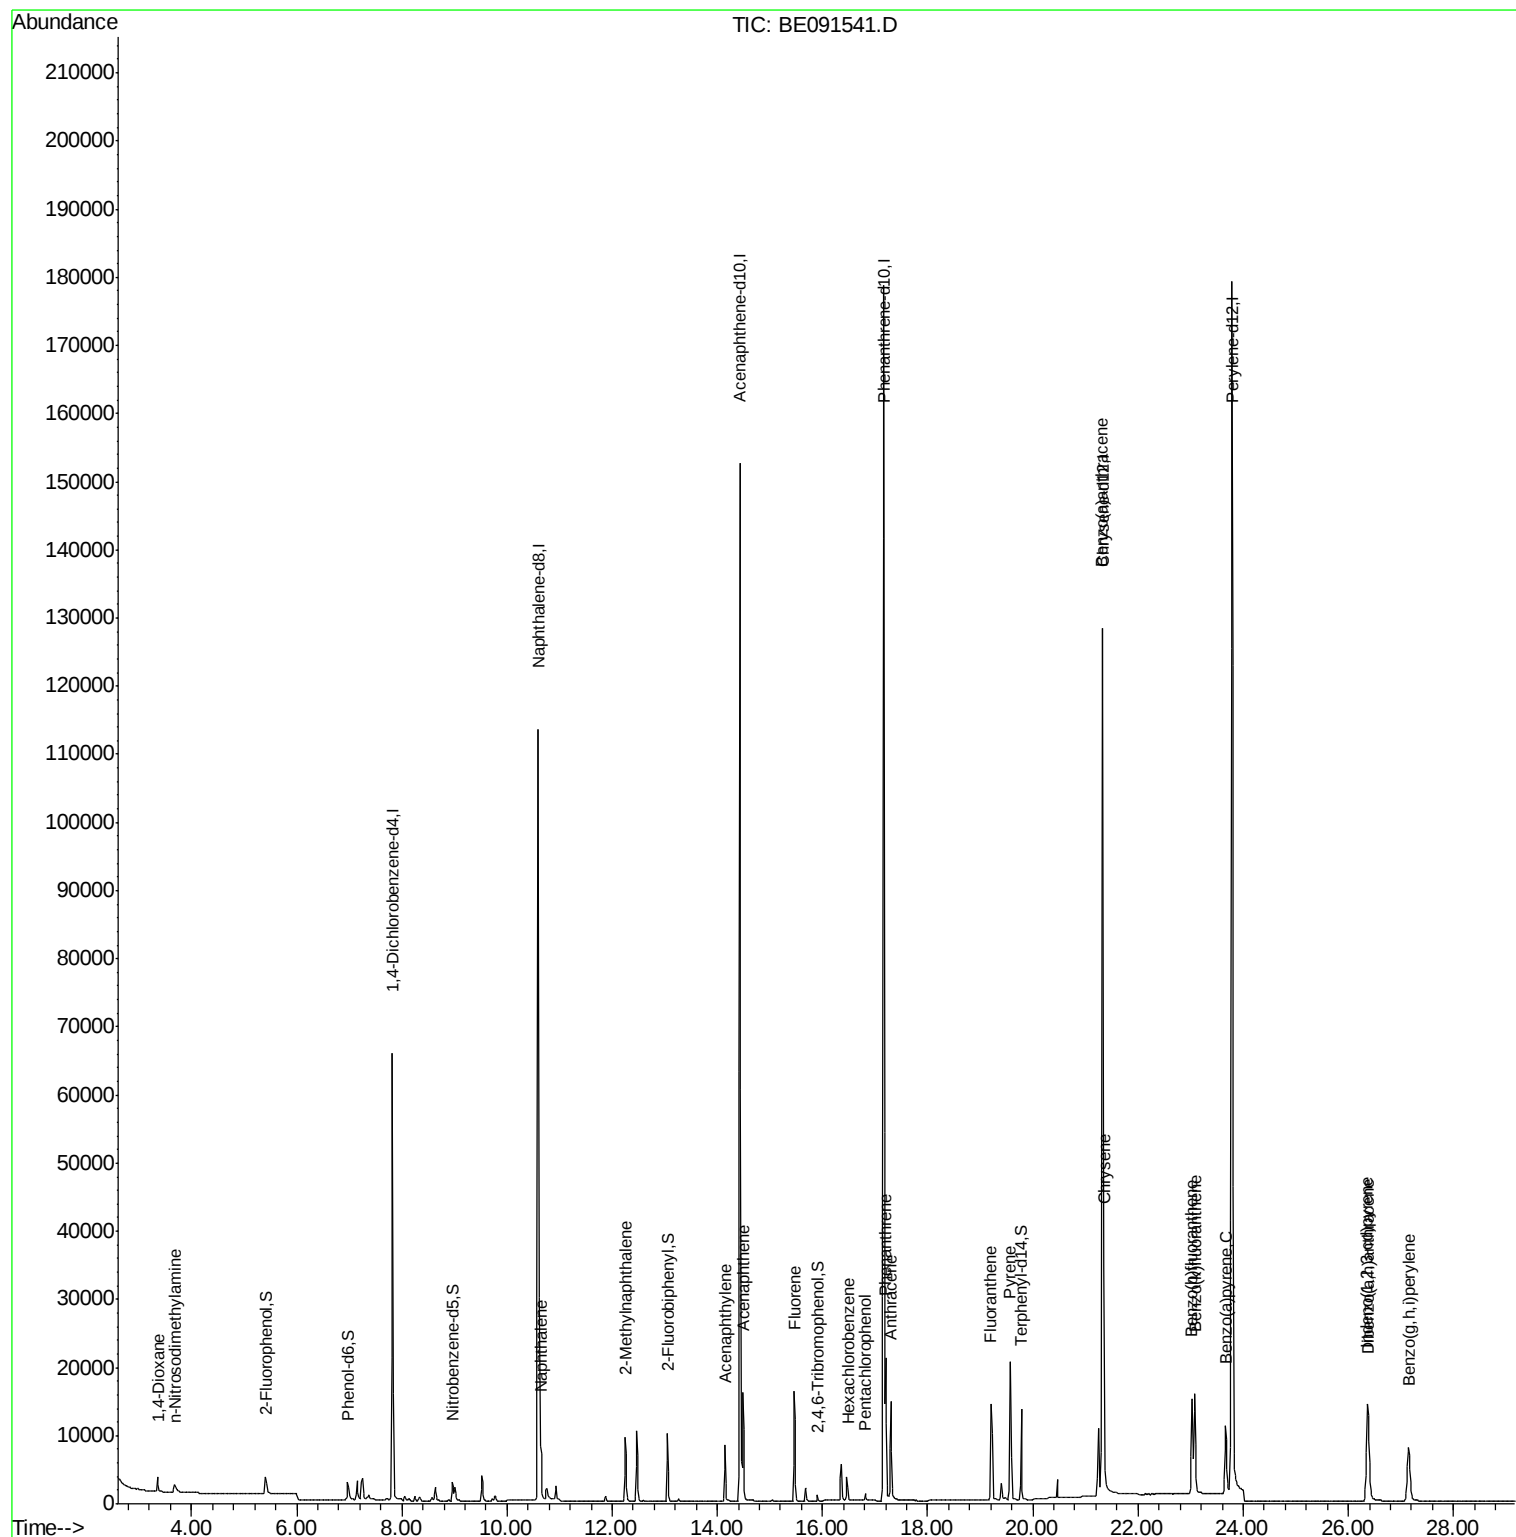

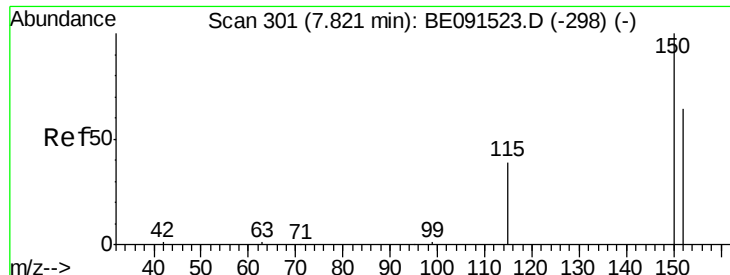





#1
 1,4-Dichlorobenzene-d4
 Concen: 5.00 ng
 RT: 7.82 min Scan# 301
 Delta R.T. 0.00 min
 Lab File: BE091541.D
 Acq: 28 Mar 2016 15:57

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion	Ratio	Lower	Upper
152	100		
150	153.4	122.2	183.2
115	60.0	45.9	68.9




Manual Integrations
 APPROVED


Sohil
 3/29/2016 5:05:46 PM

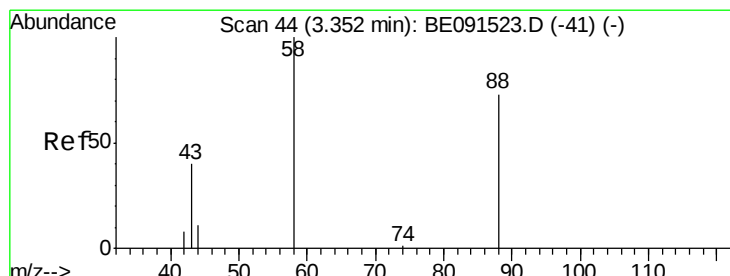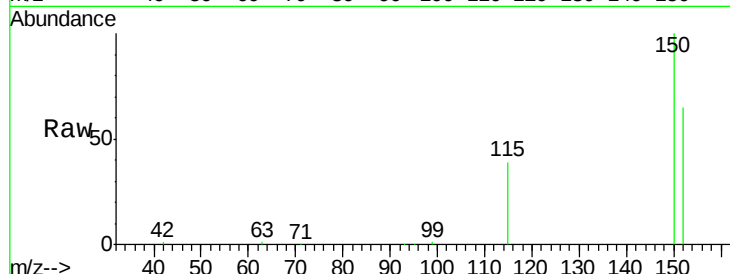

#2
 1,4-Dioxane
 Concen: 0.41 ng
 RT: 3.37 min Scan# 45
 Delta R.T. 0.00 min
 Lab File: BE091541.D
 Acq: 28 Mar 2016 15:57

Tgt Ion	Ratio	Lower	Upper
88	100		
58	76.8	61.0	91.6
43	39.0	25.4	38.2

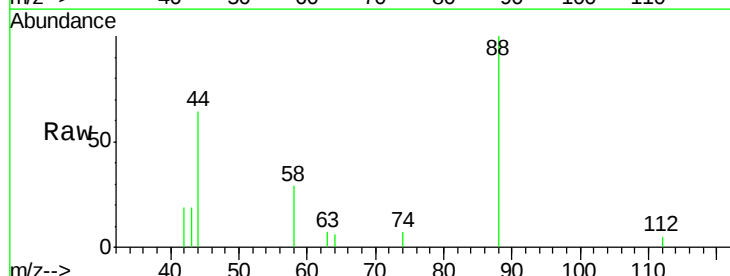

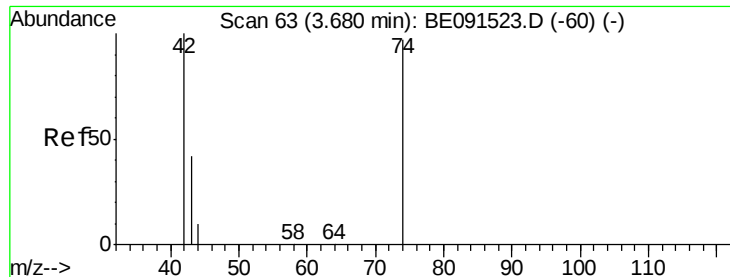

#3





n-Nitrosodimethylamine
Concen: 0.41 ng
RT: 3.68 min Scan# 63
Delta R.T. 0.00 min
Lab File: BE091541.D
Acq: 28 Mar 2016 15:57

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion	Ratio	Lower	Upper
42	100		
74	100.4	84.3	126.5
44	14.5	6.7	10.1

Manual Integrations
APPROVED




Sohil
3/29/2016 5:05:46 PM

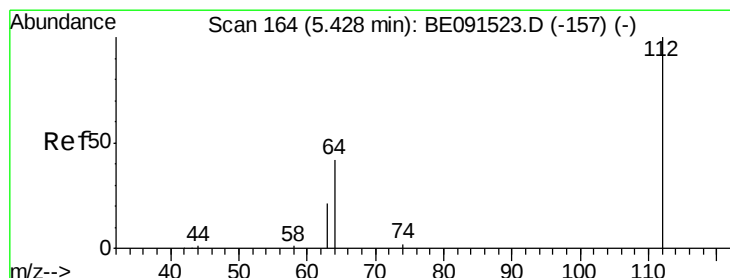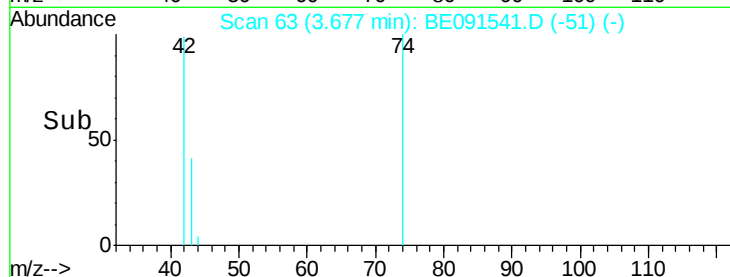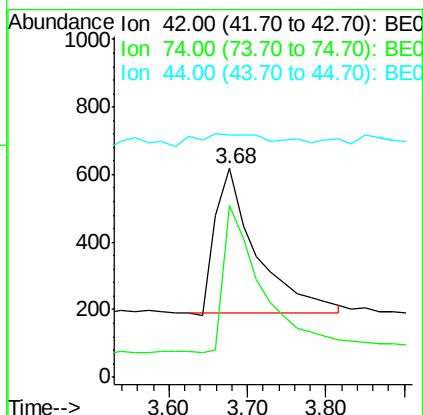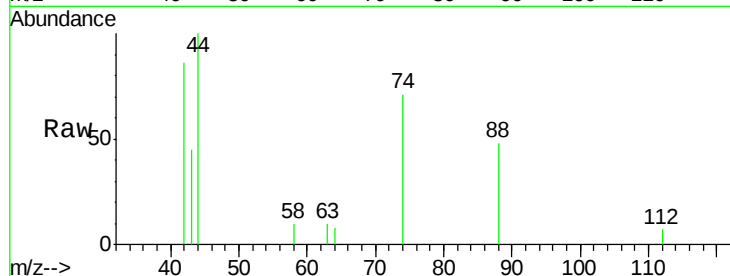


#4

2-Fluorophenol
Concen: 0.40 ng
RT: 5.41 min Scan# 163
Delta R.T. -0.02 min
Lab File: BE091541.D
Acq: 28 Mar 2016 15:57

Tgt Ion	Ratio	Lower	Upper
112	100		
64	70.6	53.3	79.9
63	38.3	29.8	44.8

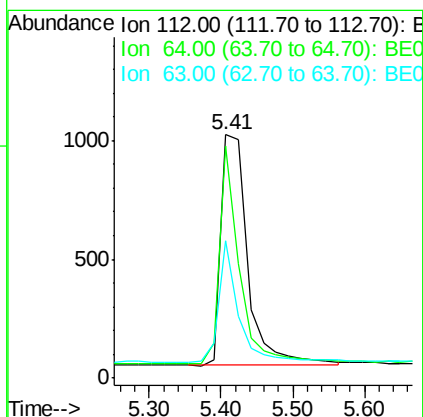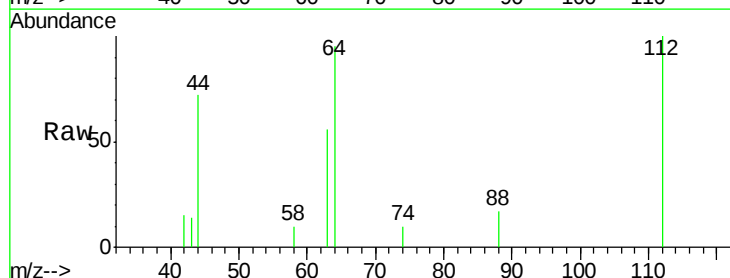



#5

Phenol-d6

Concen: 0.38 ng

RT: 6.97 min Scan# 252

Delta R.T. -0.02 min

Lab File: BE091541.D

Acq: 28 Mar 2016 15:57

Instrument :

BNA_E


ClientSampleId :

SSTDCCC0.4EC




Tgt Ion:	99	Resp:	3357
Ion Ratio	Lower	Upper	
99	100		
42	28.6	20.6	30.8
71	36.6	29.0	43.4

Manual Integrations
APPROVED

Sohil
3/29/2016 5:05:46 PM



Abundance Ion 99.00 (98.70 to 99.70): BE0
Ion 42.00 (41.70 to 42.70): BE0
Ion 71.00 (70.70 to 71.70): BE0

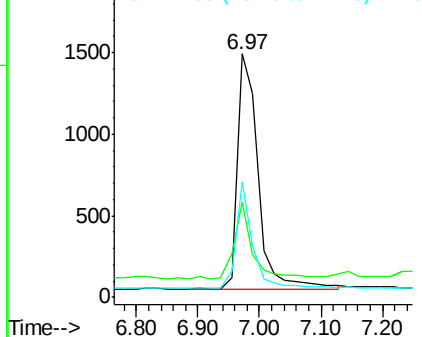

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.59 min Scan# 512




Delta R.T. 0.00 min


Lab File: BE091541.D

Acq: 28 Mar 2016 15:57

Tgt Ion:	136	Resp:	157726
Ion Ratio	Lower	Upper	
136	100		
137	10.9	8.8	13.2
54	7.3	5.2	7.8
68	5.3	4.1	6.1

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BE0
Ion 68.00 (67.70 to 68.70): BE0

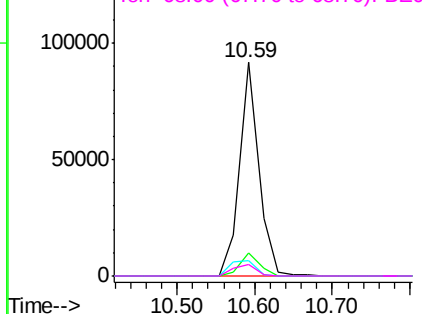



#7

Nitrobenzene-d5

Concen: 0.39 ng

RT: 8.97 min Scan# 393

Delta R.T. -0.01 min

Lab File: BE091541.D

Acq: 28 Mar 2016 15:57

Instrument :

BNA_E


ClientSampleId :

SSTDCCC0.4EC

Tgt Ion:	82	Resp:	2702
Ion Ratio	Lower	Upper	
82	100		
128	31.7	23.5	35.3
54	61.9	52.4	78.6

Manual Integrations
APPROVED




Sohil
3/29/2016 5:05:46 PM



Abundance Ion 82.00 (81.70 to 82.70): BE091541.D (-377) (-)

Ion 128.00 (127.70 to 128.70): BE091541.D (-377) (-)

Ion 54.00 (53.70 to 54.70): BE091541.D (-377) (-)

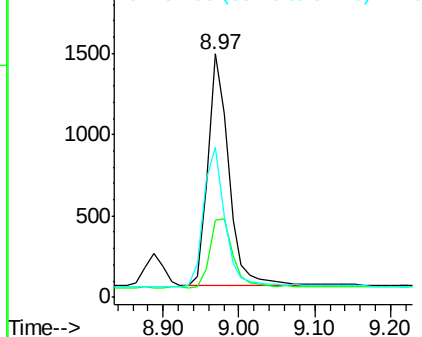

#8

Naphthalene

Concen: 0.40 ng

RT: 10.65 min Scan# 515

Delta R.T. 0.00 min

Lab File: BE091541.D




Acq: 28 Mar 2016 15:57


Tgt Ion:	128	Resp:	12797
Ion Ratio	Lower	Upper	
128	100		
129	12.8	8.2	12.2#
127	11.8	11.8	17.8#

Abundance Ion 128.00 (127.70 to 128.70): BE091541.D (-505) (-)

Ion 129.00 (128.70 to 129.70): BE091541.D (-505) (-)

Ion 127.00 (126.70 to 127.70): BE091541.D (-505) (-)

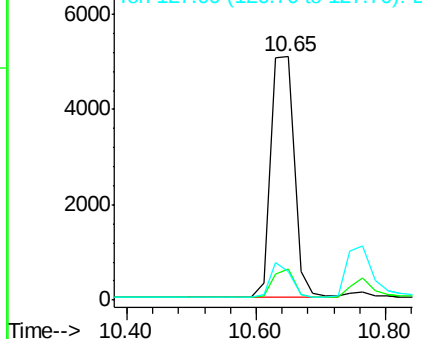

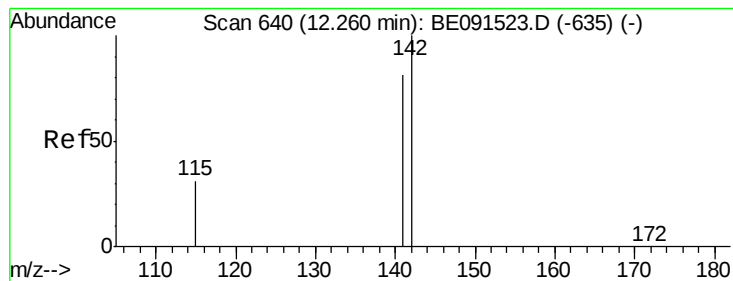

#9

2-Methylnaphthalene

Concen: 0.38 ng

RT: 12.25 min Scan# 639

Delta R.T. -0.01 min

Lab File: BE091541.D

Acq: 28 Mar 2016 15:57

Instrument :

BNA_E





ClientSampleId :

SSTDCCC0.4EC

Tgt Ion:	142	Resp:	7566
Ion Ratio	Lower	Upper	
142	100		
141	93.0	66.9	100.3
115	40.2	25.1	37.7#

Manual Integrations
APPROVED

Sohil
3/29/2016 5:05:46 PM

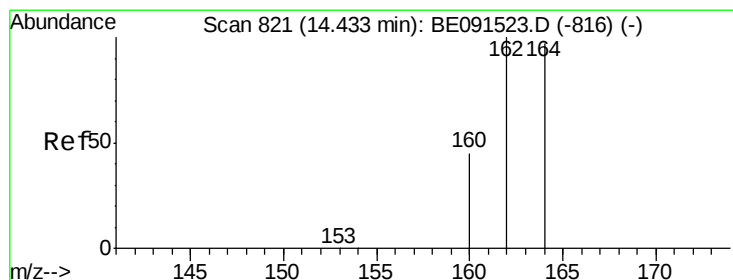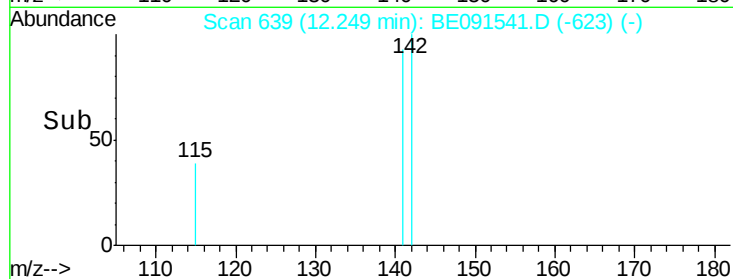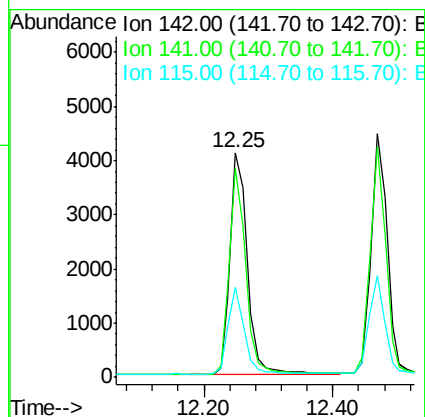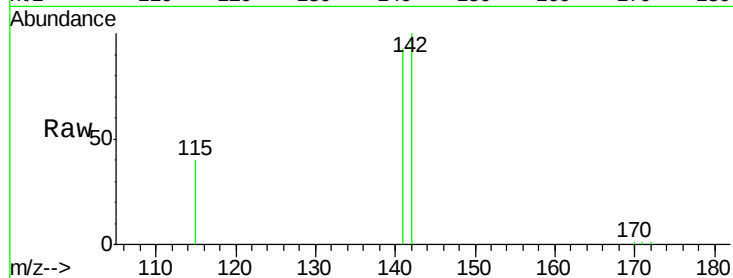

#10

Acenaphthene-d10

Concen: 5.00 ng




RT: 14.43 min Scan# 821


Delta R.T. -0.01 min

Lab File: BE091541.D

Acq: 28 Mar 2016 15:57

Tgt Ion:	164	Resp:	90173
Ion Ratio	Lower	Upper	
164	100		
162	105.9	84.4	126.6
160	47.7	37.7	56.5

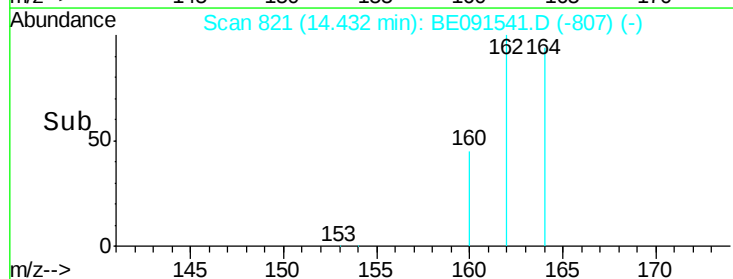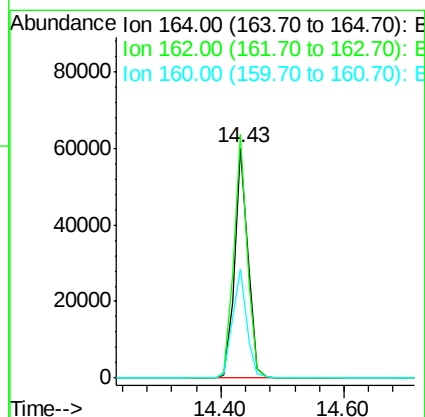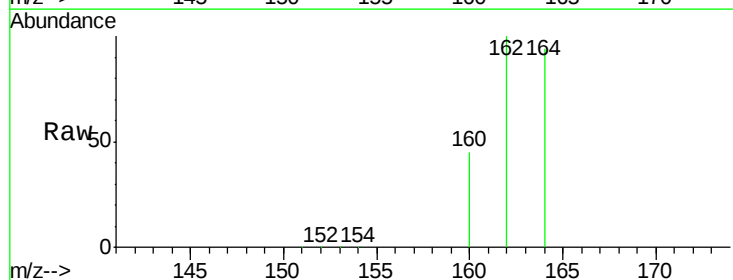

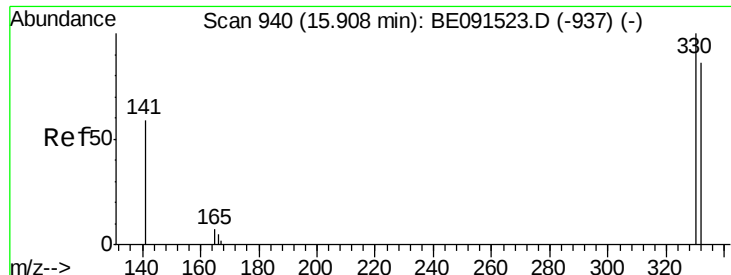





#11
 2,4,6-Tribromophenol
 Concen: 0.41 ng m
 RT: 15.91 min Scan# 940
 Delta R.T. -0.01 min
 Lab File: BE091541.D
 Acq: 28 Mar 2016 15:57

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion	Ratio	Lower	Upper
330	100		
332	177.6	79.2	118.8#
141	52.6	28.1	42.1#




Manual Integrations
 APPROVED


Sohil
 3/29/2016 5:05:46 PM

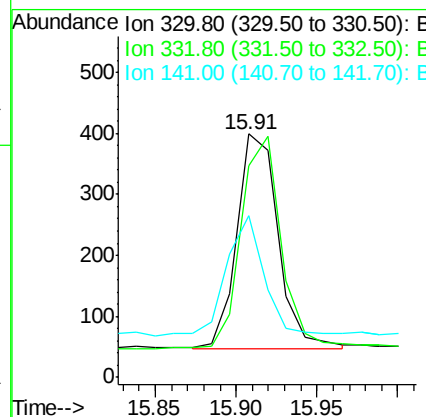

#12
 2-Fluorobiphenyl
 Concen: 0.40 ng
 RT: 13.06 min Scan# 709
 Delta R.T. -0.01 min
 Lab File: BE091541.D
 Acq: 28 Mar 2016 15:57

Tgt Ion	Ratio	Lower	Upper
172	100		
171	33.1	29.8	44.8
170	22.0	21.4	32.2

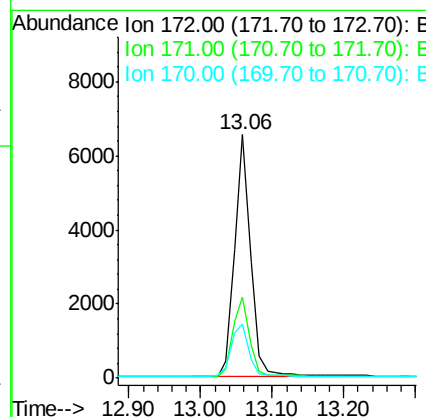



#13

Acenaphthylene

Concen: 0.38 ng

RT: 14.15 min Scan# 800

Delta R.T. 0.00 min

Lab File: BE091541.D

Acq: 28 Mar 2016 15:57

Instrument :

BNA_E





ClientSampleId :

SSTDCCC0.4EC

Tgt Ion:	152	Resp:	11972
Ion Ratio	Lower	Upper	
152	100		
151	18.6	16.3	24.5
153	12.8	11.1	16.7

Manual Integrations
APPROVED

Sohil
3/29/2016 5:05:46 PM

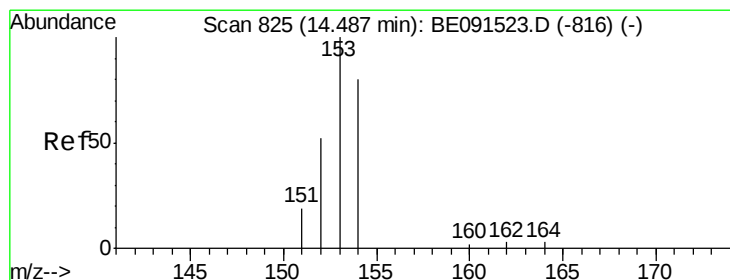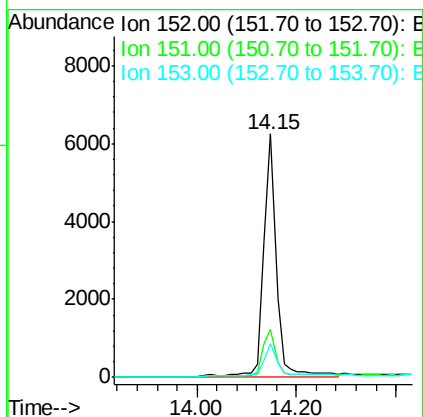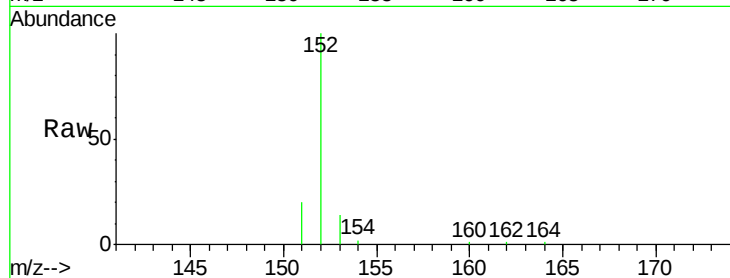

#14

Acenaphthene

Concen: 0.41 ng




RT: 14.49 min Scan# 825


Delta R.T. -0.01 min

Lab File: BE091541.D

Acq: 28 Mar 2016 15:57

Tgt Ion:	154	Resp:	9127
Ion Ratio	Lower	Upper	
154	100		
153	108.1	87.3	130.9
152	54.6	42.9	64.3

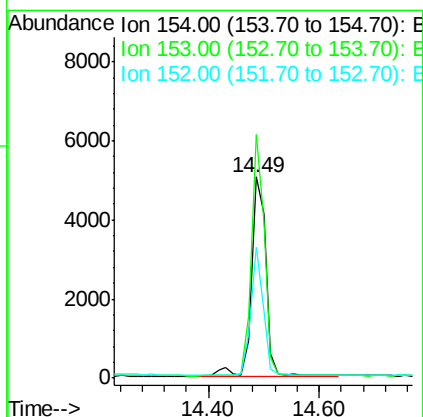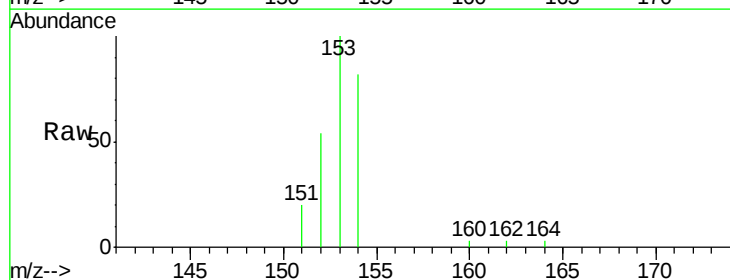



#15

Fluorene

Concen: 0.39 ng

RT: 15.47 min Scan# 902

Delta R.T. -0.01 min

Lab File: BE091541.D

Acq: 28 Mar 2016 15:57

Instrument :

BNA_E


ClientSampleId :

SSTDCCC0.4EC




Manual Integrations
APPROVED

Sohil

3/29/2016 5:05:46 PM

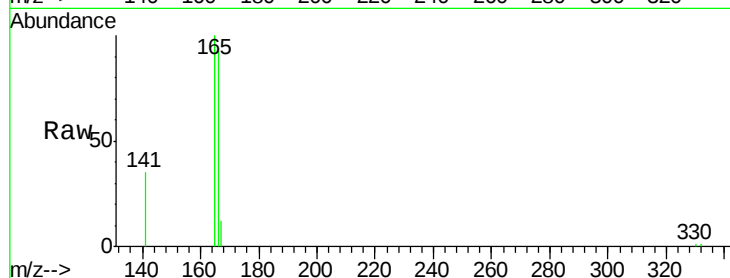

Tgt Ion:	166	Resp:	10649
Ion Ratio	Lower	Upper	
166	100		
165	99.2	79.2	118.8
167	13.5	10.8	16.2

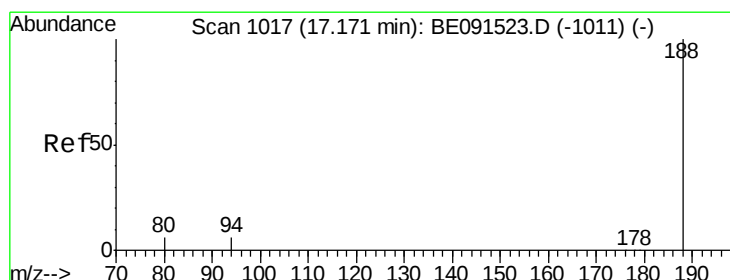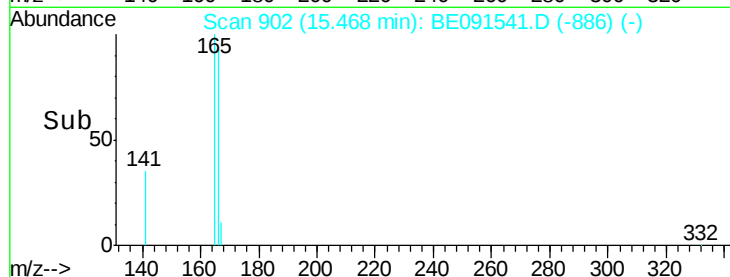

#16

Phenanthrene-d10

Concen: 5.00 ng




RT: 17.17 min Scan# 1018


Delta R.T. -0.00 min

Lab File: BE091541.D

Acq: 28 Mar 2016 15:57

Tgt Ion:	188	Resp:	237725
Ion Ratio	Lower	Upper	
188	100		
94	5.5	5.4	8.2
80	4.8	5.0	7.4#

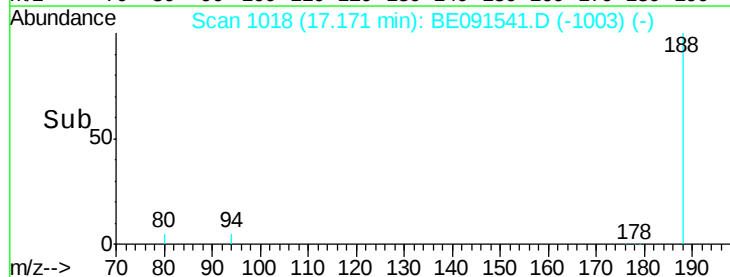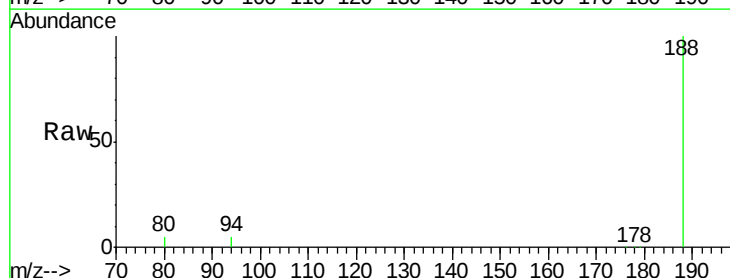

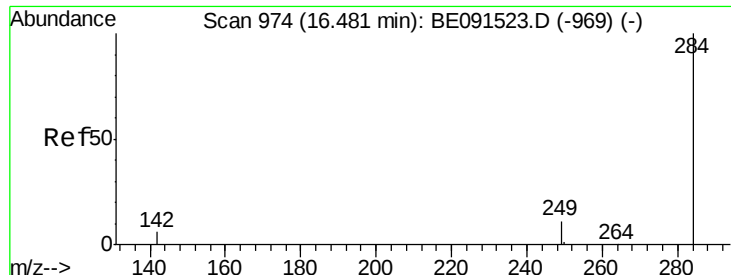





#17
Hexachlorobenzene
Concen: 0.39 ng m
RT: 16.48 min Scan# 975
Delta R.T. -0.00 min
Lab File: BE091541.D
Acq: 28 Mar 2016 15:57

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion	Ratio	Lower	Upper
284	100		
142	43.3	31.0	46.4
249	32.9	25.8	38.8




Manual Integrations
APPROVED


Sohil
3/29/2016 5:05:46 PM



#18
Pentachlorophenol
Concen: 0.46 ng
RT: 16.81 min Scan# 994
Delta R.T. -0.02 min
Lab File: BE091541.D
Acq: 28 Mar 2016 15:57

Tgt Ion	Ratio	Lower	Upper
266	100		
268	62.2	48.2	72.2
264	66.5	52.1	78.1



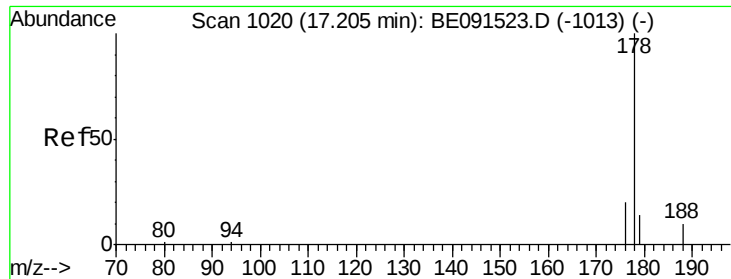





#19
Phenanthrene
Concen: 0.40 ng
RT: 17.21 min Scan# 1021
Delta R.T. -0.00 min
Lab File: BE091541.D
Acq: 28 Mar 2016 15:57

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion	Ratio	Lower	Upper
178	100		
176	19.4	15.5	23.3
179	16.3	13.1	19.7




Manual Integrations
APPROVED


Sohil
3/29/2016 5:05:46 PM

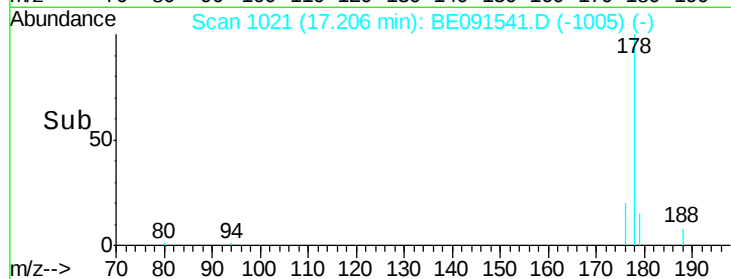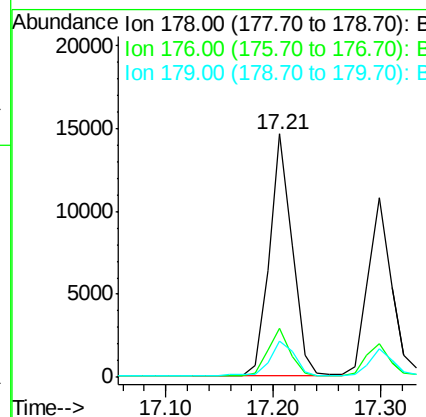

#20
Anthracene
Concen: 0.38 ng
RT: 17.30 min Scan# 1029
Delta R.T. -0.00 min
Lab File: BE091541.D
Acq: 28 Mar 2016 15:57

Tgt Ion	Ratio	Lower	Upper
178	100		
176	18.7	14.9	22.3
179	15.2	12.2	18.4

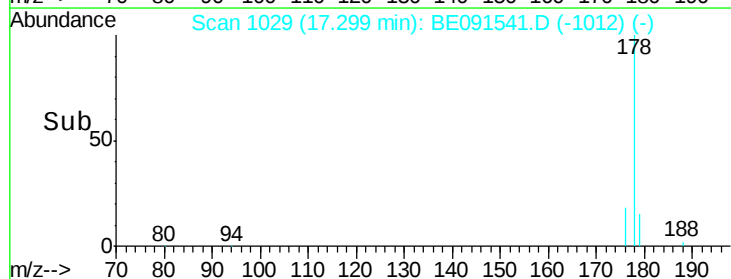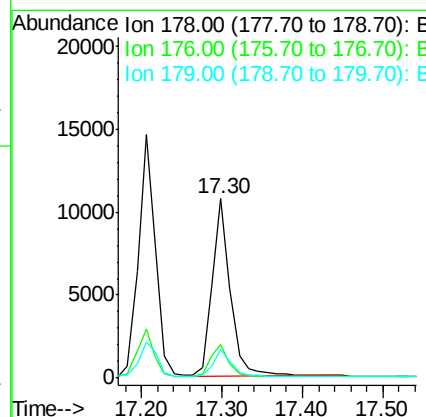

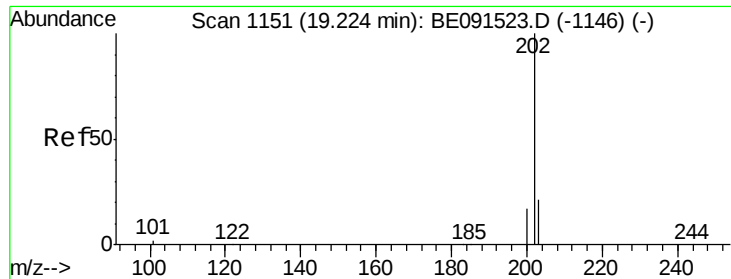


#21
 Fluoranthene
 Concen: 0.39 ng
 RT: 19.21 min Scan# 1151
 Delta R.T. -0.02 min
 Lab File: BE091541.D
 Acq: 28 Mar 2016 15:57

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC0.4EC

Tgt	Ion	Ratio	Resp	Lower	Upper
202	100		19613		
101	11.2	8.3	12.5		
203	17.3	13.9	20.9		

Manual Integrations
 APPROVED

Sohil
 3/29/2016 5:05:46 PM






Abundance

Ion 202.00 (201.70 to 202.70): E


Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

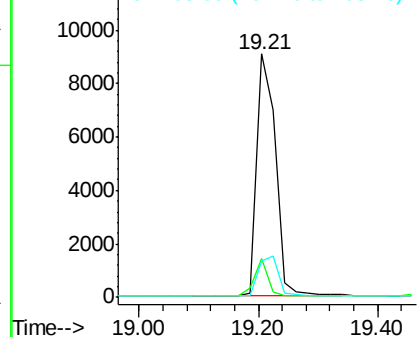

#22
 Chrysene-d12
 Concen: 5.00 ng
 RT: 21.34 min Scan# 1249
 Delta R.T. -0.00 min
 Lab File: BE091541.D
 Acq: 28 Mar 2016 15:57

Tgt	Ion	Ratio	Resp	Lower	Upper
240	100		238198		
120	1.0	4.0	6.0#		
236	21.2	23.0	34.4#		






Abundance

Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

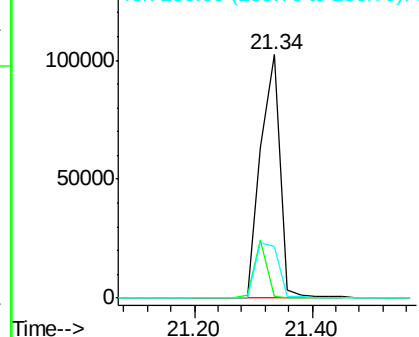







#23
Pyrene
Concen: 0.39 ng
RT: 19.57 min Scan# 1170
Delta R.T. -0.00 min
Lab File: BE091541.D
Acq: 28 Mar 2016 15:57

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion	Ratio	Lower	Upper
202	100		
200	21.9	16.4	24.6
203	17.3	14.6	21.8




Manual Integrations
APPROVED


Sohil
3/29/2016 5:05:46 PM

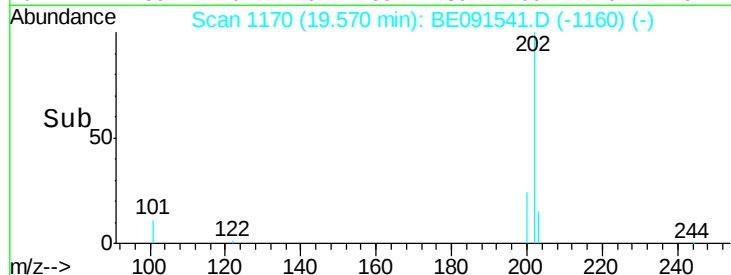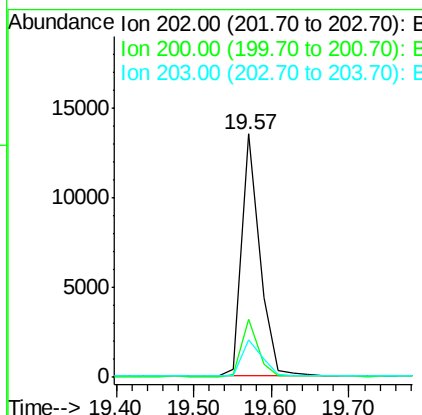

#24
Terphenyl-d14
Concen: 0.41 ng
RT: 19.78 min Scan# 1181
Delta R.T. -0.00 min
Lab File: BE091541.D
Acq: 28 Mar 2016 15:57

Tgt Ion	Ratio	Lower	Upper
244	100		
212	8.5	5.8	8.8
122	3.3	1.8	2.8









#25
Benzo(a)anthracene
Concen: 0.39 ng m
RT: 21.31 min Scan# 1248
Delta R.T. -0.00 min
Lab File: BE091541.D
Acq: 28 Mar 2016 15:57

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion	Ratio	Lower	Upper
228	100		
226	21.6	24.0	36.0#
229	22.6	13.8	20.6#




Manual Integrations
APPROVED


Sohil
3/29/2016 5:05:46 PM

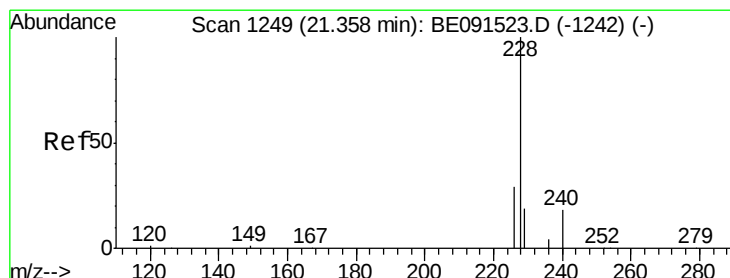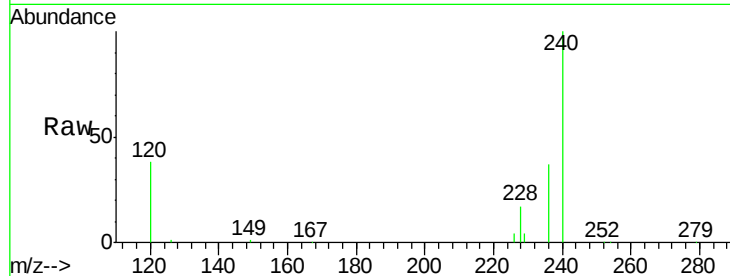

#26
Chrysene
Concen: 0.42 ng m
RT: 21.36 min Scan# 1250
Delta R.T. -0.00 min
Lab File: BE091541.D
Acq: 28 Mar 2016 15:57

Tgt Ion	Ratio	Lower	Upper
228	100		
226	28.5	18.9	28.3#
229	19.3	19.1	28.7

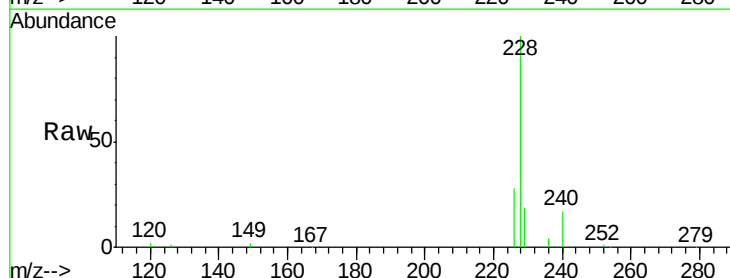

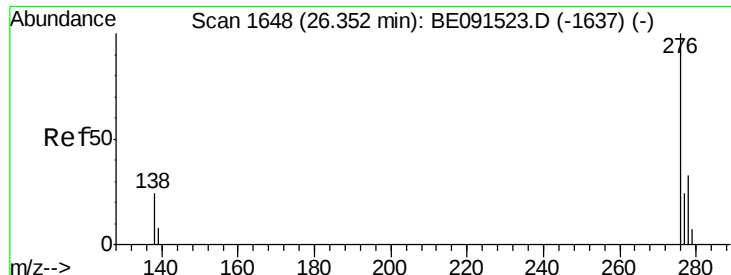


#27
 Indeno(1,2,3-cd)pyrene
 Concen: 0.40 ng
 RT: 26.36 min Scan# 1650
 Delta R.T. -0.01 min
 Lab File: BE091541.D
 Acq: 28 Mar 2016 15:57

Instrument :
 BNA_E
 ClientSampleId :
 SSTCCCC0.4EC

Tgt Ion	Ratio	Resp Lower	Resp Upper
276	100		
138	26.1	20.2	30.4
277	24.8	19.8	29.8

Manual Integrations
 APPROVED

Sohil
 3/29/2016 5:05:46 PM






Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

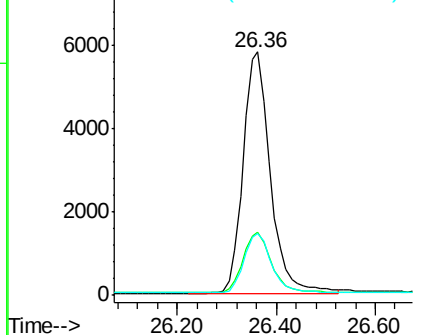

#28
 Perylene-d12
 Concen: 5.00 ng
 RT: 23.78 min Scan# 1429
 Delta R.T. -0.01 min
 Lab File: BE091541.D
 Acq: 28 Mar 2016 15:57




Tgt Ion	Ratio	Resp Lower	Resp Upper
264	100		
260	24.9	20.1	30.1
265	21.9	18.3	27.5


Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

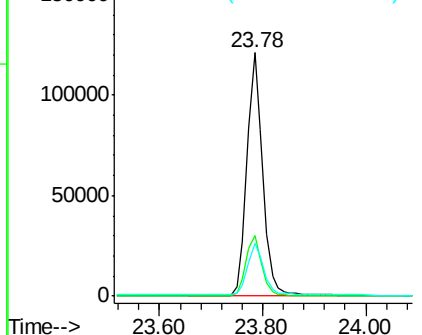

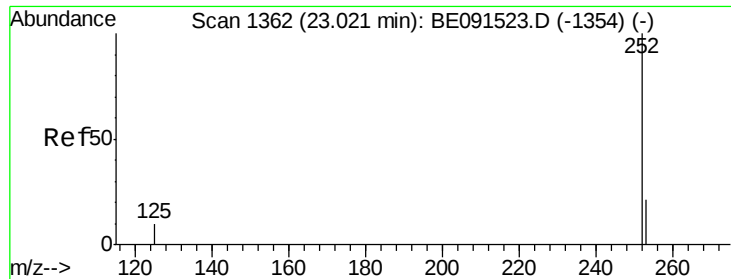

#29

Benzo(b)fluoranthene

Concen: 0.41 ng

RT: 23.02 min Scan# 1363

Delta R.T. -0.01 min

Lab File: BE091541.D


Acq: 28 Mar 2016 15:57

Instrument :

BNA_E

ClientSampleId :



SSTDCCC0.4EC



Tgt Ion:	252	Resp:	23703
Ion Ratio	Lower	Upper	
252	100		
253	21.9	18.7	28.1
125	12.7	9.8	14.6

Manual Integrations
APPROVED

Sohil
3/29/2016 5:05:46 PM

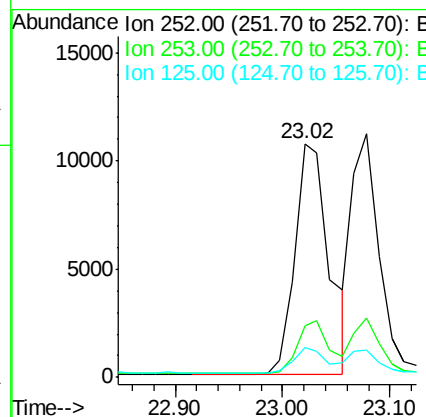

#30

Benzo(k)fluoranthene


Concen: 0.35 ng

RT: 23.08 min Scan# 1368



Delta R.T. -0.00 min


Lab File: BE091541.D

Acq: 28 Mar 2016 15:57



Tgt Ion:	252	Resp:	20006
Ion Ratio	Lower	Upper	
252	100		
253	24.1	20.2	30.4
125	11.0	9.4	14.2

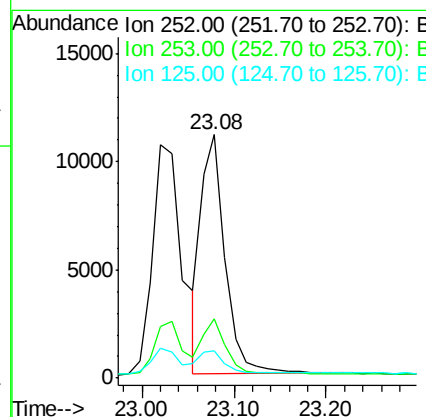

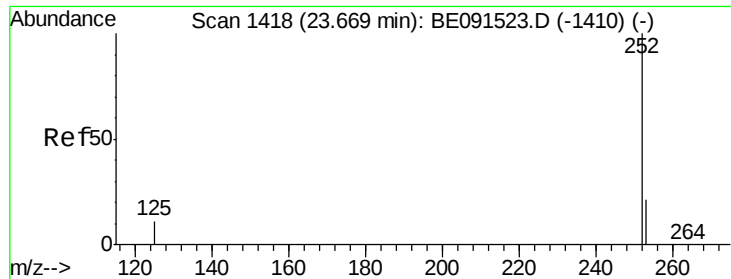





#31
Benzo(a)pyrene
Concen: 0.49 ng
RT: 23.67 min Scan# 1419
Delta R.T. -0.01 min
Lab File: BE091541.D
Acq: 28 Mar 2016 15:57

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.0	19.4	29.0
125	14.2	11.4	17.2




Manual Integrations
APPROVED


Sohil
3/29/2016 5:05:46 PM

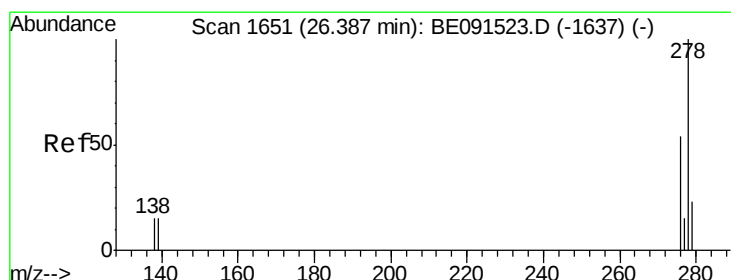

#32
Dibenzo(a,h)anthracene
Concen: 0.37 ng
RT: 26.39 min Scan# 1652
Delta R.T. -0.01 min
Lab File: BE091541.D
Acq: 28 Mar 2016 15:57

Tgt Ion	Ratio	Lower	Upper
278	100		
139	16.9	14.2	21.4
279	25.2	19.6	29.4



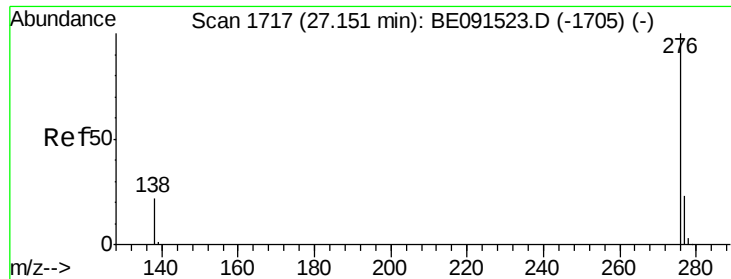

#33

Benzo(g,h,i)perylene

Concen: 0.37 ng

RT: 27.15 min Scan# 1718

Delta R.T. -0.01 min

Lab File: BE091541.D


Acq: 28 Mar 2016 15:57

Instrument :

BNA_E

ClientSampleId :

SSTDCCC0.4EC



Tgt Ion:	276	Resp:	19745
Ion Ratio	Lower	Upper	
276	100		
277	24.4	19.4	29.2
138	22.6	18.2	27.4

Manual Integrations
APPROVED

Sohil
3/29/2016 5:05:46 PM

