


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE032816\
 Data File : BE091531.D
 Acq On : 28 Mar 2016 9:21
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 25 19:00:32 2016

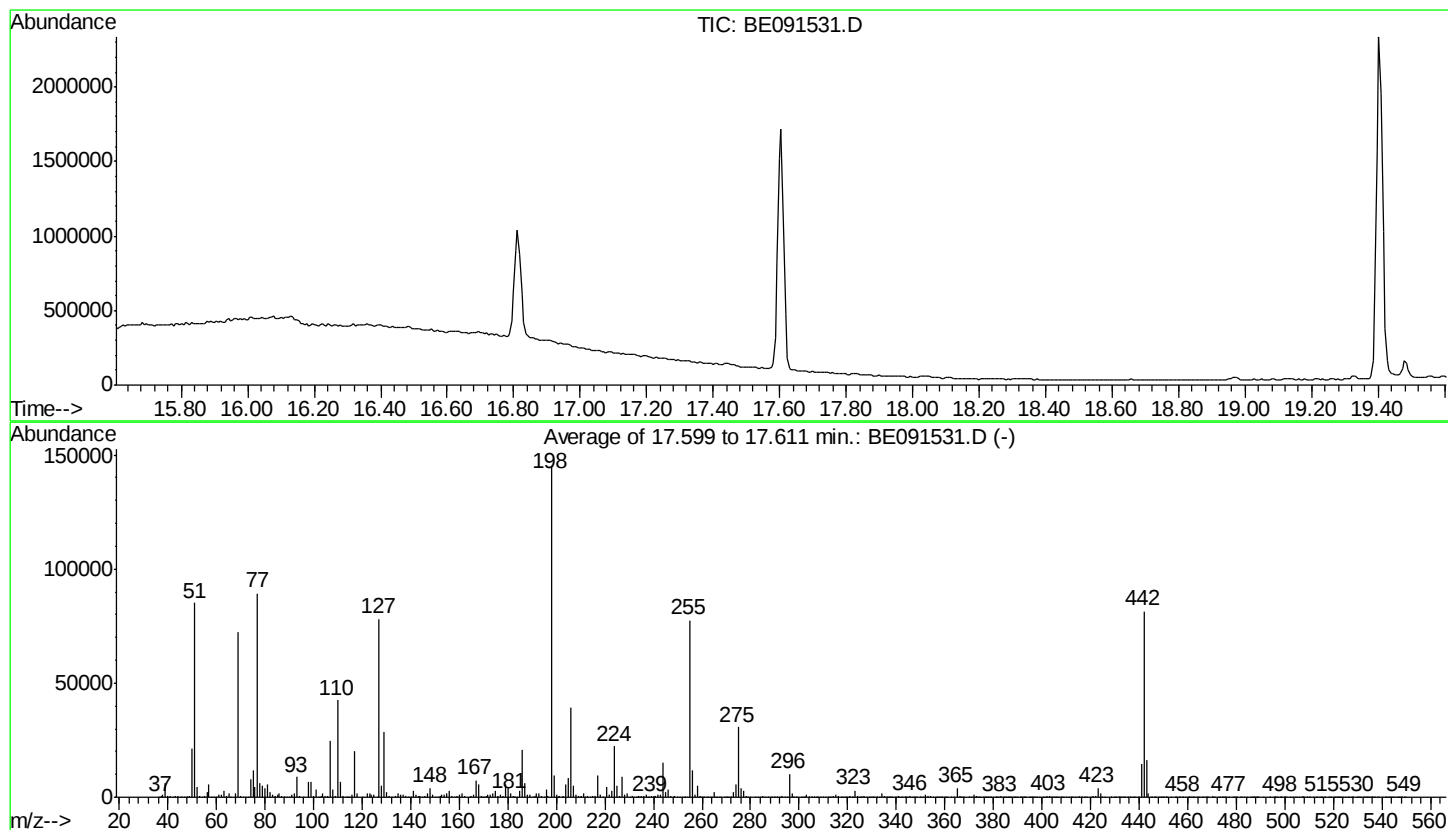

AutoFind: Scans 2555, 2556, 2557; Background Corrected with Scan 2548

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.6	85073	PASS
68	69	0.00	2	2.0	1427	PASS
69	198	0.00	100	49.8	72412	PASS
70	69	0.00	2	0.5	395	PASS
127	198	10	80	53.7	78026	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	145281	PASS
199	198	5	9	6.8	9810	PASS
275	198	10	60	21.1	30666	PASS
365	198	1	100	2.9	4164	PASS
441	442	0.01	24	18.0	14681	PASS
442	198	50	100	56.0	81428	PASS
443	442	15	24	20.3	16492	PASS