

Data Path : Z:\HPCHEM1\BNA E\DATA\BE032817\
 Data File : BE092835.D
 Acq On : 28 Mar 2017 13:49
 Operator : SJ/MA
 Sample : SSTDICC010
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Mar 28 14:21:07 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE032817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 28 13:07:38 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	7557	5.00	ng	0.00
7) Naphthalene-d8	10.54	136	34909	5.00	ng	0.00
12) Acenaphthene-d10	14.40	164	18251	5.00	ng	0.00
18) Phenanthrene-d10	17.16	188	38051	5.00	ng	0.00
24) Chrysene-d12	21.30	240	47556	5.00	ng	0.00
31) Perylene-d12	23.71	264	40969	5.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.36	112	18965	11.86	ng	0.00
5) Phenol-d6	6.94	99	29475	15.48	ng	0.00
8) Nitrobenzene-d5	8.93	82	25660	12.03	ng	0.00
13) 2,4,6-Tribromophenol	15.88	330	4433	9.23	ng	0.00
14) 2-Fluorobiphenyl	13.02	172	60017	13.94	ng	-0.01
26) Terphenyl-d14	19.76	244	81394	14.18	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.31	88	9597	8.55	ng	96
3) n-Nitrosodimethylamine	3.59	42	11672	9.20	ng	82
6) bis(2-Chloroethyl)ether	7.20	93	26105	12.57	ng	# 45
9) Naphthalene	10.58	128	78009	10.45	ng	# 95
10) Hexachlorobutadiene	10.89	225	10305	9.58	ng	99
11) 2-Methylnaphthalene	12.21	142	51480	10.66	ng	95
15) Acenaphthylene	14.11	152	341659	12.18	ng	100
16) Acenaphthene	14.45	154	52617	13.40	ng	97
17) Fluorene	15.44	166	62402	11.69	ng	99
19) Hexachlorobenzene	16.47	284	15436	9.92	ng	# 67
20) Pentachlorophenol	16.81	266	6259	11.92	ng	# 87
21) Phenanthrene	17.18	178	98484	10.79	ng	# 94
22) Anthracene	17.27	178	103450	11.24	ng	98
23) Fluoranthene	19.18	202	483522	10.88	ng	99
25) Pyrene	19.54	202	525764	12.21	ng	99
27) Benzo(a)anthracene	21.26	228	124856	2.61	ng	97
28) Chrysene	21.31	228	119180	2.73	ng	# 88
29) Bis(2-ethylhexyl)phthalate	21.23	149	57994	11.12	ng	# 72
30) Indeno(1,2,3-cd)pyrene	26.25	276	490348	10.38	ng	# 93
32) Benzo(b)fluoranthene	22.97	252	116678	10.69	ng	98
33) Benzo(k)fluoranthene	23.02	252	107294	9.77	ng	95
34) Benzo(a)pyrene	23.60	252	105114	10.59	ng	96
35) Dibenzo(a,h)anthracene	26.29	278	106081	11.19	ng	95
36) Benzo(g,h,i)perylene	27.04	276	423047	10.43	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE032817\
Data File : BE092835.D
Acq On : 28 Mar 2017 13:49
Operator : SJ/MA
Sample : SSTDICC010
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Mar 28 14:21:07 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE032817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 28 13:07:38 2017
Response via : Initial Calibration









#1

1,4-Dichlorobenzene-d4
Concen: 5.00 ng
RT: 7.80 min Scan# 556
Delta R.T. -0.00 min
Lab File: BE092835.D
Acq: 28 Mar 2017 13:49

Instrument :
BNA_E
ClientSampled :




Tot Ion:152 Resp: 7557
Ion Ratio Lower Upper
152 100
150 128.3 106.0 159.0
115 32.7 31.2 46.8



#2

1,4-Dioxane
Concen: 8.55 ng
RT: 3.31 min Scan# 62
Delta R.T. -0.01 min
Lab File: BE092835.D
Acq: 28 Mar 2017 13:49

Tgt Ion: 88 Resp: 9597
Ion Ratio Lower Upper
88 100
58 78.3 63.6 95.4
43 29.7 28.0 42.0





#3

n-Nitrosodimethylamine

Concen: 9.20 ng

RT: 3.59 min Scan# 87

Delta R.T. -0.01 min

Lab File: BE092835.D

Acq: 28 Mar 2017 13:49

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 42 Resp: 11672

Ion Ratio Lower Upper

42 100

74 127.3 86.0 129.0




44 6.6 5.1 7.7



Abundance Ion 42.00 (41.70 to 42.70): BE0

Ion 74.00 (73.70 to 74.70): BE0

Ion 44.00 (43.70 to 44.70): BE0



#4

2-Fluorophenol

Concen: 11.86 ng

RT: 5.36 min Scan# 267

Delta R.T. -0.00 min

Lab File: BE092835.D

Acq: 28 Mar 2017 13:49


Tgt Ion: 112 Resp: 18965

Ion Ratio Lower Upper

112 100

64 69.1 53.5 80.3



63 35.6 27.9 41.9




Abundance Ion 112.00 (111.70 to 112.70): BE0

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0





#5

Phenol-d6

Concen: 15.48 ng

RT: 6.94 min Scan# 519

Delta R.T. -0.00 min

Lab File: BE092835.D

Acq: 28 Mar 2017 13:49

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 99 Resp: 29475

Ion Ratio Lower Upper

99 100

42 0.0 16.0 24.0#




71 32.1 30.6 45.8



Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0



#6

bis(2-Chloroethyl)ether

Concen: 12.57 ng

RT: 7.20 min Scan# 530

Delta R.T. -0.00 min

Lab File: BE092835.D

Acq: 28 Mar 2017 13:49


Tgt Ion: 93 Resp: 26105

Ion Ratio Lower Upper

93 100

63 83.3 16.0 24.0#



95 30.3 24.0 36.0




Abundance Ion 93.00 (92.70 to 93.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

Ion 95.00 (94.70 to 95.70): BE0





#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.54 min Scan# 679

Delta R.T. 0.00 min

Lab File: BE092835.D

Acq: 28 Mar 2017 13:49

Instrument :

BNA_E

ClientSampleId :

Tot Ion:136 Resp: 34909





Ion Ratio Lower Upper

136 100

137 11.4 8.2 12.4

54 5.7 9.6 14.4#

68 5.4 6.7 10.1#



#8

Nitrobenzene-d5

Concen: 12.03 ng

RT: 8.93 min Scan# 605

Delta R.T. -0.00 min

Lab File: BE092835.D

Acq: 28 Mar 2017 13:49




Tgt Ion: 82 Resp: 25660


Ion Ratio Lower Upper

82 100

128 40.4 39.0 58.4

54 31.0 44.8 67.2#





#9

Naphthalene

Concen: 10.45 ng

RT: 10.58 min Scan# 681

Delta R.T. 0.00 min

Lab File: BE092835.D

Acq: 28 Mar 2017 13:49

Instrument :

BNA_E

ClientSampleId :





Tot Ion:128 Resp: 78009

Ion Ratio Lower Upper

128 100

129 10.4 11.2 16.8#

127 13.8 11.6 17.4



#10

Hexachlorobutadiene

Concen: 9.58 ng

RT: 10.89 min Scan# 697

Delta R.T. 0.00 min

Lab File: BE092835.D

Acq: 28 Mar 2017 13:49




Tgt Ion:225 Resp: 10305


Ion Ratio Lower Upper

225 100

223 62.6 50.6 76.0

227 64.4 51.4 77.0



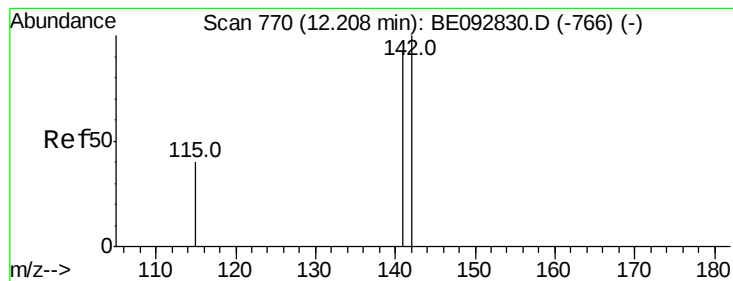

#11

2-Methylnaphthalene

Concen: 10.66 ng

RT: 12.21 min Scan# 770

Delta R.T. 0.00 min

Lab File: BE092835.D

Acq: 28 Mar 2017 13:49

Instrument :

BNA_E

ClientSampleId :


Tot Ion:142 Resp: 51480

Ion Ratio Lower Upper

142 100

141 89.3 73.7 110.5




115 36.9 34.0 51.0



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E



#12

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.40 min Scan# 933

Delta R.T. 0.00 min

Lab File: BE092835.D

Acq: 28 Mar 2017 13:49


Tgt Ion:164 Resp: 18251

Ion Ratio Lower Upper

164 100

162 98.0 71.4 107.0



160 41.5 27.4 41.2#



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E









#13
 2,4,6-Tribromophenol
 Concen: 9.23 ng
 RT: 15.88 min Scan# 1042
 Delta R.T. -0.00 min
 Lab File: BE092835.D
 Acq: 28 Mar 2017 13:49




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:330 Resp: 4433
 Ion Ratio Lower Upper
 330 100
 332 96.5 75.4 113.0
 141 55.9 31.0 46.6#



#14
 2-Fluorobiphenyl
 Concen: 13.94 ng
 RT: 13.02 min Scan# 840
 Delta R.T. -0.01 min
 Lab File: BE092835.D
 Acq: 28 Mar 2017 13:49

Tgt Ion:172 Resp: 60017
 Ion Ratio Lower Upper
 172 100
 171 37.8 30.1 45.1
 170 26.5 21.8 32.6









#15
Acenaphthylene
Concen: 12.18 ng
RT: 14.11 min Scan# 916
Delta R.T. 0.00 min
Lab File: BE092835.D
Acq: 28 Mar 2017 13:49




Instrument :
BNA_E
ClientSampleId :


Tot Ion:152 Resp: 341659
Ion Ratio Lower Upper
152 100
151 4.9 3.9 5.9
153 13.2 10.4 15.6



#16
Acenaphthene
Concen: 13.40 ng
RT: 14.45 min Scan# 936
Delta R.T. 0.00 min
Lab File: BE092835.D
Acq: 28 Mar 2017 13:49

Tgt Ion:154 Resp: 52617
Ion Ratio Lower Upper
154 100
153 448.0 350.8 526.2
152 215.3 171.1 256.7





#17

Fluorene

Concen: 11.69 ng

RT: 15.44 min Scan# 1004

Delta R.T. -0.00 min

Lab File: BE092835.D

Acq: 28 Mar 2017 13:49

Instrument :

BNA_E

ClientSampled :





Tot Ion:166 Resp: 62402

Ion Ratio Lower Upper

166 100

165 99.3 78.2 117.4

167 14.1 11.0 16.4



#18

Phenanthrene-d10

Concen: 5.00 ng

RT: 17.16 min Scan# 1110

Delta R.T. 0.00 min

Lab File: BE092835.D

Acq: 28 Mar 2017 13:49




Tgt Ion:188 Resp: 38051

Ion Ratio Lower Upper

188 100

94 2.9 3.2 4.8#

80 2.4 2.6 3.8#









#19
Hexachlorobenzene
Concen: 9.92 ng
RT: 16.47 min Scan# 1080
Delta R.T. -0.00 min
Lab File: BE092835.D
Acq: 28 Mar 2017 13:49




Instrument :
BNA_E
ClientSampleId :




Tot Ion:284 Resp: 15436
Ion Ratio Lower Upper
284 100
142 0.0 29.1 43.7#
249 36.5 27.9 41.9



#20
Pentachlorophenol
Concen: 11.92 ng
RT: 16.81 min Scan# 1095
Delta R.T. -0.00 min
Lab File: BE092835.D
Acq: 28 Mar 2017 13:49

Tgt Ion:266 Resp: 6259
Ion Ratio Lower Upper
266 100
268 74.9 62.5 93.7
264 52.2 57.2 85.8#





#21

Phenanthrene

Concen: 10.79 ng

RT: 17.18 min Scan# 1111

Delta R.T. -0.00 min

Lab File: BE092835.D

Acq: 28 Mar 2017 13:49

Instrument :

BNA_E

ClientSampleId :





Tot Ion:178 Resp: 98484

Ion Ratio Lower Upper

178 100

176 20.4 15.8 23.8

179 14.9 16.0 24.0#



#22

Anthracene

Concen: 11.24 ng

RT: 17.27 min Scan# 1115

Delta R.T. -0.00 min

Lab File: BE092835.D

Acq: 28 Mar 2017 13:49


Tgt Ion:178 Resp: 103450


Ion Ratio Lower Upper

178 100

176 19.5 15.0 22.4

179 14.6 12.2 18.2









#23
 Fluoranthene
 Concen: 10.88 ng
 RT: 19.18 min Scan# 1199
 Delta R.T. 0.00 min
 Lab File: BE092835.D
 Acq: 28 Mar 2017 13:49




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:202 Resp: 483522
 Ion Ratio Lower Upper
 202 100
 101 3.2 2.2 3.4
 203 17.6 13.7 20.5



#24
 Chrysene-d12
 Concen: 5.00 ng
 RT: 21.30 min Scan# 1321
 Delta R.T. 0.00 min
 Lab File: BE092835.D
 Acq: 28 Mar 2017 13:49

Tgt Ion:240 Resp: 47556
 Ion Ratio Lower Upper
 240 100
 120 1.3 2.6 4.0#
 236 21.0 24.6 37.0#





#25

Pvrene

Concen: 12.21 ng

RT: 19.54 min Scan# 1220

Delta R.T. 0.00 min

Lab File: BE092835.D

Acq: 28 Mar 2017 13:49

Instrument :

BNA_E

ClientSampleId :


Tot Ion:202 Resp: 525764

Ion Ratio Lower Upper




202 100

200 5.1 4.2 6.4

203 17.7 13.9 20.9



Abundance Ion 202.00 (201.70 to 202.70): E
Ion 200.00 (199.70 to 200.70): E
Ion 203.00 (202.70 to 203.70): E



#26

Terphenyl-d14

Concen: 14.18 ng

RT: 19.76 min Scan# 1233

Delta R.T. 0.00 min

Lab File: BE092835.D

Acq: 28 Mar 2017 13:49


Tgt Ion:244 Resp: 81394

Ion Ratio Lower Upper



244 100


212 7.1 6.7 10.1

122 1.4 3.6 5.4#



Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E





#27

Benzo(a)anthracene

Concen: 2.61 ng

RT: 21.26 min Scan# 1319

Delta R.T. 0.00 min

Lab File: BE092835.D

Acq: 28 Mar 2017 13:49

Instrument :

BNA_E

ClientSampleId :


Tot Ion:228 Resp: 124856

Ion Ratio Lower Upper

228 100

226 31.6 23.6 35.4




229 16.7 13.3 19.9



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E



#28

Chrysene

Concen: 2.73 ng

RT: 21.31 min Scan# 1322

Delta R.T. 0.00 min

Lab File: BE092835.D

Acq: 28 Mar 2017 13:49


Tgt Ion:228 Resp: 119180

Ion Ratio Lower Upper

228 100

226 36.5 36.3 54.5



229 16.1 10.6 16.0#



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E





#29

Bis(2-ethylhexyl)phthalate

Concen: 11.12 ng

RT: 21.23 min Scan# 1317

Delta R.T. 0.00 min

Lab File: BE092835.D

Acq: 28 Mar 2017 13:49

Instrument :

BNA_E

ClientSampleId :





Tot Ion:149 Resp: 57994

Ion Ratio Lower Upper

149 100

167 28.0 16.0 24.0#

279 2.6 16.0 24.0#



#30

Indeno(1,2,3-cd)pyrene

Concen: 10.38 ng

RT: 26.25 min Scan# 1704

Delta R.T. -0.00 min

Lab File: BE092835.D

Acq: 28 Mar 2017 13:49




Tgt Ion:276 Resp: 490348


Ion Ratio Lower Upper

276 100

138 32.3 20.3 30.5#

277 25.1 19.7 29.5









#31
Pervlene-d12
Concen: 5.00 ng
RT: 23.71 min Scan# 1493
Delta R.T. 0.00 min
Lab File: BE092835.D
Acq: 28 Mar 2017 13:49




Instrument :
BNA_E
ClientSampleId :


Tot Ion:264 Resp: 40969
Ion Ratio Lower Upper
264 100
260 24.7 20.1 30.1
265 22.0 17.9 26.9



#32
Benzo(b)fluoranthene
Concen: 10.69 ng
RT: 22.97 min Scan# 1429
Delta R.T. 0.00 min
Lab File: BE092835.D
Acq: 28 Mar 2017 13:49

Tgt Ion:252 Resp: 116678
Ion Ratio Lower Upper
252 100
253 22.8 18.7 28.1
125 11.9 10.5 15.7









#33
Benzo(k)fluoranthene
Concen: 9.77 ng
RT: 23.02 min Scan# 1433
Delta R.T. 0.00 min
Lab File: BE092835.D
Acq: 28 Mar 2017 13:49




Instrument :
BNA_E
ClientSampleId :


Tot Ion:252 Resp: 107294
Ion Ratio Lower Upper
252 100
253 22.1 20.3 30.5
125 12.5 9.6 14.4



#34
Benzo(a)pyrene
Concen: 10.59 ng
RT: 23.60 min Scan# 1483
Delta R.T. 0.00 min
Lab File: BE092835.D
Acq: 28 Mar 2017 13:49

Tgt Ion:252 Resp: 105114
Ion Ratio Lower Upper
252 100
253 20.8 19.0 28.6
125 14.6 11.8 17.8









#35
Dibenzo(a,h)anthracene
Concen: 11.19 ng
RT: 26.29 min Scan# 1706
Delta R.T. -0.00 min
Lab File: BE092835.D
Acq: 28 Mar 2017 13:49

Instrument :
BNA_E
ClientSampleId :

Tot Ion:278 Resp: 106081
Ion Ratio Lower Upper
278 100
139 19.6 13.8 20.8
279 24.2 21.4 32.2



#36
Benzo(g,h,i)perylene
Concen: 10.43 ng
RT: 27.04 min Scan# 1750
Delta R.T. 0.02 min
Lab File: BE092835.D
Acq: 28 Mar 2017 13:49

Tgt Ion:276 Resp: 423047
Ion Ratio Lower Upper
276 100
277 23.5 19.8 29.8
138 26.6 19.8 29.6

