

Data Path : Z:\HPCHEM1\BNA E\DATA\BE032817\
 Data File : BE092836.D
 Acq On : 28 Mar 2017 14:25
 Operator : SJ/MA
 Sample : SSTDICV0.4
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 ICVBE032817

Manual Integrations
 APPROVED

mohammad
 3/29/2017 2:37:26 PM

Quant Time: Mar 28 15:01:45 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE032817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 28 14:58:05 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	7284	5.00	ng	0.00
7) Naphthalene-d8	10.54	136	33054	5.00	ng	0.00
12) Acenaphthene-d10	14.40	164	16098	5.00	ng	0.00
18) Phenanthrene-d10	17.16	188	35489	5.00	ng	0.00
24) Chrysene-d12	21.28	240	42258	5.00	ng	-0.02
31) Perylene-d12	23.71	264	36961	5.00	ng	0.00

System Monitoring Compounds						
4) 2-Fluorophenol	5.36	112	653	0.38	ng	0.00
5) Phenol-d6	6.94	99	944	0.38	ng	0.00
8) Nitrobenzene-d5	8.93	82	739	0.39	ng	0.00
13) 2,4,6-Tribromophenol	15.88	330	82	0.33	ng	0.00
14) 2-Fluorobiphenyl	13.02	172	2146	0.40	ng	-0.01
26) Terphenyl-d14	19.76	244	2720	0.37	ng	0.00

Target Compounds						Qvalue
2) 1,4-Dioxane	3.31	88	413	0.42	ng	91
3) n-Nitrosodimethylamine	3.61	42	386	0.38	ng	# 80
6) bis(2-Chloroethyl)ether	7.20	93	948	0.40	ng	# 43
9) Naphthalene	10.58	128	2887	0.40	ng	97
10) Hexachlorobutadiene	10.89	225	380	0.39	ng	98
11) 2-Methylnaphthalene	12.21	142	1779	0.39	ng	95
15) Acenaphthylene	14.11	152	8632	0.35	ng	100
16) Acenaphthene	14.45	154	1684	0.38	ng	85
17) Fluorene	15.44	166	2006	0.38	ng	97
19) Hexachlorobenzene	16.47	284	545	0.41	ng	# 68
20) Pentachlorophenol	16.81	266	101	0.46	ng	92
21) Phenanthrene	17.18	178	3779	0.44	ng	# 95
22) Anthracene	17.27	178	3060	0.39	ng	99
23) Fluoranthene	19.18	202	14541	0.37	ng	99
25) Pyrene	19.54	202	15655	0.37	ng	99
27) Benzo(a)anthracene	21.26	228	3736	0.37	ng	97
28) Chrysene	21.31	228	4159	0.39	ng	# 84
29) Bis(2-ethylhexyl)phthalate	21.23	149	887	0.36	ng	# 76
30) Indeno(1,2,3-cd)pyrene	26.25	276	14522	0.37	ng	# 93
32) Benzo(b)fluoranthene	22.96	252	3365m	0.34	ng	
33) Benzo(k)fluoranthene	23.02	252	3478	0.39	ng	# 97
34) Benzo(a)pyrene	23.60	252	2828	0.35	ng	# 94
35) Dibenzo(a,h)anthracene	26.29	278	3148	0.36	ng	95
36) Benzo(g,h,i)perylene	27.02	276	13419	0.37	ng	# 92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032817\
Data File : BE092836.D
Acq On : 28 Mar 2017 14:25
Operator : SJ/MA
Sample : SSTDICV0.4
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
ICVBE032817

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:26 PM

Quant Time: Mar 28 15:01:45 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE032817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 28 14:58:05 2017
Response via : Initial Calibration

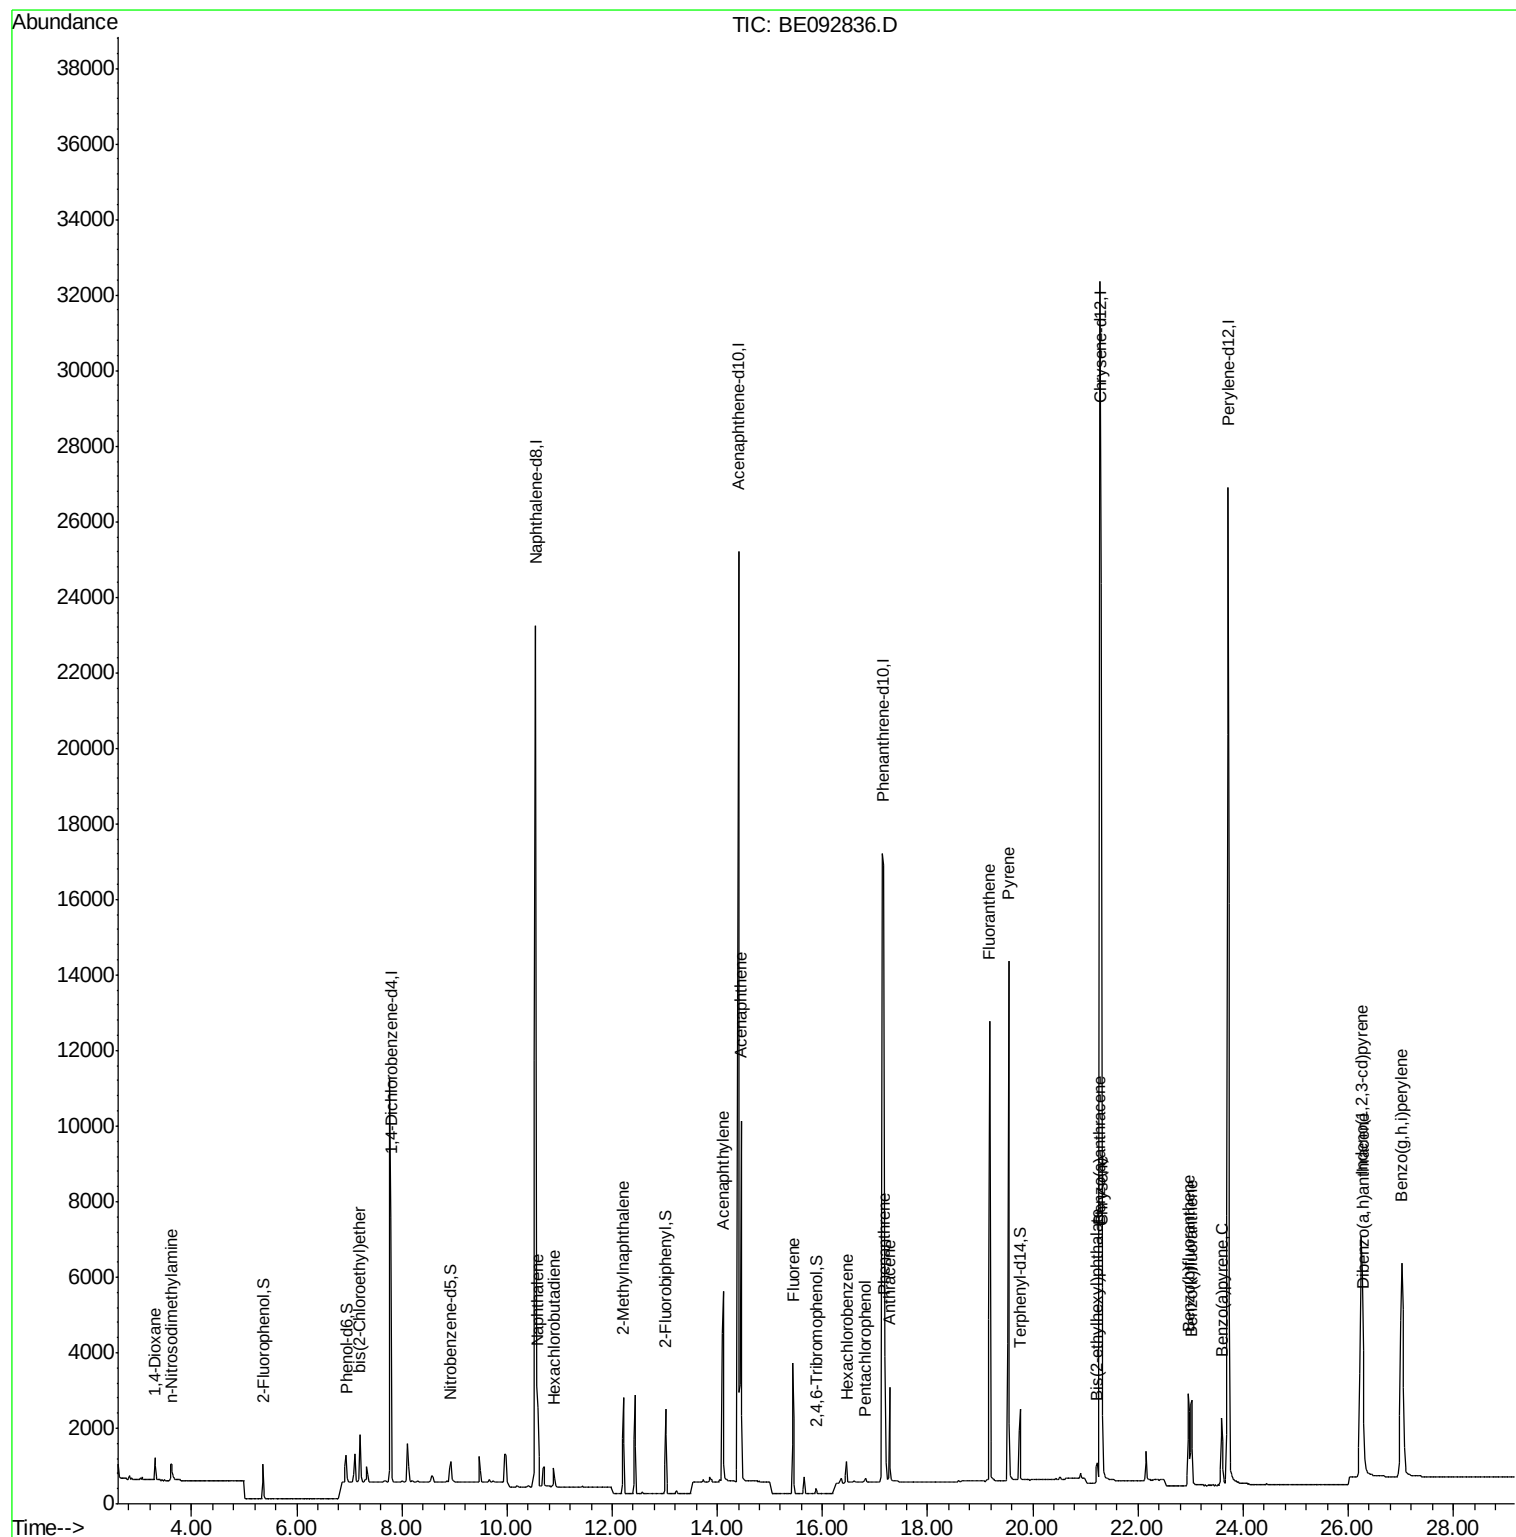

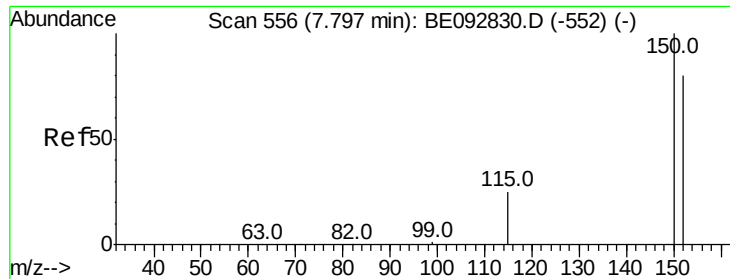

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.80 min Scan# 556

Delta R.T. -0.00 min

Lab File: BE092836.D

Acq: 28 Mar 2017 14:25

Instrument :

BNA_E





ClientSampleId :

ICVBE032817

Tot Ion	Ratio	Lower	Upper
152	100		
150	123.4	106.0	159.0
115	31.0	31.2	46.8

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:26 PM

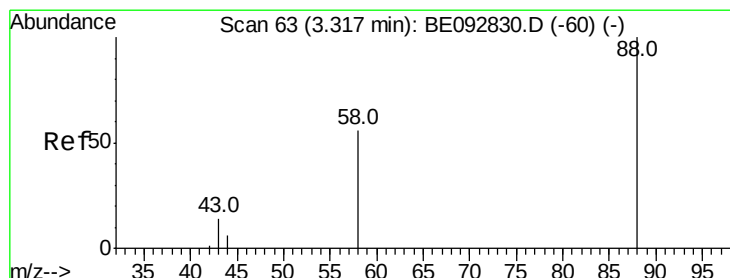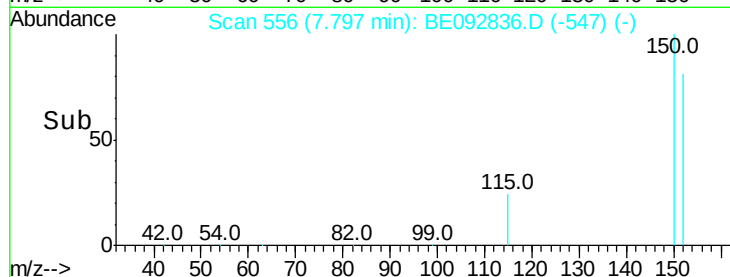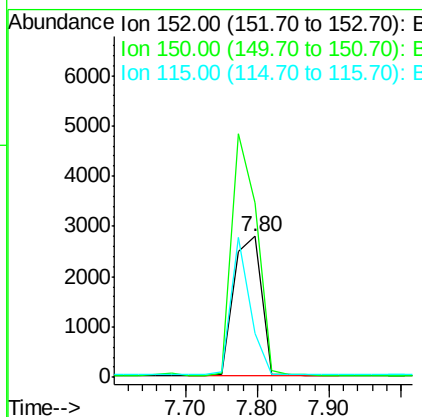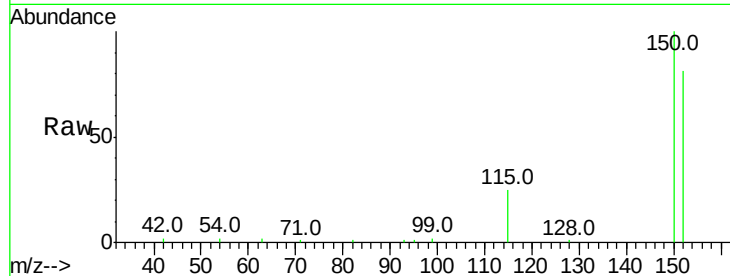

#2

1,4-Dioxane

Concen: 0.42 ng




RT: 3.31 min Scan# 62


Delta R.T. -0.01 min

Lab File: BE092836.D

Acq: 28 Mar 2017 14:25

Tgt Ion	Ratio	Lower	Upper
88	100		
58	72.2	63.6	95.4
43	28.6	28.0	42.0

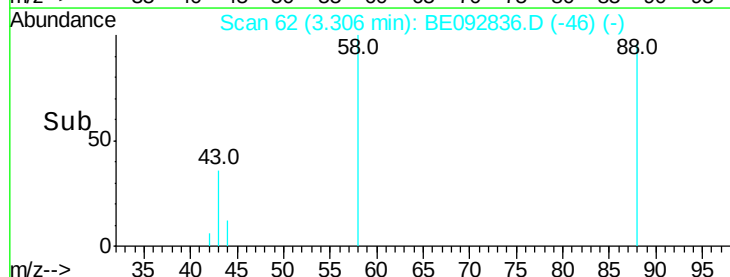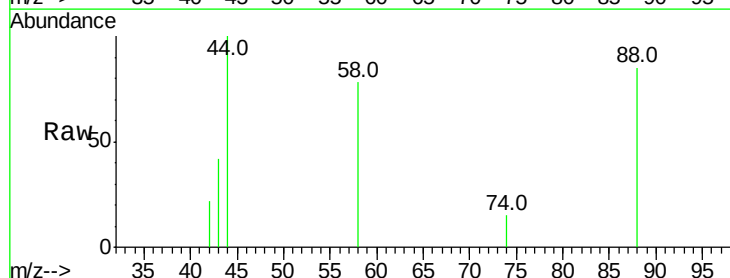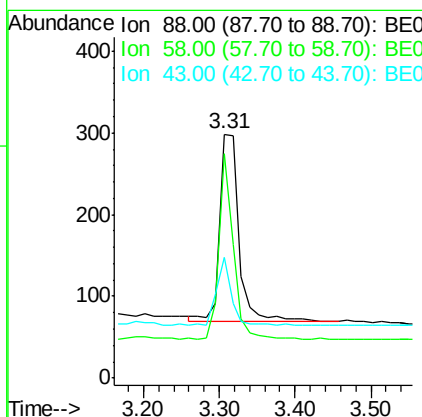



#3

n-Nitrosodimethylamine

Concen: 0.38 ng

RT: 3.61 min Scan# 88

Delta R.T. 0.00 min

Lab File: BE092836.D

Acq: 28 Mar 2017 14:25

Instrument :

BNA_E





ClientSampleId :

ICVBE032817

Tot Ion:	42	Resp:	386
Ion Ratio	Lower	Upper	
42	100		
74	127.5	86.0	129.0
44	18.4	5.1	7.7#

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:26 PM

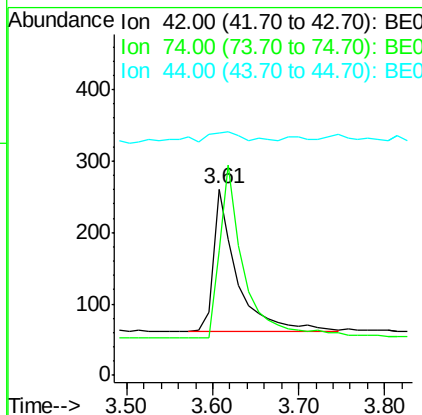

#4

2-Fluorophenol

Concen: 0.38 ng




RT: 5.36 min Scan# 267




Delta R.T. -0.00 min

Lab File: BE092836.D

Acq: 28 Mar 2017 14:25

Tgt Ion:	112	Resp:	653
Ion Ratio	Lower	Upper	
112	100		
64	70.3	53.5	80.3
63	37.7	27.9	41.9

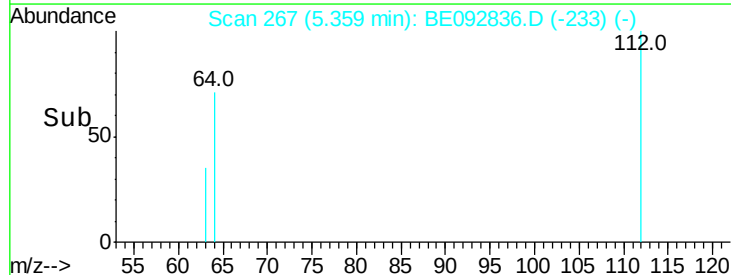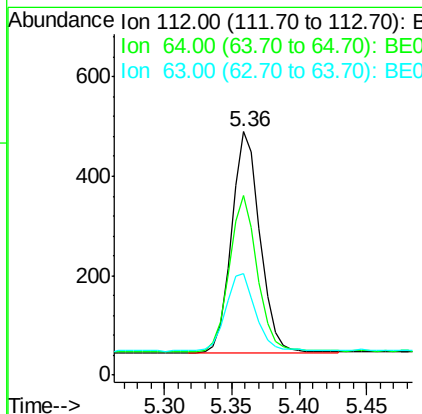



#5

Phenol-d6

Concen: 0.38 ng

RT: 6.94 min Scan# 519

Delta R.T. -0.00 min

Lab File: BE092836.D

Acq: 28 Mar 2017 14:25

Tot Ion:	99	Resp:	944
Ion	Ratio	Lower	Upper
99	100		
42	0.0	16.0	24.0#
71	0.0	30.6	45.8#

Instrument :





BNA_E

ClientSampleId :

ICVBE032817

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:26 PM

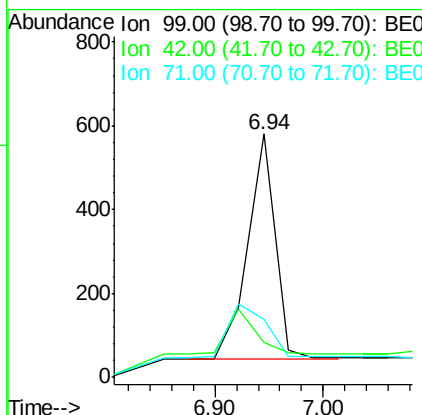

#6

bis(2-Chloroethyl)ether

Concen: 0.40 ng


RT: 7.20 min Scan# 530


Delta R.T. -0.00 min

Lab File: BE092836.D

Acq: 28 Mar 2017 14:25

Tgt Ion:	93	Resp:	948
Ion	Ratio	Lower	Upper
93	100		
63	83.6	16.0	24.0#
95	31.6	24.0	36.0

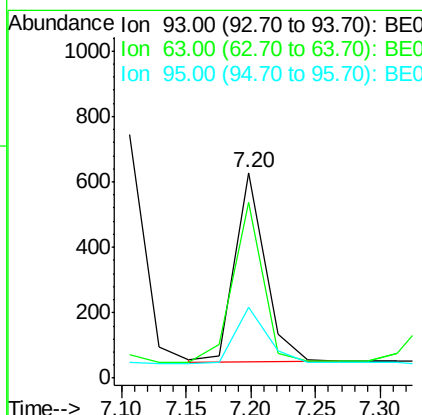



#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.54 min Scan# 679

Delta R.T. 0.00 min

Lab File: BE092836.D

Acq: 28 Mar 2017 14:25

Instrument :

BNA_E





ClientSampleId :

ICVBE032817

Tot Ion	Ratio	Resp	Lower	Upper
136	100			
137	11.5	8.2	12.4	
54	5.2	9.6	14.4	
68	5.1	6.7	10.1	

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:26 PM

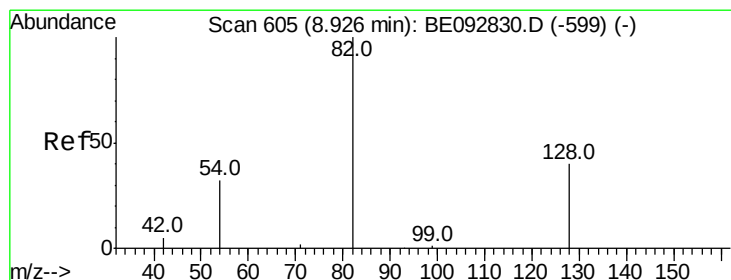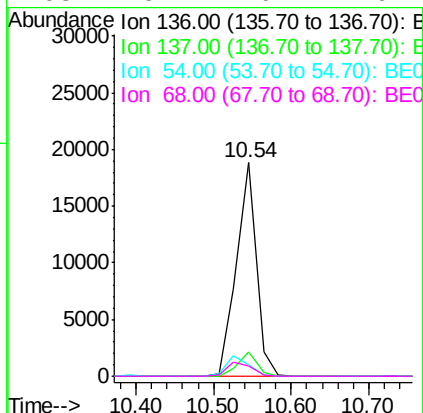

#8

Nitrobenzene-d5

Concen: 0.39 ng




RT: 8.93 min Scan# 605


Delta R.T. -0.00 min

Lab File: BE092836.D

Acq: 28 Mar 2017 14:25

Tgt Ion	Ratio	Resp	Lower	Upper
82	100			
128	51.5	39.0	58.4	
54	41.0	44.8	67.2	

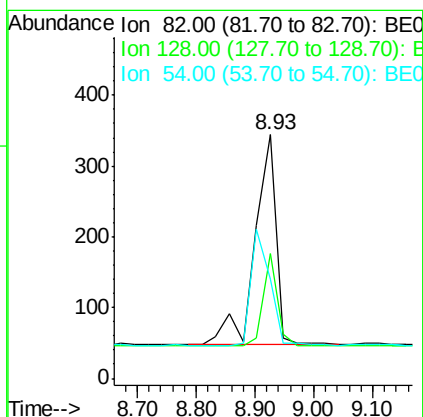



#9

Naphthalene

Concen: 0.40 ng

RT: 10.58 min Scan# 681

Delta R.T. 0.00 min

Lab File: BE092836.D

Acq: 28 Mar 2017 14:25

Instrument :

BNA_E





ClientSampleId :

ICVBE032817

Tot Ion:	128	Resp:	2887
Ion	Ratio	Lower	Upper
128	100		
129	12.9	11.2	16.8
127	15.5	11.6	17.4

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:26 PM

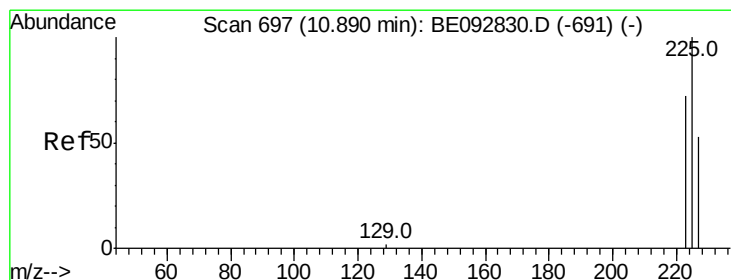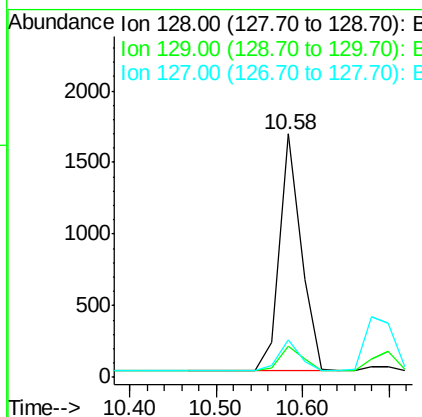

#10

Hexachlorobutadiene

Concen: 0.39 ng




RT: 10.89 min Scan# 697




Delta R.T. 0.00 min

Lab File: BE092836.D

Acq: 28 Mar 2017 14:25

Tgt Ion:	225	Resp:	380
Ion	Ratio	Lower	Upper
225	100		
223	65.8	50.6	76.0
227	63.2	51.4	77.0

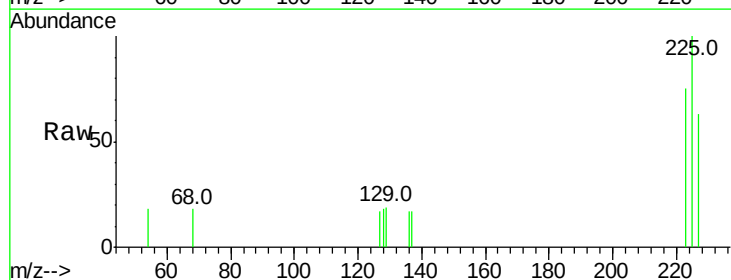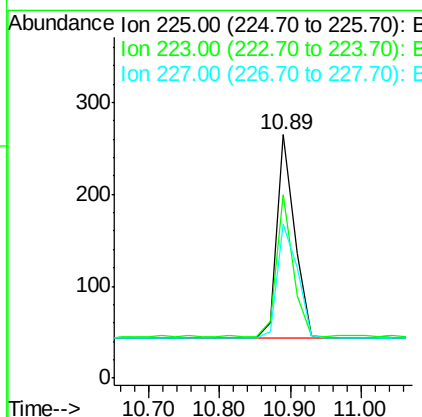

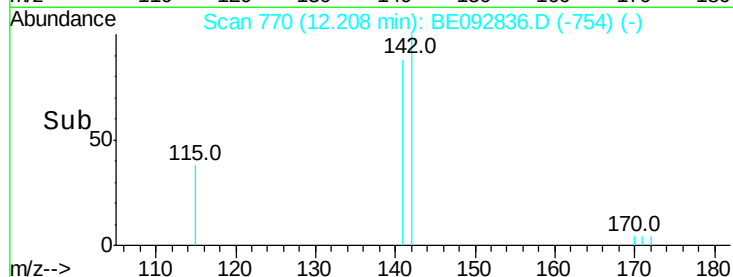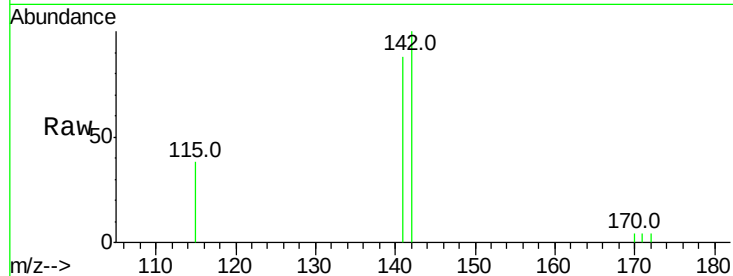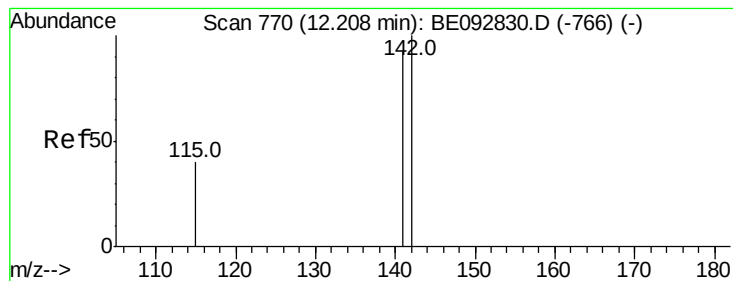

#11

2-Methylnaphthalene

Concen: 0.39 ng

RT: 12.21 min Scan# 770

Delta R.T. 0.00 min

Lab File: BE092836.D

Acq: 28 Mar 2017 14:25

Tot Ion:	142	Resp:	1779
Ion	Ratio	Lower	Upper
142	100		
141	88.0	73.7	110.5
115	38.0	34.0	51.0

Instrument :





BNA_E

ClientSampleId :

ICVBE032817

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:26 PM

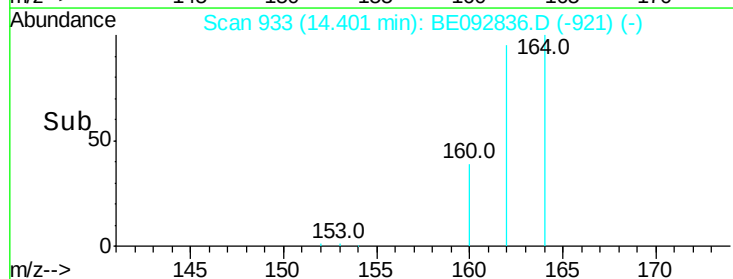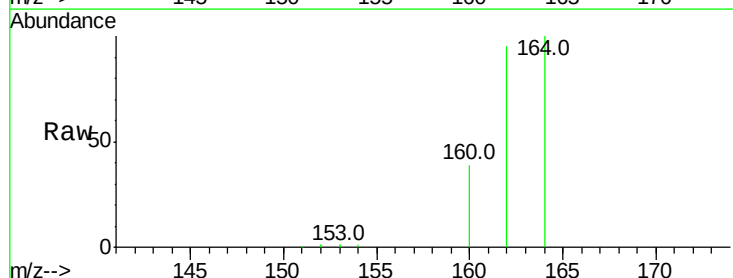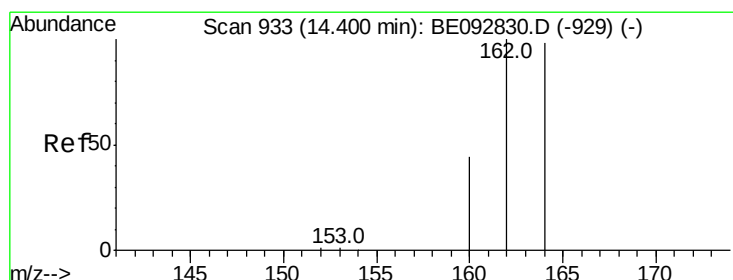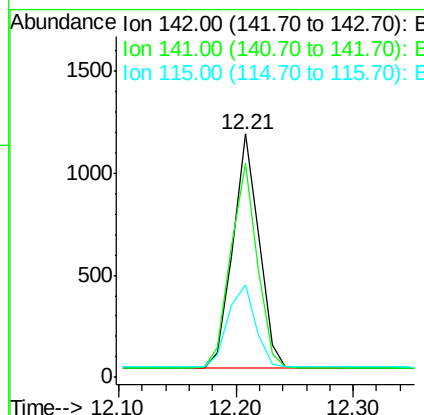

#12

Acenaphthene-d10

Concen: 5.00 ng


RT: 14.40 min Scan# 933


Delta R.T. 0.00 min

Lab File: BE092836.D

Acq: 28 Mar 2017 14:25

Tgt Ion:	164	Resp:	16098
Ion	Ratio	Lower	Upper
164	100		
162	95.5	71.4	107.0
160	39.4	27.4	41.2

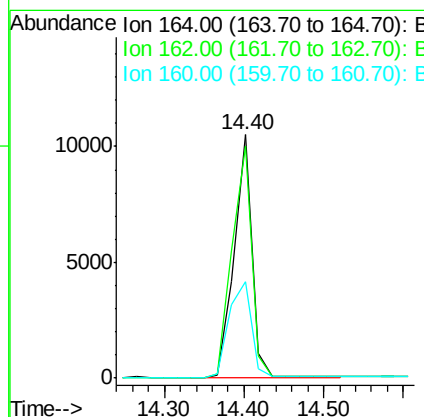

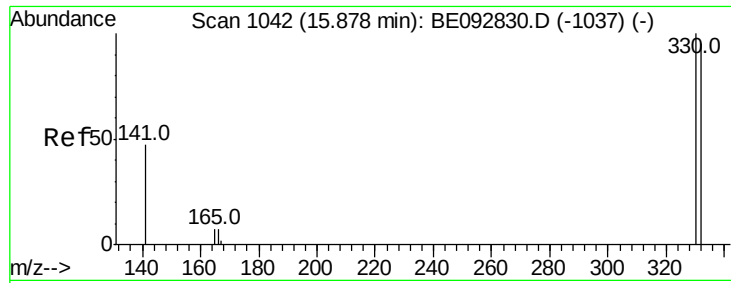





#13
 2,4,6-Tribromophenol
 Concen: 0.33 ng
 RT: 15.88 min Scan# 1042
 Delta R.T. -0.00 min
 Lab File: BE092836.D
 Acq: 28 Mar 2017 14:25

Instrument :
 BNA_E
 ClientSampleId :
 ICVBE032817

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.3	75.4	113.0
141	59.8	31.0	46.6




Manual Integrations
 APPROVED


mohammad
 3/29/2017 2:37:26 PM

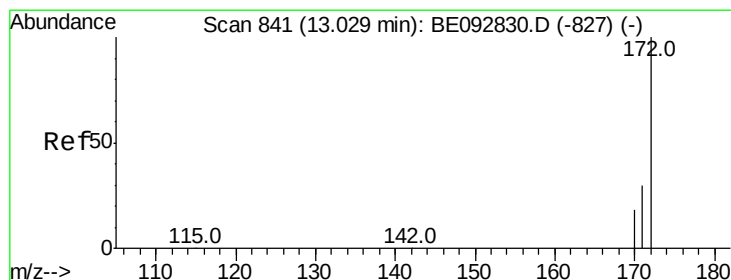

#14
 2-Fluorobiphenyl
 Concen: 0.40 ng
 RT: 13.02 min Scan# 840
 Delta R.T. -0.01 min
 Lab File: BE092836.D
 Acq: 28 Mar 2017 14:25

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.9	30.1	45.1
170	27.8	21.8	32.6

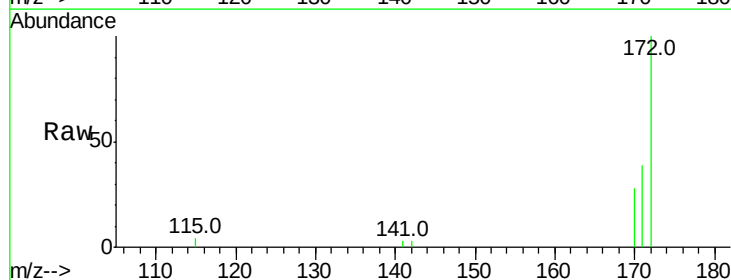







#15
Acenaphthylene
Concen: 0.35 ng
RT: 14.11 min Scan# 916
Delta R.T. 0.00 min
Lab File: BE092836.D
Acq: 28 Mar 2017 14:25

Instrument :
BNA_E
ClientSampleId :
ICVBE032817

Tot Ion	Ratio	Lower	Upper
152	100		
151	4.9	3.9	5.9
153	13.2	10.4	15.6




Manual Integrations
APPROVED


mohammad
3/29/2017 2:37:26 PM

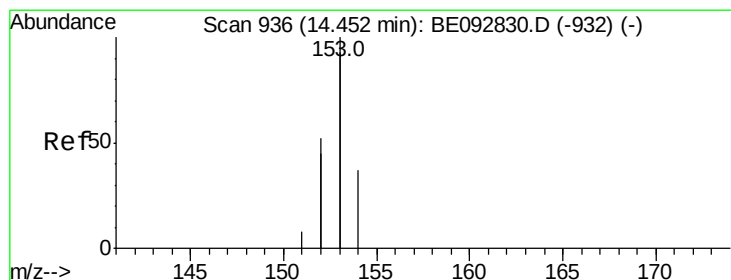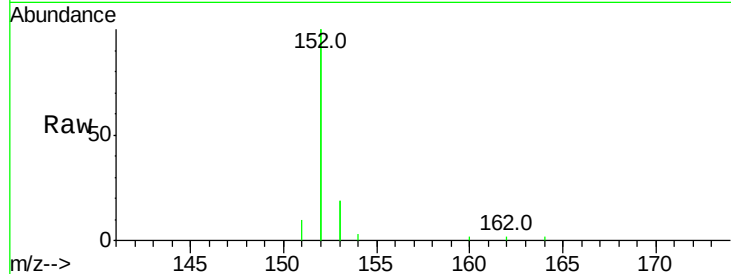

#16
Acenaphthene
Concen: 0.38 ng
RT: 14.45 min Scan# 936
Delta R.T. 0.00 min
Lab File: BE092836.D
Acq: 28 Mar 2017 14:25

Tgt Ion	Ratio	Lower	Upper
154	100		
153	480.1	350.8	526.2
152	231.1	171.1	256.7









#17
Fluorene
Concen: 0.38 ng
RT: 15.44 min Scan# 1004
Delta R.T. -0.00 min
Lab File: BE092836.D
Acq: 28 Mar 2017 14:25

Instrument :
BNA_E
ClientSampleId :
ICVBE032817

Tot Ion	Ratio	Lower	Upper
166	100		
165	100.8	78.2	117.4
167	13.7	11.0	16.4




Manual Integrations
APPROVED


mohammad
3/29/2017 2:37:26 PM

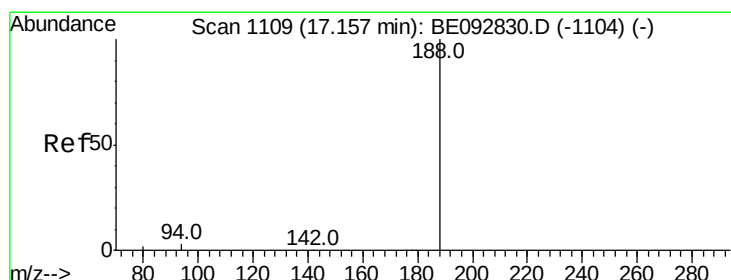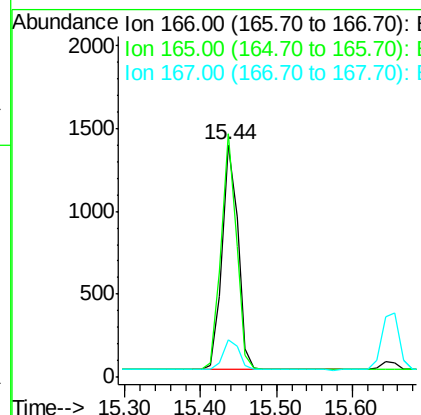

#18
Phenanthrene-d10
Concen: 5.00 ng
RT: 17.16 min Scan# 1110
Delta R.T. 0.00 min
Lab File: BE092836.D
Acq: 28 Mar 2017 14:25

Tgt Ion	Ratio	Lower	Upper
188	100		
94	2.5	3.2	4.8#
80	2.0	2.6	3.8#

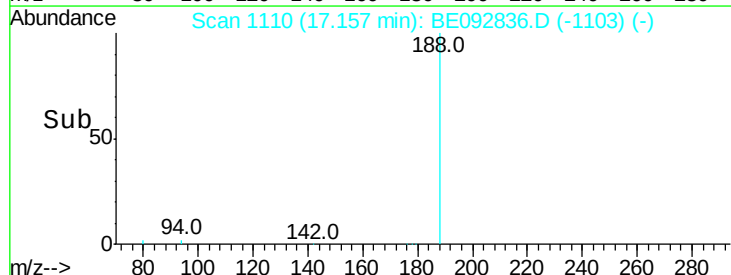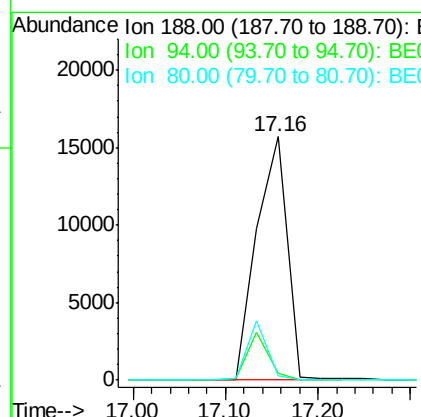







#19
Hexachlorobenzene
Concen: 0.41 ng
RT: 16.47 min Scan# 1080
Delta R.T. -0.00 min
Lab File: BE092836.D
Acq: 28 Mar 2017 14:25

Instrument :
BNA_E
ClientSampled :
ICVBE032817

Tot Ion	Ratio	Lower	Upper
284	100		
142	0.0	29.1	43.7#
249	33.8	27.9	41.9




Manual Integrations
APPROVED




mohammad
3/29/2017 2:37:26 PM



#20
Pentachlorophenol
Concen: 0.46 ng
RT: 16.81 min Scan# 1095
Delta R.T. 0.00 min
Lab File: BE092836.D
Acq: 28 Mar 2017 14:25

Tgt Ion	Ratio	Lower	Upper
266	100		
268	86.8	62.5	93.7
264	76.9	57.2	85.8



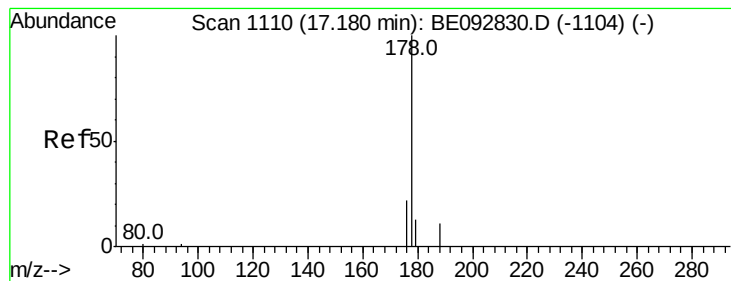

#21

Phenanthrene

Concen: 0.44 ng

RT: 17.18 min Scan# 1111

Delta R.T. -0.00 min

Lab File: BE092836.D

Acq: 28 Mar 2017 14:25

Instrument :

BNA_E





ClientSampleId :

ICVBE032817

Tot Ion	Ratio	Lower	Upper
178	100		
176	19.7	15.8	23.8
179	15.6	16.0	24.0

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:26 PM

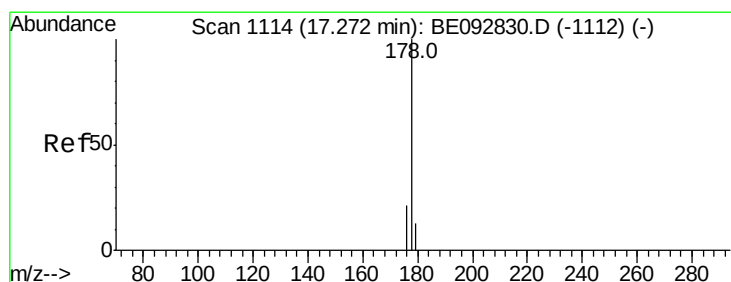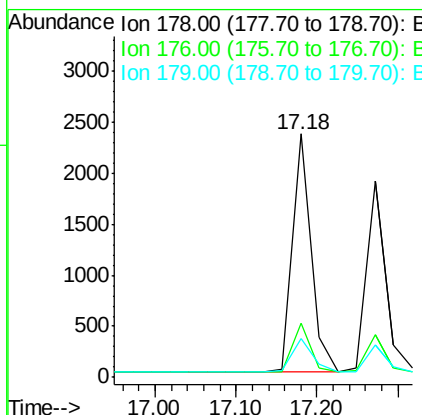

#22

Anthracene

Concen: 0.39 ng


RT: 17.27 min Scan# 1115


Delta R.T. -0.00 min

Lab File: BE092836.D

Acq: 28 Mar 2017 14:25

Tgt Ion	Ratio	Lower	Upper
178	100		
176	19.4	15.0	22.4
179	14.8	12.2	18.2

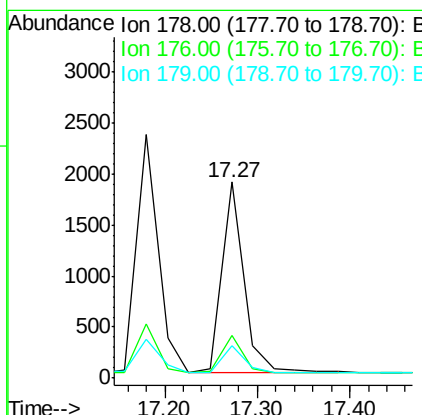



#23

Fluoranthene

Concen: 0.37 ng

RT: 19.18 min Scan# 1199

Delta R.T. 0.00 min

Lab File: BE092836.D

Acq: 28 Mar 2017 14:25

Instrument :

BNA_E


ClientSampleId :

ICVBE032817

Tot Ion:	202	Resp:	14541
Ion Ratio	Lower	Upper	
202	100		
101	3.1	2.2	3.4
203	17.6	13.7	20.5

Manual Integrations
APPROVED




mohammad
3/29/2017 2:37:26 PM



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

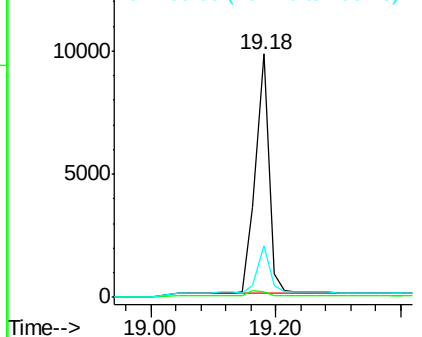

#24

Chrysene-d12

Concen: 5.00 ng


RT: 21.28 min Scan# 1320

Delta R.T. -0.02 min

Lab File: BE092836.D

Acq: 28 Mar 2017 14:25



Tgt Ion:	240	Resp:	42258
Ion Ratio	Lower	Upper	
240	100		
120	19.9	2.6	4.0#
236	33.1	24.6	37.0




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

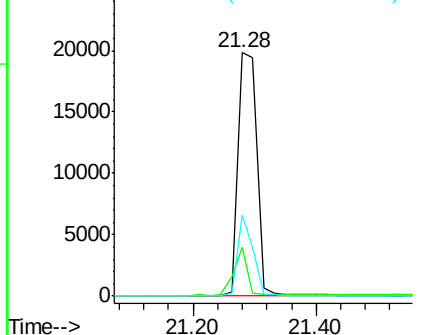







#25
Pvrene
Concen: 0.37 ng
RT: 19.54 min Scan# 1220
Delta R.T. 0.00 min
Lab File: BE092836.D
Acq: 28 Mar 2017 14:25

Instrument :
BNA_E
ClientSampleId :
ICVBE032817

Tot Ion	Ratio	Resp Lower	Upper
202	100		
200	5.0	4.2	6.4
203	17.9	13.9	20.9




Manual Integrations
APPROVED


mohammad
3/29/2017 2:37:26 PM

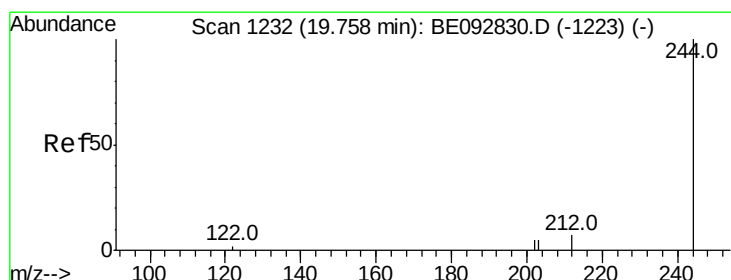

#26
Terphenyl-d14
Concen: 0.37 ng
RT: 19.76 min Scan# 1233
Delta R.T. 0.00 min
Lab File: BE092836.D
Acq: 28 Mar 2017 14:25

Tgt Ion	Ratio	Resp Lower	Upper
244	100		
212	9.1	6.7	10.1
122	3.8	3.6	5.4





#27

Benzo(a)anthracene

Concen: 0.37 ng

RT: 21.26 min Scan# 1319

Delta R.T. -0.00 min

Lab File: BE092836.D





Acq: 28 Mar 2017 14:25

Instrument :
BNA_E
ClientSampleId :
ICVBE032817

Tot Ion	Ratio	Lower	Upper
228	100		
226	30.9	23.6	35.4
229	18.5	13.3	19.9

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:26 PM

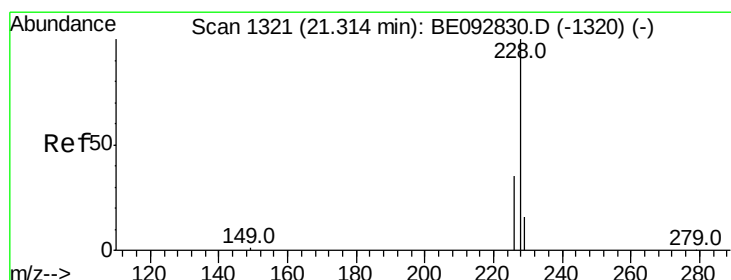

#28

Chrysene

Concen: 0.39 ng




RT: 21.31 min Scan# 1322




Delta R.T. -0.00 min

Lab File: BE092836.D

Acq: 28 Mar 2017 14:25

Tgt Ion	Ratio	Lower	Upper
228	100		
226	34.2	36.3	54.5#
229	18.5	10.6	16.0#

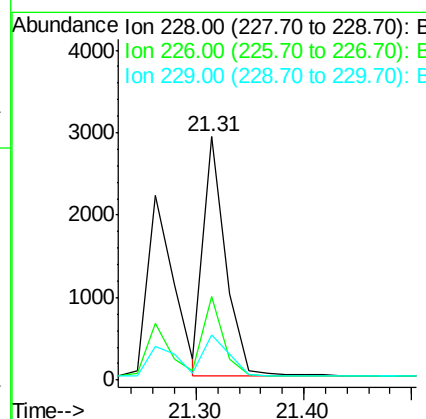



#29

Bis(2-ethylhexyl)phthalate

Concen: 0.36 ng

RT: 21.23 min Scan# 1317

Delta R.T. 0.00 min

Lab File: BE092836.D

Acq: 28 Mar 2017 14:25

Instrument :

BNA_E





ClientSampleId :

ICVBE032817

Tot Ion:	149	Resp:	887
Ion Ratio	Lower	Upper	
149	100		
167	24.6	16.0	24.0#
279	2.9	16.0	24.0#

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:26 PM

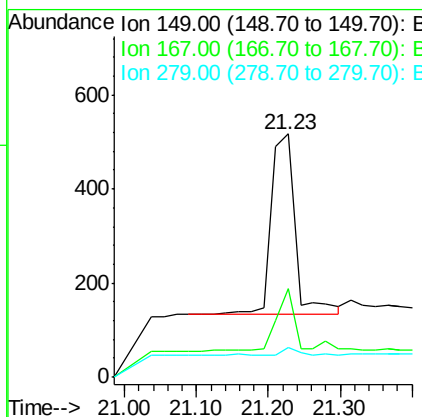

#30

Indeno(1,2,3-cd)pyrene

Concen: 0.37 ng


RT: 26.25 min Scan# 1704


Delta R.T. -0.00 min

Lab File: BE092836.D

Acq: 28 Mar 2017 14:25

Tgt Ion:	276	Resp:	14522
Ion Ratio	Lower	Upper	
276	100		
138	32.2	20.3	30.5#
277	24.8	19.7	29.5

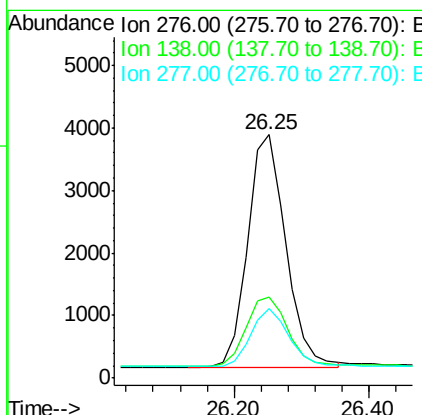

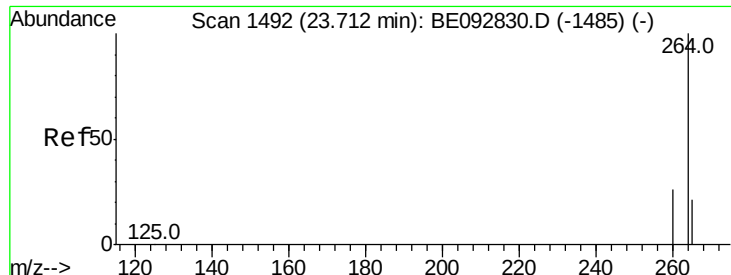





#31
Pervlene-d12
Concen: 5.00 ng
RT: 23.71 min Scan# 1493
Delta R.T. 0.00 min
Lab File: BE092836.D
Acq: 28 Mar 2017 14:25

Instrument :
BNA_E
ClientSampleId :
ICVBE032817

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.4	20.1	30.1
265	22.5	17.9	26.9




Manual Integrations
APPROVED


mohammad
3/29/2017 2:37:26 PM

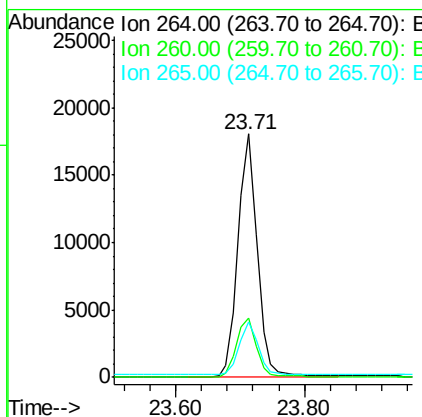

#32
Benzo(b)fluoranthene
Concen: 0.34 ng m
RT: 22.96 min Scan# 1428
Delta R.T. -0.01 min
Lab File: BE092836.D
Acq: 28 Mar 2017 14:25

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.5	18.7	28.1
125	16.2	10.5	15.7#

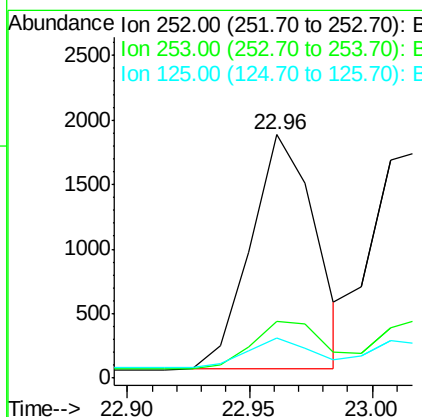



#33

Benzo(k)fluoranthene

Concen: 0.39 ng

RT: 23.02 min Scan# 1433

Delta R.T. 0.00 min

Lab File: BE092836.D

Acq: 28 Mar 2017 14:25





Instrument :
BNA_E

ClientSampleId :
ICVBE032817

Tot Ion	Ratio	Lower	Upper
252	100		
253	25.6	20.3	30.5
125	15.5	9.6	14.4

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:26 PM

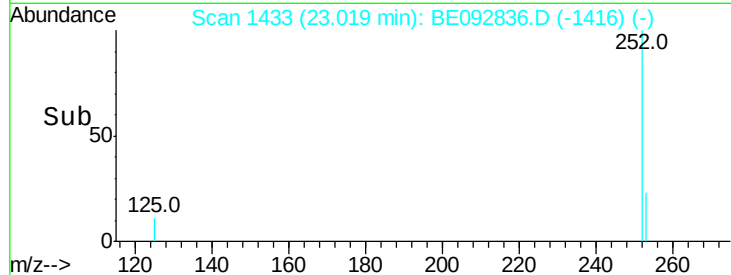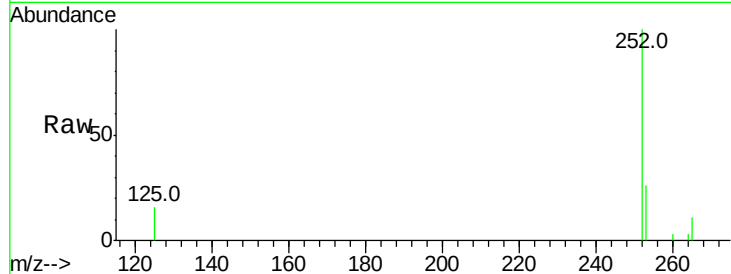

#34

Benzo(a)pyrene

Concen: 0.35 ng




RT: 23.60 min Scan# 1483


Delta R.T. 0.00 min

Lab File: BE092836.D

Acq: 28 Mar 2017 14:25

Tgt Ion	Ratio	Lower	Upper
252	100		
253	26.1	19.0	28.6
125	18.4	11.8	17.8









#35
Dibenzo(a,h)anthracene
Concen: 0.36 ng
RT: 26.29 min Scan# 1706
Delta R.T. -0.00 min
Lab File: BE092836.D
Acq: 28 Mar 2017 14:25

Instrument :
BNA_E
ClientSampleId :
ICVBE032817

Tot Ion	Ratio	Lower	Upper
278	100		
139	19.5	13.8	20.8
279	29.0	21.4	32.2

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:26 PM

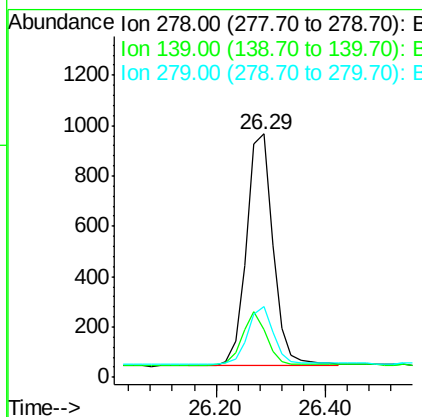

#36
Benzo(g,h,i)perylene
Concen: 0.37 ng
RT: 27.02 min Scan# 1749
Delta R.T. -0.00 min
Lab File: BE092836.D
Acq: 28 Mar 2017 14:25

Tgt Ion	Ratio	Lower	Upper
276	100		
277	27.0	19.8	29.8
138	30.3	19.8	29.6#

