

Data Path : Z:\HPCHEM1\BNA E\DATA\BE032817\
 Data File : BE092845.D
 Acq On : 28 Mar 2017 20:56
 Operator : SJ/MA
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC0.4

Manual Integrations
 APPROVED

mohammad
 3/29/2017 2:37:34 PM

Quant Time: Mar 29 05:58:01 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE032817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 28 14:58:05 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	7560	5.00	ng	-0.02
7) Naphthalene-d8	10.55	136	34153	5.00	ng	0.00
12) Acenaphthene-d10	14.40	164	16785	5.00	ng	0.00
18) Phenanthrene-d10	17.13	188	36828	5.00	ng	-0.02
24) Chrysene-d12	21.28	240	44694	5.00	ng	-0.02
31) Perylene-d12	23.71	264	38817	5.00	ng	0.00

System Monitoring Compounds

4) 2-Fluorophenol	5.36	112	658	0.37	ng	0.00
5) Phenol-d6	6.94	99	936m	0.36	ng	0.00
8) Nitrobenzene-d5	8.93	82	757	0.39	ng	0.00
13) 2,4,6-Tribromophenol	15.88	330	88	0.34	ng	0.00
14) 2-Fluorobiphenyl	13.02	172	2263	0.41	ng	-0.01
26) Terphenyl-d14	19.76	244	2832	0.37	ng	0.00

Target Compounds

						Qvalue
2) 1,4-Dioxane	3.32	88	403	0.40	ng	95
3) n-Nitrosodimethylamine	3.61	42	388	0.37	ng	# 85
6) bis(2-Chloroethyl)ether	7.20	93	998	0.41	ng	# 45
9) Naphthalene	10.58	128	2964	0.40	ng	97
10) Hexachlorobutadiene	10.89	225	387	0.39	ng	99
11) 2-Methylnaphthalene	12.21	142	1844	0.39	ng	96
15) Acenaphthylene	14.11	152	8763	0.34	ng	100
16) Acenaphthene	14.45	154	1775	0.39	ng	83
17) Fluorene	15.44	166	2113	0.39	ng	98
19) Hexachlorobenzene	16.47	284	579	0.42	ng	# 67
20) Pentachlorophenol	16.81	266	117	0.48	ng	89
21) Phenanthrene	17.18	178	4238	0.47	ng	# 95
22) Anthracene	17.27	178	3288	0.40	ng	99
23) Fluoranthene	19.18	202	19716	0.48	ng	# 70
25) Pyrene	19.54	202	16499	0.37	ng	98
27) Benzo(a)anthracene	21.26	228	3925	0.37	ng	97
28) Chrysene	21.31	228	4477	0.40	ng	# 83
29) Bis(2-ethylhexyl)phthalate	21.21	149	851	0.33	ng	# 78
30) Indeno(1,2,3-cd)pyrene	26.24	276	14394	0.34	ng	# 92
32) Benzo(b)fluoranthene	22.96	252	3603	0.35	ng	97
33) Benzo(k)fluoranthene	23.01	252	3528	0.38	ng	# 94
34) Benzo(a)pyrene	23.60	252	2804	0.33	ng	# 94
35) Dibenzo(a,h)anthracene	26.27	278	3233	0.36	ng	# 94
36) Benzo(g,h,i)perylene	27.02	276	13736	0.36	ng	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032817\
Data File : BE092845.D
Acq On : 28 Mar 2017 20:56
Operator : SJ/MA
Sample : SSTDCCC0.4
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:34 PM

Quant Time: Mar 29 05:58:01 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE032817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 28 14:58:05 2017
Response via : Initial Calibration





#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.77 min Scan# 555

Delta R.T. -0.02 min

Lab File: BE092845.D

Acq: 28 Mar 2017 20:56

Instrument :

BNA_E





ClientSampleId :

SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
152	100		
150	190.6	106.0	159.0#
115	106.3	31.2	46.8#

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:34 PM



#2

1,4-Dioxane

Concen: 0.40 ng




RT: 3.32 min Scan# 63


Delta R.T. -0.00 min

Lab File: BE092845.D

Acq: 28 Mar 2017 20:56

Tgt Ion	Ratio	Lower	Upper
88	100		
58	76.7	63.6	95.4
43	29.5	28.0	42.0





#3





n-Nitrosodimethylamine
Concen: 0.37 ng
RT: 3.61 min Scan# 88
Delta R.T. -0.00 min
Lab File: BE092845.D
Acq: 28 Mar 2017 20:56

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
42	100		
74	122.9	86.0	129.0
44	12.4	5.1	7.7#

Manual Integrations
APPROVED




mohammad
3/29/2017 2:37:34 PM






#4

2-Fluorophenol
Concen: 0.37 ng
RT: 5.36 min Scan# 267
Delta R.T. -0.00 min
Lab File: BE092845.D
Acq: 28 Mar 2017 20:56

Tgt Ion	Ratio	Lower	Upper
112	100		
64	67.9	53.5	80.3
63	35.1	27.9	41.9





#5

Phenol-d6

Concen: 0.36 ng/mL

RT: 6.94 min Scan# 519

Delta R.T. -0.00 min

Lab File: BE092845.D

Acq: 28 Mar 2017 20:56

Tot Ion	Ratio	Lower	Upper
99	100		
42	0.0	16.0	24.0#
71	0.0	30.6	45.8#

Instrument :





BNA_E

ClientSampleId :

SSTDCCC0.4

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:34 PM



#6

bis(2-Chloroethyl)ether

Concen: 0.41 ng/mL


RT: 7.20 min Scan# 530


Delta R.T. -0.00 min

Lab File: BE092845.D

Acq: 28 Mar 2017 20:56

Tgt Ion	Ratio	Lower	Upper
93	100		
63	82.0	16.0	24.0#
95	30.8	24.0	36.0





#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.55 min Scan# 679

Delta R.T. 0.00 min

Lab File: BE092845.D

Acq: 28 Mar 2017 20:56

Instrument :

BNA_E





ClientSampleId :

SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
136	100		
137	11.8	8.2	12.4
54	4.5	9.6	14.4#
68	4.5	6.7	10.1#

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:34 PM



#8

Nitrobenzene-d5

Concen: 0.39 ng




RT: 8.93 min Scan# 605


Delta R.T. -0.00 min

Lab File: BE092845.D

Acq: 28 Mar 2017 20:56

Tgt Ion	Ratio	Lower	Upper
82	100		
128	50.6	39.0	58.4
54	39.5	44.8	67.2#





#9

Naphthalene

Concen: 0.40 ng

RT: 10.58 min Scan# 681

Delta R.T. 0.00 min

Lab File: BE092845.D

Acq: 28 Mar 2017 20:56

Instrument :

BNA_E





ClientSampleId :

SSTDCCC0.4

Tot Ion:	128	Resp:	2964
Ion	Ratio	Lower	Upper
128	100		
129	12.9	11.2	16.8
127	15.7	11.6	17.4

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:34 PM



#10

Hexachlorobutadiene

Concen: 0.39 ng




RT: 10.89 min Scan# 697


Delta R.T. 0.00 min

Lab File: BE092845.D

Acq: 28 Mar 2017 20:56

Tgt Ion:	225	Resp:	387
Ion	Ratio	Lower	Upper
225	100		
223	64.1	50.6	76.0
227	64.3	51.4	77.0



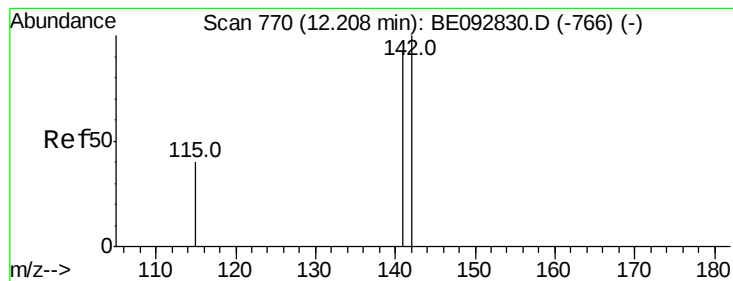

#11

2-Methylnaphthalene

Concen: 0.39 ng

RT: 12.21 min Scan# 770

Delta R.T. -0.00 min

Lab File: BE092845.D

Acq: 28 Mar 2017 20:56

Instrument :

BNA_E





ClientSampleId :

SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
142	100		
141	88.9	73.7	110.5
115	38.2	34.0	51.0

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:34 PM



#12

Acenaphthene-d10

Concen: 5.00 ng




RT: 14.40 min Scan# 933


Delta R.T. -0.00 min

Lab File: BE092845.D

Acq: 28 Mar 2017 20:56

Tgt Ion	Ratio	Lower	Upper
164	100		
162	96.0	71.4	107.0
160	40.2	27.4	41.2









#13
 2,4,6-Tribromophenol
 Concen: 0.34 ng
 RT: 15.88 min Scan# 1042
 Delta R.T. 0.00 min
 Lab File: BE092845.D
 Acq: 28 Mar 2017 20:56

Instrument :
 BNA_E
 ClientSampleId :
 SSTCCCC0.4

Tot Ion:330 Resp: 88
 Ion Ratio Lower Upper
 330 100
 332 94.3 75.4 113.0
 141 59.1 31.0 46.6#




Manual Integrations
 APPROVED


mohammad
 3/29/2017 2:37:34 PM



#14
 2-Fluorobiphenyl
 Concen: 0.41 ng
 RT: 13.02 min Scan# 840
 Delta R.T. -0.01 min
 Lab File: BE092845.D
 Acq: 28 Mar 2017 20:56

Tgt Ion:172 Resp: 2263
 Ion Ratio Lower Upper
 172 100
 171 38.6 30.1 45.1
 170 26.9 21.8 32.6





#15

Acenaphthylene

Concen: 0.34 ng

RT: 14.11 min Scan# 916

Delta R.T. -0.00 min

Lab File: BE092845.D

Acq: 28 Mar 2017 20:56

Instrument :

BNA_E





ClientSampleId :

SSTDCCC0.4

Tot Ion:	152	Resp:	8763
Ion	Ratio	Lower	Upper
152	100		
151	4.8	3.9	5.9
153	12.9	10.4	15.6

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:34 PM



#16

Acenaphthene

Concen: 0.39 ng




RT: 14.45 min Scan# 936

Delta R.T. -0.00 min

Lab File: BE092845.D

Acq: 28 Mar 2017 20:56

Tgt Ion:	154	Resp:	1775
Ion	Ratio	Lower	Upper
154	100		
153	482.6	350.8	526.2
152	237.8	171.1	256.7









#17
Fluorene
 Concen: 0.39 ng
 RT: 15.44 min Scan# 1004
 Delta R.T. -0.00 min
 Lab File: BE092845.D
 Acq: 28 Mar 2017 20:56

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
166	100		
165	100.2	78.2	117.4
167	14.1	11.0	16.4




Manual Integrations
 APPROVED

mohammad
 3/29/2017 2:37:34 PM



#18
Phenanthrene-d10
 Concen: 5.00 ng
 RT: 17.13 min Scan# 1109
 Delta R.T. -0.02 min
 Lab File: BE092845.D
 Acq: 28 Mar 2017 20:56

Tgt Ion	Ratio	Lower	Upper
188	100		
94	22.7	3.2	4.8#
80	25.5	2.6	3.8#









#19
Hexachlorobenzene
Concen: 0.42 ng
RT: 16.47 min Scan# 1080
Delta R.T. 0.00 min
Lab File: BE092845.D
Acq: 28 Mar 2017 20:56

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
284	100		
142	0.0	29.1	43.7#
249	33.2	27.9	41.9




Manual Integrations
APPROVED


mohammad
3/29/2017 2:37:34 PM



#20
Pentachlorophenol
Concen: 0.48 ng
RT: 16.81 min Scan# 1095
Delta R.T. 0.00 min
Lab File: BE092845.D
Acq: 28 Mar 2017 20:56

Tgt Ion	Ratio	Lower	Upper
266	100		
268	90.4	62.5	93.7
264	77.1	57.2	85.8









#21
Phenanthrene
Concen: 0.47 ng
RT: 17.18 min Scan# 1111
Delta R.T. 0.00 min
Lab File: BE092845.D
Acq: 28 Mar 2017 20:56

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
178	100		
176	19.5	15.8	23.8
179	15.7	16.0	24.0




Manual Integrations
APPROVED


mohammad
3/29/2017 2:37:34 PM



#22
Anthracene
Concen: 0.40 ng
RT: 17.27 min Scan# 1115
Delta R.T. 0.00 min
Lab File: BE092845.D
Acq: 28 Mar 2017 20:56

Tgt Ion	Ratio	Lower	Upper
178	100		
176	18.2	15.0	22.4
179	15.7	12.2	18.2





#23

Fluoranthene

Concen: 0.48 ng

RT: 19.18 min Scan# 1199

Delta R.T. 0.00 min

Lab File: BE092845.D

Acq: 28 Mar 2017 20:56

Instrument :

BNA_E





ClientSampleId :

SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
202	100		
101	6.3	2.2	3.4#
203	31.4	13.7	20.5#

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:34 PM



#24

Chrysene-d12

Concen: 5.00 ng




RT: 21.28 min Scan# 1320


Delta R.T. -0.02 min

Lab File: BE092845.D

Acq: 28 Mar 2017 20:56

Tgt Ion	Ratio	Lower	Upper
240	100		
120	14.1	2.6	4.0#
236	31.8	24.6	37.0









#25
Pvrene
Concen: 0.37 ng
RT: 19.54 min Scan# 1220
Delta R.T. 0.00 min
Lab File: BE092845.D
Acq: 28 Mar 2017 20:56

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Tot Ion	Ratio	Resp	Lower	Upper
202	100	16499		
200	5.0		4.2	6.4
203	18.1		13.9	20.9




Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:34 PM



#26
Terphenyl-d14
Concen: 0.37 ng
RT: 19.76 min Scan# 1233
Delta R.T. 0.00 min
Lab File: BE092845.D
Acq: 28 Mar 2017 20:56

Tgt Ion	Ratio	Resp	Lower	Upper
244	100	2832		
212	9.0		6.7	10.1
122	4.1		3.6	5.4





#27

Benzo(a)anthracene

Concen: 0.37 ng

RT: 21.26 min Scan# 1319

Delta R.T. -0.00 min

Lab File: BE092845.D





Acq: 28 Mar 2017 20:56

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
228	100		
226	30.6	23.6	35.4
229	18.8	13.3	19.9

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:34 PM



#28

Chrysene

Concen: 0.40 ng




RT: 21.31 min Scan# 1322


Delta R.T. -0.00 min

Lab File: BE092845.D

Acq: 28 Mar 2017 20:56

Tgt Ion	Ratio	Lower	Upper
228	100		
226	33.3	36.3	54.5#
229	18.8	10.6	16.0#









#29
Bis(2-ethylhexyl)phthalate
Concen: 0.33 ng
RT: 21.21 min Scan# 1316
Delta R.T. -0.02 min
Lab File: BE092845.D
Acq: 28 Mar 2017 20:56

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
149	100		
167	24.1	16.0	24.0#
279	4.2	16.0	24.0#




Manual Integrations
APPROVED


mohammad
3/29/2017 2:37:34 PM



#30
Indeno(1,2,3-cd)pyrene
Concen: 0.34 ng
RT: 26.24 min Scan# 1703
Delta R.T. -0.02 min
Lab File: BE092845.D
Acq: 28 Mar 2017 20:56

Tgt Ion	Ratio	Lower	Upper
276	100		
138	32.6	20.3	30.5#
277	25.1	19.7	29.5









#31
Pervlene-d12
Concen: 5.00 ng
RT: 23.71 min Scan# 1493
Delta R.T. -0.00 min
Lab File: BE092845.D
Acq: 28 Mar 2017 20:56

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.8	20.1	30.1
265	22.9	17.9	26.9




Manual Integrations
APPROVED


mohammad
3/29/2017 2:37:34 PM



#32
Benzo(b)fluoranthene
Concen: 0.35 ng
RT: 22.96 min Scan# 1428
Delta R.T. -0.01 min
Lab File: BE092845.D
Acq: 28 Mar 2017 20:56

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.6	18.7	28.1
125	15.6	10.5	15.7









#33
Benzo(k)fluoranthene
Concen: 0.38 ng
RT: 23.01 min Scan# 1432
Delta R.T. -0.01 min
Lab File: BE092845.D
Acq: 28 Mar 2017 20:56

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.3	20.3	30.5
125	16.4	9.6	14.4




Manual Integrations
APPROVED


mohammad
3/29/2017 2:37:34 PM



#34
Benzo(a)pyrene
Concen: 0.33 ng
RT: 23.60 min Scan# 1483
Delta R.T. -0.00 min
Lab File: BE092845.D
Acq: 28 Mar 2017 20:56

Tgt Ion	Ratio	Lower	Upper
252	100		
253	26.2	19.0	28.6
125	17.8	11.8	17.8









#35
Dibenzo(a,h)anthracene
Concen: 0.36 ng
RT: 26.27 min Scan# 1705
Delta R.T. -0.02 min
Lab File: BE092845.D
Acq: 28 Mar 2017 20:56

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
278	100		
139	23.1	13.8	20.8#
279	27.4	21.4	32.2

Manual Integrations
APPROVED

mohammad
3/29/2017 2:37:34 PM



#36
Benzo(g,h,i)perylene
Concen: 0.36 ng
RT: 27.02 min Scan# 1749
Delta R.T. 0.00 min
Lab File: BE092845.D
Acq: 28 Mar 2017 20:56

Tgt Ion	Ratio	Lower	Upper
276	100		
277	27.5	19.8	29.8
138	29.1	19.8	29.6

