


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032817\
 Data File : BE092827.D
 Acq On : 28 Mar 2017 8:51
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 28 14:58:05 2017

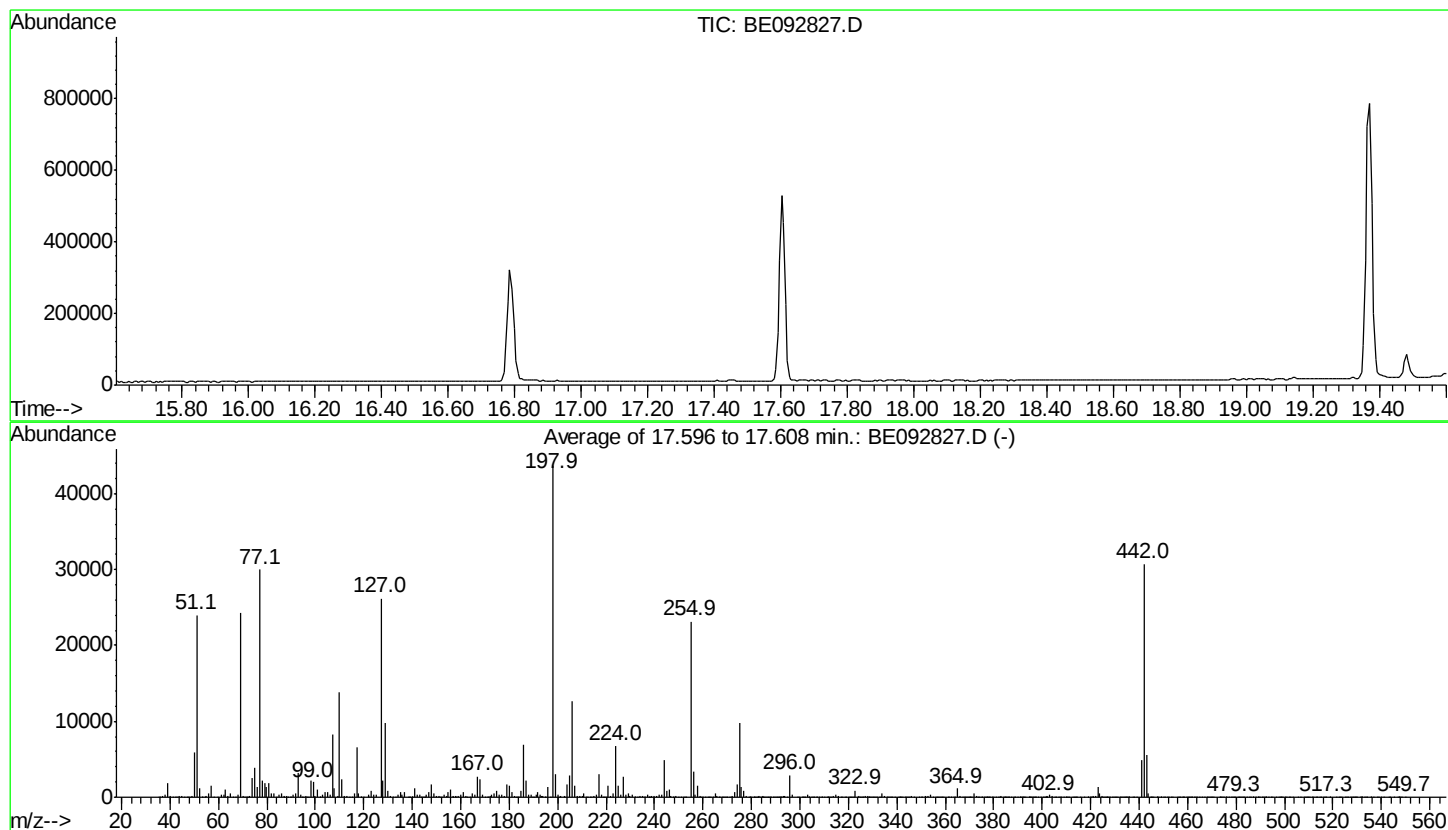

AutoFind: Scans 2554, 2555, 2556; Background Corrected with Scan 2547

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.8	23957	PASS
68	69	0.00	2	1.1	269	PASS
69	198	0.00	100	55.7	24348	PASS
70	69	0.00	2	0.5	126	PASS
127	198	10	80	59.9	26168	PASS
197	198	0.00	2	0.2	75	PASS
198	198	100	100	100.0	43679	PASS
199	198	5	9	7.1	3086	PASS
275	198	10	60	22.3	9737	PASS
365	198	1	100	2.6	1117	PASS
441	442	0.01	24	15.7	4835	PASS
442	198	50	100	70.3	30725	PASS
443	442	15	24	18.3	5634	PASS