


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032817\
 Data File : BE092844.D
 Acq On : 28 Mar 2017 19:41
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE032817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 28 14:58:05 2017

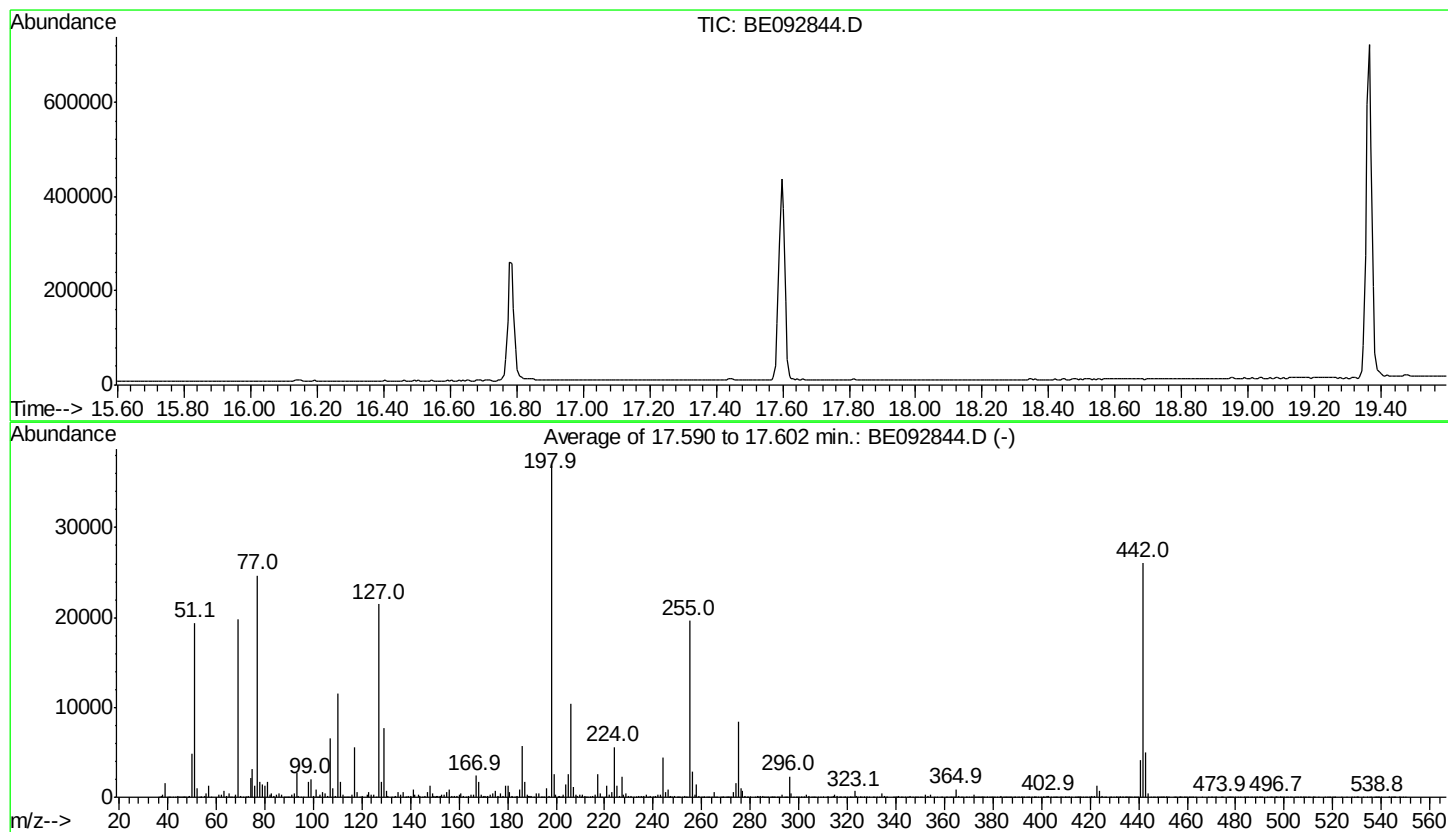

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2544

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.7	19440	PASS
68	69	0.00	2	1.6	310	PASS
69	198	0.00	100	53.7	19814	PASS
70	69	0.00	2	0.5	108	PASS
127	198	10	80	58.2	21487	PASS
197	198	0.00	2	0.3	129	PASS
198	198	100	100	100.0	36908	PASS
199	198	5	9	6.9	2543	PASS
275	198	10	60	22.6	8355	PASS
365	198	1	100	2.4	878	PASS
441	442	0.01	24	16.1	4195	PASS
442	198	50	100	70.7	26108	PASS
443	442	15	24	19.1	4987	PASS