
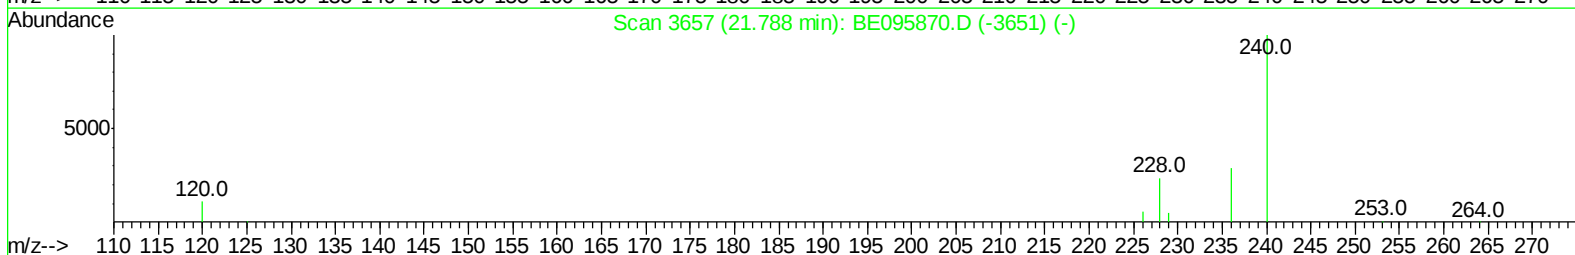
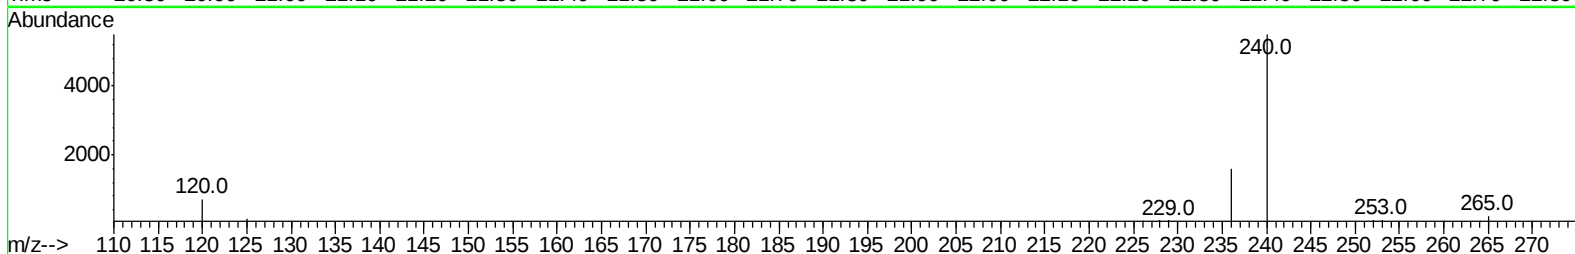


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095879.D
Acq On : 28 Mar 2018 16:34
Operator : SJ/JU
Sample : J1950-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Mar 29 04:33:26 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 16:31:37 2018
Response via : Initial Calibration

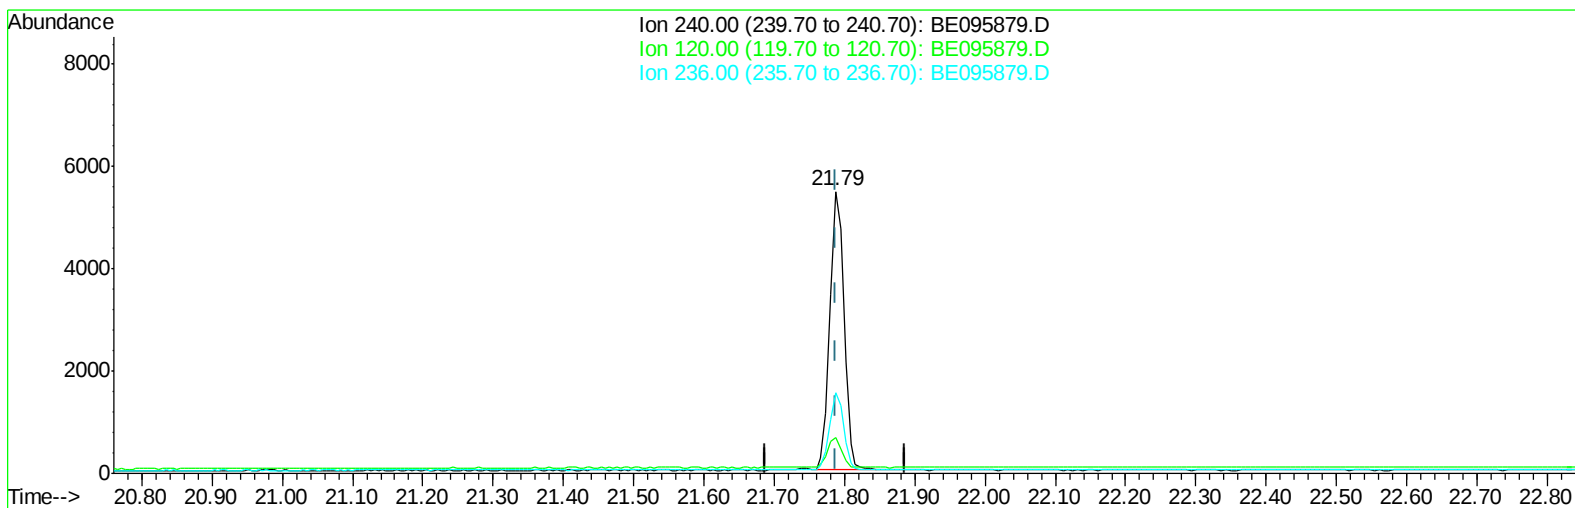

TIC: BE095879.D

(16) Chrysene-d12 (I)

21.787min (-0.000) 0.40ng/ul m

response 7512

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	12.87#
236.00	34.90	28.58
0.00	0.00	0.00