
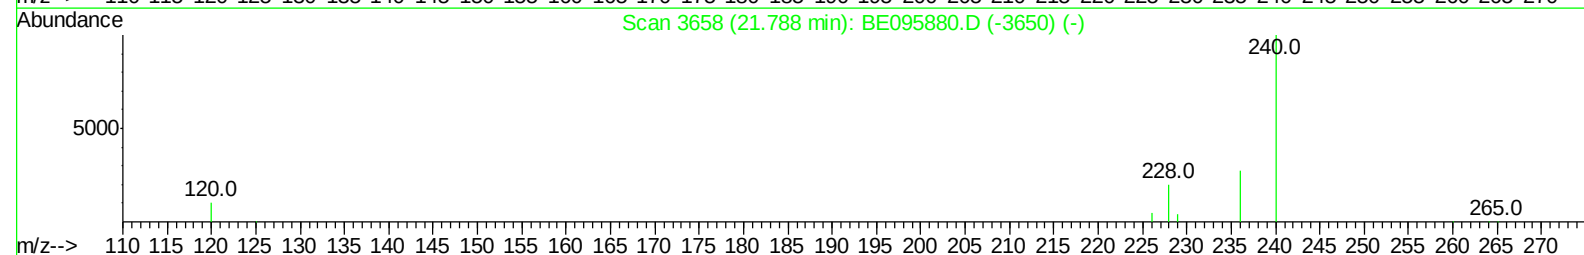
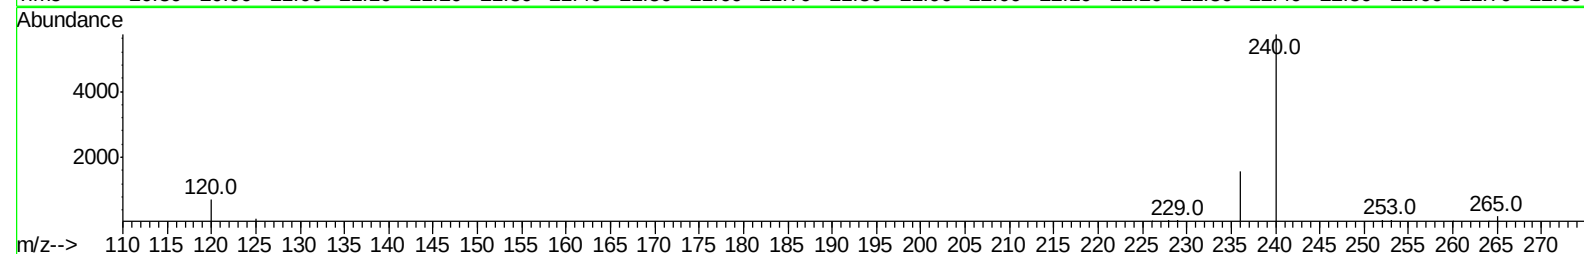


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095882.D
Acq On : 28 Mar 2018 18:19
Operator : SJ/JU
Sample : J1950-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Mar 29 04:43:34 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 04:43:20 2018
Response via : Initial Calibration

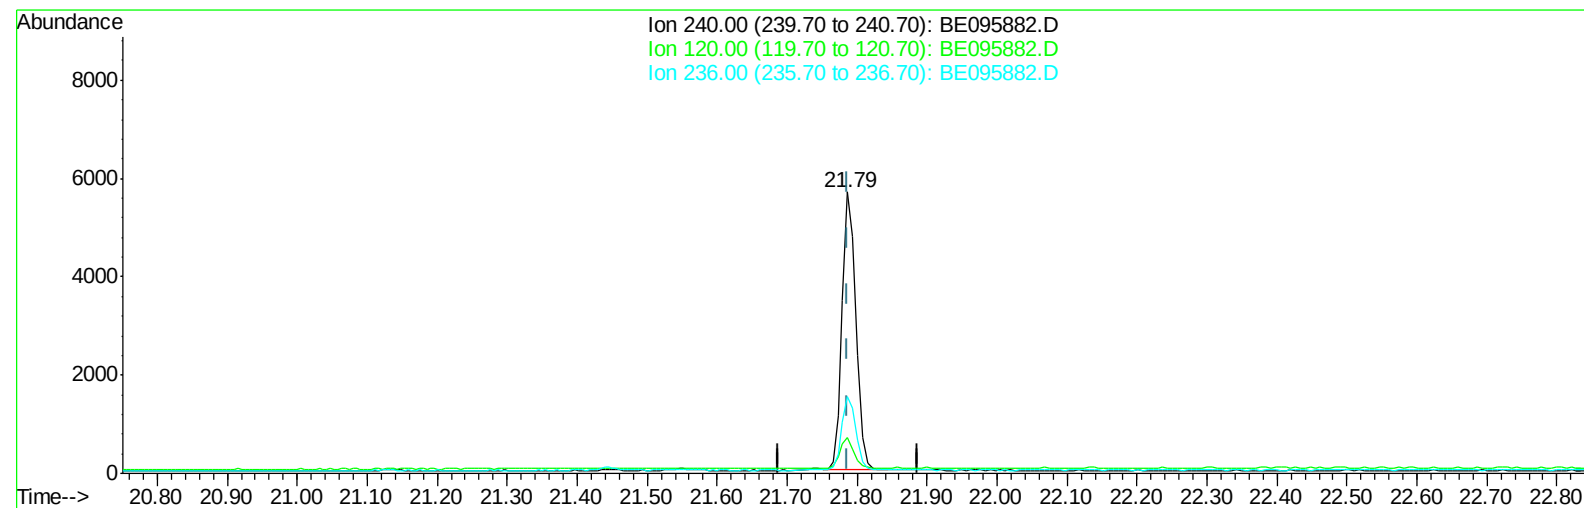

TIC: BE095882.D

(16) Chrysene-d12 (I)

21.787min (-0.001) 0.40ng/ul m

response 7755

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	12.52#
236.00	34.90	27.39#
0.00	0.00	0.00