
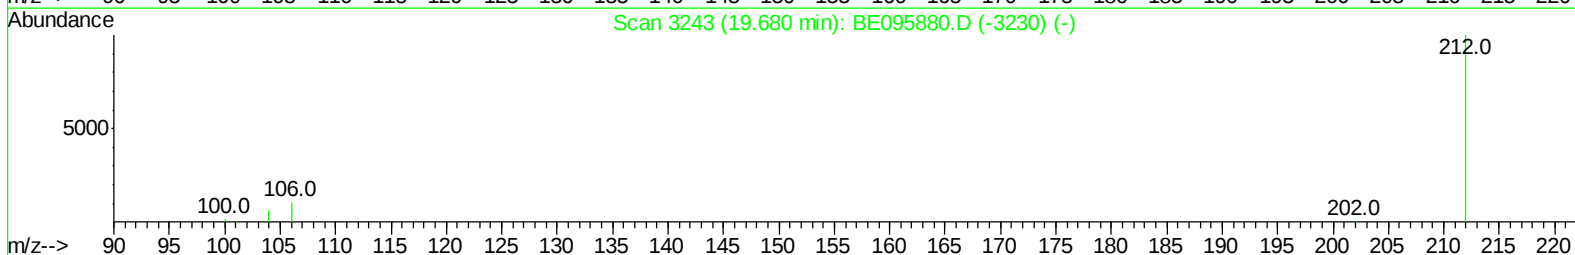
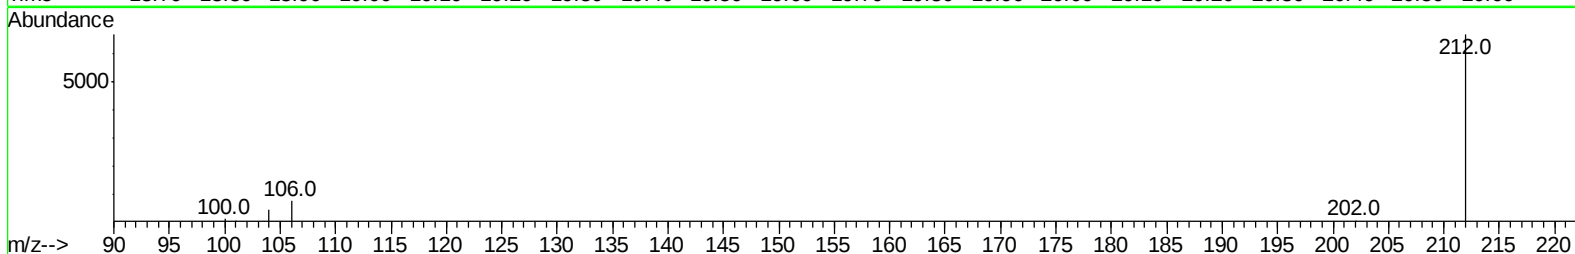


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095882.D
Acq On : 28 Mar 2018 18:19
Operator : SJ/JU
Sample : J1950-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Mar 29 05:13:41 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 04:43:20 2018
Response via : Initial Calibration

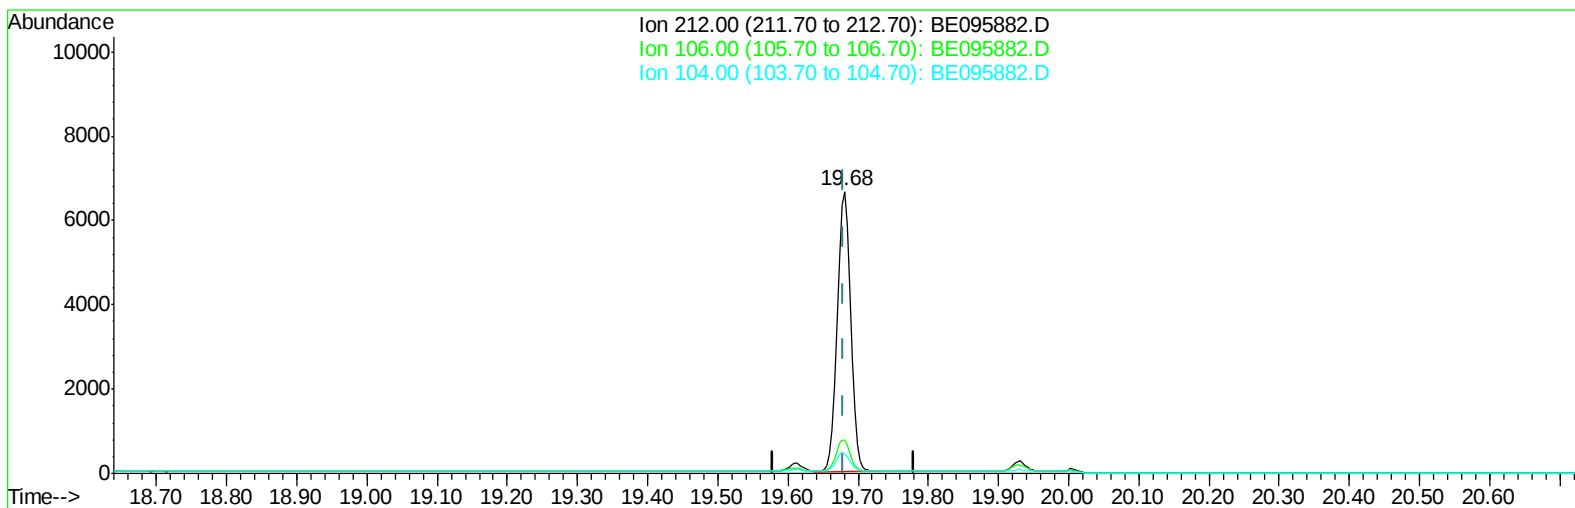

TIC: BE095882.D

(14) Fluoranthene-d10 (SURRE)

19.681min (+0.000) 0.36ng/ul m

response 8684

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00