
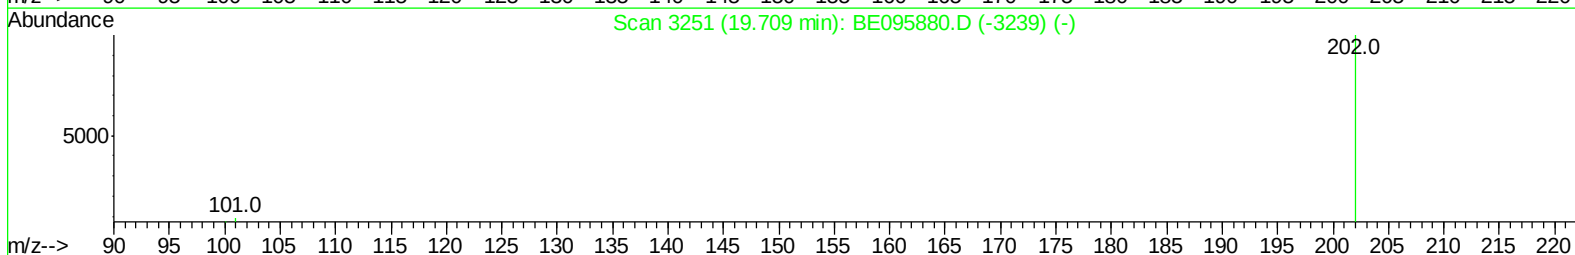
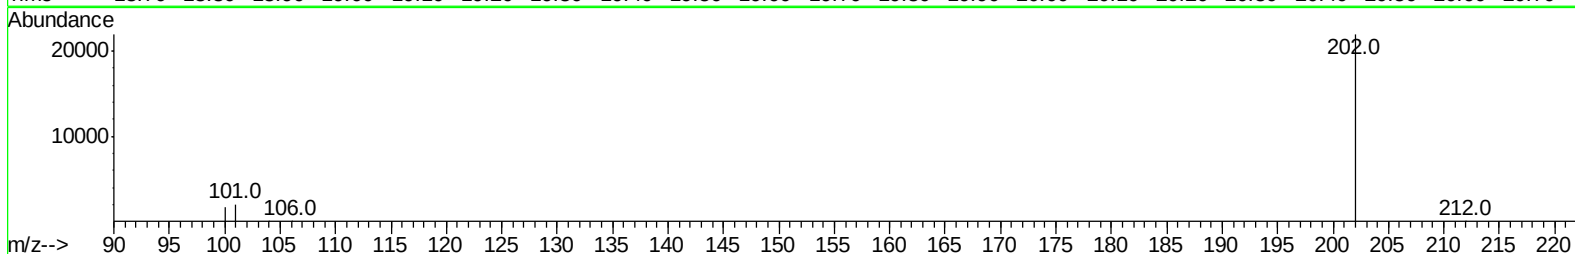


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095885.D
Acq On : 28 Mar 2018 20:06
Operator : SJ/JU
Sample : J1951-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Mar 29 05:30:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 04:43:20 2018
Response via : Initial Calibration

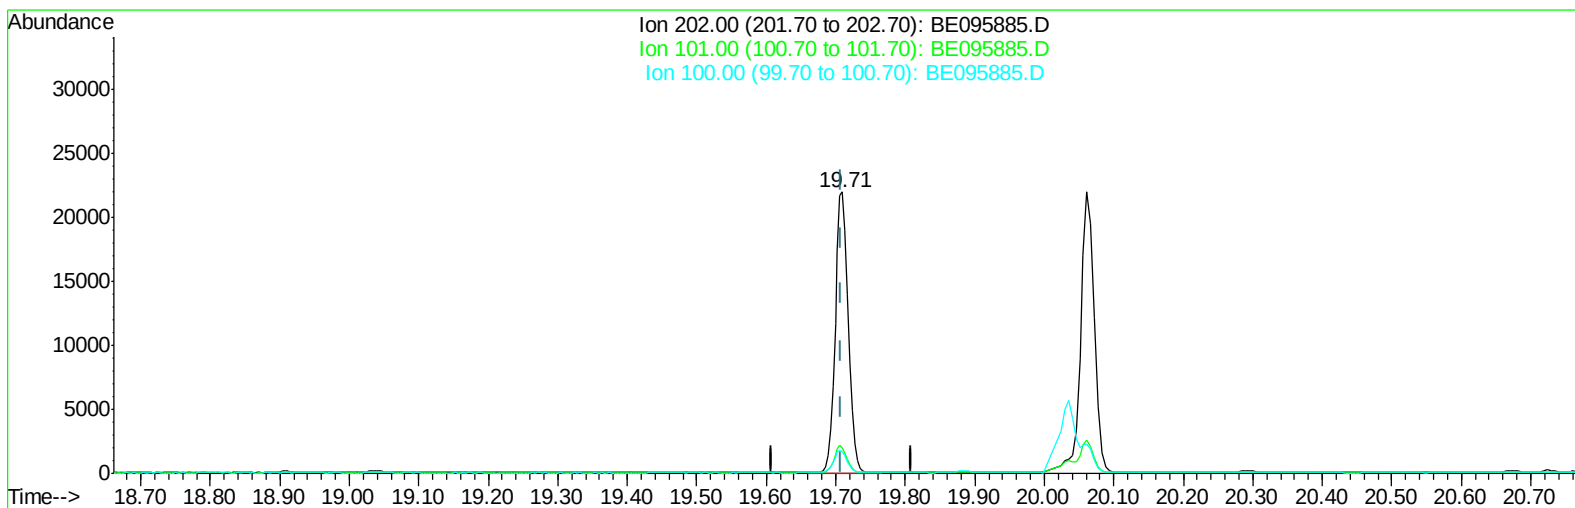

TIC: BE095885.D

(15) Fluoranthene (C)

19.710min (+0.001) 1.07ng/ul m

response 29296

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	9.27
100.00	19.50	7.56
0.00	0.00	0.00