
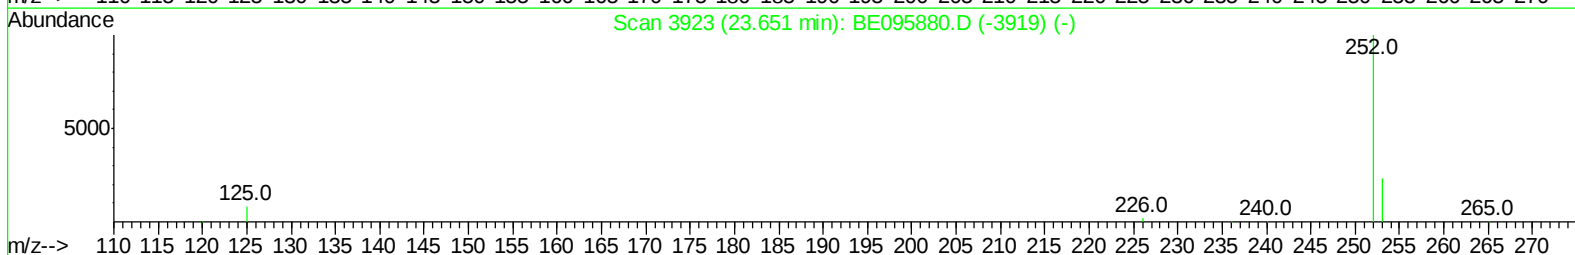
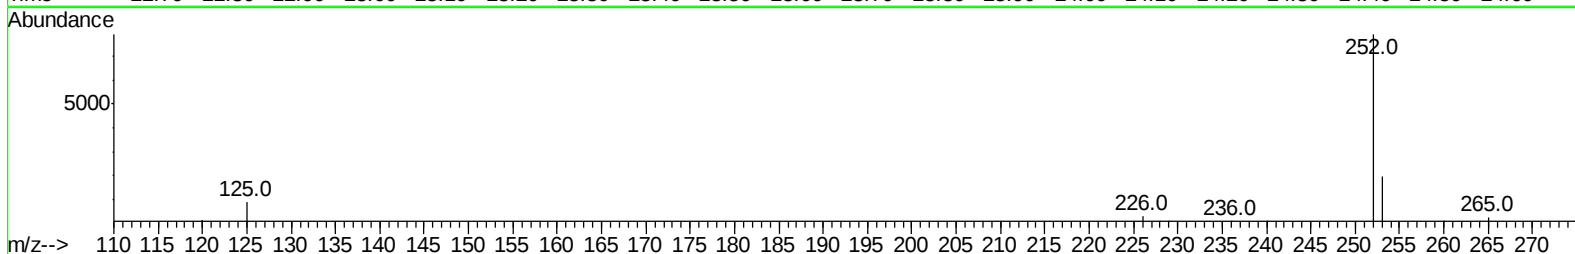


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095885.D
Acq On : 28 Mar 2018 20:06
Operator : SJ/JU
Sample : J1951-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Mar 29 05:30:37 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 04:43:20 2018
Response via : Initial Calibration

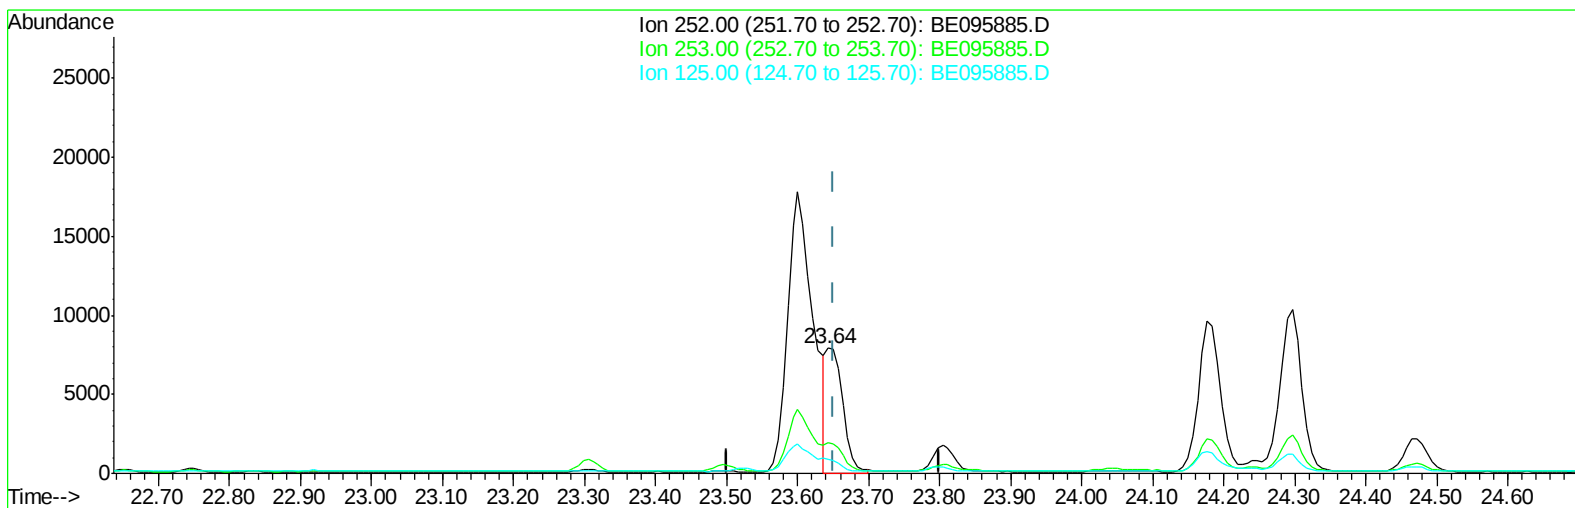

TIC: BE095885.D

(22) Benzo(k)fluoranthene

23.643min (-0.009) 0.46ng/ul m

response 13045

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	24.42#
125.00	17.10	11.09#
0.00	0.00	0.00