
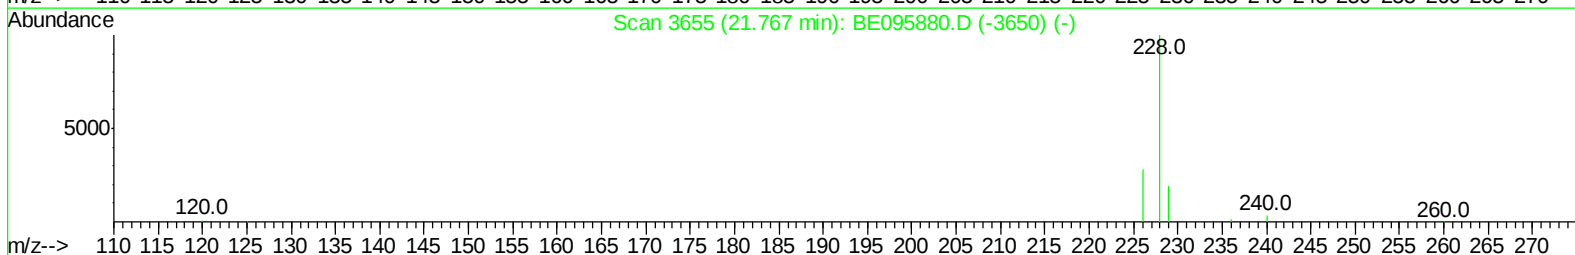
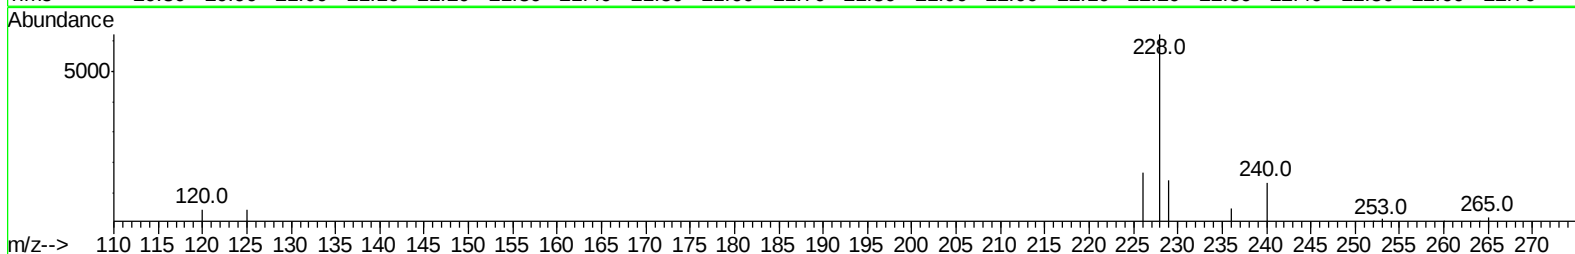


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095888.D
Acq On : 28 Mar 2018 21:54
Operator : SJ/JU
Sample : J2059-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Mar 29 05:49:07 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 04:43:20 2018
Response via : Initial Calibration

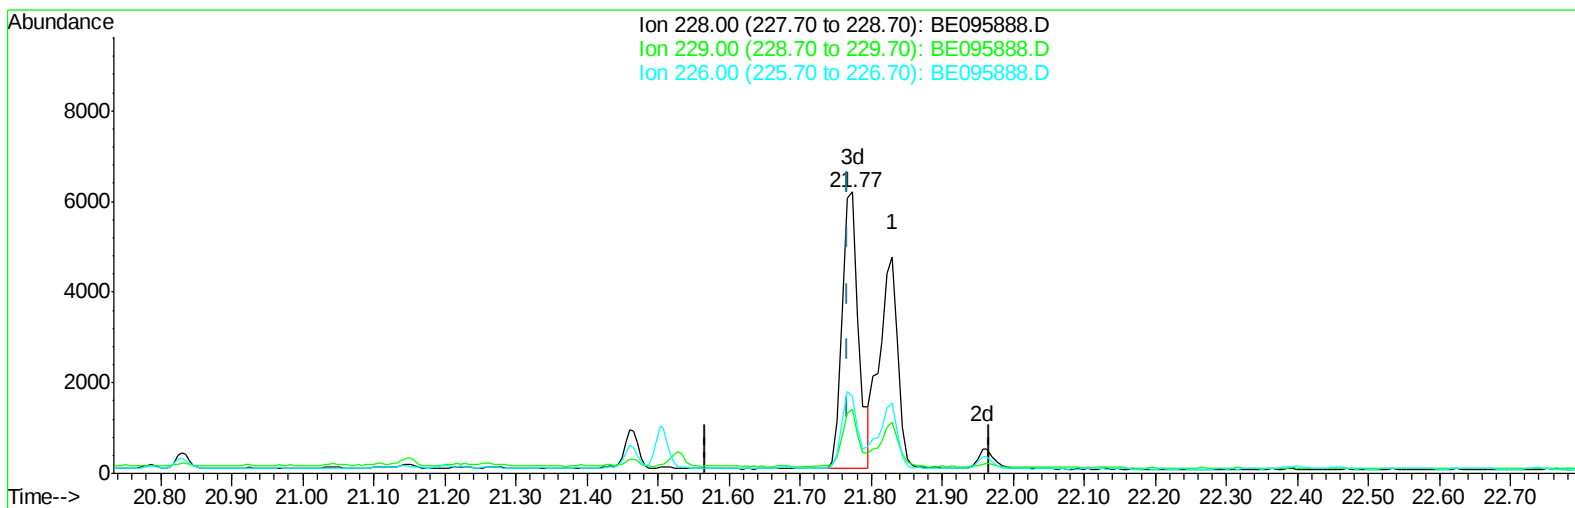

TIC: BE095888.D

(18) Benzo(a)anthracene

21.774min (+0.007) 0.41ng/ul m

response 9574

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	22.62#
226.00	21.30	27.25#
0.00	0.00	0.00