
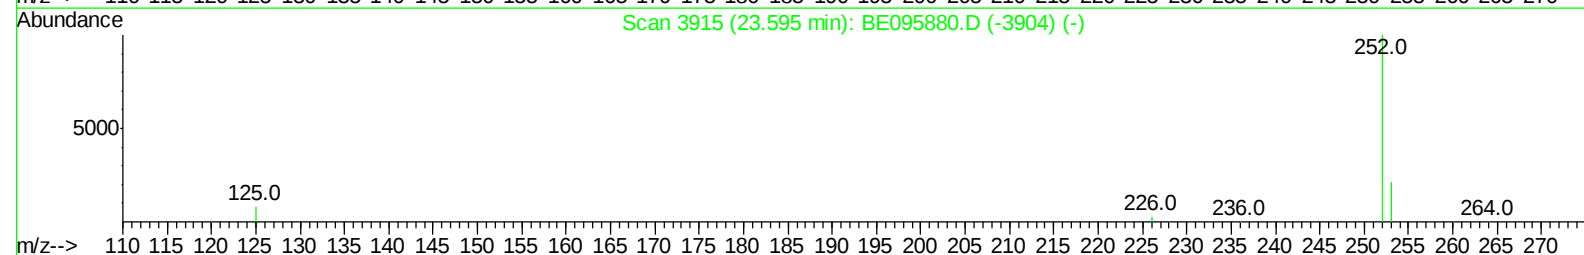
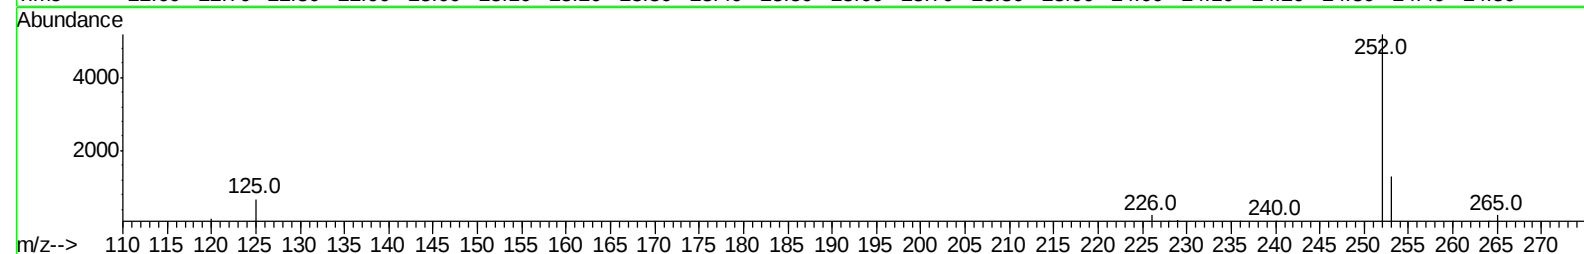


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095888.D
Acq On : 28 Mar 2018 21:54
Operator : SJ/JU
Sample : J2059-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Mar 29 05:49:07 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 04:43:20 2018
Response via : Initial Calibration

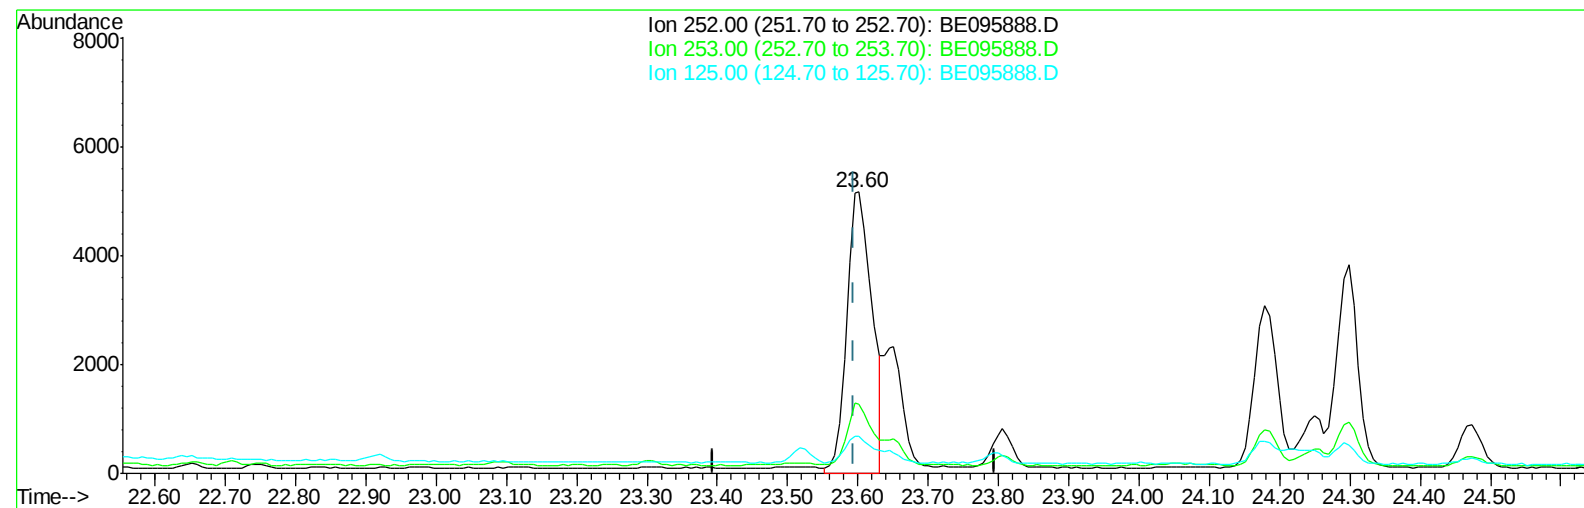

TIC: BE095888.D

(21) Benzo(b)fluoranthene

23.602min (+0.007) 0.42ng/ul m

response 12942

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	24.77
125.00	17.50	13.06
0.00	0.00	0.00