
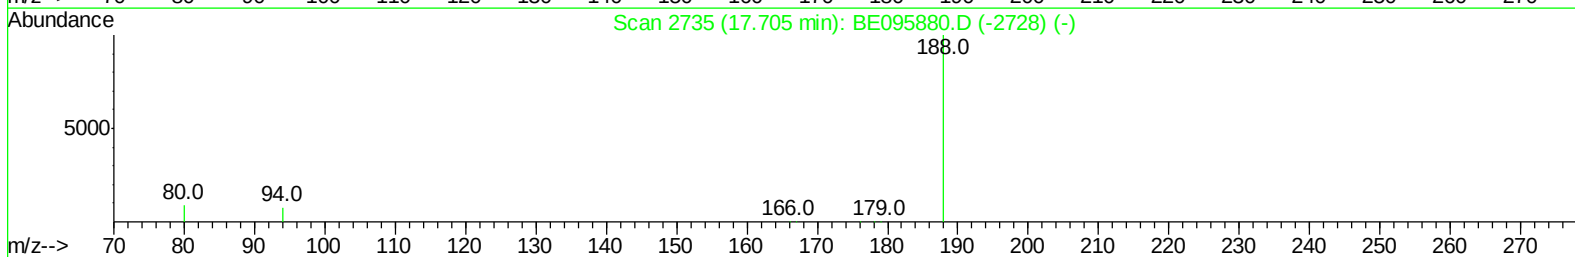
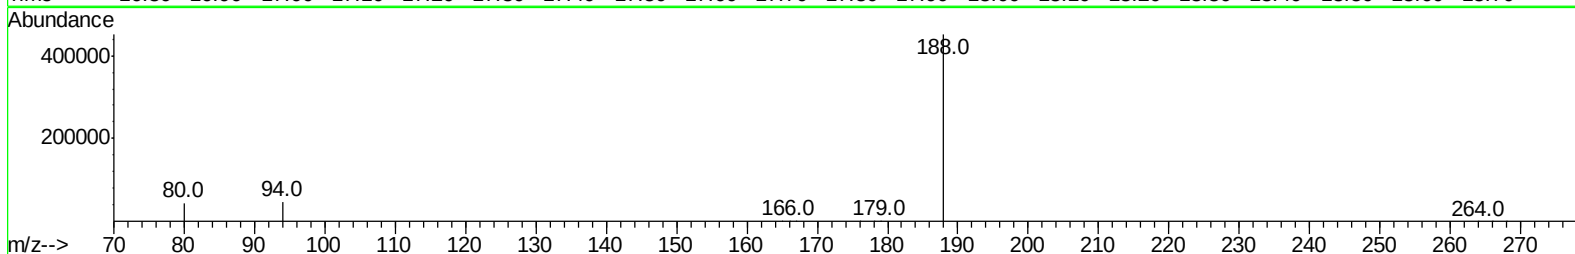


Data Path : Z:\HPCHEM1\BNA E\DATA\BE032818\
Data File : BE095890.D
Acq On : 28 Mar 2018 23:05
Operator : SJ/JU
Sample : J2059-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Mar 29 04:44:32 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 29 04:43:20 2018
Response via : Initial Calibration

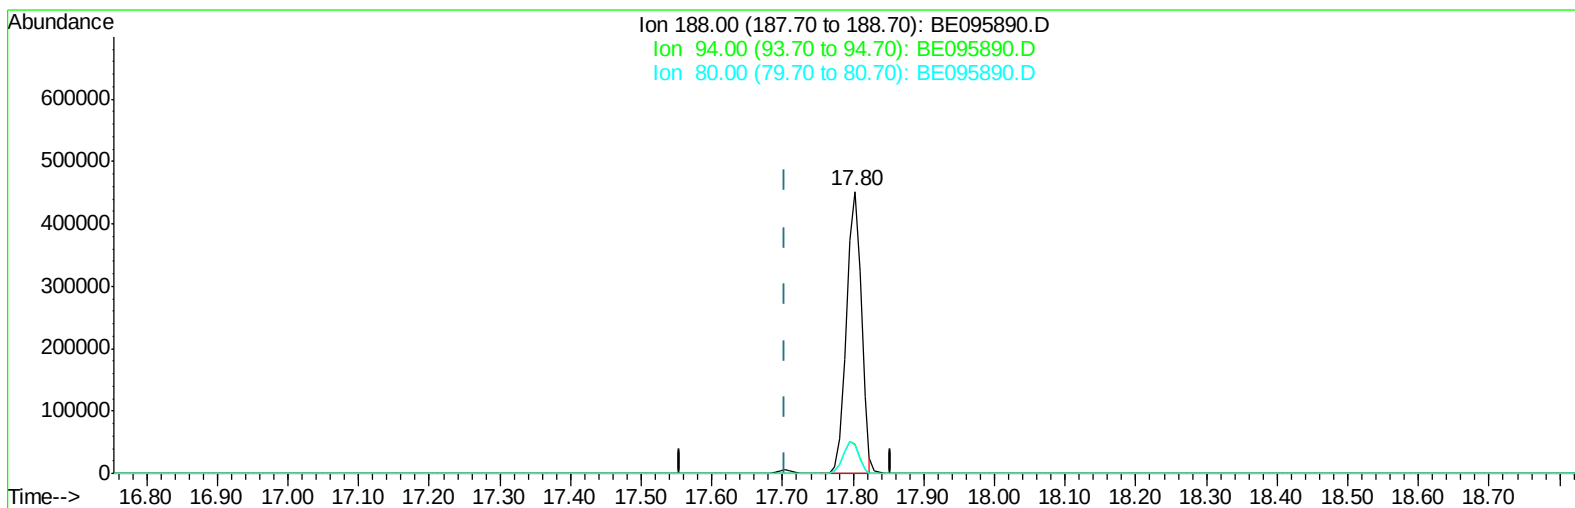

TIC: BE095890.D

(10) Phenanthrene-d10 (I)

17.802min (+0.097) 0.40ng/ul

response 653185

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.31
80.00	11.80	9.83
0.00	0.00	0.00